
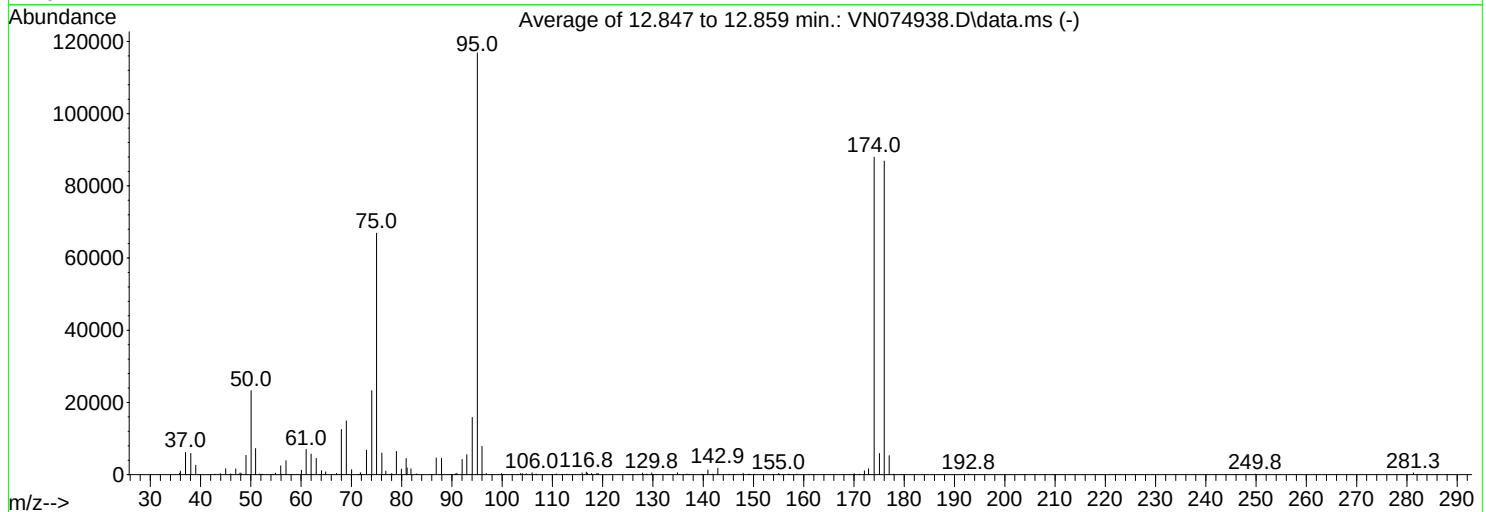


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102022\
Data File : VN074938.D
Acq On : 20 Oct 2022 13:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
Title : SW846 8260
Last Update : Fri Oct 21 09:37:47 2022

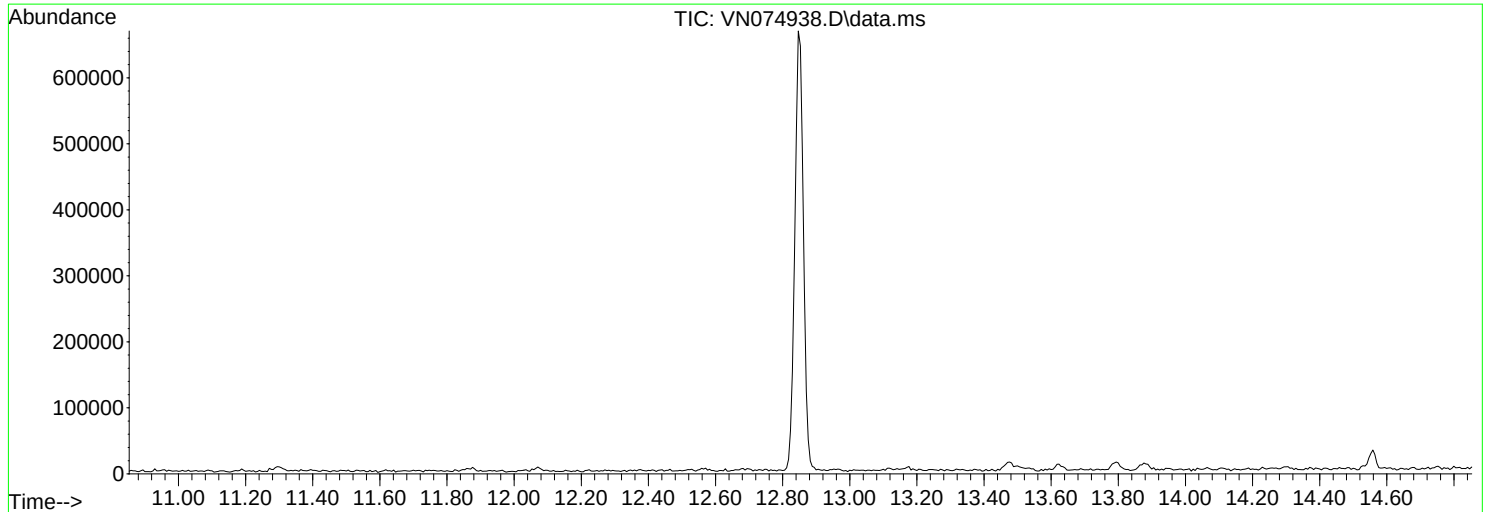

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1825

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	23293	PASS
75	95	30	60	57.2	66883	PASS
95	95	100	100	100.0	116851	PASS
96	95	5	9	6.7	7871	PASS
173	174	0.00	2	1.9	1653	PASS
174	95	50	100	75.3	87947	PASS
175	174	5	9	6.7	5862	PASS
176	174	95	101	98.8	86883	PASS
177	176	5	9	6.1	5272	PASS

Average of 12.847 to 12.859 min.: VN074938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	368	47.60	154	55.95	2447	68.00	12484
36.00	963	47.85	478	57.00	3917	69.00	14884
37.00	6174	48.10	260	57.90	56	70.05	1384
38.05	5894	49.05	5363	58.20	84	71.40	71
39.05	2638	50.05	23293	60.05	1235	71.80	527
39.90	149	50.95	7233	61.00	7000	73.00	6788
42.90	132	51.80	162	62.00	5716	74.05	23288
43.90	327	52.10	123	63.00	4500	75.00	66883
45.00	1636	52.30	85	64.05	1109	76.05	5966
46.00	241	54.25	111	64.90	767	76.85	992
47.00	1578	54.90	428	67.05	344	77.70	148

Average of 12.847 to 12.859 min.: VN074938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.05	321	91.00	410	103.70	301	117.80	311
78.95	6420	92.05	4202	104.05	259	118.85	346
79.95	1541	92.95	5525	104.80	283	119.10	364
80.90	4489	94.05	15885	105.95	553	125.20	89
81.10	1858	95.05	116851	106.80	163	126.00	51
81.85	1633	96.00	7871	110.75	236	127.90	437
83.00	210	96.85	350	112.85	128	128.10	77
86.90	4593	99.20	69	114.50	71	128.70	177
87.95	4528	99.85	308	115.90	477	128.90	84
89.90	51	100.30	111	116.75	731	129.75	494
90.70	227	103.00	113	117.00	409	130.70	52

Average of 12.847 to 12.859 min.: VN074938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
132.90	92	146.20	52	161.00	82	177.90	134
134.90	521	147.95	407	161.80	63	192.80	123
135.20	68	149.10	197	169.10	75	249.80	181
136.75	202	150.10	166	170.05	291	279.10	67
137.00	103	153.90	82	171.10	146	281.30	505
137.20	86	155.00	298	172.05	1060	282.20	134
139.75	132	155.20	121	172.90	1653	282.90	81
140.95	1297	156.90	177	174.00	87947		
141.85	148	157.10	50	175.05	5862		
142.90	1757	158.65	196	176.00	86883		
145.10	108	160.20	70	177.00	5272		

Instrument :

MSVOA_N

ClientSampleId :

BFB