
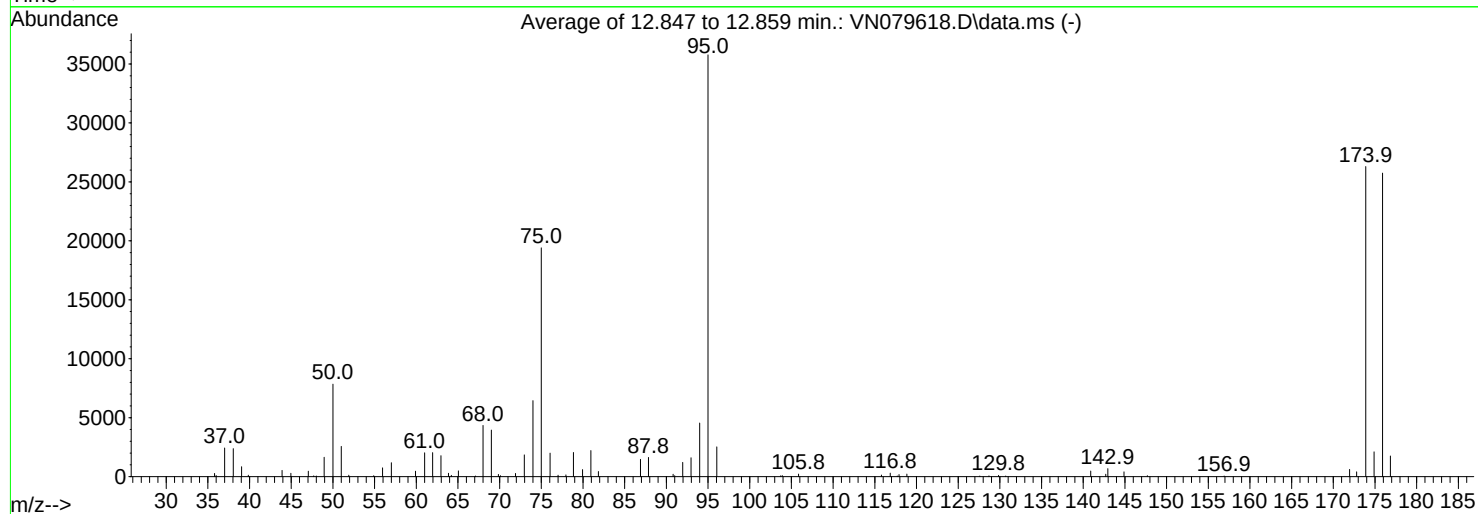


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN102023\  
Data File : VN079618.D  
Acq On : 20 Oct 2023 10:06  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N101723W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Wed Oct 18 02:19:15 2023

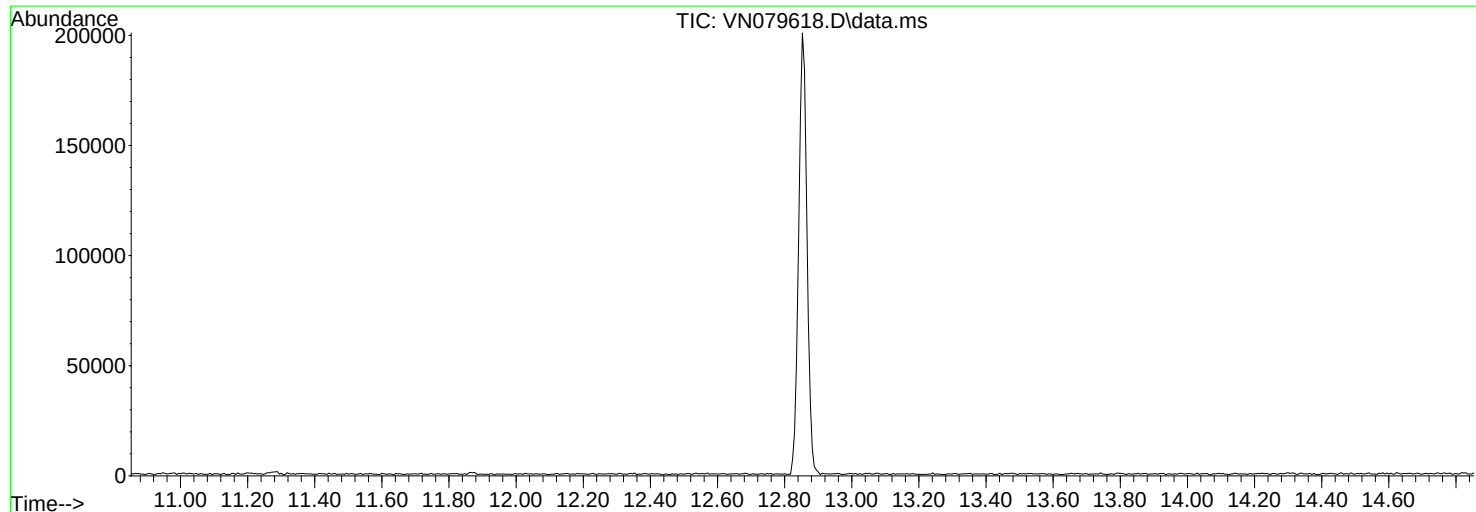

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1846

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.9  | 7838  | PASS      |
| 75     | 95      | 30     | 60     | 54.2  | 19408 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 35776 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 2520  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.5   | 402   | PASS      |
| 174    | 95      | 50     | 100    | 73.5  | 26304 | PASS      |
| 175    | 174     | 5      | 9      | 8.0   | 2099  | PASS      |
| 176    | 174     | 95     | 101    | 97.9  | 25739 | PASS      |
| 177    | 176     | 5      | 9      | 6.8   | 1754  | PASS      |