

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102120\
 Data File : VN064225.D
 Acq On : 21 Oct 2020 16:45
 Operator : JC/MD
 Sample : L4434-02
 Misc : 5.00µ/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 16757-SME

Quant Time: Oct 22 01:49:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102120W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 21 12:48:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	236670	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	415148	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	421478	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	204319	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.98	65	180575	51.38	ug/l	0.00
Spiked Amount			Recovery	=	102.76%	
35) Dibromofluoromethane	7.54	113	136552	49.47	ug/l	0.00
Spiked Amount			Recovery	=	98.94%	
50) Toluene-d8	10.06	98	517664	51.70	ug/l	0.00
Spiked Amount			Recovery	=	103.40%	
62) 4-Bromofluorobenzene	12.38	95	235689	58.07	ug/l	0.00
Spiked Amount			Recovery	=	116.14%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Methyl Iodide	3.88	142	702	0.214	ug/l #	85
13) Acrolein	3.62	56	76	0.257	ug/l #	1
16) Acetone	3.79	43	2987	2.970	ug/l	91
17) Carbon Disulfide	3.99	76	1753	0.277	ug/l #	75
18) Methyl Acetate	4.29	43	851	0.332	ug/l	92
25) 2-Butanone	6.78	43	684	0.428	ug/l #	51
29) Tetrahydrofuran	7.16	42	769	0.805	ug/l #	49
31) Cyclohexane	7.62	56	7996	1.919	ug/l #	58
36) 1,1-Dichloropropene	7.62	75	19888	4.805	ug/l #	48
38) Carbon Tetrachloride	7.62	117	26808	5.693	ug/l #	13
39) Methylcyclohexane	9.04	83	3778	1.004	ug/l	92
40) Benzene	8.00	78	8651	0.757	ug/l	97
43) Isopropyl Acetate	8.21	43	24822	3.544	ug/l #	57
51) 4-Methyl-2-Pentanone	9.96	43	6698	1.790	ug/l	91
52) Toluene	10.13	92	17176	2.350	ug/l	95
59) 2-Hexanone	10.72	43	948	0.347	ug/l #	49
67) Ethyl Benzene	11.48	91	16450	1.026	ug/l	100
68) m/p-Xylenes	11.59	106	27404	4.613	ug/l	89
69) o-Xylene	11.92	106	19447	3.385	ug/l	94
70) Styrene	11.93	104	3135	0.326	ug/l #	1
74) N-amyl acetate	12.03	43	1526	0.227	ug/l #	49
76) 1,2,3-Trichloropropane	12.38	75	126915	29.465	ug/l #	100
78) n-propylbenzene	12.57	91	4295	0.244	ug/l	97
80) 1,3,5-Trimethylbenzene	12.71	105	9936	0.754	ug/l	100
81) trans-1,4-Dichloro-2-buten	12.38	75	126915	74.390	ug/l #	9
84) 1,2,4-Trimethylbenzene	13.02	105	19924	1.519	ug/l	95
95) Naphthalene	15.10	128	121712	11.284	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102120\
Data File : VN064225.D
Acq On : 21 Oct 2020 16:45
Operator : JC/MD
Sample : L4434-02
Misc : 5.00µl/10mL/100µL/5.00mL/MSVOA_N/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
16757-SME

Quant Time: Oct 22 01:49:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N102120W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 21 12:48:40 2020
Response via : Initial Calibration

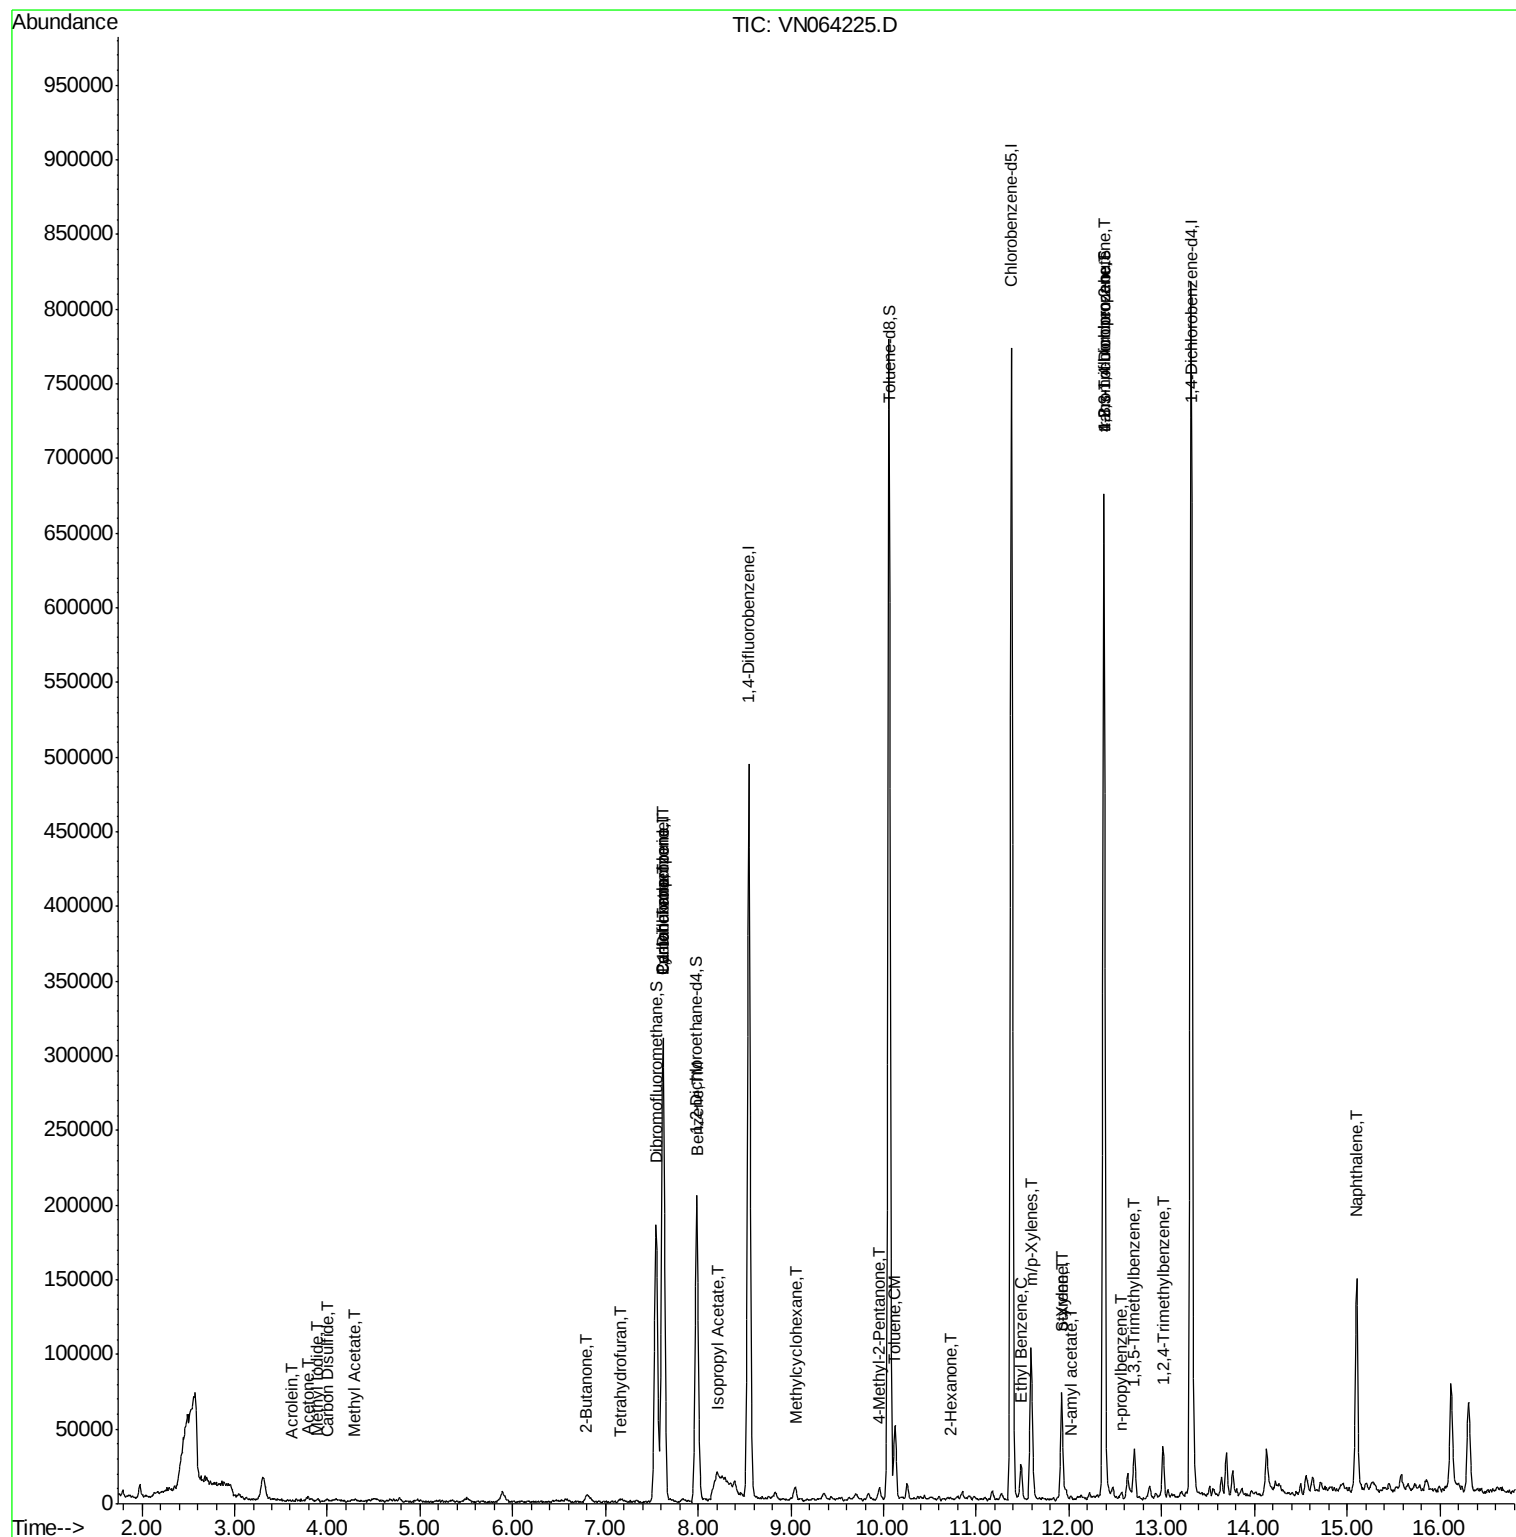



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1829

Delta R.T. -0.00 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampleId :


16757-SME

Tot Ion:168 Resp: 236670

Ion Ratio Lower Upper

168 100

99 66.3 54.0 81.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.62

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

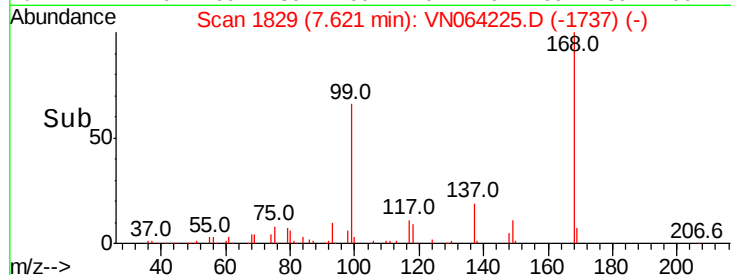

#10

Methyl Iodide

Concen: 0.214 ug/l

RT: 3.88 min Scan# 665

Delta R.T. -0.04 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45


Tgt Ion:142 Resp: 702

Ion Ratio Lower Upper

142 100

127 45.0 41.0 61.6

141 0.0 11.3 16.9#



Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

3.88


600


400

200

0

Time--> 3.84 3.86 3.88





#13

Acrolein

Concen: 0.257 ug/l

RT: 3.62 min Scan# 585

Delta R.T. 0.05 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampleId :


16757-SME

Tot Ion: 56 Resp: 76

Ion Ratio Lower Upper




56 100

55 365.8 56.1 84.1#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

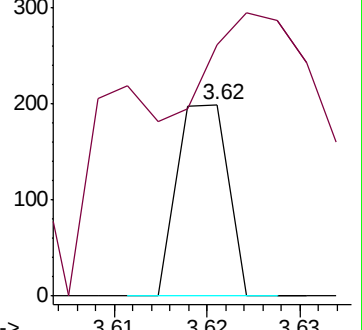

#16

Acetone

Concen: 2.970 ug/l

RT: 3.79 min Scan# 639

Delta R.T. 0.02 min

Lab File: VN064225.D


Acq: 21 Oct 2020 16:45

Tgt Ion: 43 Resp: 2987

Ion Ratio Lower Upper



43 100


58 30.9 21.0 31.4



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




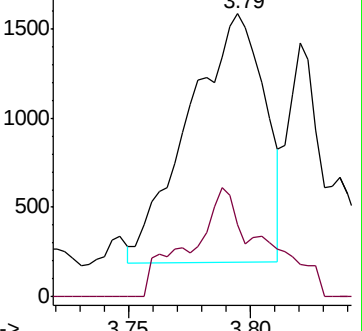


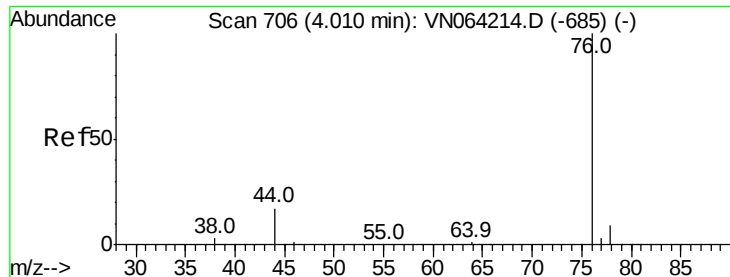

#17
Carbon Disulfide
Concen: 0.277 ug/l
RT: 3.99 min Scan# 700
Delta R.T. -0.02 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45




Instrument :
MSVOA_N
ClientSampleId :
16757-SME


Tot Ion: 76 Resp: 1753
Ion Ratio Lower Upper
76 100
78 0.0 7.1 10.7#

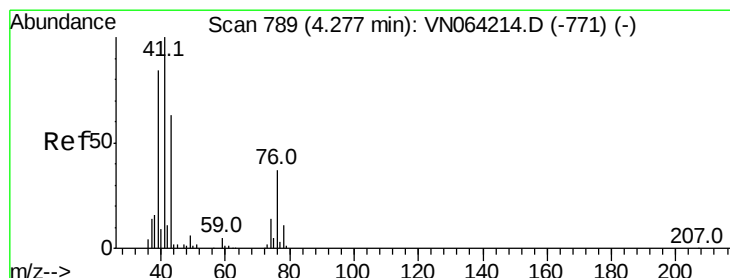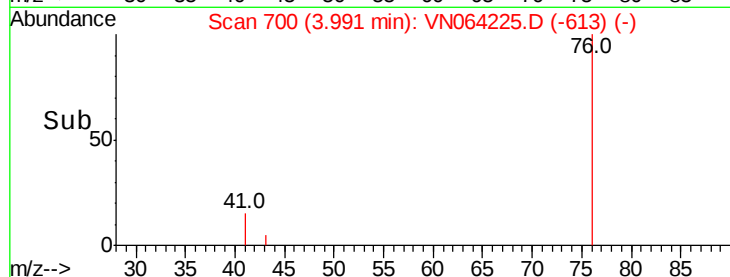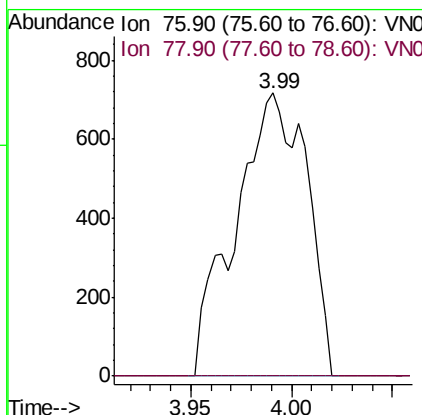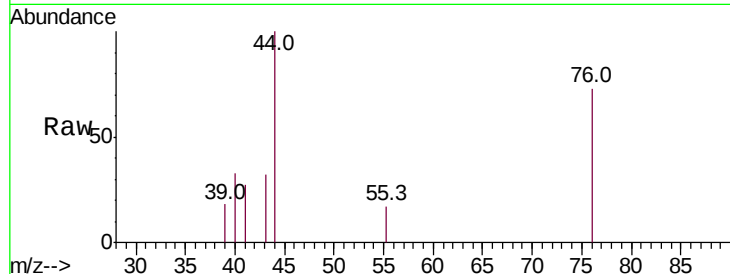

#18
Methyl Acetate
Concen: 0.332 ug/l
RT: 4.29 min Scan# 792
Delta R.T. 0.01 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion: 43 Resp: 851
Ion Ratio Lower Upper
43 100
74 18.3 17.9 26.9


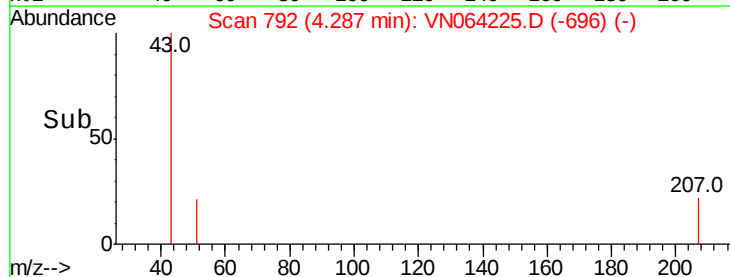
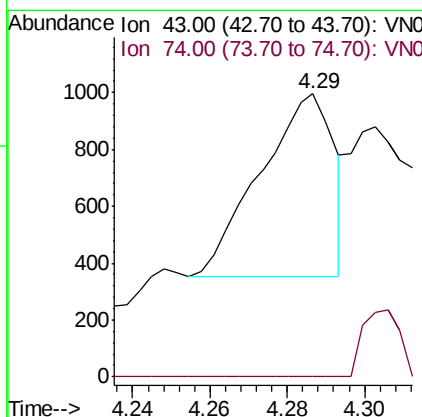
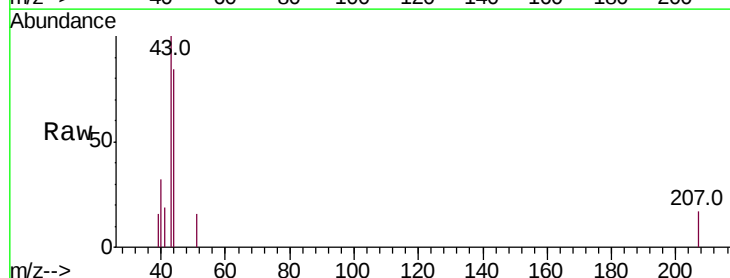




#25
2-Butanone
Concen: 0.428 ug/l
RT: 6.78 min Scan# 1568
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45




Instrument :
MSVOA_N
ClientSampled :
16757-SME


Tot Ion: 43 Resp: 684
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.0#

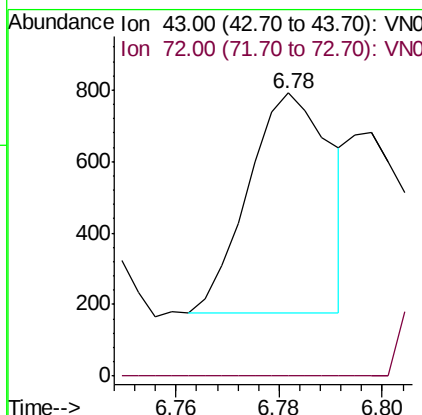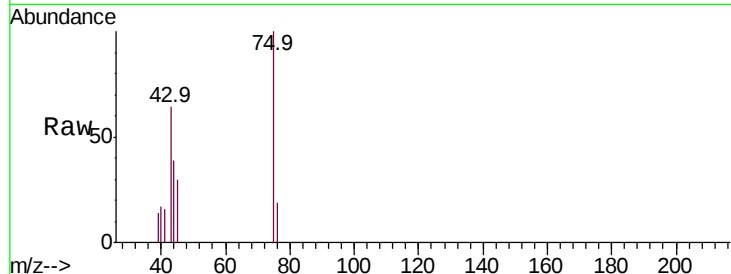

#29
Tetrahydrofuran
Concen: 0.805 ug/l
RT: 7.16 min Scan# 1686
Delta R.T. -0.01 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion: 42 Resp: 769
Ion Ratio Lower Upper
42 100
72 0.0 30.8 46.2#
71 13.8 29.0 43.6#

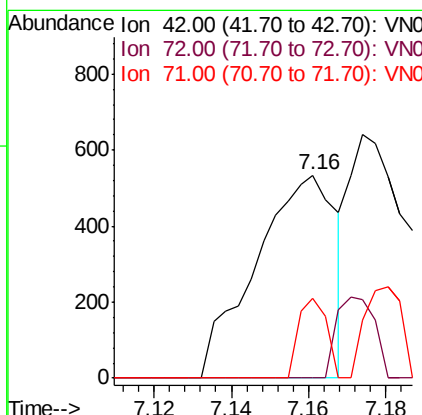



#31

Cyclohexane

Concen: 1.919 ug/l

RT: 7.62 min Scan# 1828

Delta R.T. 0.00 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampled :

16757-SME


Tot Ion: 56 Resp: 7996

Ion Ratio Lower Upper

56 100

69 113.3 29.8 44.6#




84 81.0 68.1 102.1



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

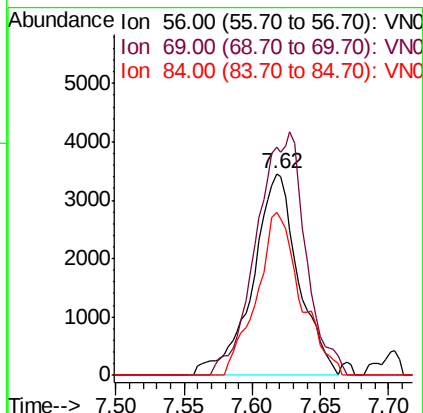

#33

1,2-Dichloroethane-d4

Concen: 51.377 ug/l

RT: 7.98 min Scan# 1942

Delta R.T. -0.00 min

Lab File: VN064225.D


Acq: 21 Oct 2020 16:45

Tgt Ion: 65 Resp: 180575

Ion Ratio Lower Upper



65 100


67 49.4 0.0 100.2



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

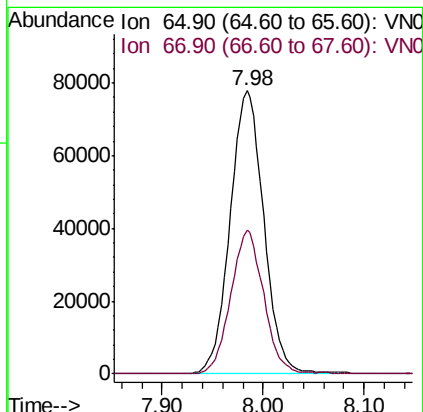



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2117

Delta R.T. -0.00 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampleId :

16757-SME


Tot Ion:114 Resp: 415148

Ion Ratio Lower Upper

114 100

63 24.0 0.0 44.0




88 17.4 0.0 34.2



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

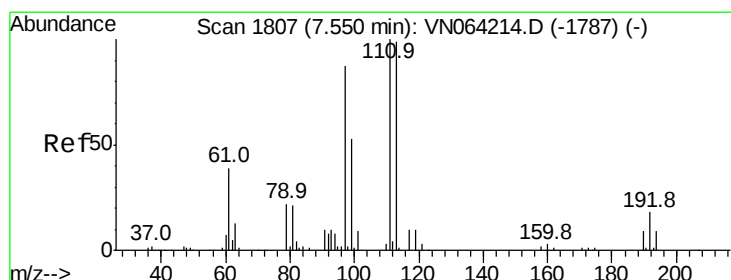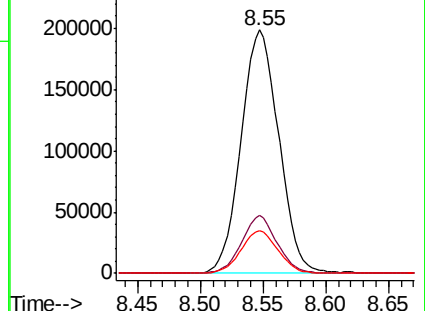

#35

Dibromofluoromethane

Concen: 49.474 ug/l

RT: 7.54 min Scan# 1805

Delta R.T. -0.01 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45


Tgt Ion:113 Resp: 136552

Ion Ratio Lower Upper

113 100

111 103.4 84.2 126.2



192 19.3 15.2 22.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



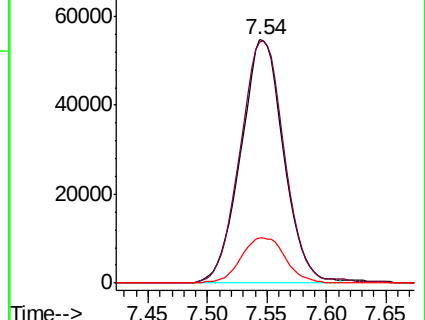





#36
 1,1-Dichloropropene
 Concen: 4.805 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN064225.D
 Acq: 21 Oct 2020 16:45




Instrument :
 MSVOA_N
 ClientSampleId :
 16757-SME


Tot Ion: 75 Resp: 19888
 Ion Ratio Lower Upper
 75 100
 110 6.7 17.2 51.6#
 77 0.0 24.9 37.3#

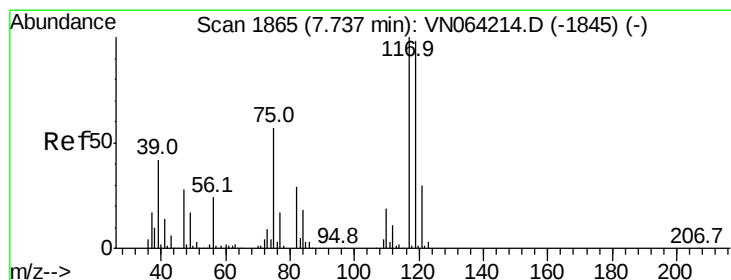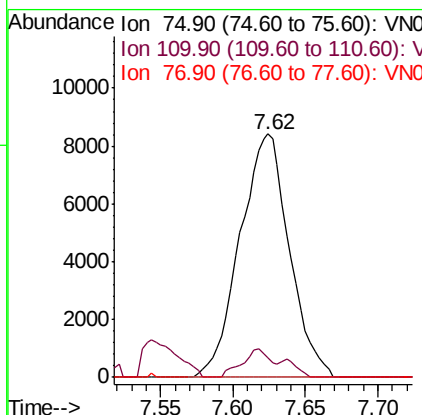

#38
 Carbon Tetrachloride
 Concen: 5.693 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.11 min
 Lab File: VN064225.D
 Acq: 21 Oct 2020 16:45

Tgt Ion: 117 Resp: 26808
 Ion Ratio Lower Upper
 117 100
 119 2.6 78.5 117.7#
 121 0.0 24.3 36.5#

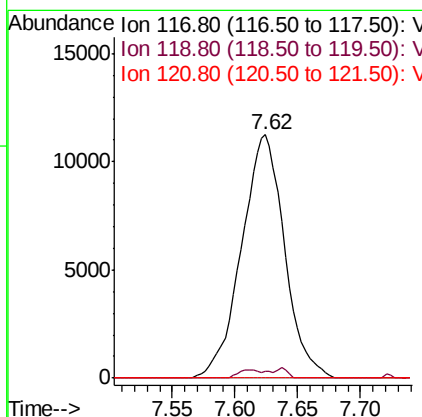


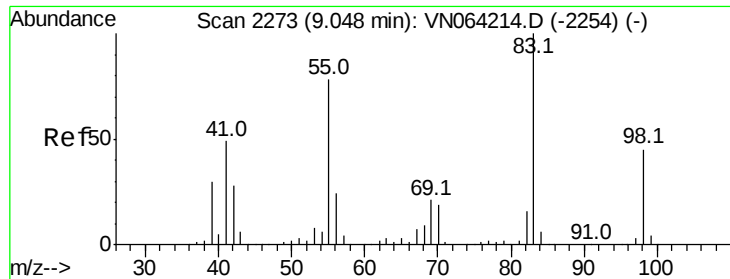




#39
Methvlcvclohexane
Concen: 1.004 ug/l
RT: 9.04 min Scan# 2271
Delta R.T. -0.01 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Instrument :
MSVOA_N
ClientSampleId :
16757-SME

Tot Ion: 83 Resp: 3778
Ion Ratio Lower Upper
83 100
55 71.6 62.2 93.2
98 38.9 35.9 53.9

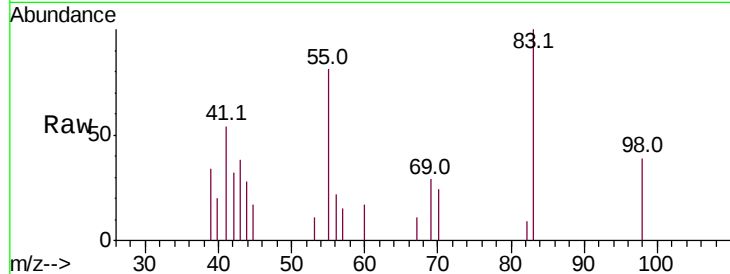


Abundance Ion 83.00 (82.70 to 83.70): VN0
Ion 55.00 (54.70 to 55.70): VN0
Ion 98.00 (97.70 to 98.70): VN0

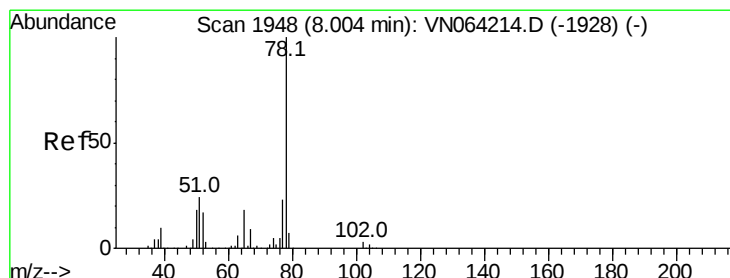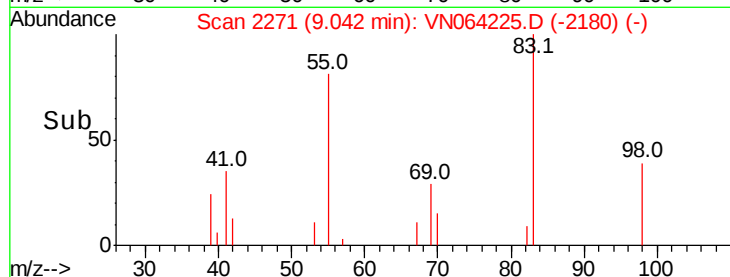
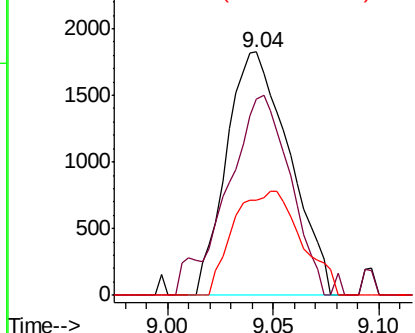



#40
Benzene
Concen: 0.757 ug/l
RT: 8.00 min Scan# 1947
Delta R.T. -0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion: 78 Resp: 8651
Ion Ratio Lower Upper
78 100
77 24.2 18.3 27.5

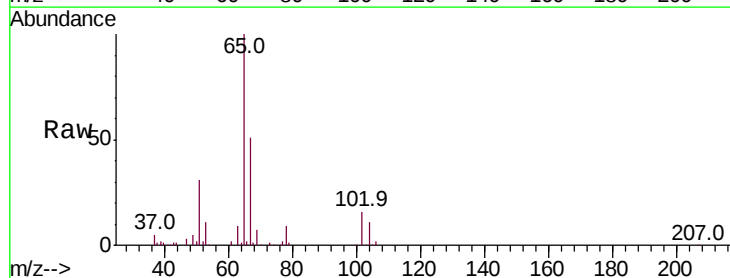

Abundance Ion 78.00 (77.70 to 78.70): VN0
Ion 77.00 (76.70 to 77.70): VN0

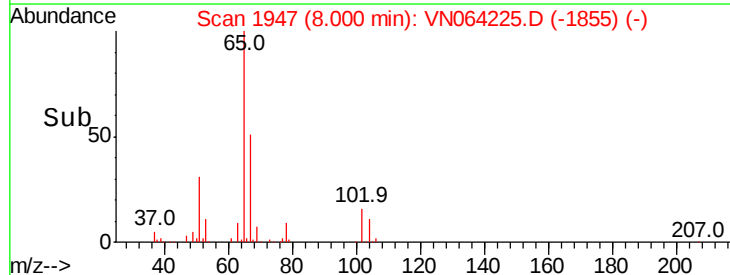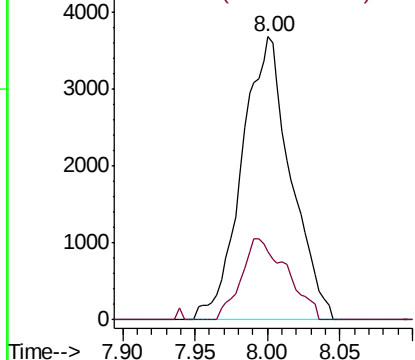



#43

Isopropyl Acetate

Concen: 3.544 ug/l

RT: 8.21 min Scan# 2013

Delta R.T. 0.09 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampleId :

16757-SME


Tot Ion: 43 Resp: 24822

Ion Ratio Lower Upper

43 100

61 0.0 19.6 29.4#




87 0.0 9.8 14.6#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

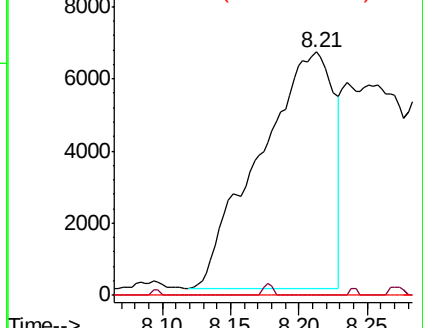

#50

Toluene-d8

Concen: 51.703 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN064225.D


Acq: 21 Oct 2020 16:45

Tgt Ion: 98 Resp: 517664

Ion Ratio Lower Upper



98 100


100 65.0 50.8 76.2



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0




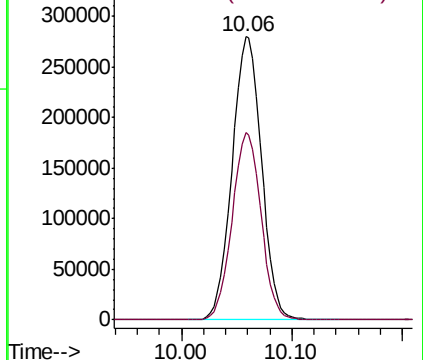




#51
4-Methyl-2-Pentanone
Concen: 1.790 ug/l
RT: 9.96 min Scan# 2555
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45




Instrument :
MSVOA_N
ClientSampleId :
16757-SME


Tot Ion: 43 Resp: 6698
Ion Ratio Lower Upper
43 100
58 30.6 28.6 42.8

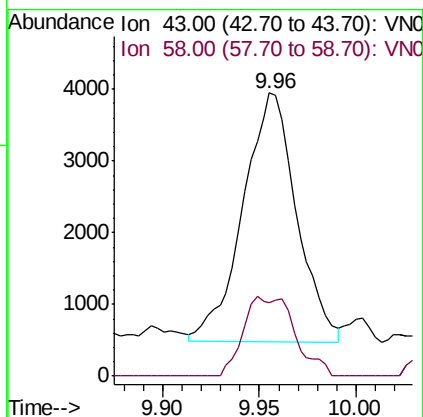

#52
Toluene
Concen: 2.350 ug/l
RT: 10.13 min Scan# 2608
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion: 92 Resp: 17176
Ion Ratio Lower Upper
92 100
91 179.4 137.4 206.2



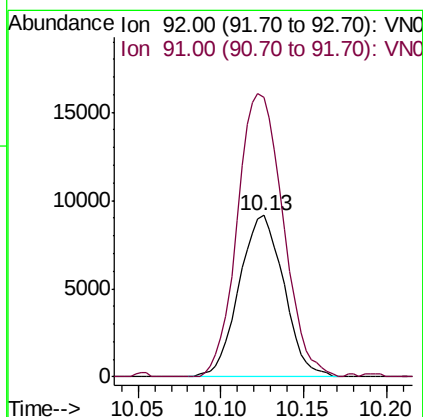





#59
2-Hexanone
Concen: 0.347 ug/l
RT: 10.72 min Scan# 2794
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45




Instrument :
MSVOA_N
ClientSampled :
16757-SME


Tot Ion: 43 Resp: 948
Ion Ratio Lower Upper
43 100
58 14.5 24.8 74.3#

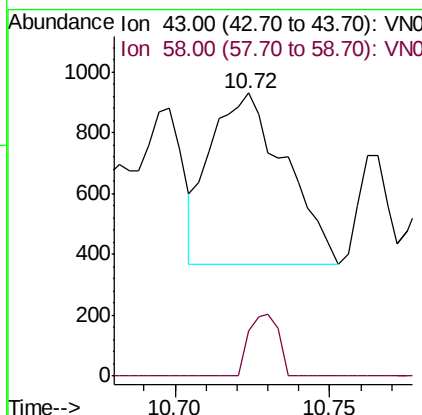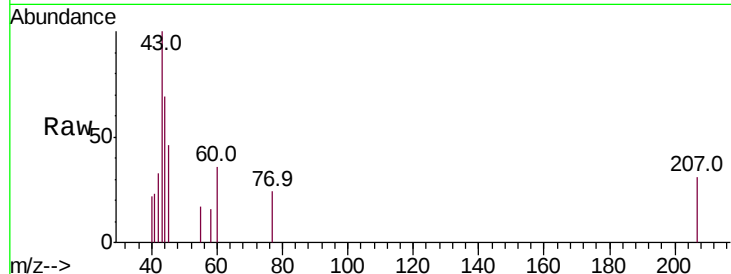

#62
4-Bromofluorobenzene
Concen: 58.067 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion: 95 Resp: 235689
Ion Ratio Lower Upper
95 100
174 72.9 0.0 144.4
176 69.9 0.0 139.2



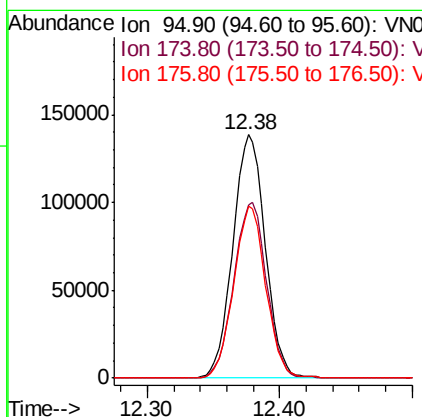





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45




Instrument :
MSVOA_N
ClientSampleId :
16757-SME


Tot Ion:117 Resp: 421478
Ion Ratio Lower Upper
117 100
82 59.9 48.8 73.2
119 32.1 24.7 37.1

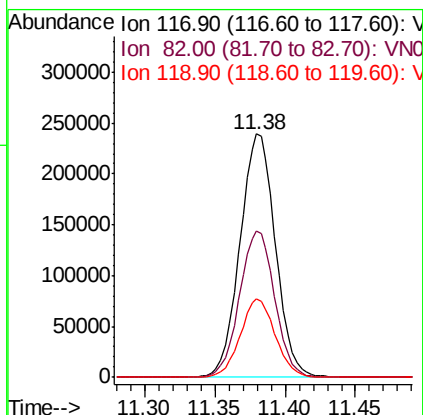

#67
Ethyl Benzene
Concen: 1.026 ug/l
RT: 11.48 min Scan# 3030
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion: 91 Resp: 16450
Ion Ratio Lower Upper
91 100
106 30.8 24.8 37.2

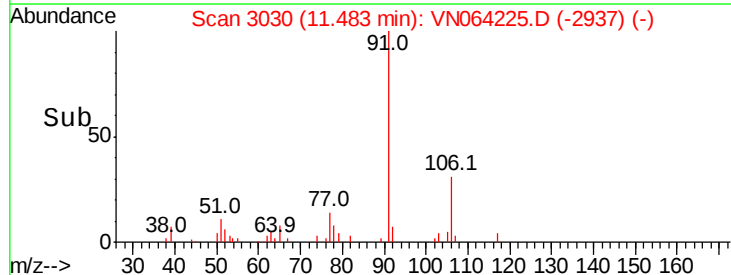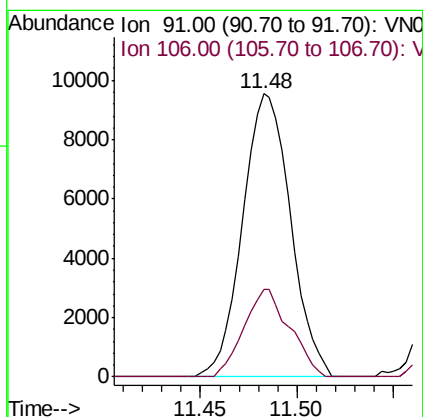







#68
m/p-Xylenes
Concen: 4.613 ug/l
RT: 11.59 min Scan# 3064
Delta R.T. -0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Instrument :
MSVOA_N
ClientSampleId :
16757-SME

Tot Ion:106 Resp: 27404
Ion Ratio Lower Upper
106 100
91 232.5 172.2 258.2




Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN


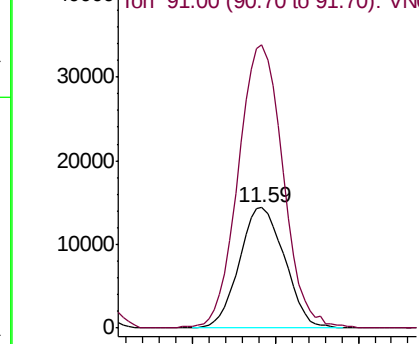



#69
o-Xylene
Concen: 3.385 ug/l
RT: 11.92 min Scan# 3166
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion:106 Resp: 19447
Ion Ratio Lower Upper
106 100
91 210.3 109.9 329.6



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN




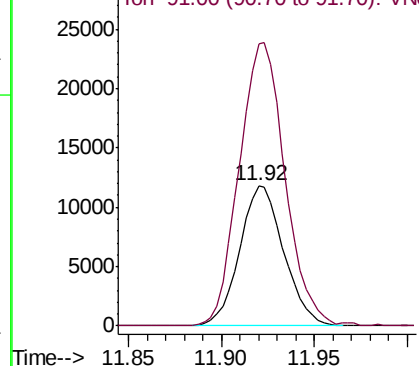


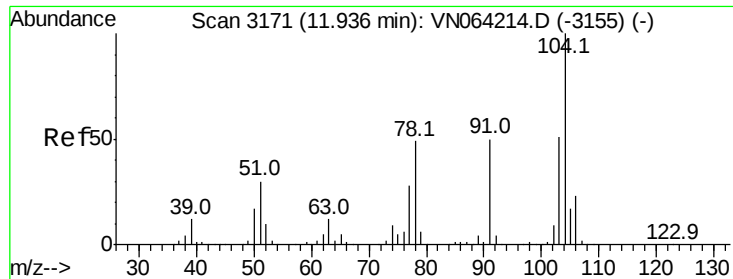

#70
Stvrene
Concen: 0.326 ug/l
RT: 11.93 min Scan# 3170
Delta R.T. -0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45




Instrument :
MSVOA_N
ClientSampleId :
16757-SME


Tot Ion:104 Resp: 3135
Ion Ratio Lower Upper
104 100
78 152.4 43.8 65.6#
103 103.4 43.4 65.2#

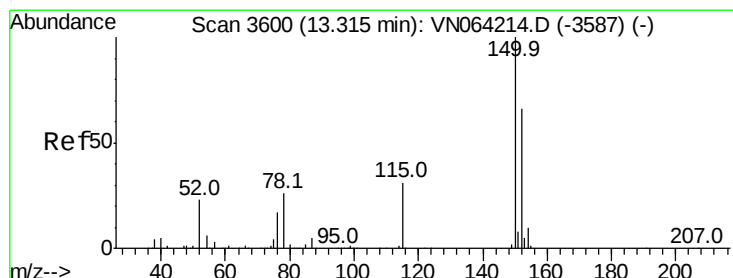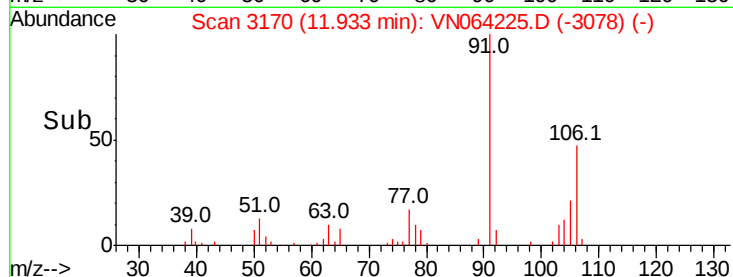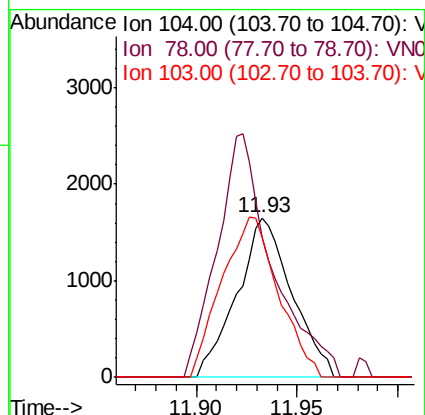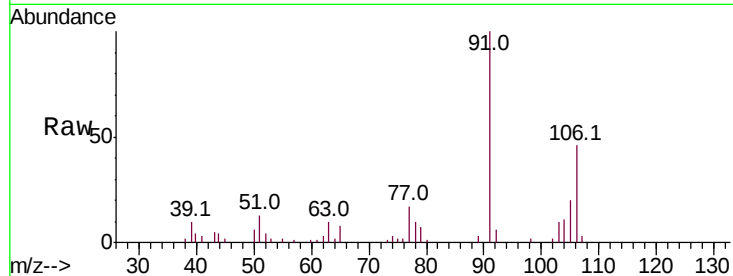

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Tgt Ion:152 Resp: 204319
Ion Ratio Lower Upper
152 100
115 63.4 32.0 96.2
150 160.3 0.0 356.6

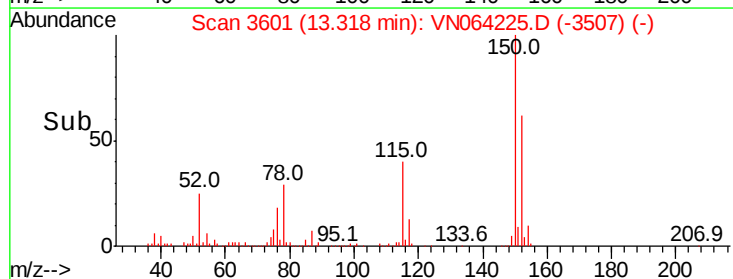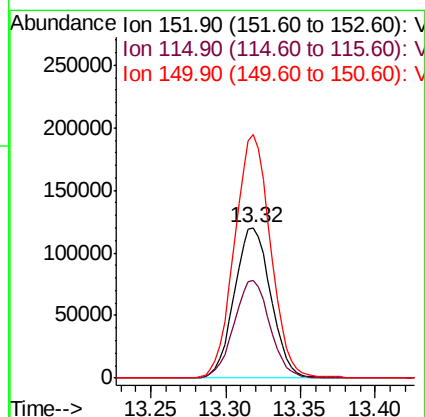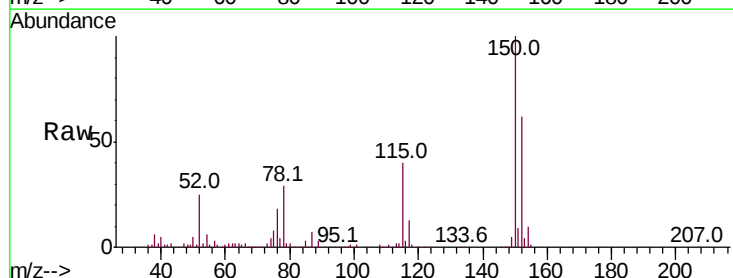



#74

N-amvl acetate

Concen: 0.227 ug/l

RT: 12.03 min Scan# 3201

Delta R.T. -0.01 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampleId :

16757-SME

Tot Ion: 43 Resp: 1526


Ion Ratio Lower Upper

43 100

70 4.4 30.2 45.4#

55 0.0 18.0 27.0#

61 0.0 17.4 26.2#






Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

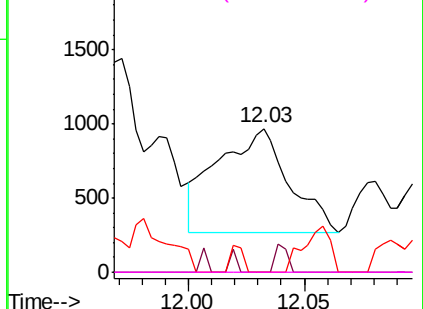

#76

1,2,3-Trichloropropane

Concen: 29.465 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064225.D


Acq: 21 Oct 2020 16:45

Tgt Ion: 75 Resp: 126915

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

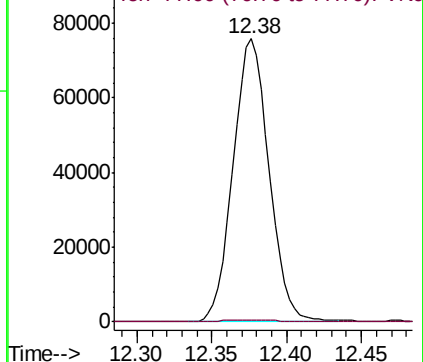



#78

n-propylbenzene

Concen: 0.244 ug/l

RT: 12.57 min Scan# 3367

Delta R.T. 0.00 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampled :


16757-SME

Tot Ion: 91 Resp: 4295

Ion Ratio Lower Upper




91 100

120 20.7 11.1 33.1



Abundance Ion 91.00 (90.70 to 91.70): VN064214.D (-3355) (-)

Ion 120.00 (119.70 to 120.70): VN064214.D (-3355) (-)

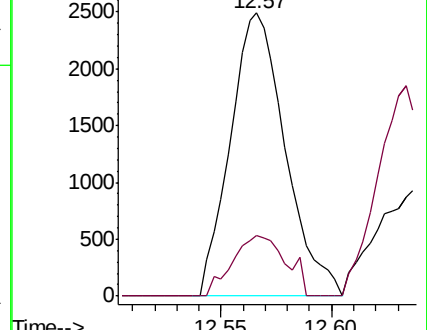

#80

1,3,5-Trimethylbenzene

Concen: 0.754 ug/l

RT: 12.71 min Scan# 3411

Delta R.T. 0.00 min

Lab File: VN064225.D


Acq: 21 Oct 2020 16:45

Tgt Ion: 105 Resp: 9936

Ion Ratio Lower Upper



105 100


120 46.7 23.4 70.0



Abundance Ion 105.00 (104.70 to 105.70): VN064214.D (-3394) (-)

Ion 120.00 (119.70 to 120.70): VN064214.D (-3394) (-)

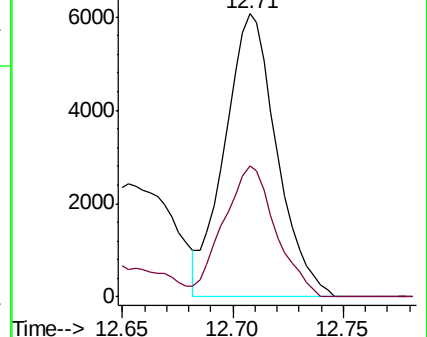



#81

trans-1,4-Dichloro-2-butene

Concen: 74.390 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064225.D

Acq: 21 Oct 2020 16:45

Instrument :

MSVOA_N

ClientSampleId :

16757-SME


Tot Ion: 75 Resp: 126915

Ion Ratio Lower Upper

75 100

53 0.0 81.0 121.4#




89 0.0 38.7 58.1#



Abundance Ion 74.90 (74.60 to 75.60): VN064225.D (-3183) (-)

Ion 53.00 (52.70 to 53.70): VN064225.D (-3183) (-)

Ion 88.90 (88.60 to 89.60): VN064225.D (-3183) (-)

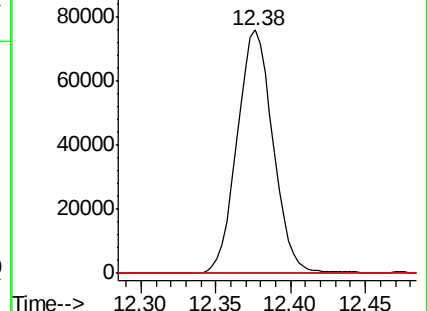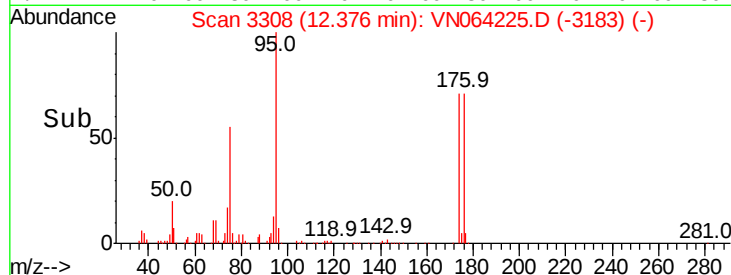

#84

1,2,4-Trimethylbenzene

Concen: 1.519 ug/l

RT: 13.02 min Scan# 3507

Delta R.T. 0.00 min

Lab File: VN064225.D


Acq: 21 Oct 2020 16:45

Tgt Ion: 105 Resp: 19924

Ion Ratio Lower Upper



105 100


120 40.1 21.5 64.5



Abundance Ion 105.00 (104.70 to 105.70): VN064225.D (-3413) (-)

Ion 120.00 (119.70 to 120.70): VN064225.D (-3413) (-)

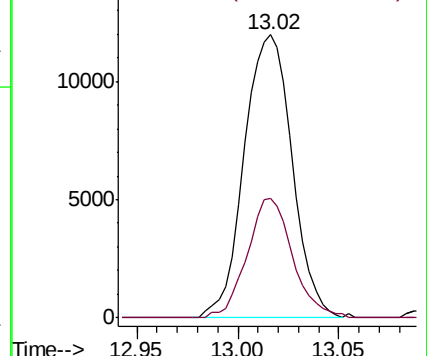




#95
Naphthalene
Concen: 11.284 ug/l
RT: 15.10 min Scan# 4156
Delta R.T. 0.00 min
Lab File: VN064225.D
Acq: 21 Oct 2020 16:45

Instrument :
MSVOA_N
ClientSampleId :
16757-SME

Tot Ion	Ratio	Lower	Upper
128	100		
127	12.6	10.5	15.7
129	11.2	8.6	12.8



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

