
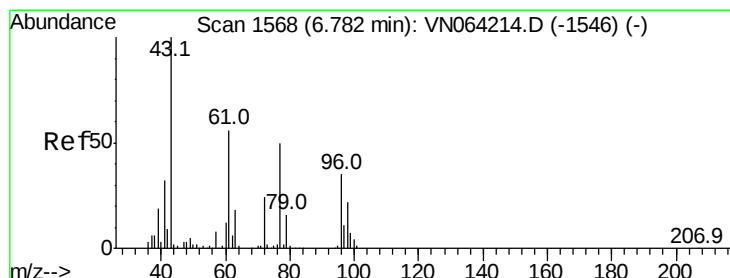
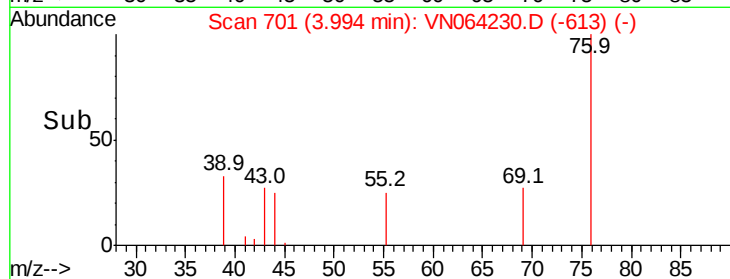
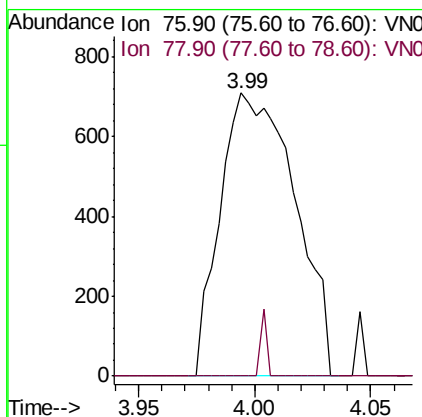


#17
Carbon Disulfide
Concen: 0.257 ug/l
RT: 3.99 min Scan# 701
Delta R.T. -0.02 min
Lab File: VN064230.D
Acq: 21 Oct 2020 18:43




Instrument :
MSVOA_N
ClientSampleId :
16757-A


Tot Ion: 76 Resp: 1589
Ion Ratio Lower Upper
76 100
78 0.0 7.1 10.7#

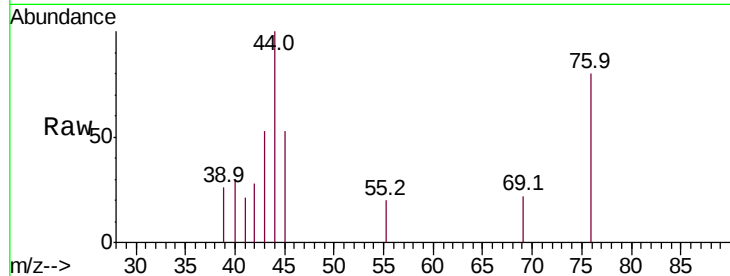

#25
2-Butanone
Concen: 9.026 ug/l
RT: 6.79 min Scan# 1570
Delta R.T. 0.01 min
Lab File: VN064230.D
Acq: 21 Oct 2020 18:43

Tgt Ion: 43 Resp: 14076
Ion Ratio Lower Upper
43 100
72 19.5 19.4 29.0


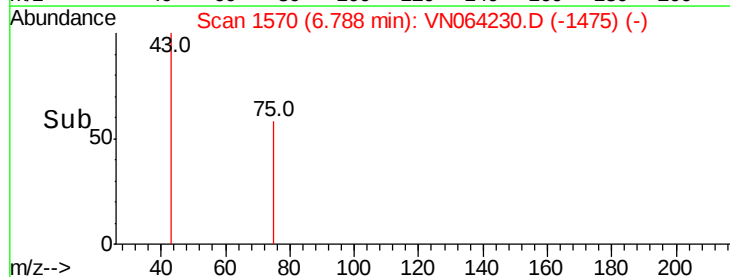
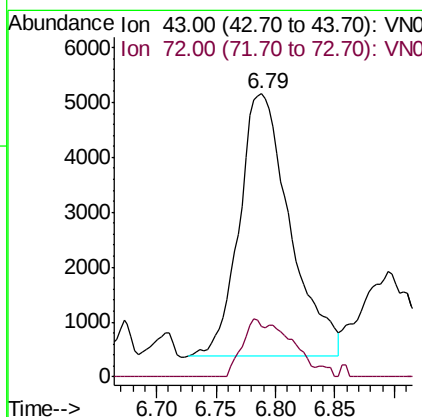
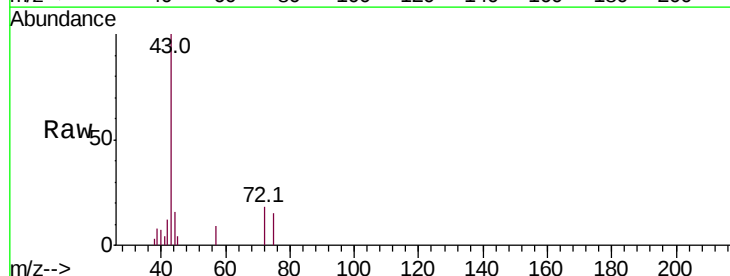


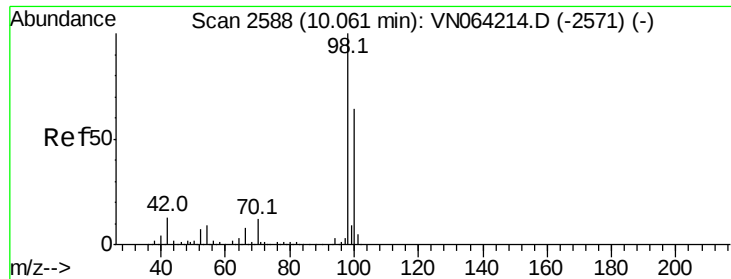

#50
Toluene-d8
Concen: 51.725 ug/l
RT: 10.06 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN064230.D
Acq: 21 Oct 2020 18:43

Instrument :
MSVOA_N
ClientSampled :
16757-A

Tot Ion: 98 Resp: 512955
Ion Ratio Lower Upper
98 100
100 64.2 50.8 76.2

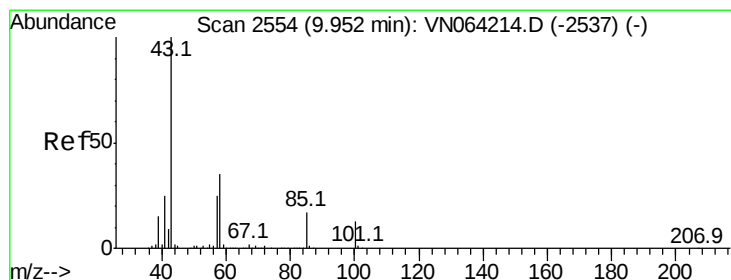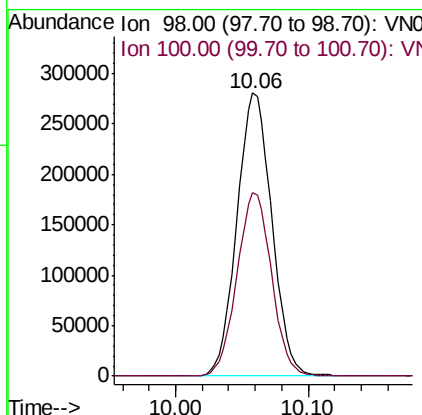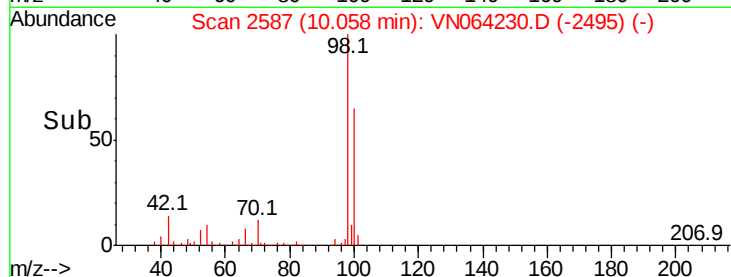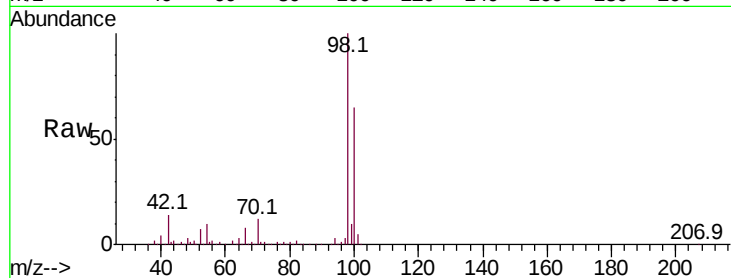

#51
4-Methyl-2-Pentanone
Concen: 0.722 ug/l
RT: 9.95 min Scan# 2553
Delta R.T. -0.00 min
Lab File: VN064230.D
Acq: 21 Oct 2020 18:43

Tgt Ion: 43 Resp: 2675
Ion Ratio Lower Upper
43 100
58 27.2 28.6 42.8#

