


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102120\
 Data File : VN064210.D
 Acq On : 21 Oct 2020 9:11
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102120W.M
 Title : SW846 8260
 Last Update : Wed Oct 21 12:48:40 2020

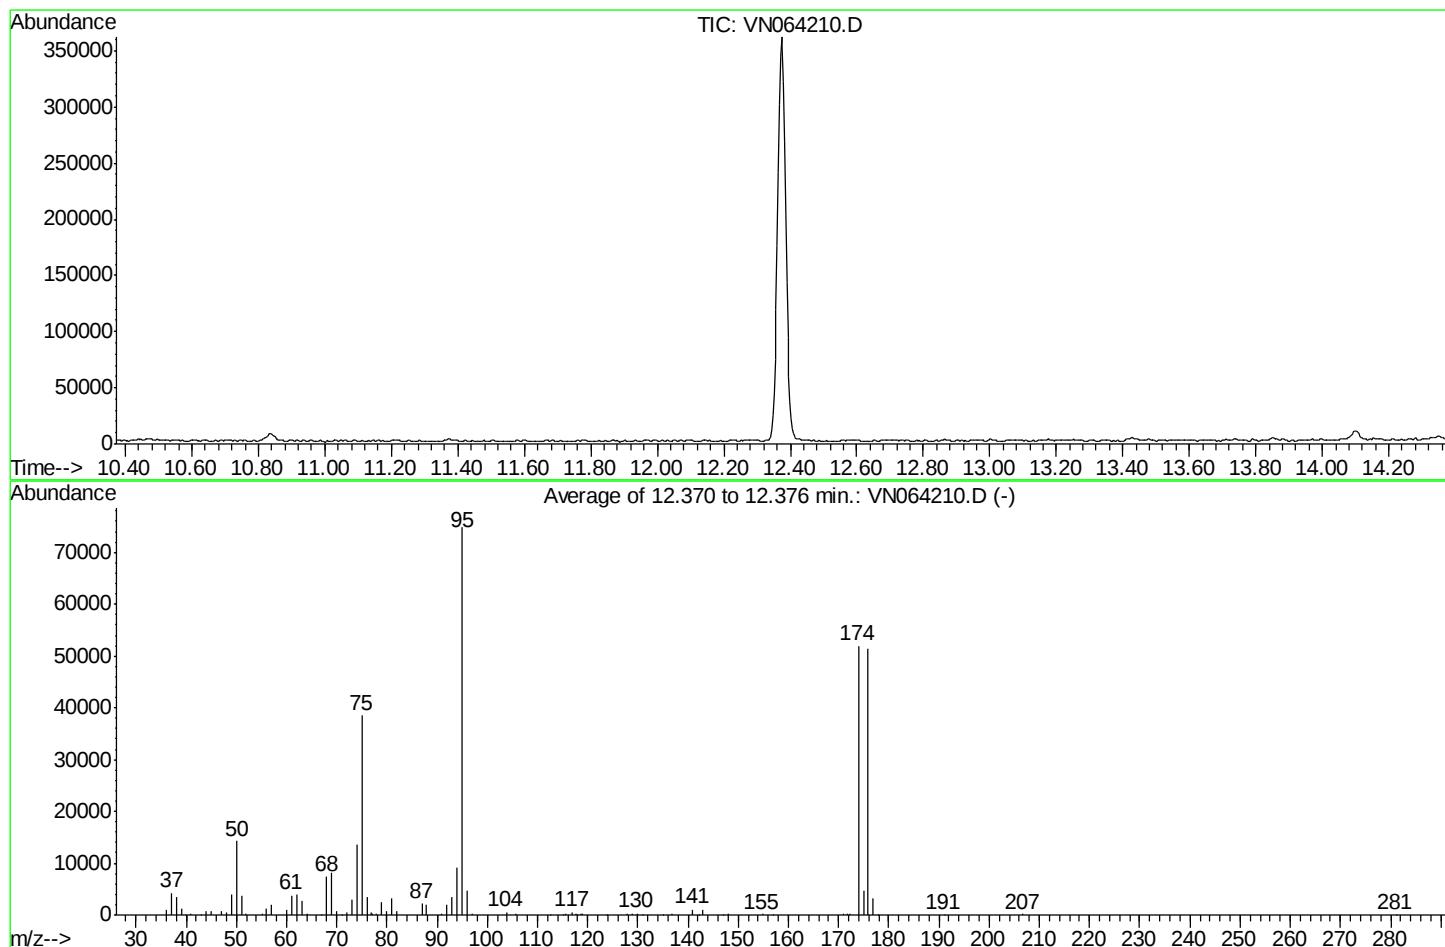

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	14238	PASS
75	95	30	60	51.4	38442	PASS
95	95	100	100	100.0	74845	PASS
96	95	5	9	6.3	4705	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.5	52000	PASS
175	174	5	9	8.9	4620	PASS
176	174	95	101	98.7	51309	PASS
177	176	5	9	6.3	3251	PASS