


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102120\
Data File : VN064236.D
Acq On : 21 Oct 2020 23:21
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102120W.M
Title : SW846 8260
Last Update : Wed Oct 21 12:48:40 2020

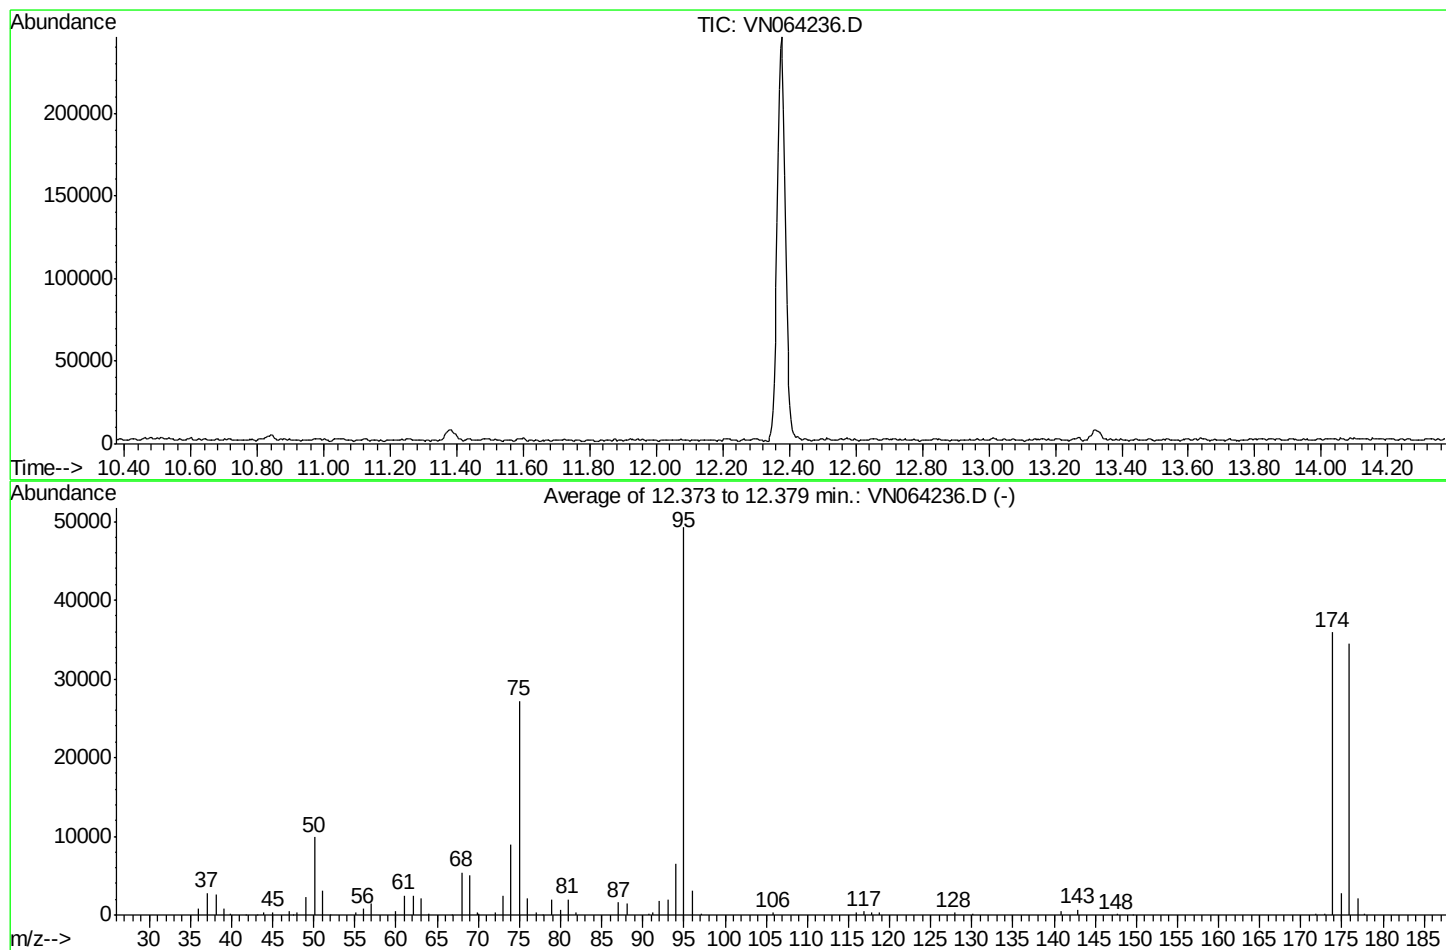

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	9902	PASS
75	95	30	60	55.2	27181	PASS
95	95	100	100	100.0	49253	PASS
96	95	5	9	6.3	3100	PASS
173	174	0.00	2	0.5	174	PASS
174	95	50	100	72.9	35928	PASS
175	174	5	9	7.8	2788	PASS
176	174	95	101	96.0	34498	PASS
177	176	5	9	6.2	2129	PASS