

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102121\
 Data File : VN069086.D
 Acq On : 21 Oct 2021 14:22
 Operator : JC/MD
 Sample : M4253-11 10X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 22 01:33:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	338861	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	587761	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	557101	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	219524	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	220503	49.354	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.700%
35) Dibromofluoromethane	8.024	113	172722	50.509	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.020%
50) Toluene-d8	10.443	98	738241	53.955	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.900%
62) 4-Bromofluorobenzene	12.733	95	269031	52.115	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	104.220%


Target Compounds				Qvalue		
5) Bromomethane	2.880	94	733	0.317	ug/l #	26
16) Acetone	4.291	43	440	0.264	ug/l #	81
19) Methyl tert-butyl Ether	5.621	73	10859	0.891	ug/l #	37
20) Methylene Chloride	5.087	84	829	0.216	ug/l	92
31) Cyclohexane	8.096	56	18688	2.690	ug/l #	62
36) 1,1-Dichloropropene	8.088	75	27696	5.517	ug/l #	45
38) Carbon Tetrachloride	8.088	117	35399	6.420	ug/l #	16
39) Methylcyclohexane	9.464	83	9902	1.532	ug/l	98
40) Benzene	8.464	78	39814	2.604	ug/l	98
41) Methacrylonitrile	7.850	41	714	0.273	ug/l #	1
52) Toluene	10.507	92	101271	10.296	ug/l	98
55) 1,1,2-Trichloroethane	10.878	97	963	0.248	ug/l #	14
67) Ethyl Benzene	11.953	91	567229	28.967	ug/l #	71
68) m/p-Xylenes	11.953	106	271859	36.622	ug/l	100
69) o-Xylene	12.283	106	207937	27.985	ug/l	98
70) Styrene	12.283	104	10792	0.892	ug/l #	1
71) Bromoform	12.736	173	1565	0.473	ug/l #	1
76) 1,2,3-Trichloropropane	12.733	75	140973	30.181	ug/l #	1
78) n-propylbenzene	12.986	91	22664	1.104	ug/l #	1
79) 2-Chlorotoluene	12.986	91	22664	1.791	ug/l #	42
80) 1,3,5-Trimethylbenzene	13.063	105	104485	6.865	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.733	75	140973	72.207	ug/l #	12
82) 4-Chlorotoluene	13.061	91	10864	0.888	ug/l #	42
83) tert-Butylbenzene	13.372	119	16397	1.238	ug/l #	67
84) 1,2,4-Trimethylbenzene	13.372	105	137301	9.363	ug/l	99
85) sec-Butylbenzene	13.372	105	137301	7.483	ug/l #	57
89) n-Butylbenzene	13.881	91	13476	1.100	ug/l #	44
90) Hexachloroethane	14.222	117	3240	1.048	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.579	75	253	0.249	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.271	180	479	2.725	ug/l #	11
95) Naphthalene	15.507	128	16949	5.349	ug/l	99
96) 1,2,3-Trichlorobenzene	15.708	180	446	2.634	ug/l #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102121\
Data File : VN069086.D
Acq On : 21 Oct 2021 14:22
Operator : JC/MD
Sample : M4253-11 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Oct 22 01:33:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration




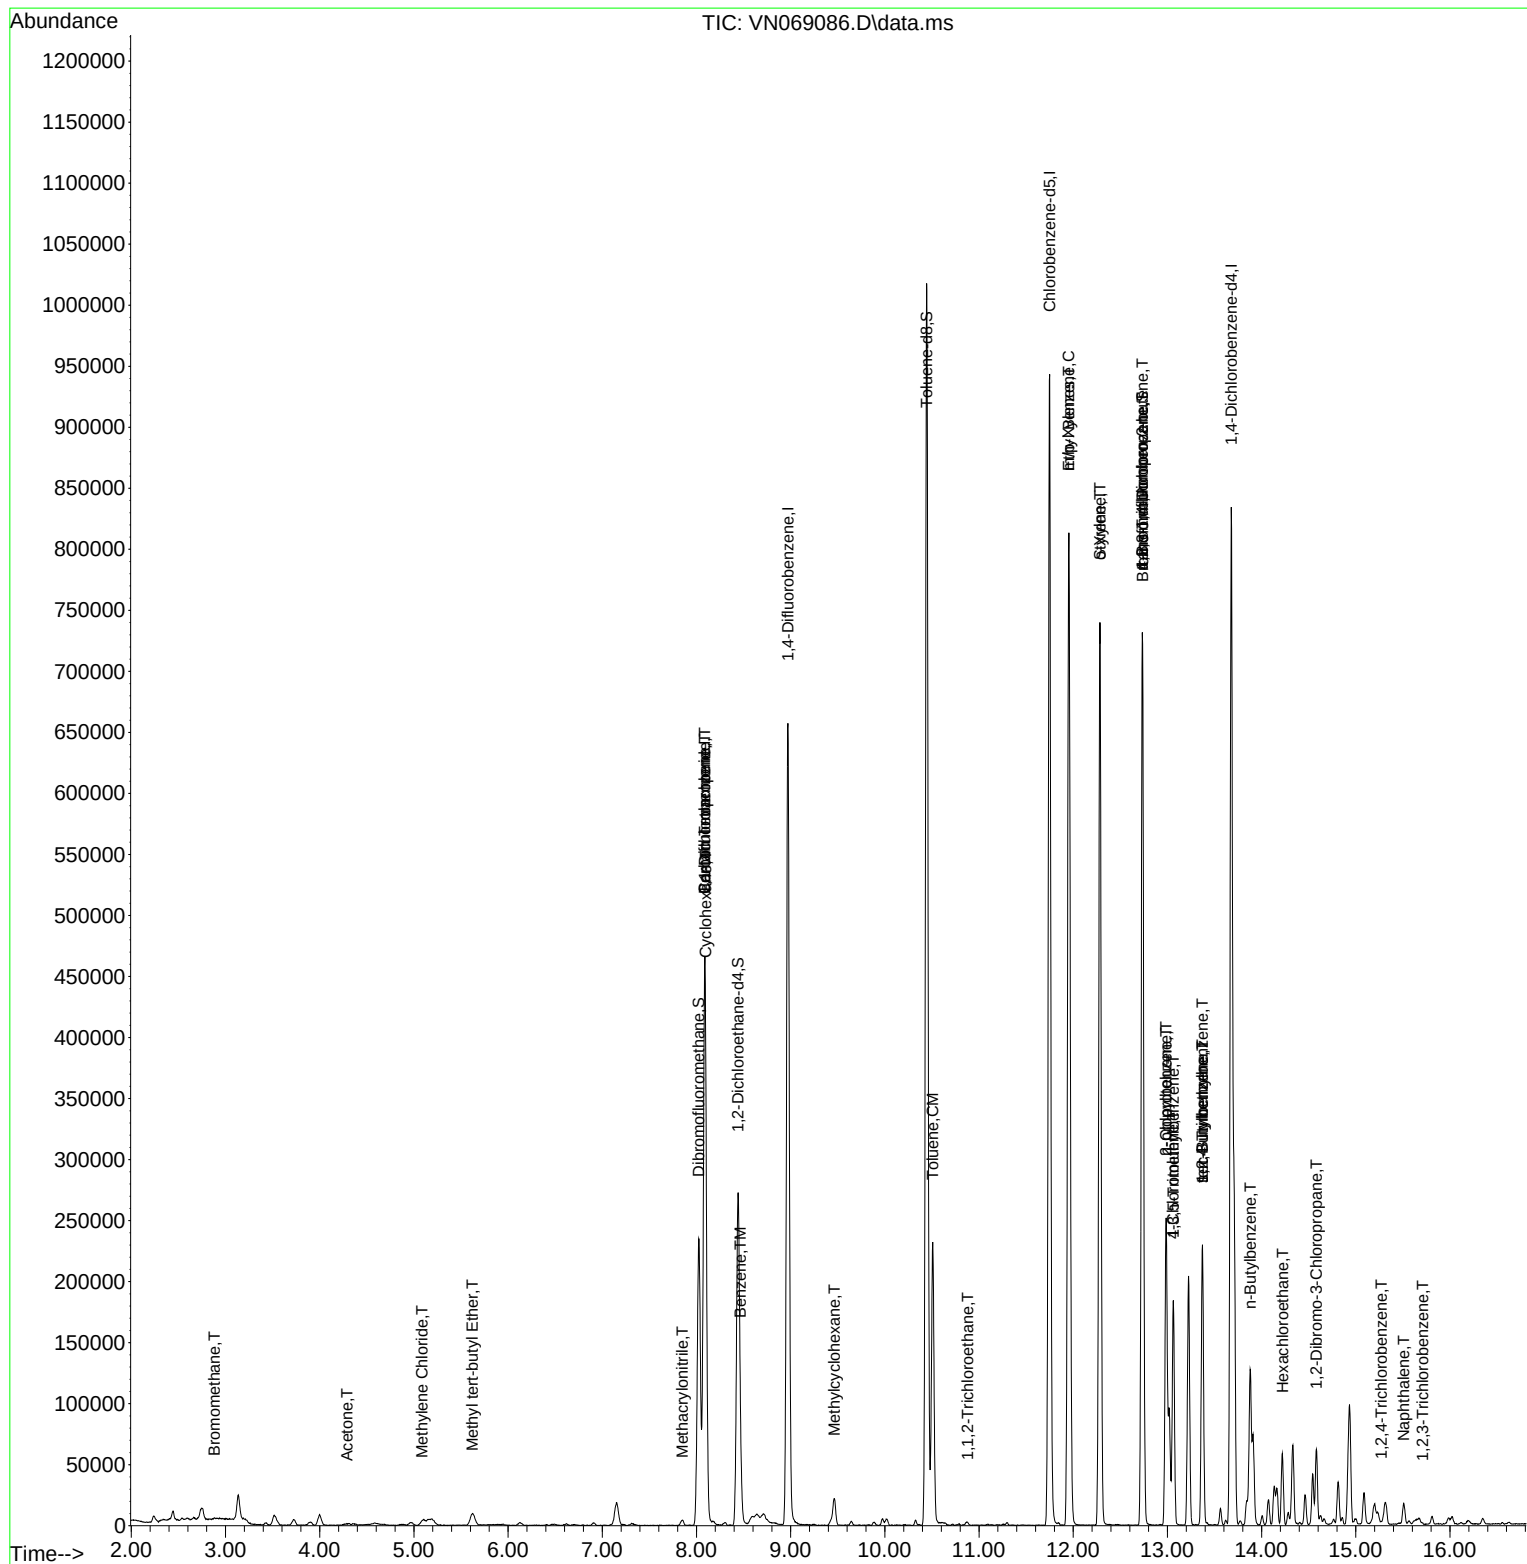


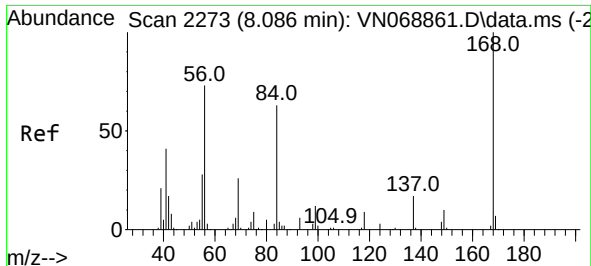

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 338861
Ion Ratio Lower Upper
168 100
99 60.7 48.9 73.3

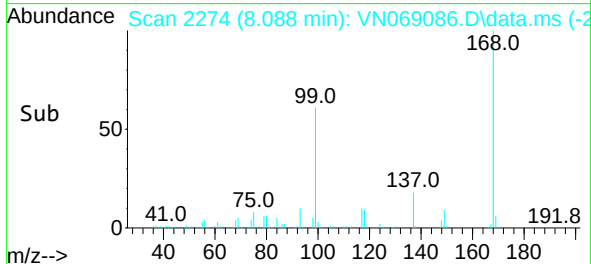

#5
Bromomethane
Concen: 0.317 ug/l
RT: 2.880 min Scan# 332
Delta R.T. 0.043 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 94 Resp: 733
Ion Ratio Lower Upper
94 100
96 21.6 74.2 111.4#




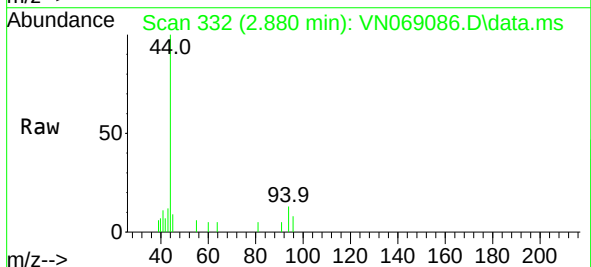


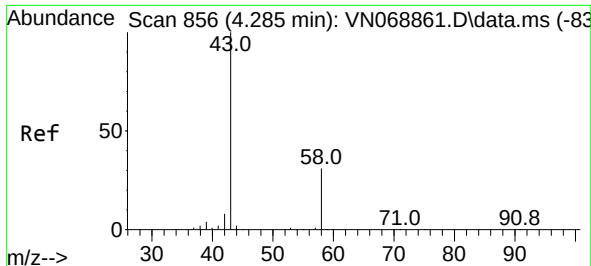

#16
Acetone
Concen: 0.264 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.005 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 440
Ion Ratio Lower Upper
43 100
58 41.1 24.5 36.7#

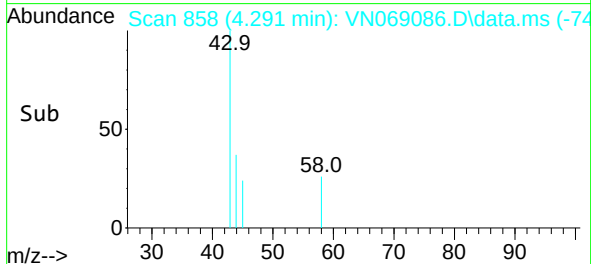

#19
Methyl tert-butyl Ether
Concen: 0.891 ug/l
RT: 5.621 min Scan# 1354
Delta R.T. 0.005 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 73 Resp: 10859
Ion Ratio Lower Upper
73 100
57 51.6 17.3 25.9#

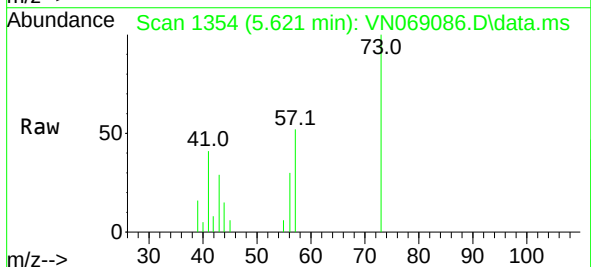

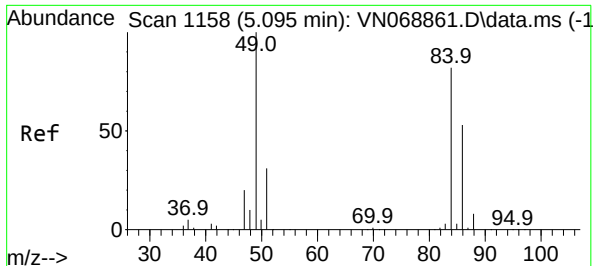

#20

Methylene Chloride

Concen: 0.216 ug/l

RT: 5.087 min Scan# 1155

Delta R.T. -0.008 min

Lab File: VN069086.D

Acq: 21 Oct 2021 14:22

Tgt Ion: 84 Resp: 829





Ion Ratio Lower Upper

84 100

49 110.8 97.6 146.4

51 35.6 30.3 45.5

86 59.4 51.8 77.6

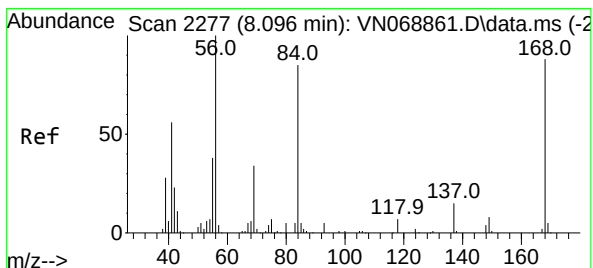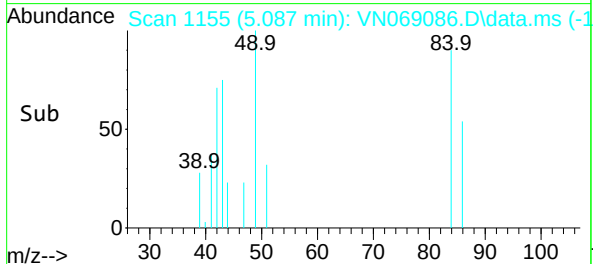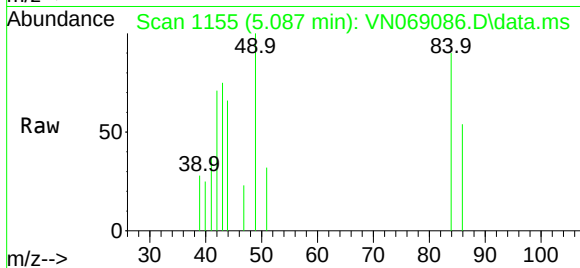

#31

Cyclohexane

Concen: 2.690 ug/l

RT: 8.096 min Scan# 2277

Delta R.T. 0.000 min

Lab File: VN069086.D

Acq: 21 Oct 2021 14:22




Tgt Ion: 56 Resp: 18688


Ion Ratio Lower Upper

56 100

69 86.5 26.9 40.3#

84 99.1 67.6 101.4


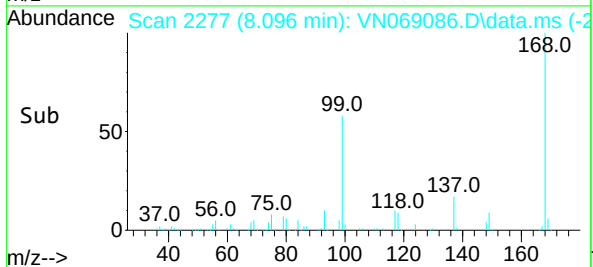

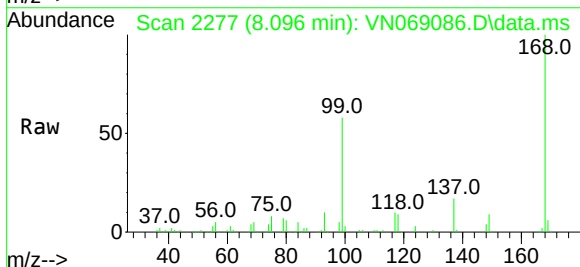




#33
 1,2-Dichloroethane-d4
 Concen: 49.354 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. 0.000 min
 Lab File: VN069086.D
 Acq: 21 Oct 2021 14:22




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 65 Resp: 220503
 Ion Ratio Lower Upper
 65 100
 67 52.2 0.0 103.8

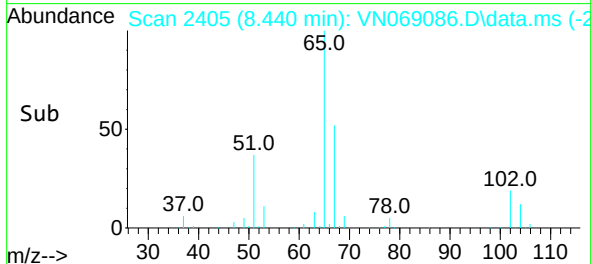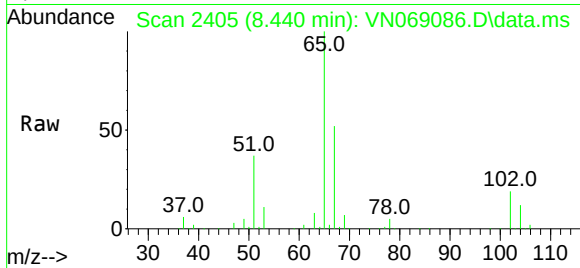

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.003 min
 Lab File: VN069086.D
 Acq: 21 Oct 2021 14:22

Tgt Ion: 114 Resp: 587761
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 42.6
 88 16.0 0.0 32.0




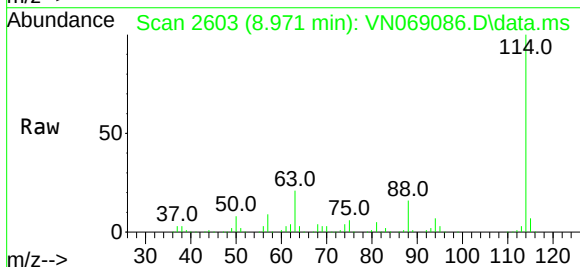




#35
Dibromofluoromethane
Concen: 50.509 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:113 Resp: 172722
Ion Ratio Lower Upper
113 100
111 103.2 83.2 124.8
192 18.1 15.0 22.4

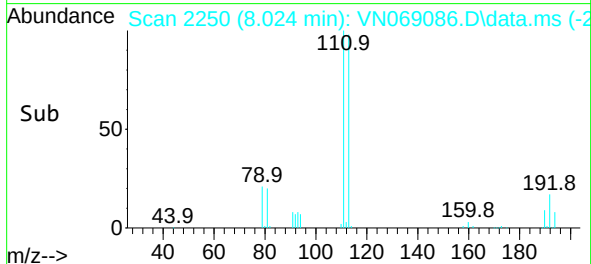

#36
1,1-Dichloropropene
Concen: 5.517 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22


Tgt Ion: 75 Resp: 27696
Ion Ratio Lower Upper
75 100
110 4.5 17.9 53.8#
77 0.0 24.7 37.1#

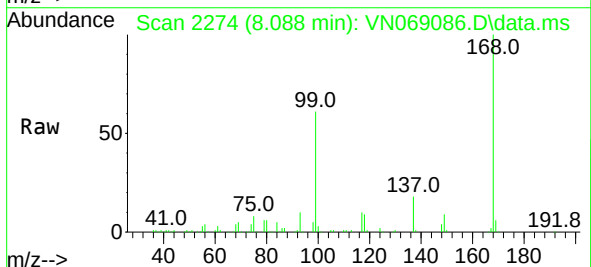






#38
Carbon Tetrachloride
Concen: 6.420 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:117 Resp: 35399
Ion Ratio Lower Upper
117 100
119 5.0 76.9 115.3#
121 0.0 24.6 37.0#

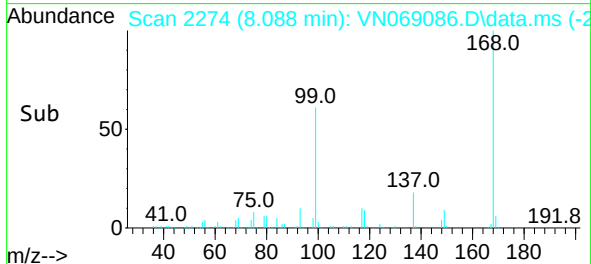


#39
Methylcyclohexane
Concen: 1.532 ug/l
RT: 9.464 min Scan# 2787
Delta R.T. 0.003 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

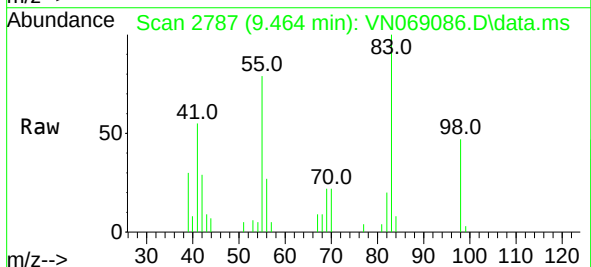

Tgt Ion: 83 Resp: 9902
Ion Ratio Lower Upper
83 100
55 78.5 61.4 92.0
98 47.4 36.4 54.6



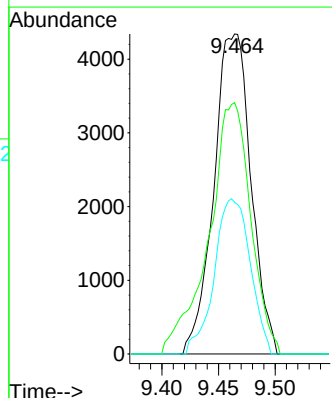



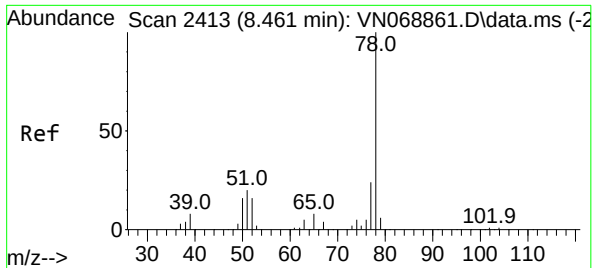

#40
Benzene
Concen: 2.604 ug/l
RT: 8.464 min Scan# 2414
Delta R.T. 0.003 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 78 Resp: 39814
Ion Ratio Lower Upper
78 100
77 23.1 19.1 28.7

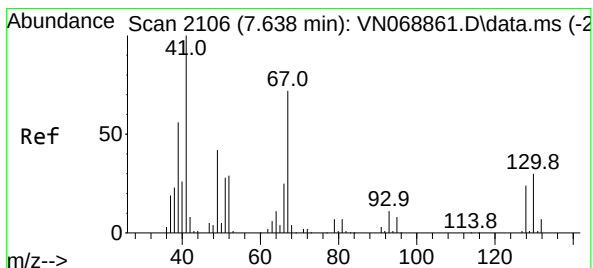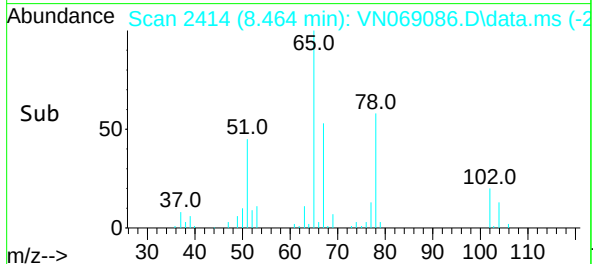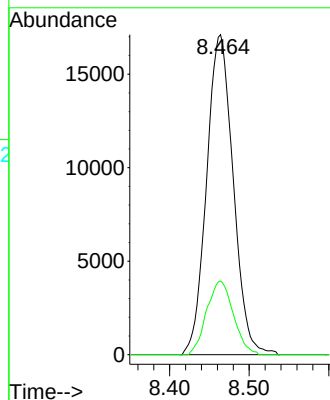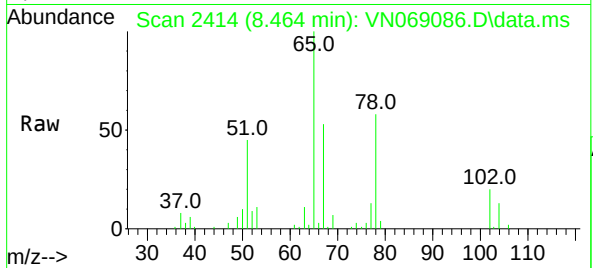

#41
Methacrylonitrile
Concen: 0.273 ug/l
RT: 7.850 min Scan# 2185
Delta R.T. 0.212 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 41 Resp: 714
Ion Ratio Lower Upper
41 100
39 80.4 44.9 67.3#
67 636.3 62.6 93.8#
52 0.0 26.2 39.4#


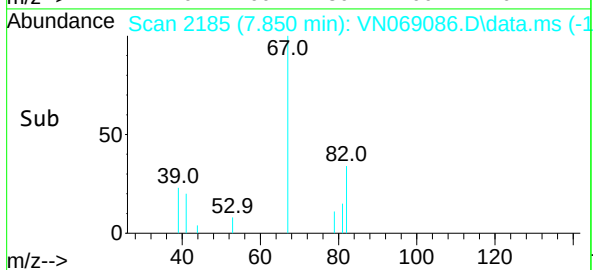
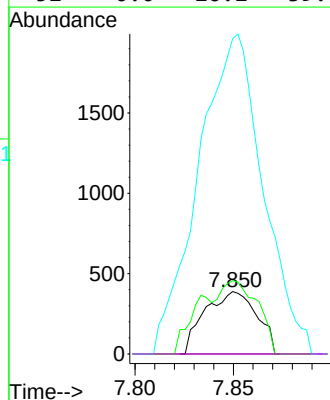
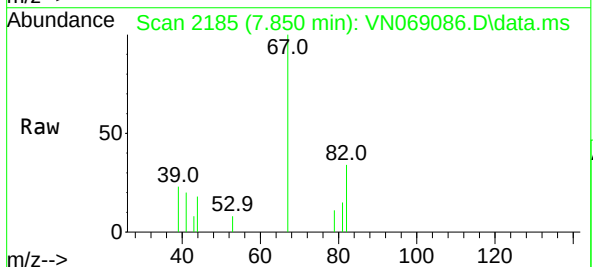




#50
Toluene-d8
Concen: 53.955 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 738241
Ion Ratio Lower Upper
98 100
100 63.8 51.5 77.3

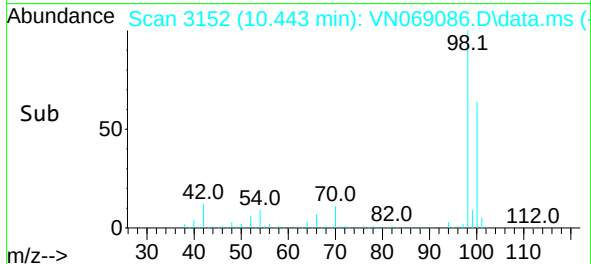

#52
Toluene
Concen: 10.296 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. 0.000 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22


Tgt Ion: 92 Resp: 101271
Ion Ratio Lower Upper
92 100
91 175.2 138.5 207.7

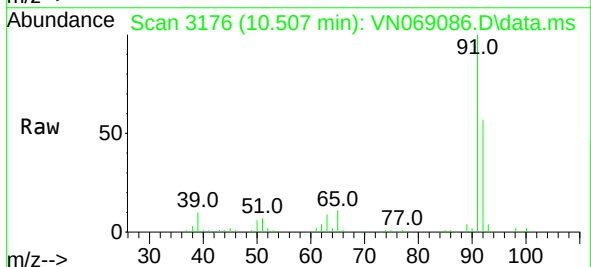






#55
1,1,2-Trichloroethane
Concen: 0.248 ug/l
RT: 10.878 min Scan# 3314
Delta R.T. -0.021 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 97	Resp: 963
Ion Ratio	Lower Upper
97 100	
83 0.0	70.5 105.7#
85 0.0	45.3 67.9#
99 0.0	50.7 76.1#

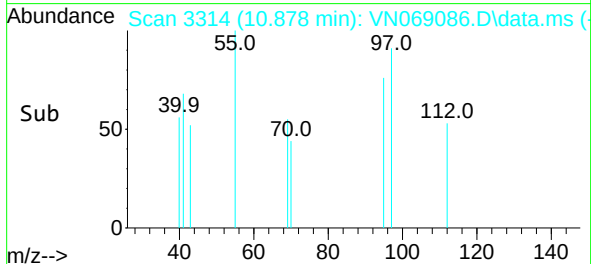

#62
4-Bromofluorobenzene
Concen: 52.115 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 95	Resp: 269031
Ion Ratio	Lower Upper
95 100	
174 73.0	0.0 144.8
176 70.6	0.0 140.0




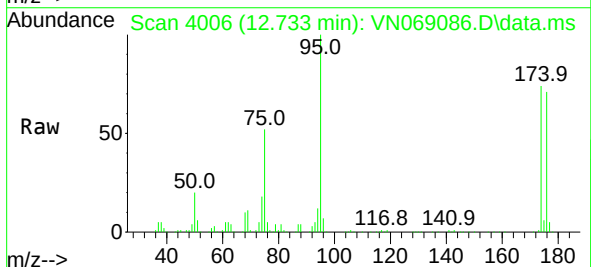


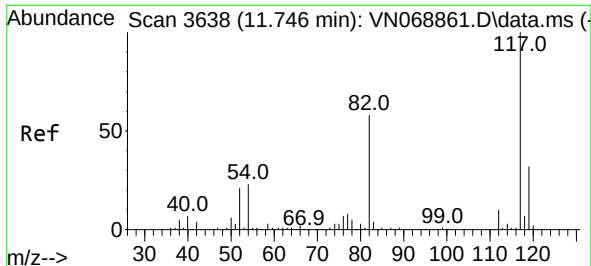

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 557101
Ion Ratio Lower Upper
117 100
82 55.7 46.4 69.6
119 31.9 26.0 39.0

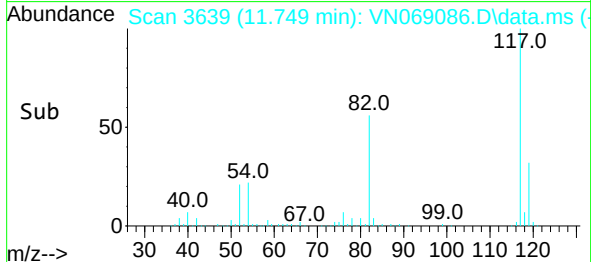

#67
Ethyl Benzene
Concen: 28.967 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. 0.107 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 91 Resp: 567229
Ion Ratio Lower Upper
91 100
106 47.1 24.8 37.2#


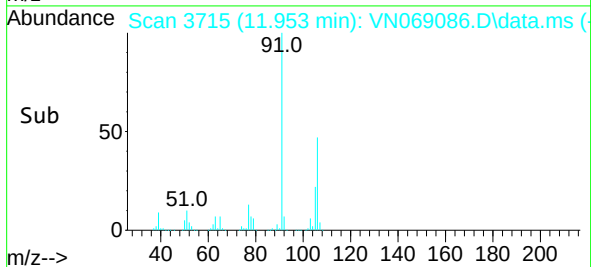

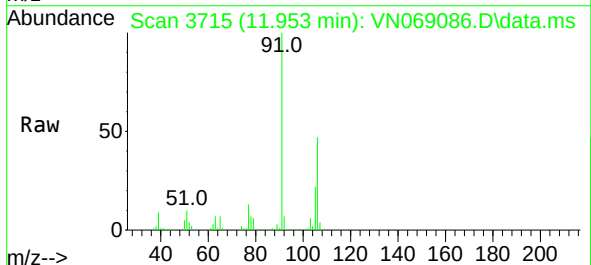


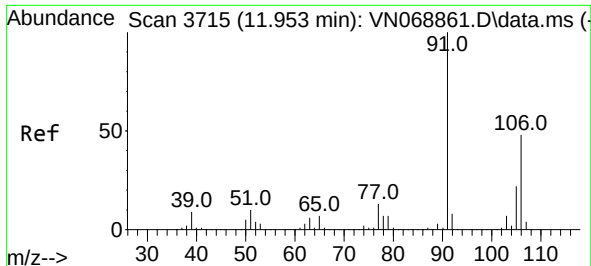

#68
m/p-Xylenes
Concen: 36.622 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. 0.000 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 271859
Ion Ratio Lower Upper
106 100
91 208.6 166.8 250.2

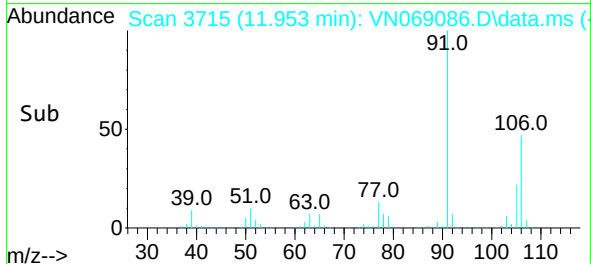

#69
o-Xylene
Concen: 27.985 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. 0.000 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion:106 Resp: 207937
Ion Ratio Lower Upper
106 100
91 221.8 109.6 328.6




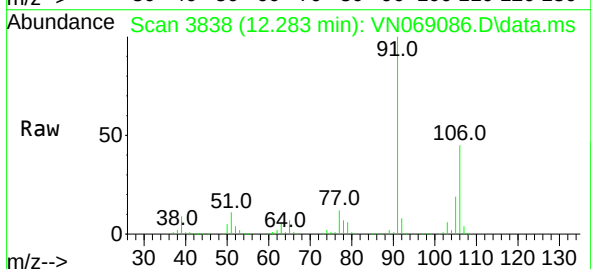




#70
Styrene
Concen: 0.892 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.013 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:104 Resp: 10792
Ion Ratio Lower Upper
104 100
78 307.6 42.2 63.4#
103 270.3 44.4 66.6#

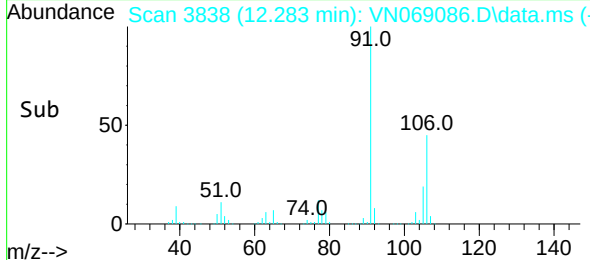

#71
Bromoform
Concen: 0.473 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.276 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion:173 Resp: 1565
Ion Ratio Lower Upper
173 100
175 885.7 23.8 71.5#
254 0.0 0.0 0.0


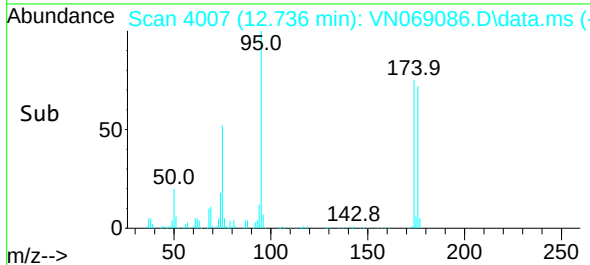

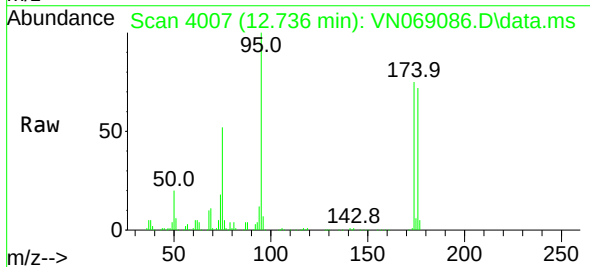


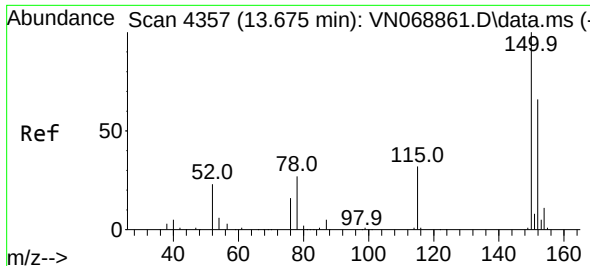

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 4358
 Delta R.T. 0.003 min
 Lab File: VN069086.D
 Acq: 21 Oct 2021 14:22




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:152 Resp: 219524
 Ion Ratio Lower Upper
 152 100
 115 67.3 31.4 94.3
 150 159.4 0.0 351.0

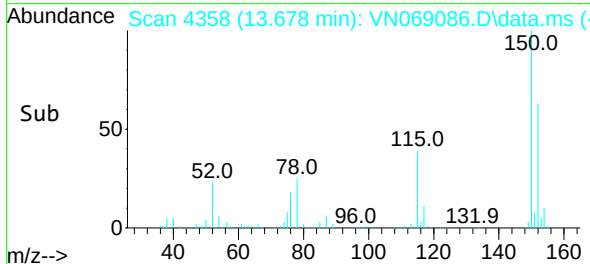

#76
 1,2,3-Trichloropropane
 Concen: 30.181 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. -0.147 min
 Lab File: VN069086.D
 Acq: 21 Oct 2021 14:22

Tgt Ion: 75 Resp: 140973
 Ion Ratio Lower Upper
 75 100
 77 1.0 96.2 288.4#




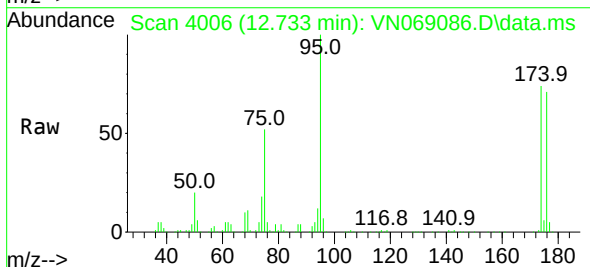


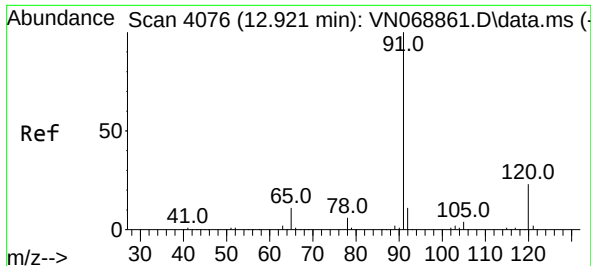

#78
n-propylbenzene
Concen: 1.104 ug/l
RT: 12.986 min Scan# 4100
Delta R.T. 0.064 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 22664
Ion Ratio Lower Upper
91 100
120 237.0 11.4 34.1#

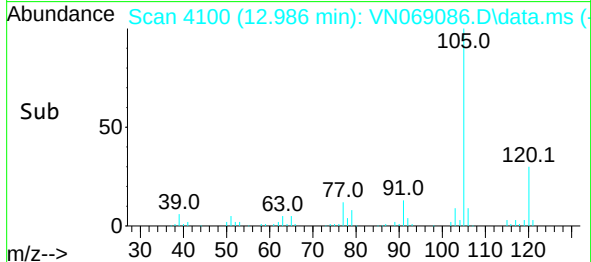

#79
2-Chlorotoluene
Concen: 1.791 ug/l
RT: 12.986 min Scan# 4100
Delta R.T. -0.024 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 91 Resp: 22664
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.4#


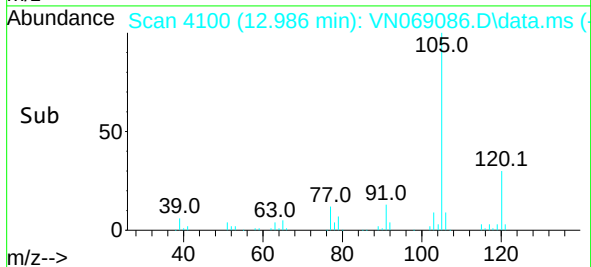

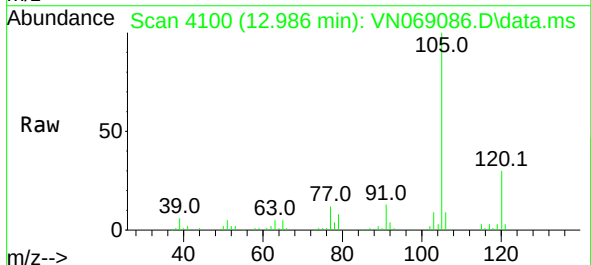




#80
1,3,5-Trimethylbenzene
Concen: 6.865 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.003 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 104485
Ion Ratio Lower Upper
105 100
120 47.9 23.4 70.2

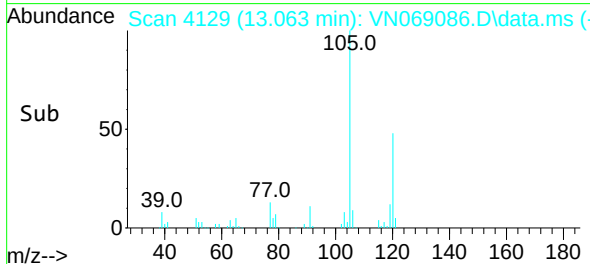

#81
trans-1,4-Dichloro-2-butene
Concen: 72.207 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 75 Resp: 140973
Ion Ratio Lower Upper
75 100
53 0.0 75.4 113.2#
89 0.0 36.9 55.3#


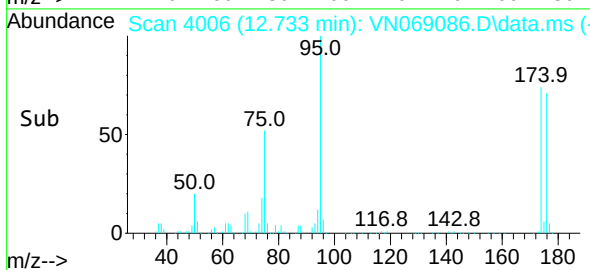

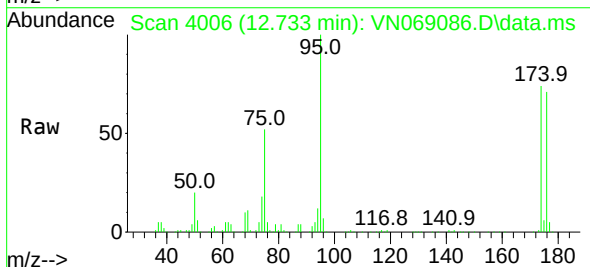


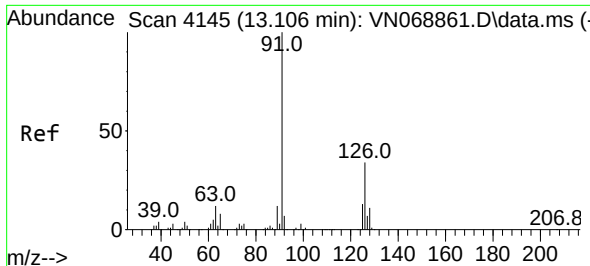

#82
4-Chlorotoluene
Concen: 0.888 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.046 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 10864
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

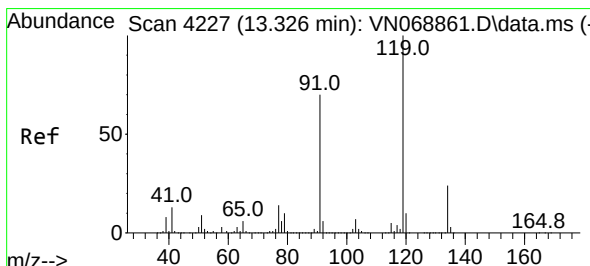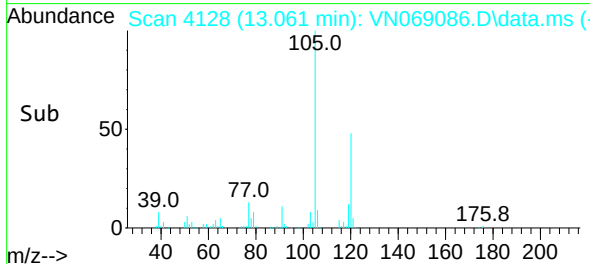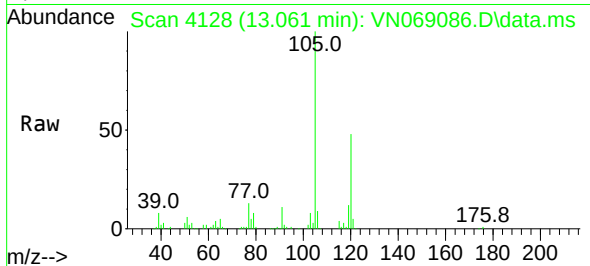

#83
tert-Butylbenzene
Concen: 1.238 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.046 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 119 Resp: 16397
Ion Ratio Lower Upper
119 100
91 91.2 34.6 103.9
134 0.0 12.6 37.6#

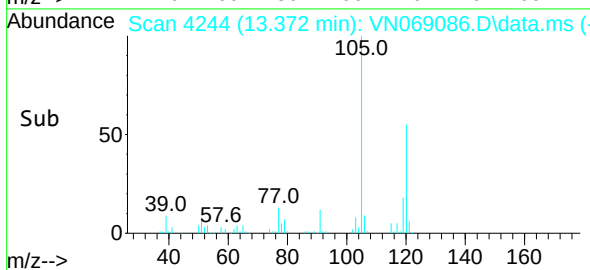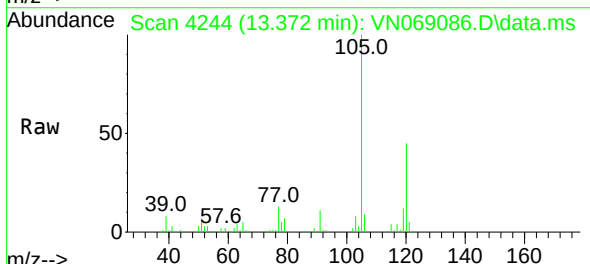



#84

1,2,4-Trimethylbenzene

Concen: 9.363 ug/l

RT: 13.372 min Scan# 4244

Delta R.T. 0.003 min

Lab File: VN069086.D





Acq: 21 Oct 2021 14:22

Tgt Ion:105 Resp: 137301

Ion Ratio Lower Upper

105 100

120 44.3 21.9 65.5

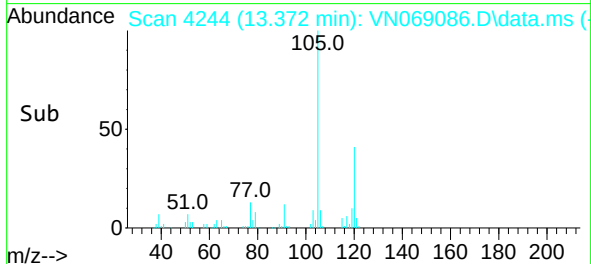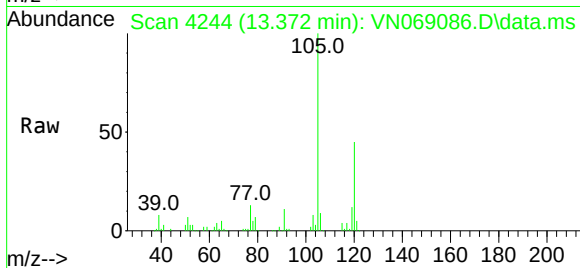

#85

sec-Butylbenzene

Concen: 7.483 ug/l

RT: 13.372 min Scan# 4244

Delta R.T. -0.131 min

Lab File: VN069086.D




Acq: 21 Oct 2021 14:22


Tgt Ion:105 Resp: 137301

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#




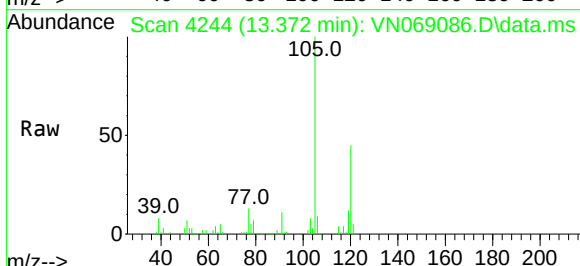


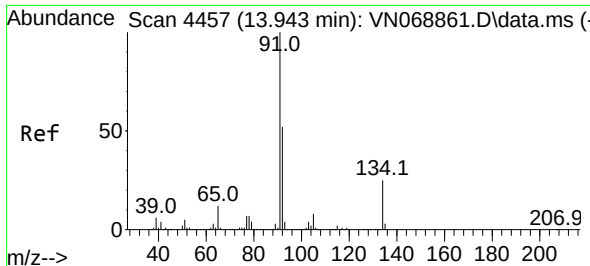

#89
n-Butylbenzene
Concen: 1.100 ug/l
RT: 13.881 min Scan# 4434
Delta R.T. -0.062 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 13476
Ion Ratio Lower Upper
91 100
92 10.2 26.0 78.0#
134 0.0 12.5 37.5#

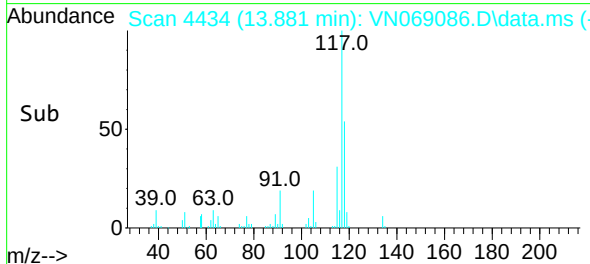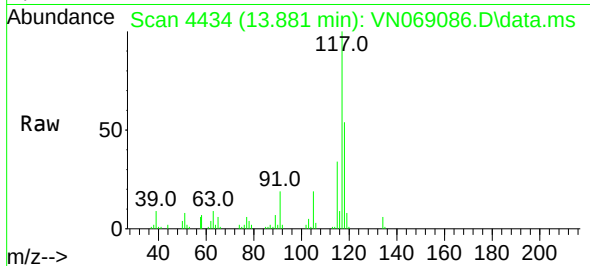

#90
Hexachloroethane
Concen: 1.048 ug/l
RT: 14.222 min Scan# 4561
Delta R.T. 0.008 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion: 117 Resp: 3240
Ion Ratio Lower Upper
117 100
201 0.0 37.1 111.5#


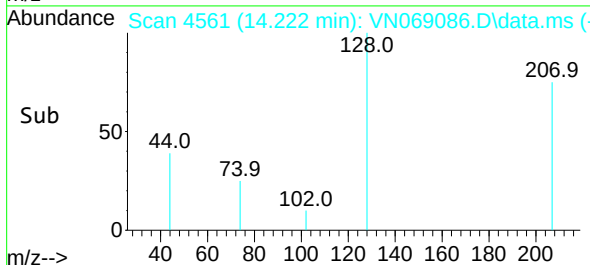

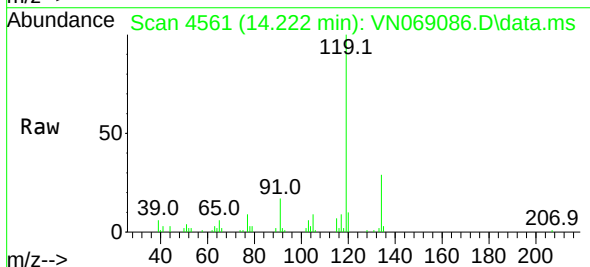




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.249 ug/l
RT: 14.579 min Scan# 4694
Delta R.T. -0.027 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 253
Ion Ratio Lower Upper
75 100
155 0.0 38.8 116.4#
157 0.0 50.2 150.6#

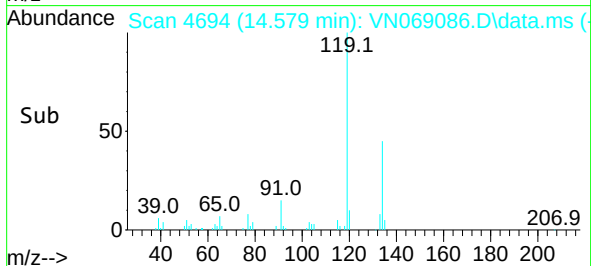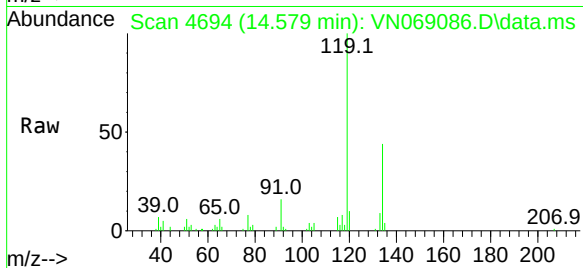

#93
1,2,4-Trichlorobenzene
Concen: 2.725 ug/l
RT: 15.271 min Scan# 4952
Delta R.T. 0.006 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion:180 Resp: 479
Ion Ratio Lower Upper
180 100
182 54.5 47.9 143.7
145 159.3 16.4 49.2#




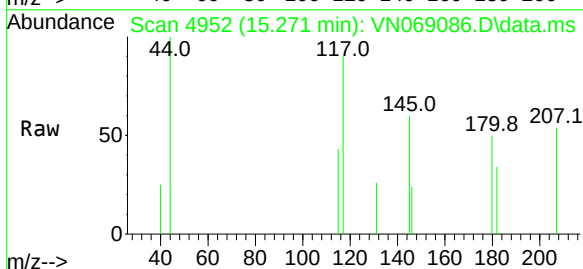


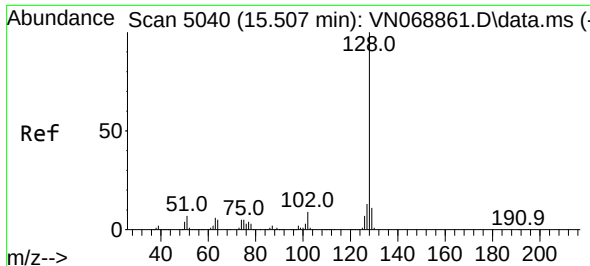

#95
Naphthalene
Concen: 5.349 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion:128	Resp:	16949
Ion Ratio	Lower	Upper
128	100	
127	13.6	10.5 15.7
129	11.5	8.9 13.3

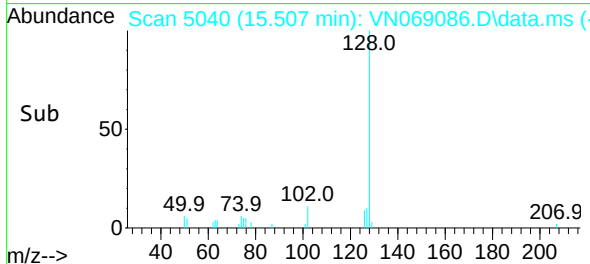

#96
1,2,3-Trichlorobenzene
Concen: 2.634 ug/l
RT: 15.708 min Scan# 5115
Delta R.T. 0.006 min
Lab File: VN069086.D
Acq: 21 Oct 2021 14:22

Tgt Ion:180	Resp:	446
Ion Ratio	Lower	Upper
180	100	
182	99.6	48.1 144.3
145	0.0	17.4 52.2#

