


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102121\
 Data File : VN069077.D
 Acq On : 21 Oct 2021 9:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Title : SW846 8260
 Last Update : Wed Oct 13 05:44:40 2021

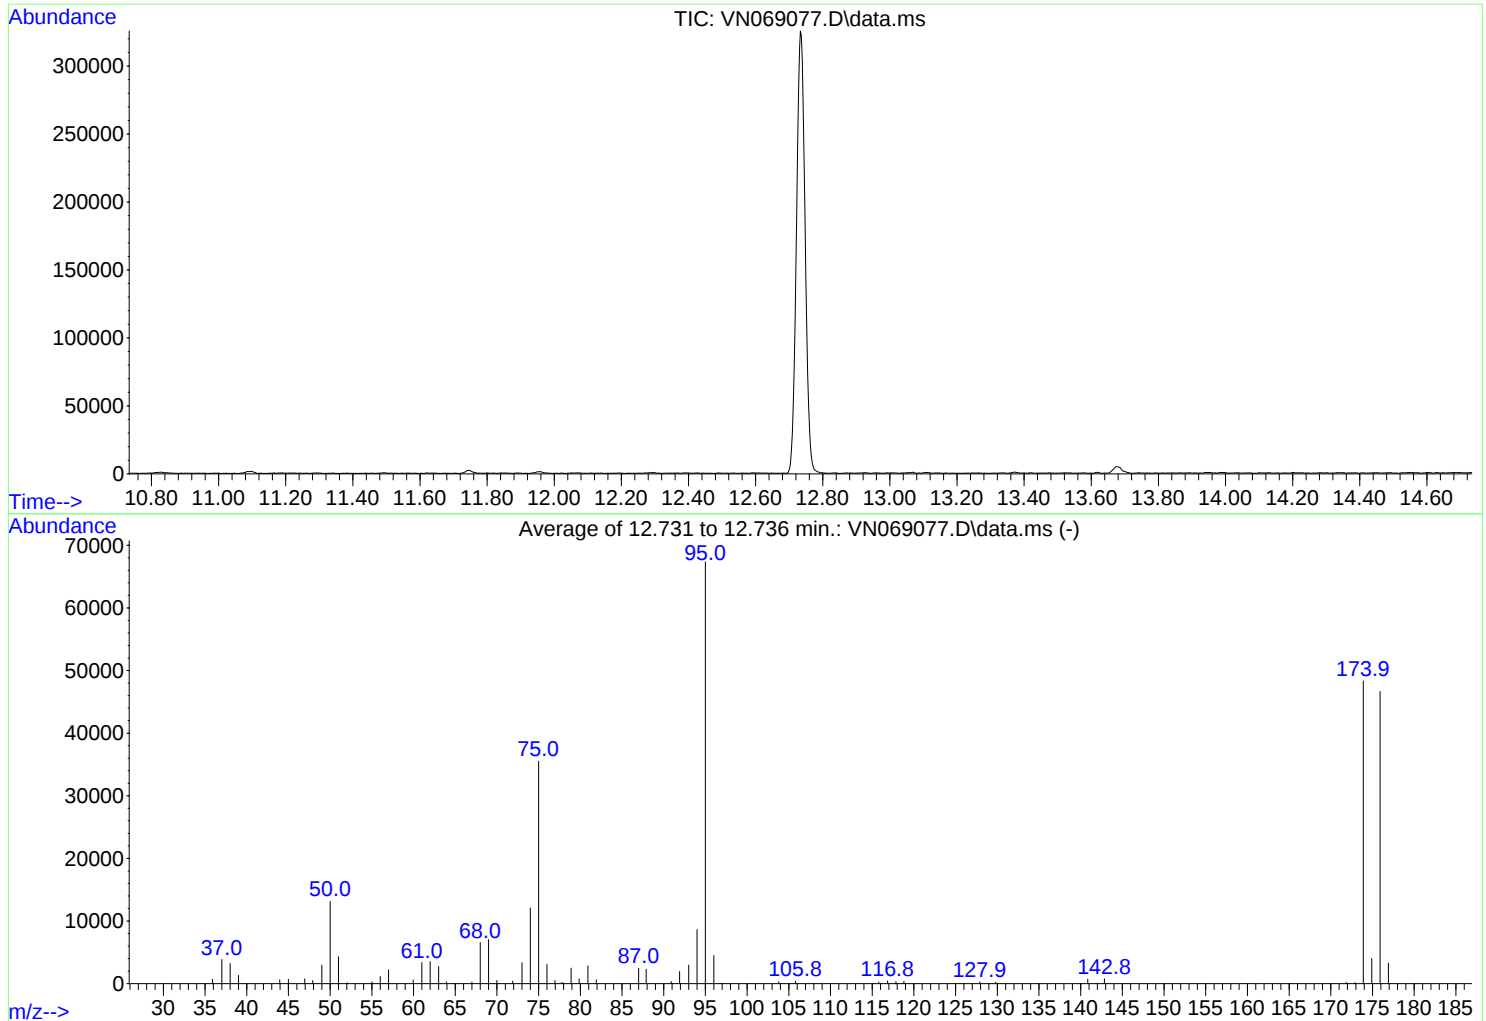

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	13142	PASS
75	95	30	60	52.8	35531	PASS
95	95	100	100	100.0	67357	PASS
96	95	5	9	6.6	4474	PASS
173	174	0.00	2	0.4	180	PASS
174	95	50	100	71.7	48312	PASS
175	174	5	9	8.3	4013	PASS
176	174	95	101	96.6	46661	PASS
177	176	5	9	7.0	3276	PASS