

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102122\
 Data File : VN074962.D
 Acq On : 21 Oct 2022 15:23
 Operator : JC\MD
 Sample : N5222-08
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-4

Quant Time: Oct 22 02:53:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 21 09:37:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	800874	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	1322077	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	1301280	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	701006	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	860292	40.430	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	80.860%		
35) Dibromofluoromethane	8.171	113	675975	42.957	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	85.920%		
50) Toluene-d8	10.571	98	2738189	45.353	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	90.700%		
62) 4-Bromofluorobenzene	12.847	95	939712	44.124	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	88.240%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	3327	Below Cal	#	81
4) Vinyl Chloride	2.518	62	940	Below Cal	#	63
5) Bromomethane	2.912	94	1182	Below Cal	#	4
6) Chloroethane	3.101	64	2192	Below Cal	#	42
7) Trichlorofluoromethane	3.230	101	98	Below Cal		91
11) Tert butyl alcohol	5.506	59	3053	0.679 ug/l	#	72
12) 1,1-Dichloroethene	4.306	96	287	Below Cal	#	1
13) Acrolein	4.206	56	1097	Below Cal	#	82
16) Acetone	4.448	43	9621	Below Cal		91
17) Carbon Disulfide	4.718	76	498	Below Cal	#	78
20) Methylene Chloride	5.283	84	3647	Below Cal	#	50
21) trans-1,2-Dichloroethene	5.800	96	55	Below Cal	#	16
25) 2-Butanone	7.500	43	3023	0.233 ug/l	#	73
30) Chloroform	7.977	83	21109	0.678 ug/l		88
31) Cyclohexane	8.236	56	19088	0.878 ug/l	#	41
36) 1,1-Dichloropropene	8.230	75	70218	3.543 ug/l	#	50
38) Carbon Tetrachloride	8.236	117	89077	4.129 ug/l	#	15
52) Toluene	10.635	92	11205	0.281 ug/l		97
58) 2-Chloroethyl Vinyl ether	10.177	63	116	3.619 ug/l	#	45
60) Dibromochloromethane	11.106	129	8213	0.468 ug/l	#	10
64) Tetrachloroethene	11.112	164	6016	0.565 ug/l	#	89
67) Ethyl Benzene	11.965	91	80564	1.153 ug/l		97
68) m/p-Xylenes	12.076	106	79173	2.907 ug/l		98
71) Bromoform	12.847	173	9306	0.831 ug/l	#	1
76) 1,2,3-Trichloropropane	12.847	75	513651	27.019 ug/l	#	1
78) n-propylbenzene	13.035	91	16115	0.240 ug/l		96
80) 1,3,5-Trimethylbenzene	13.176	105	18137	0.367 ug/l		100
81) trans-1,4-Dichloro-2-b...	12.847	75	513651	86.630 ug/l	#	10
84) 1,2,4-Trimethylbenzene	13.482	105	132186	2.646 ug/l		96
85) sec-Butylbenzene	13.482	105	132186	2.151 ug/l	#	57
95) Naphthalene	15.641	128	385105	9.042 ug/l		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102122\
Data File : VN074962.D
Acq On : 21 Oct 2022 15:23
Operator : JC\MD
Sample : N5222-08
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-4

Quant Time: Oct 22 02:53:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 21 09:37:47 2022
Response via : Initial Calibration




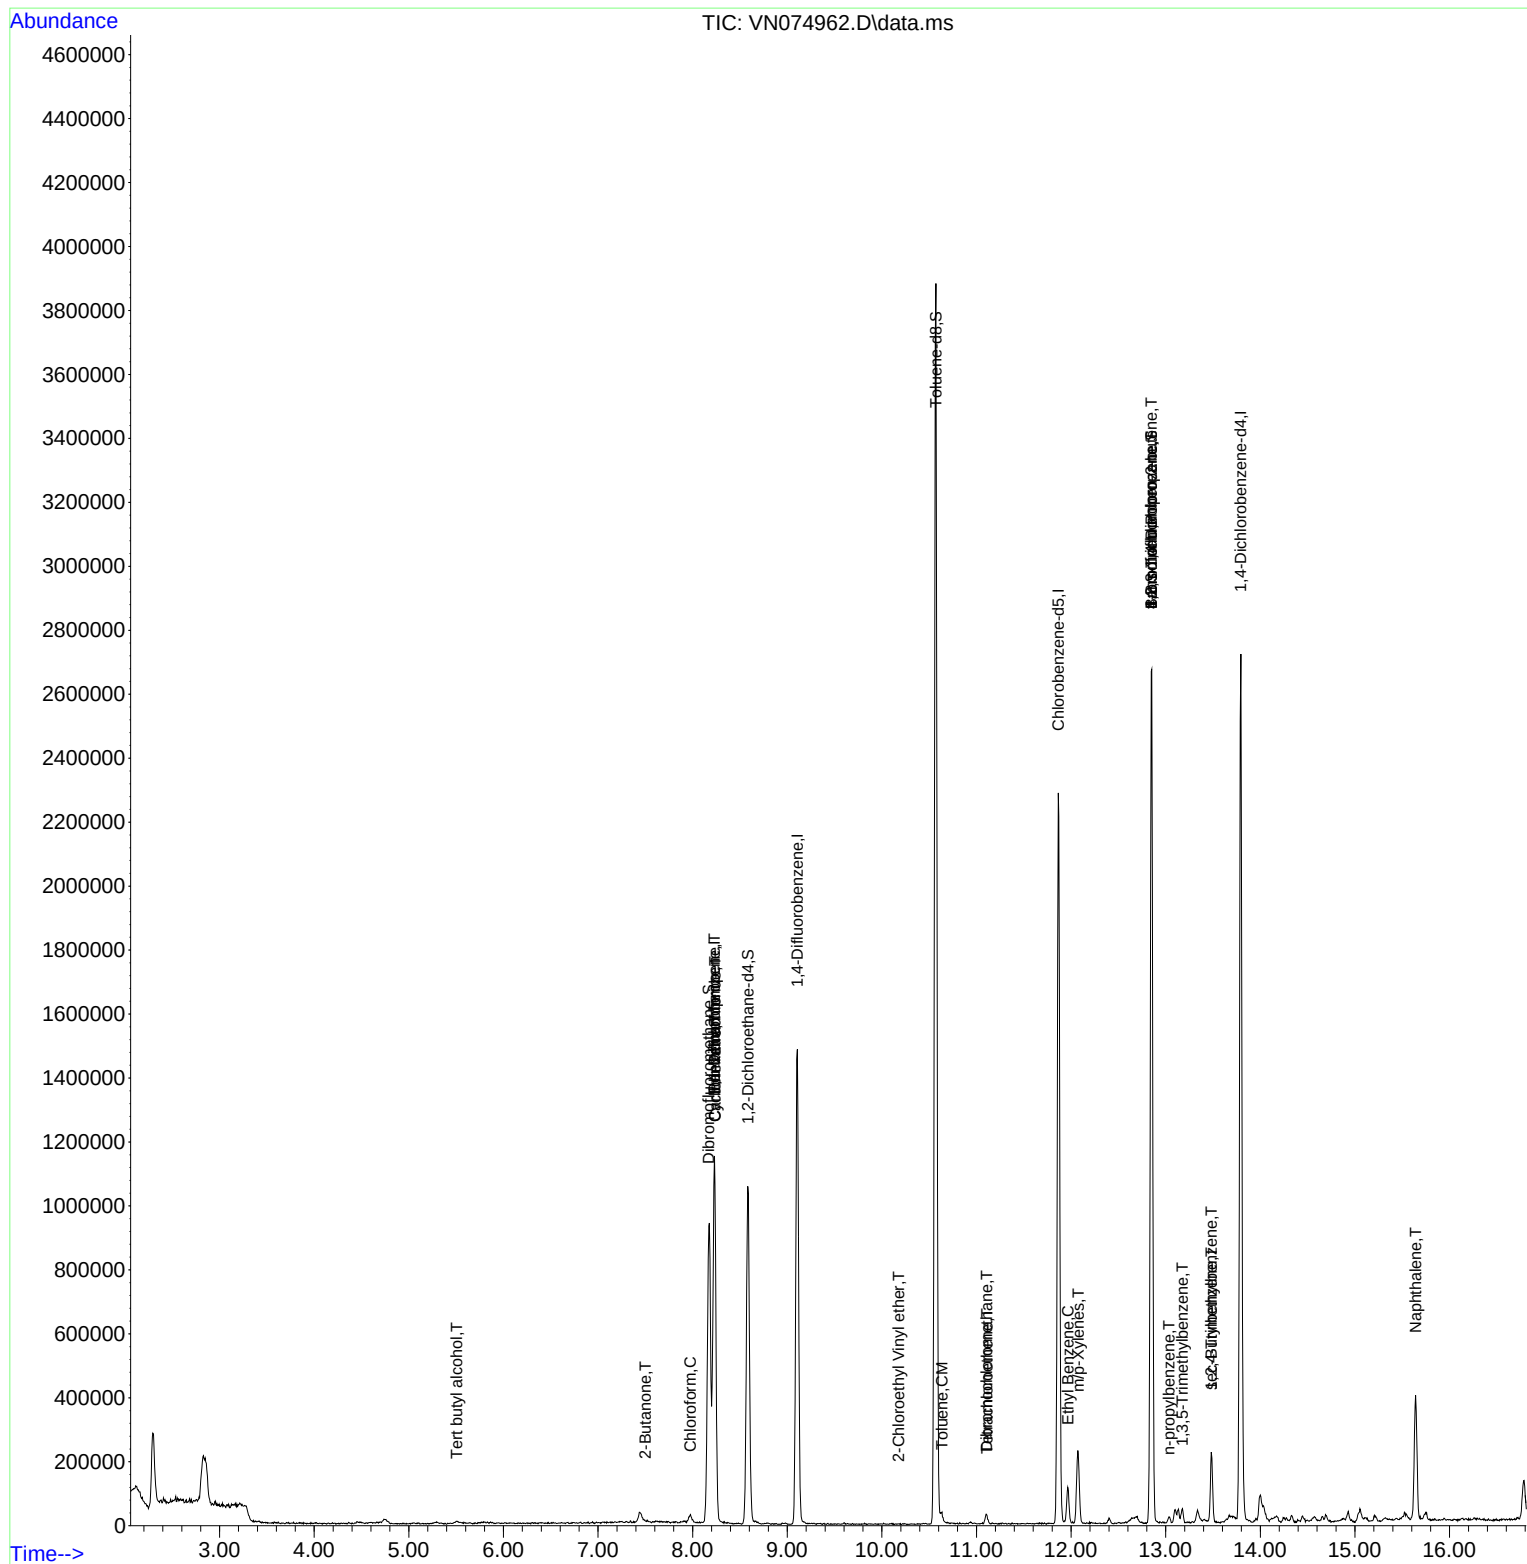




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:168 Resp: 800874
Ion Ratio Lower Upper
168 100
99 65.0 52.2 78.4



#3
Chloromethane
Concen: Below Cal
RT: 2.377 min Scan# 55
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 50 Resp: 3327
Ion Ratio Lower Upper
50 100
52 24.8 28.8 43.2#


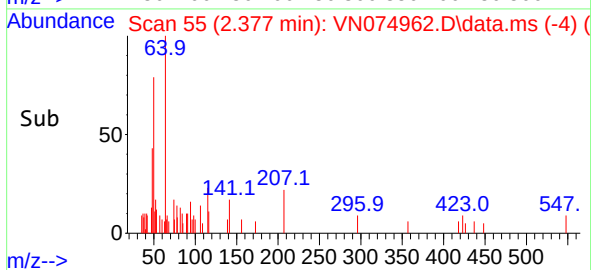




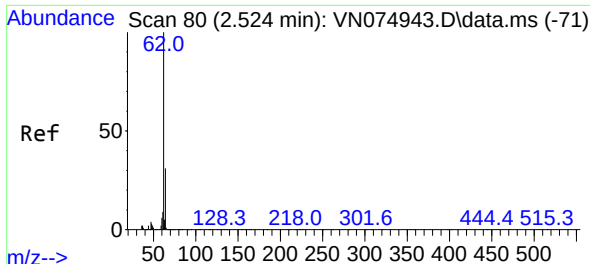

#4
 Vinyl Chloride
 Concen: Below Cal
 RT: 2.518 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: VN074962.D
 Acq: 21 Oct 2022 15:23




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-4


Tgt Ion: 62 Resp: 940
 Ion Ratio Lower Upper
 62 100
 64 10.4 24.5 36.7#

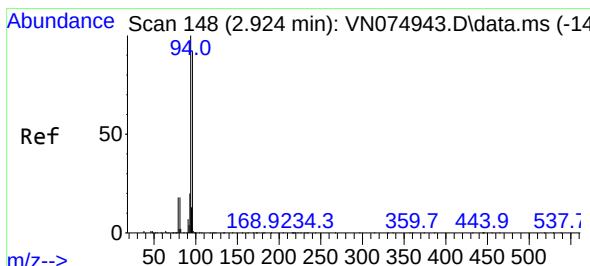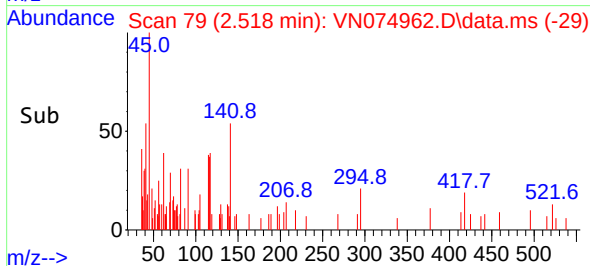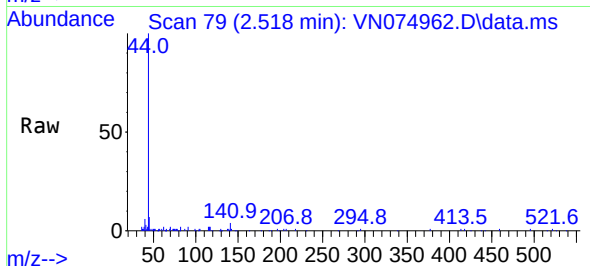

#5
 Bromomethane
 Concen: Below Cal
 RT: 2.912 min Scan# 146
 Delta R.T. -0.012 min
 Lab File: VN074962.D
 Acq: 21 Oct 2022 15:23

Tgt Ion: 94 Resp: 1182
 Ion Ratio Lower Upper
 94 100
 96 0.0 73.5 110.3#


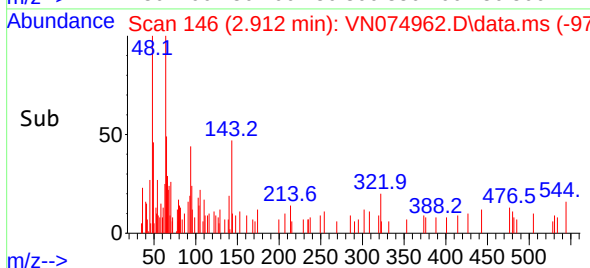
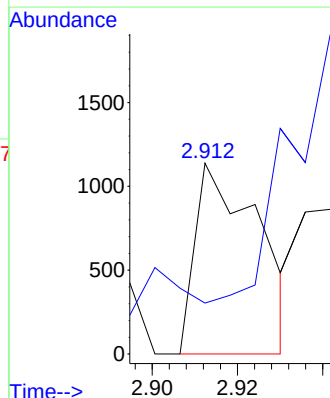
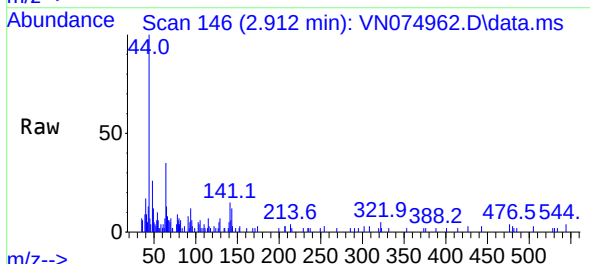




#6
Chloroethane
Concen: Below Cal
RT: 3.101 min Scan# 11
Delta R.T. -0.005 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 64 Resp: 2192
Ion Ratio Lower Upper
64 100
66 1.6 27.9 41.9#

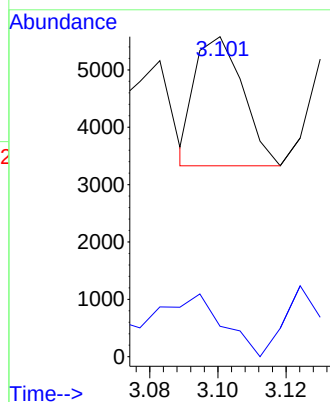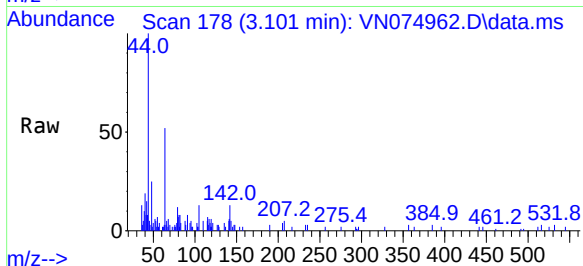

#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.230 min Scan# 200
Delta R.T. -0.265 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion:101 Resp: 98
Ion Ratio Lower Upper
101 100
103 71.2 51.5 77.3


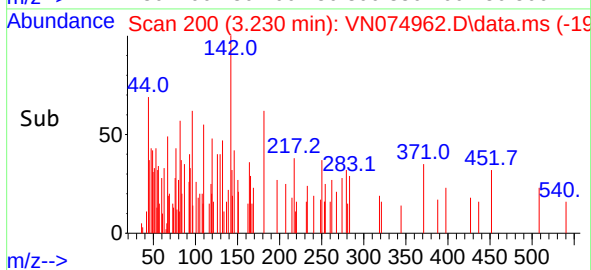
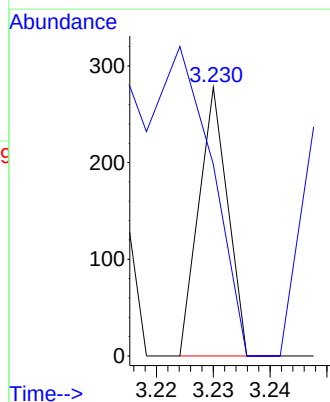
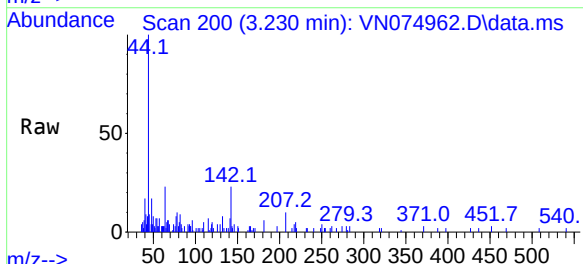




#11
Tert butyl alcohol
Concen: 0.679 ug/l
RT: 5.506 min Scan# 51
Delta R.T. -0.029 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 59 Resp: 3053
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

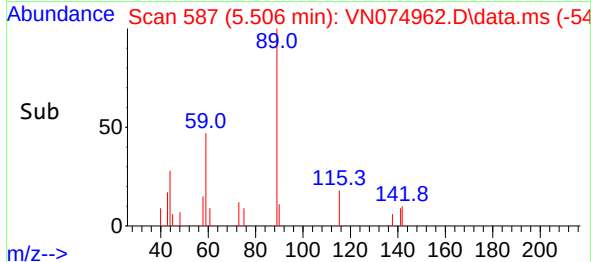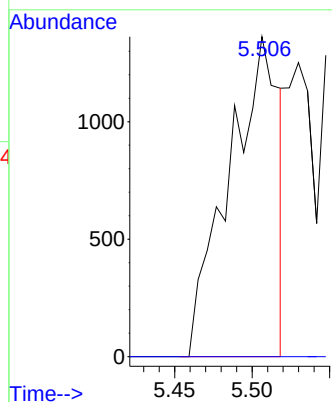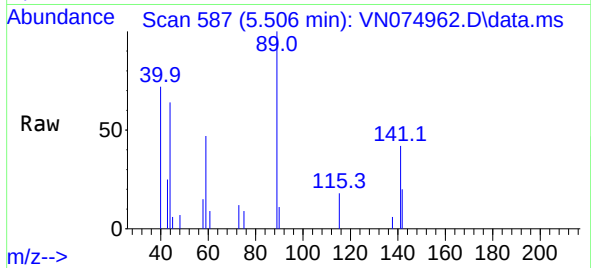

#12
1,1-Dichloroethene
Concen: Below Cal
RT: 4.306 min Scan# 383
Delta R.T. -0.041 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 96 Resp: 287
Ion Ratio Lower Upper
96 100
61 0.0 128.9 193.3#
98 0.0 51.8 77.8#


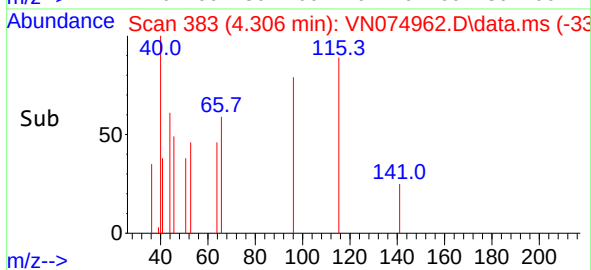






#13
Acrolein
Concen: Below Cal
RT: 4.206 min Scan# 30
Delta R.T. 0.017 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 56 Resp: 1097
Ion Ratio Lower Upper
56 100
55 81.9 53.7 80.5#



#16
Acetone
Concen: Below Cal
RT: 4.448 min Scan# 407
Delta R.T. 0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 43 Resp: 9621
Ion Ratio Lower Upper
43 100
58 37.3 25.7 38.5


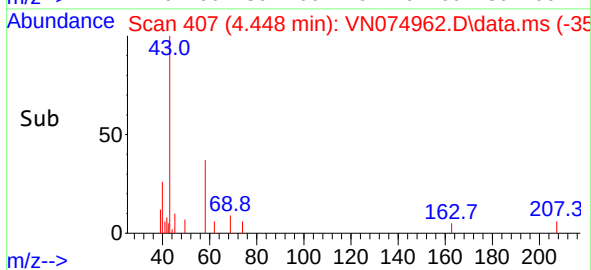






#17
Carbon Disulfide
Concen: Below Cal
RT: 4.718 min Scan# 417
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 76 Resp: 498
Ion Ratio Lower Upper
76 100
78 1.5 7.4 11.2#



#20
Methylene Chloride
Concen: Below Cal
RT: 5.283 min Scan# 549
Delta R.T. -0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 84 Resp: 3647
Ion Ratio Lower Upper
84 100
49 54.5 88.6 133.0#
51 21.7 26.7 40.1#
86 14.5 49.7 74.5#


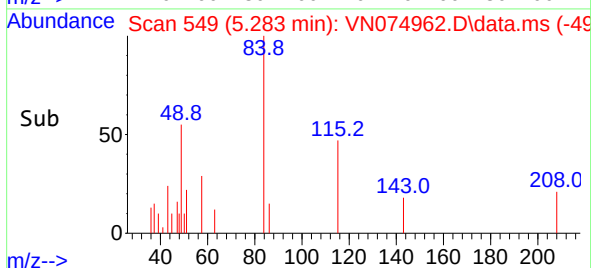
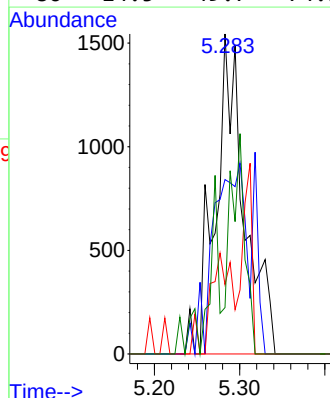





#21
trans-1,2-Dichloroethene
Concen: Below Cal
RT: 5.800 min Scan# 61
Delta R.T. 0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 96 Resp: 55
Ion Ratio Lower Upper
96 100
61 98.1 112.6 169.0#
98 215.4 52.4 78.6#

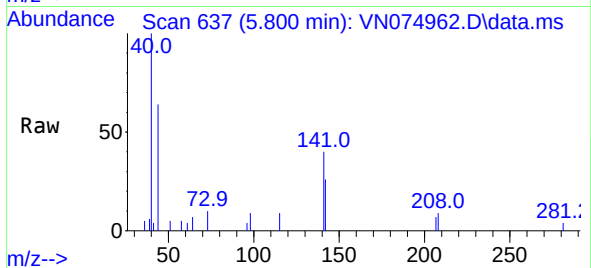

#25
2-Butanone
Concen: 0.233 ug/l
RT: 7.500 min Scan# 926
Delta R.T. 0.012 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 43 Resp: 3023
Ion Ratio Lower Upper
43 100
72 15.2 23.9 35.9#


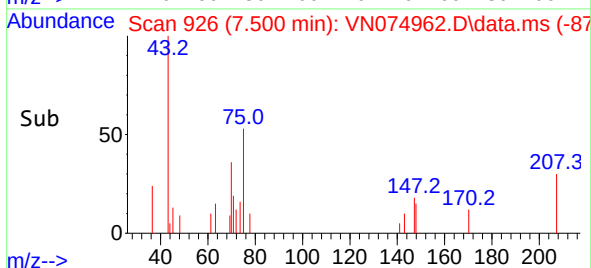
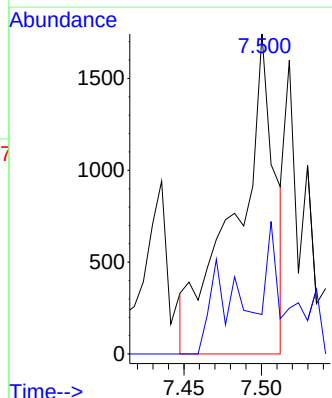



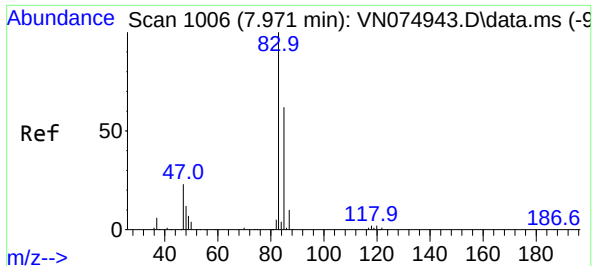

#30
Chloroform
Concen: 0.678 ug/l
RT: 7.977 min Scan# 1007
Delta R.T. 0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 83 Resp: 21109
Ion Ratio Lower Upper
83 100
85 71.8 49.9 74.9

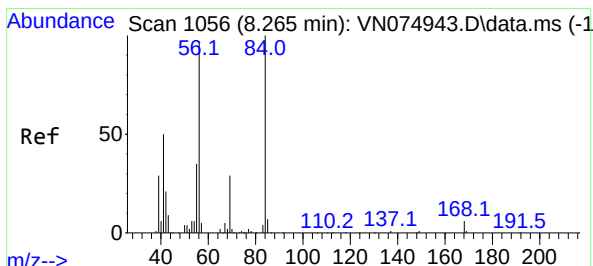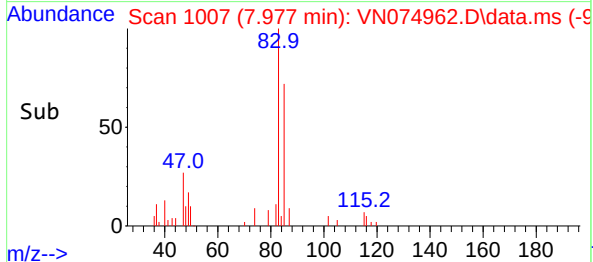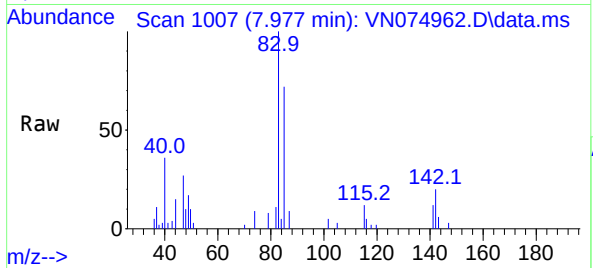

#31
Cyclohexane
Concen: 0.878 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.029 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 56 Resp: 19088
Ion Ratio Lower Upper
56 100
69 151.3 24.2 36.2#
84 115.2 82.8 124.2


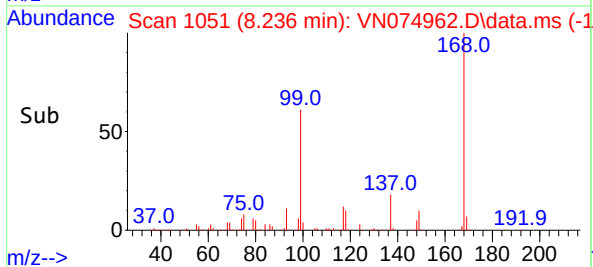

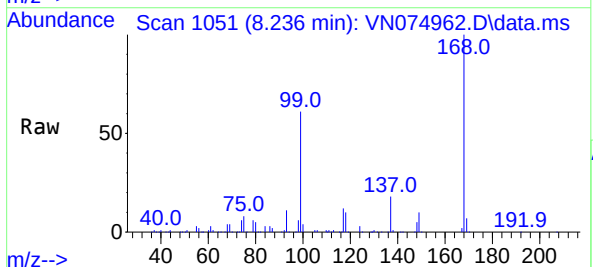


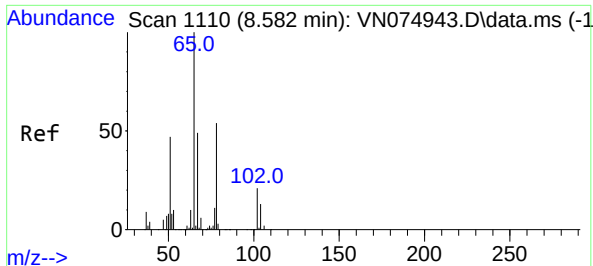

#33
1,2-Dichloroethane-d4
Concen: 40.430 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 65 Resp: 860292
Ion Ratio Lower Upper
65 100
67 51.8 0.0 102.6

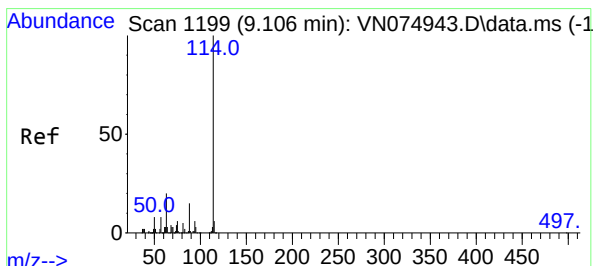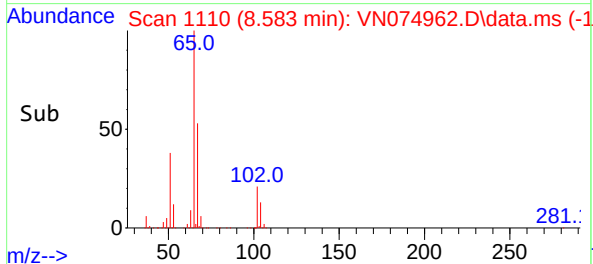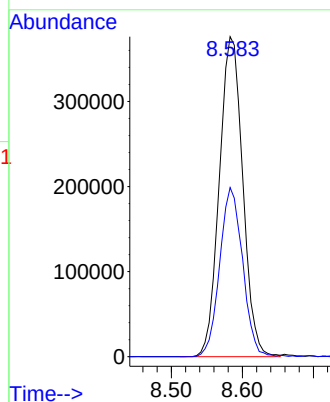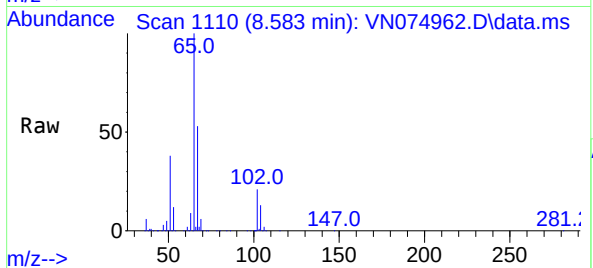

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 114 Resp: 1322077
Ion Ratio Lower Upper
114 100
63 20.1 0.0 39.8
88 16.3 0.0 30.4


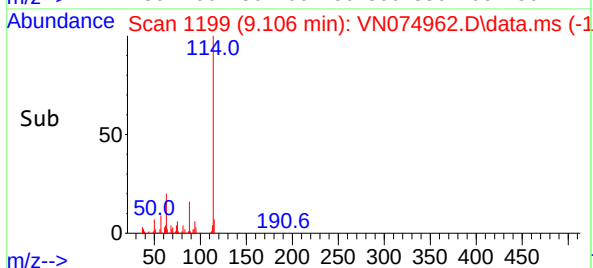

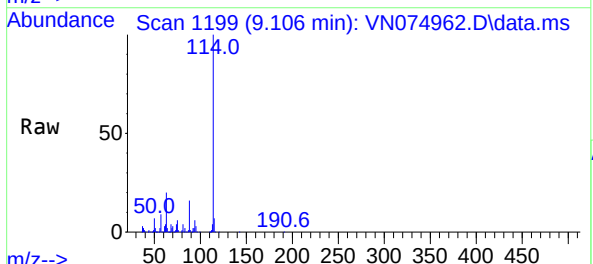


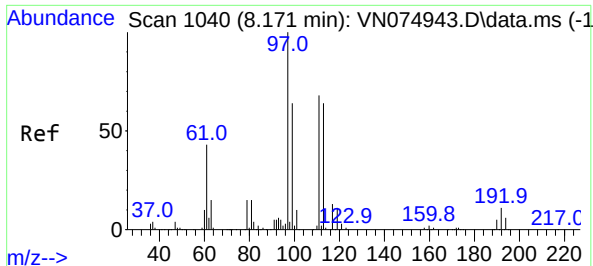

#35
Dibromofluoromethane
Concen: 42.957 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:113 Resp: 675975
Ion Ratio Lower Upper
113 100
111 104.3 83.4 125.2
192 16.7 13.3 19.9

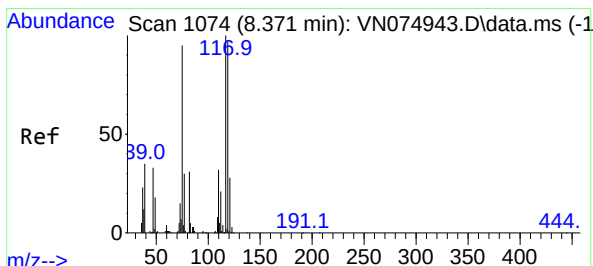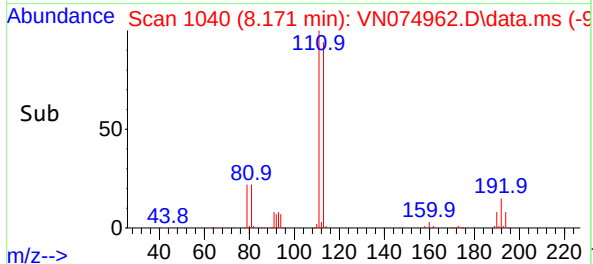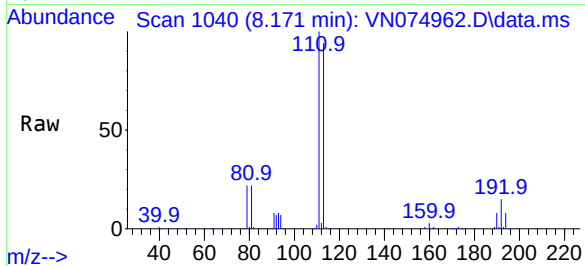

#36
1,1-Dichloropropene
Concen: 3.543 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.141 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 75 Resp: 70218
Ion Ratio Lower Upper
75 100
110 10.2 18.1 54.4#
77 0.2 25.0 37.4#


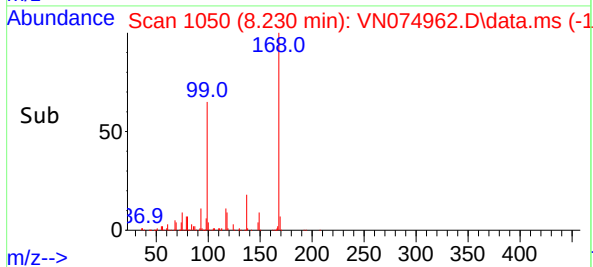

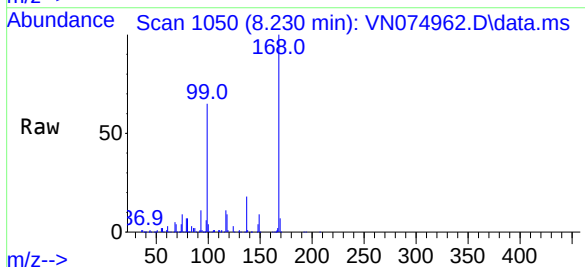


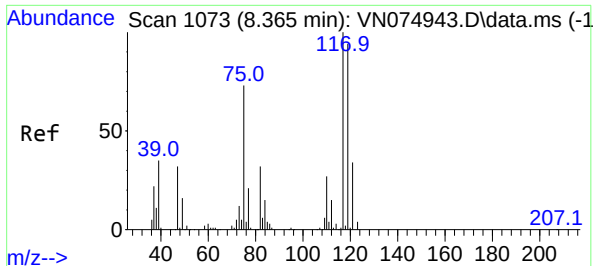

#38
Carbon Tetrachloride
Concen: 4.129 ug/l
RT: 8.236 min Scan# 1073
Delta R.T. -0.129 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:117 Resp: 89077
Ion Ratio Lower Upper
117 100
119 3.4 75.2 112.8#
121 0.0 27.0 40.6#

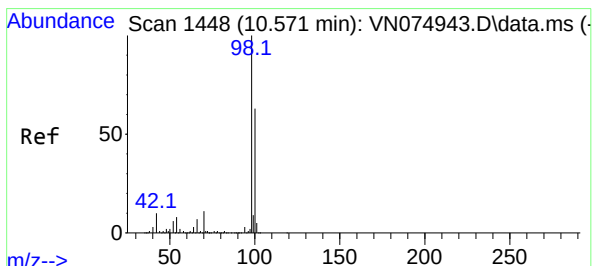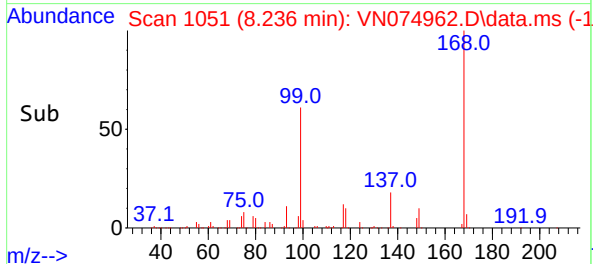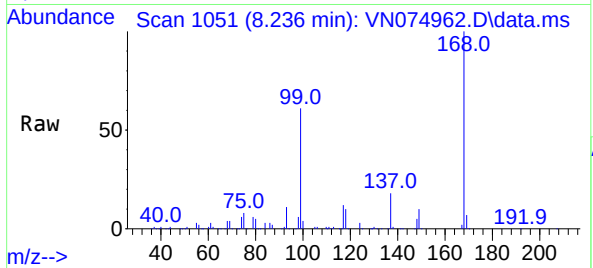

#50
Toluene-d8
Concen: 45.353 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 98 Resp: 2738189
Ion Ratio Lower Upper
98 100
100 64.0 51.4 77.2


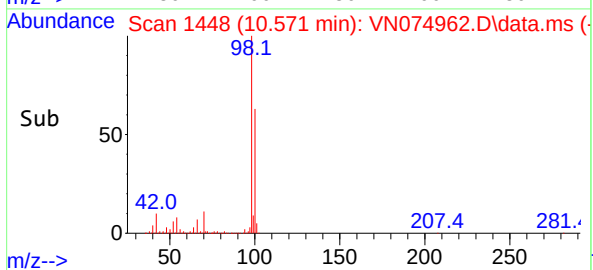

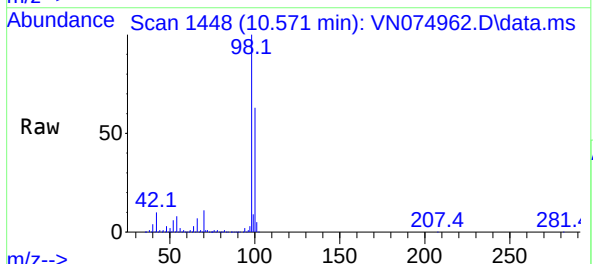


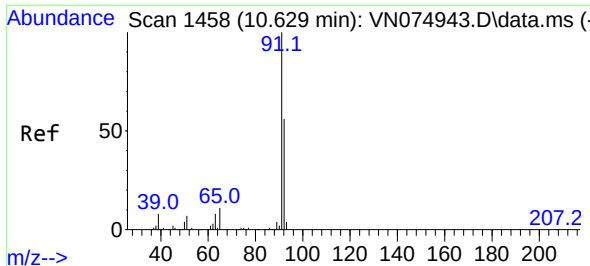

#52
Toluene
Concen: 0.281 ug/l
RT: 10.635 min Scan# 1458
Delta R.T. 0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 92 Resp: 11205
Ion Ratio Lower Upper
92 100
91 169.3 139.2 208.8

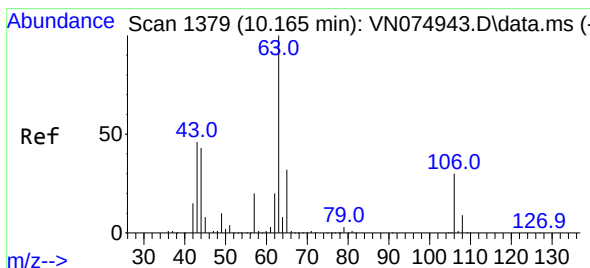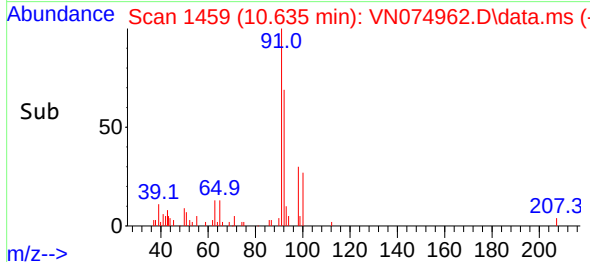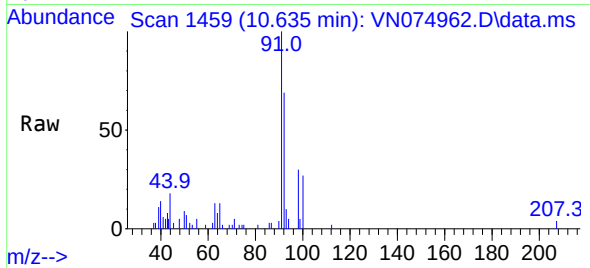

#58
2-Chloroethyl Vinyl ether
Concen: 3.619 ug/l
RT: 10.177 min Scan# 1381
Delta R.T. 0.012 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 63 Resp: 116
Ion Ratio Lower Upper
63 100
106 0.0 24.1 36.1#


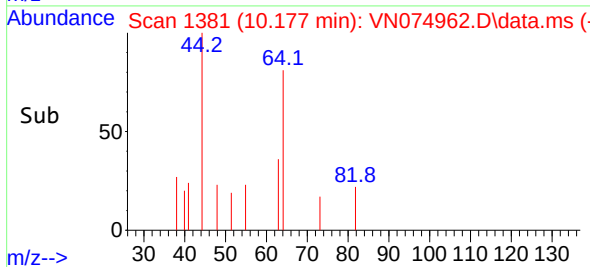

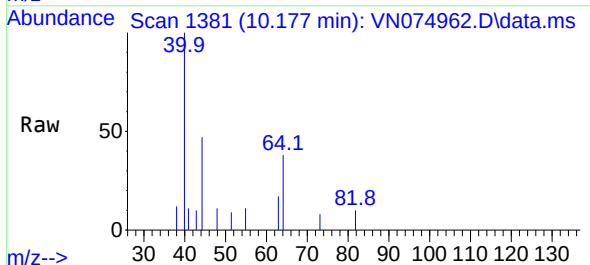




#60
Dibromochloromethane
Concen: 0.468 ug/l
RT: 11.106 min Scan# 11
Delta R.T. -0.253 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:129 Resp: 8213
Ion Ratio Lower Upper
129 100
127 0.0 39.0 116.9#

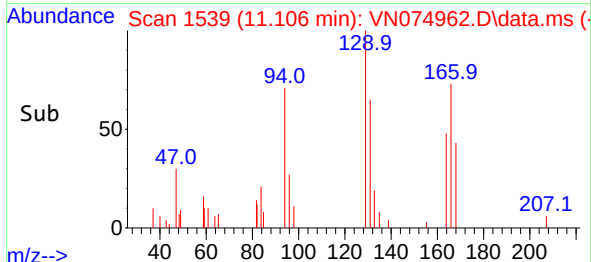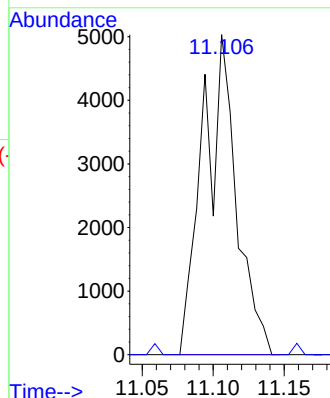

#62
4-Bromofluorobenzene
Concen: 44.124 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 95 Resp: 939712
Ion Ratio Lower Upper
95 100
174 71.8 0.0 143.0
176 70.1 0.0 138.2


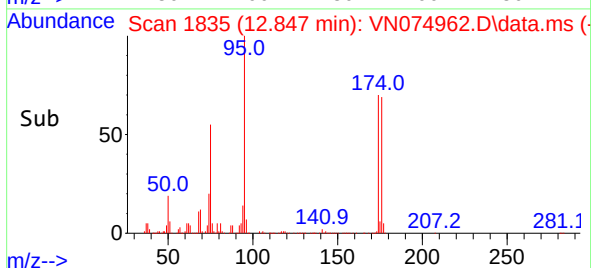






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:117 Resp: 1301280
Ion Ratio Lower Upper
117 100
82 59.8 45.6 68.4
119 31.8 25.1 37.7



#64
Tetrachloroethene
Concen: 0.565 ug/l
RT: 11.112 min Scan# 1540
Delta R.T. 0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion:164 Resp: 6016
Ion Ratio Lower Upper
164 100
166 122.9 98.6 148.0
129 128.8 81.2 121.8#
131 90.3 79.0 118.6


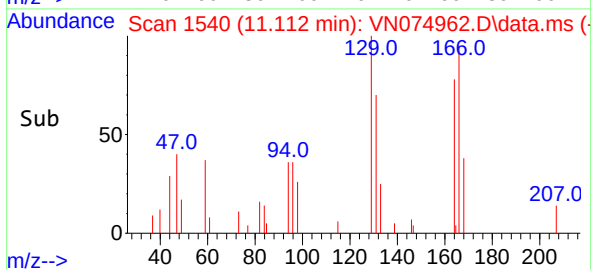






#67
Ethyl Benzene
Concen: 1.153 ug/l
RT: 11.965 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 91 Resp: 80564
Ion Ratio Lower Upper
91 100
106 29.9 25.4 38.2

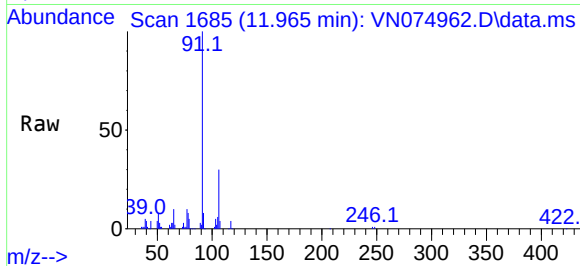

#68
m/p-Xylenes
Concen: 2.907 ug/l
RT: 12.076 min Scan# 1704
Delta R.T. 0.006 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 106 Resp: 79173
Ion Ratio Lower Upper
106 100
91 196.8 159.7 239.5


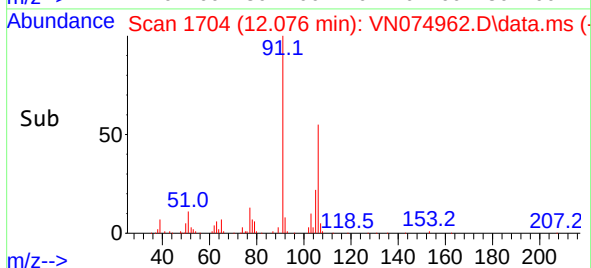

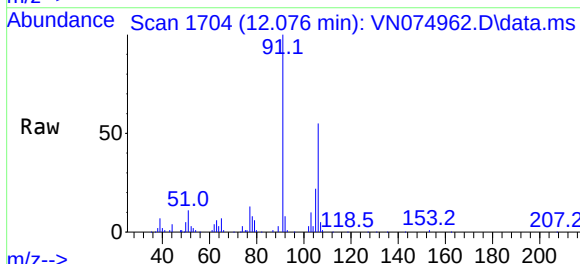




#71
Bromoform
Concen: 0.831 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.265 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:173 Resp: 9306
Ion Ratio Lower Upper
173 100
175 485.6 24.8 74.3#
254 0.0 0.1 0.1#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion:152 Resp: 701006
Ion Ratio Lower Upper
152 100
115 63.0 31.3 93.8
150 159.5 0.0 349.6


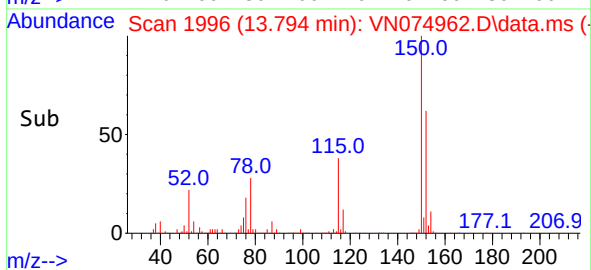






#76
1,2,3-Trichloropropane
Concen: 27.019 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.147 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 75 Resp: 513651
Ion Ratio Lower Upper
75 100
77 1.0 81.0 243.0#

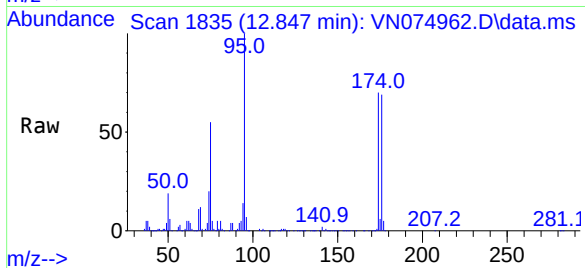

#78
n-propylbenzene
Concen: 0.240 ug/l
RT: 13.035 min Scan# 1867
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 91 Resp: 16115
Ion Ratio Lower Upper
91 100
120 24.9 11.5 34.4


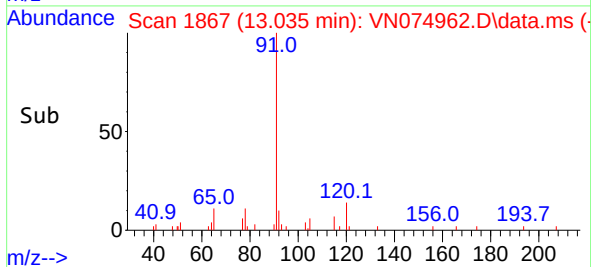

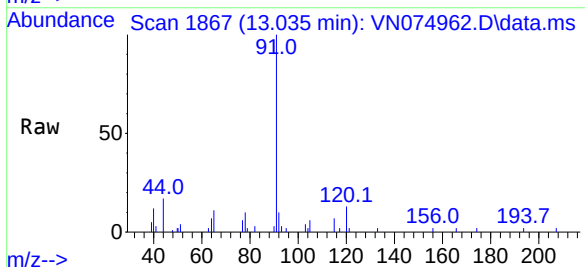




#80
1,3,5-Trimethylbenzene
Concen: 0.367 ug/l
RT: 13.176 min Scan# 1891
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:105 Resp: 18137
Ion Ratio Lower Upper
105 100
120 48.7 24.3 72.9

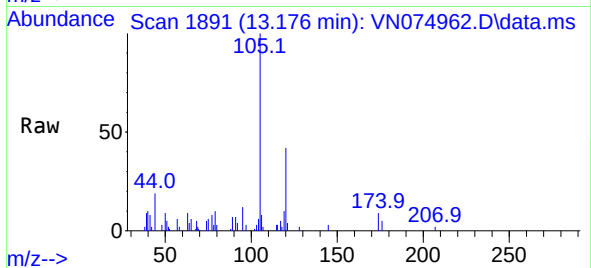

#81
trans-1,4-Dichloro-2-butene
Concen: 86.630 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.112 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion: 75 Resp: 513651
Ion Ratio Lower Upper
75 100
53 0.0 79.2 118.8#
89 0.0 37.9 56.9#


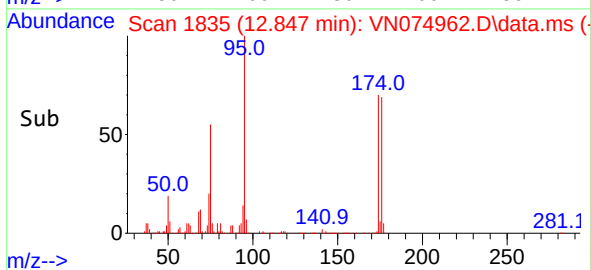






#84
1,2,4-Trimethylbenzene
Concen: 2.646 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:105 Resp: 132186
Ion Ratio Lower Upper
105 100
120 42.7 22.9 68.5

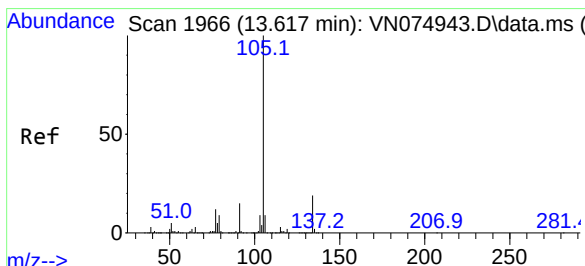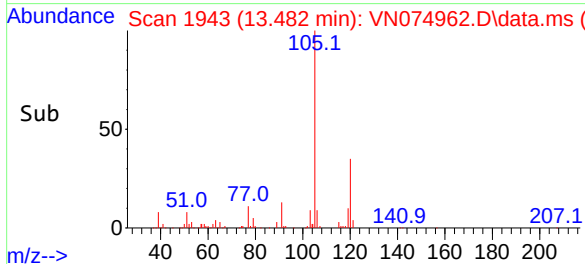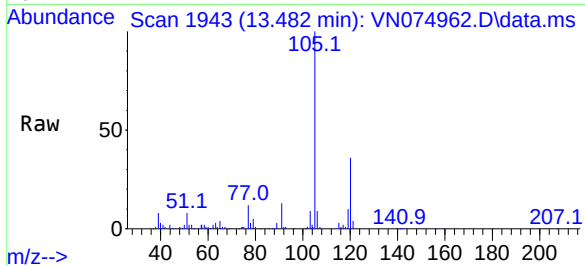

#85
sec-Butylbenzene
Concen: 2.151 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. -0.135 min
Lab File: VN074962.D
Acq: 21 Oct 2022 15:23

Tgt Ion:105 Resp: 132186
Ion Ratio Lower Upper
105 100
134 0.0 9.7 29.1#

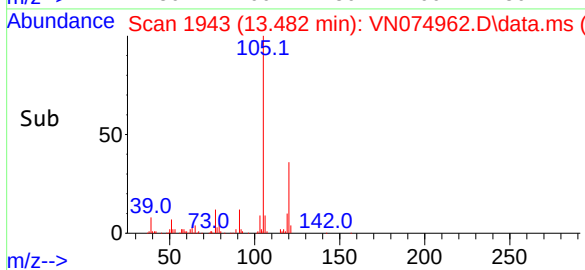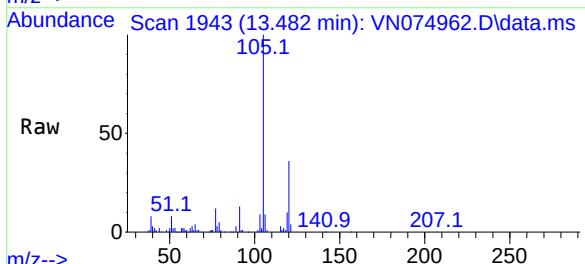



#95

Naphthalene

Concen: 9.042 ug/l

RT: 15.641 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN074962.D


Acq: 21 Oct 2022 15:23

Instrument :

MSVOA_N

ClientSampleId :

MW-4

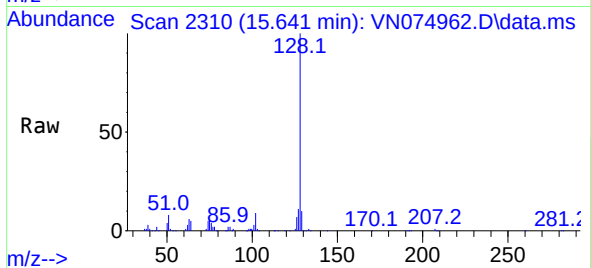

Tgt Ion:128 Resp: 385105

Ion Ratio Lower Upper

128 100

127 12.6 10.4 15.6

129 10.3 8.6 12.8

