

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102122\
 Data File : VN074969.D
 Acq On : 21 Oct 2022 18:12
 Operator : JC\MD
 Sample : N5222-15
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1A

Quant Time: Oct 22 02:55:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 21 09:37:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	796800	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	1341837	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	1319102	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	634513	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	878195	41.482	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	82.960%		
35) Dibromofluoromethane	8.177	113	694475	43.483	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	86.960%		
50) Toluene-d8	10.571	98	2855773	46.604	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	93.200%		
62) 4-Bromofluorobenzene	12.847	95	895297	41.420	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	82.840%#		
Target Compounds					Qvalue	
3) Chloromethane	2.377	50	3724	Below Cal		92
4) Vinyl Chloride	2.512	62	356	Below Cal	#	48
5) Bromomethane	2.906	94	983	Below Cal	#	4
6) Chloroethane	2.830	64	83158	3.628	ug/l #	45
7) Trichlorofluoromethane	3.506	101	321	Below Cal	#	18
11) Tert butyl alcohol	5.536	59	5529	1.235	ug/l #	78
12) 1,1-Dichloroethene	4.300	96	70	Below Cal	#	1
13) Acrolein	4.206	56	901	Below Cal	#	16
16) Acetone	4.453	43	26576	Below Cal		90
17) Carbon Disulfide	4.724	76	2914	Below Cal	#	74
19) Methyl tert-butyl Ether	5.824	73	15049	0.293	ug/l #	20
20) Methylene Chloride	5.283	84	3938	Below Cal	#	40
21) trans-1,2-Dichloroethene	5.553	96	243	Below Cal	#	1
25) 2-Butanone	7.500	43	8783	0.681	ug/l #	59
31) Cyclohexane	8.230	56	22913	1.059	ug/l #	18
36) 1,1-Dichloropropene	8.230	75	73096	3.634	ug/l #	49
38) Carbon Tetrachloride	8.236	117	88907	4.060	ug/l #	15
39) Methylcyclohexane	9.606	83	7296	0.306	ug/l #	64
40) Benzene	8.612	78	131606	2.122	ug/l	99
51) 4-Methyl-2-Pentanone	10.447	43	17097	0.703	ug/l	93
52) Toluene	10.635	92	116440	2.878	ug/l	99
58) 2-Chloroethyl Vinyl ether	10.159	63	85	3.616	ug/l #	45
67) Ethyl Benzene	11.965	91	52462	0.741	ug/l #	87
68) m/p-Xylenes	12.071	106	28166	1.020	ug/l	87
69) o-Xylene	12.394	106	5662	0.205	ug/l	90
76) 1,2,3-Trichloropropane	12.853	75	498935	28.996	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	498935	92.966	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.488	105	48884	1.081	ug/l	100
90) Hexachloroethane	14.335	117	2060	0.232	ug/l #	20
95) Naphthalene	15.647	128	109990	2.853	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102122\
Data File : VN074969.D
Acq On : 21 Oct 2022 18:12
Operator : JC\MD
Sample : N5222-15
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1A

Quant Time: Oct 22 02:55:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 21 09:37:47 2022
Response via : Initial Calibration




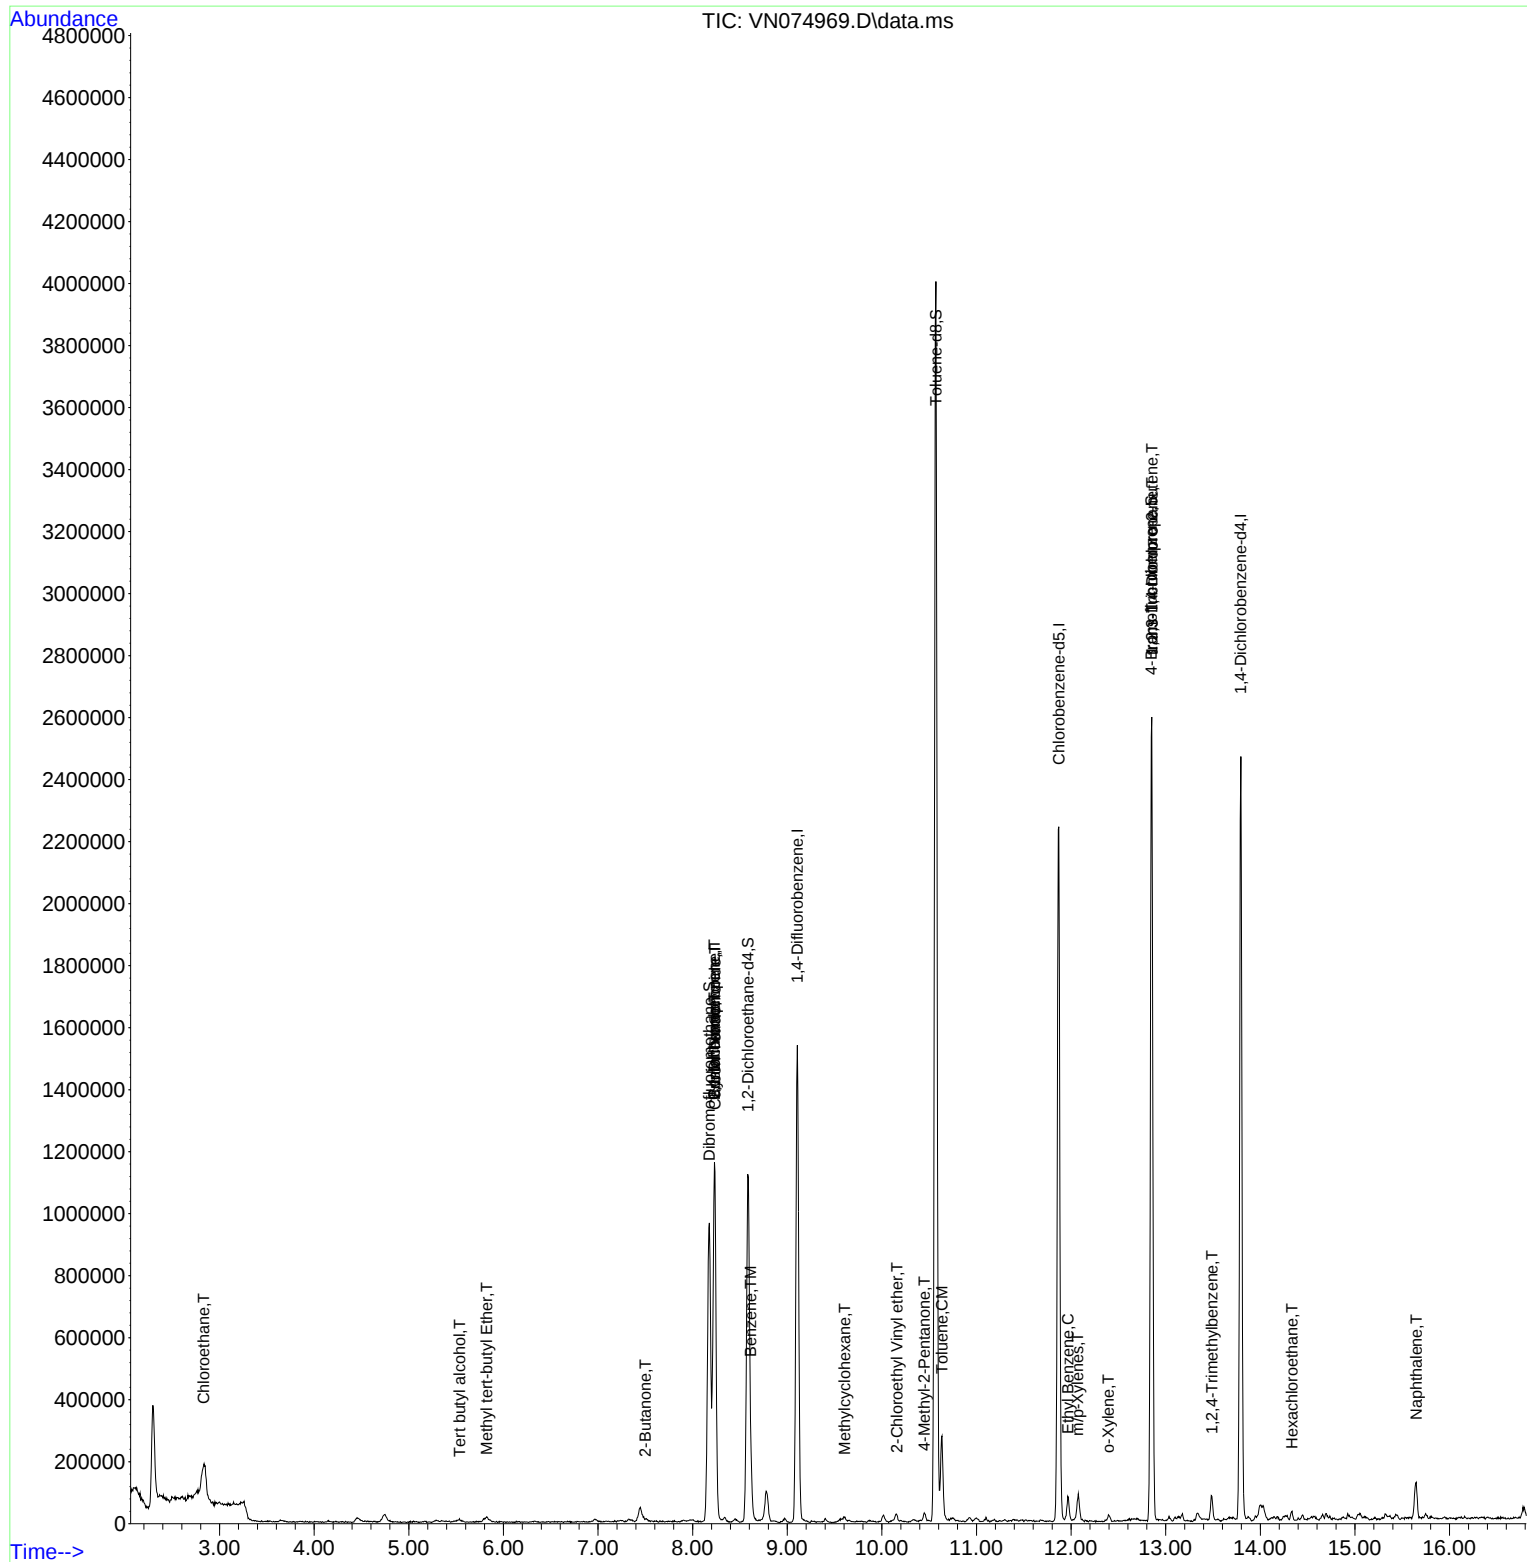




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion:168 Resp: 796800
Ion Ratio Lower Upper
168 100
99 65.1 52.2 78.4

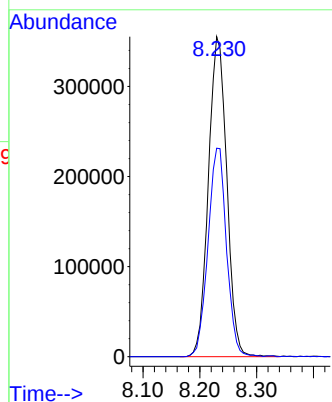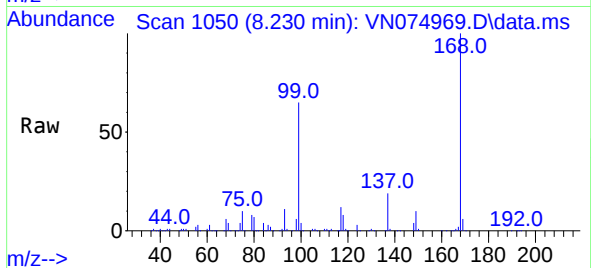

#3
Chloromethane
Concen: Below Cal
RT: 2.377 min Scan# 55
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 50 Resp: 3724
Ion Ratio Lower Upper
50 100
52 31.0 28.8 43.2


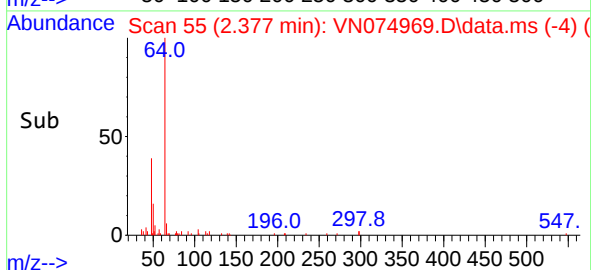






#4
Vinyl Chloride
Concen: Below Cal
RT: 2.512 min Scan# 71
Delta R.T. -0.012 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 62 Resp: 356
Ion Ratio Lower Upper
62 100
64 59.1 24.5 36.7#

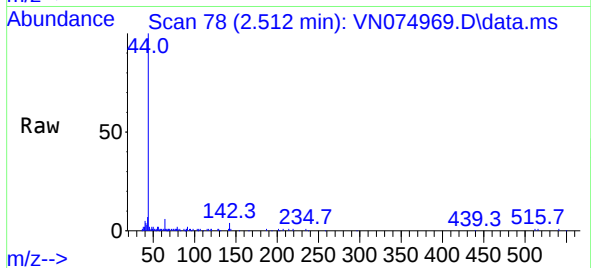

#5
Bromomethane
Concen: Below Cal
RT: 2.906 min Scan# 145
Delta R.T. -0.018 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 94 Resp: 983
Ion Ratio Lower Upper
94 100
96 0.0 73.5 110.3#


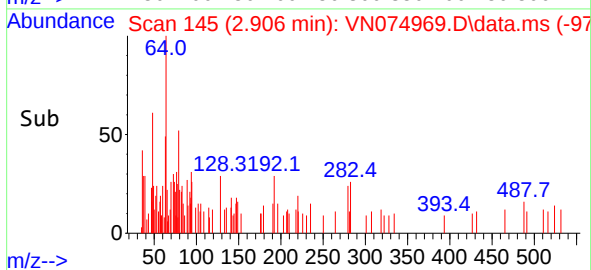






#6
Chloroethane
Concen: 3.628 ug/l
RT: 2.830 min Scan# 11
Delta R.T. -0.276 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 64 Resp: 83158
Ion Ratio Lower Upper
64 100
66 3.3 27.9 41.9#



#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.506 min Scan# 247
Delta R.T. 0.011 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion:101 Resp: 321
Ion Ratio Lower Upper
101 100
103 0.0 51.5 77.3#

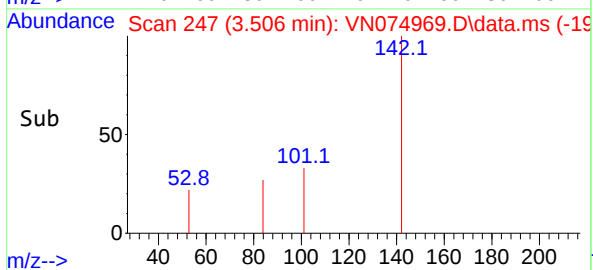



#11

Tert butyl alcohol

Concen: 1.235 ug/l

RT: 5.536 min Scan# 59

Delta R.T. 0.000 min

Lab File: VN074969.D

Acq: 21 Oct 2022 18:12

Instrument :

MSVOA_N

ClientSampleId :





MW-1A

Tgt Ion: 59 Resp: 5529

Ion Ratio Lower Upper

59 100

57 2.0 8.2 12.4#

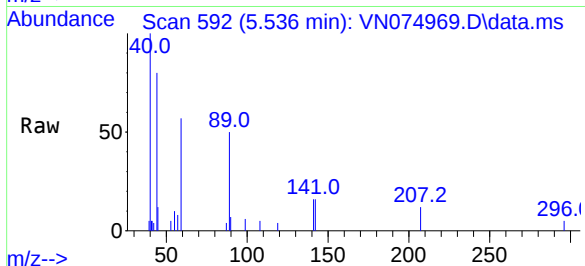

#12

1,1-Dichloroethene

Concen: Below Cal

RT: 4.300 min Scan# 382

Delta R.T. -0.047 min

Lab File: VN074969.D

Acq: 21 Oct 2022 18:12




Tgt Ion: 96 Resp: 70


Ion Ratio Lower Upper

96 100

61 0.0 128.9 193.3#

98 0.0 51.8 77.8#


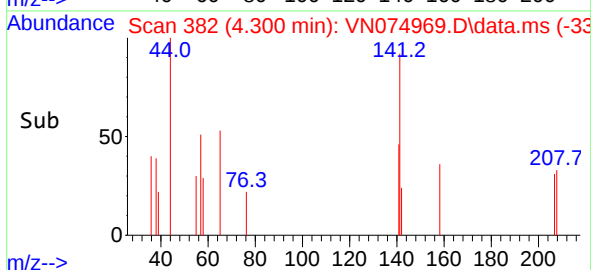
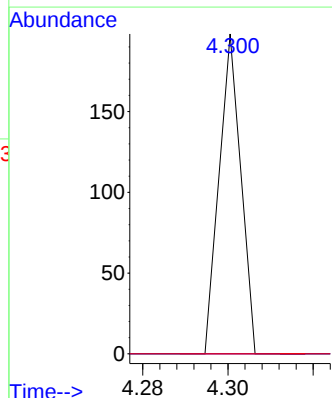
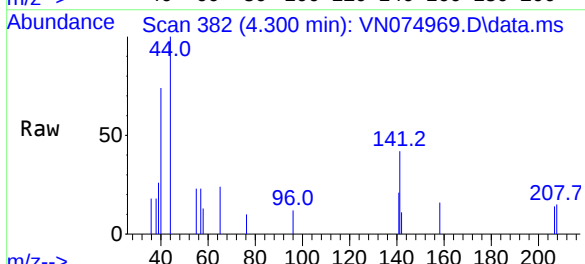




#13
Acrolein
Concen: Below Cal
RT: 4.206 min Scan# 301
Delta R.T. 0.017 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 56 Resp: 901
Ion Ratio Lower Upper
56 100
55 0.0 53.7 80.5#

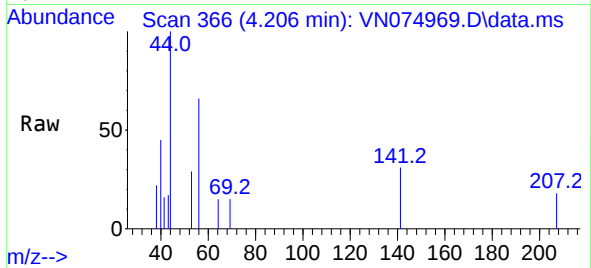

#16
Acetone
Concen: Below Cal
RT: 4.453 min Scan# 408
Delta R.T. 0.011 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 43 Resp: 26576
Ion Ratio Lower Upper
43 100
58 37.8 25.7 38.5


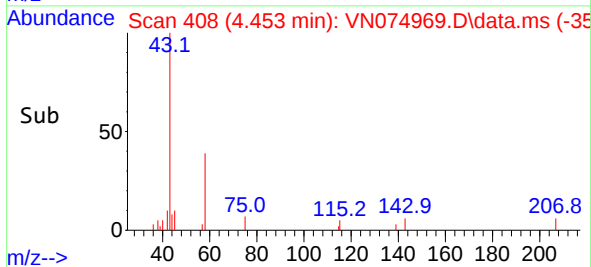

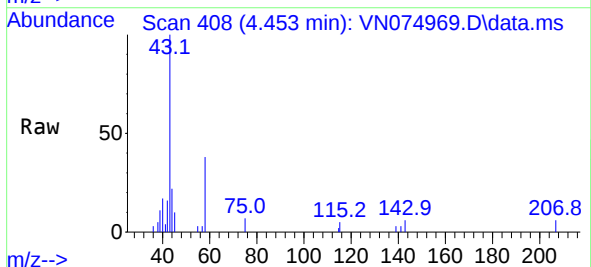




#17
Carbon Disulfide
Concen: Below Cal
RT: 4.724 min Scan# 411
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 76 Resp: 2914
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.2#

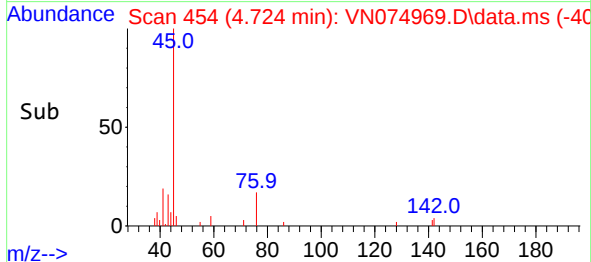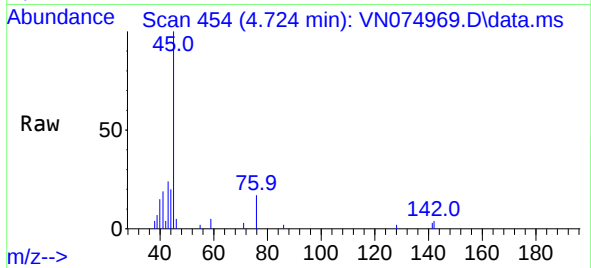

#19
Methyl tert-butyl Ether
Concen: 0.293 ug/l
RT: 5.824 min Scan# 641
Delta R.T. 0.018 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 73 Resp: 15049
Ion Ratio Lower Upper
73 100
57 58.6 16.9 25.3#


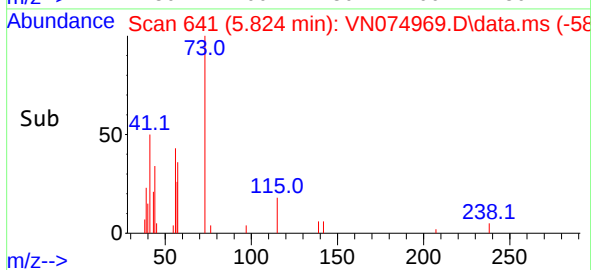






#20
Methylene Chloride
Concen: Below Cal
RT: 5.283 min Scan# 54
Delta R.T. -0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 84 Resp: 3938
Ion Ratio Lower Upper
84 100
49 47.8 88.6 133.0#
51 0.0 26.7 40.1#
86 13.8 49.7 74.5#

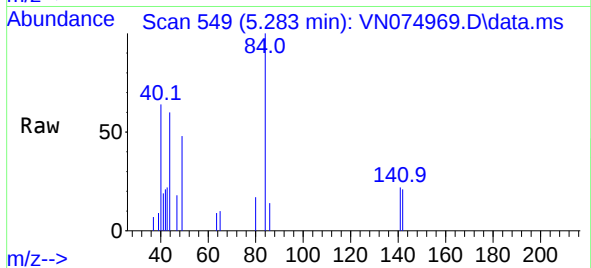

#21
trans-1,2-Dichloroethene
Concen: Below Cal
RT: 5.553 min Scan# 595
Delta R.T. -0.241 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 96 Resp: 243
Ion Ratio Lower Upper
96 100
61 0.0 112.6 169.0#
98 0.0 52.4 78.6#


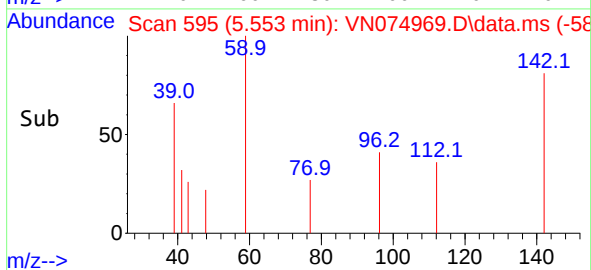






#25
2-Butanone
Concen: 0.681 ug/l
RT: 7.500 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 43 Resp: 8783
Ion Ratio Lower Upper
43 100
72 7.8 23.9 35.9#

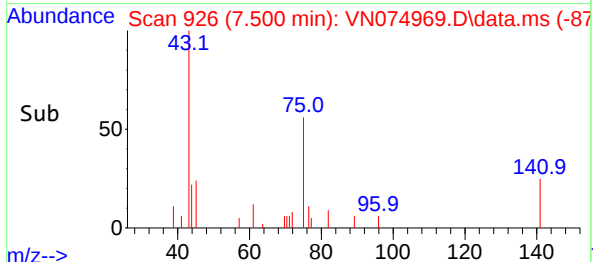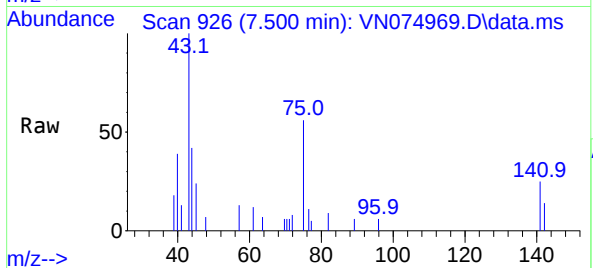

#31
Cyclohexane
Concen: 1.059 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.035 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 56 Resp: 22913
Ion Ratio Lower Upper
56 100
69 142.2 24.2 36.2#
84 150.7 82.8 124.2#


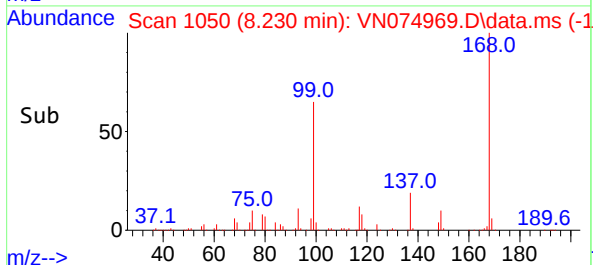
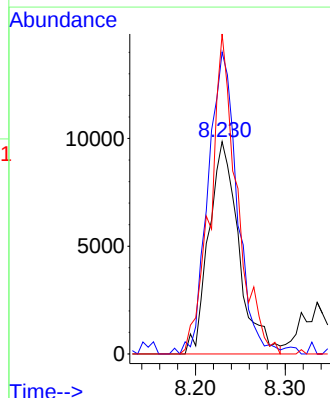
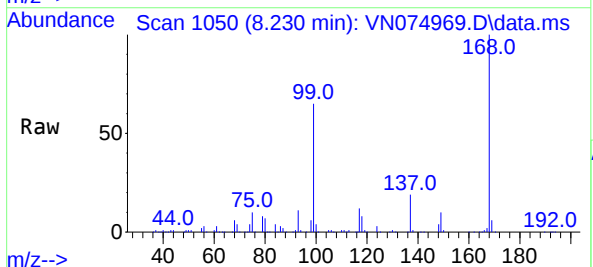




#33
1,2-Dichloroethane-d4
Concen: 41.482 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 65 Resp: 878195
Ion Ratio Lower Upper
65 100
67 52.5 0.0 102.6

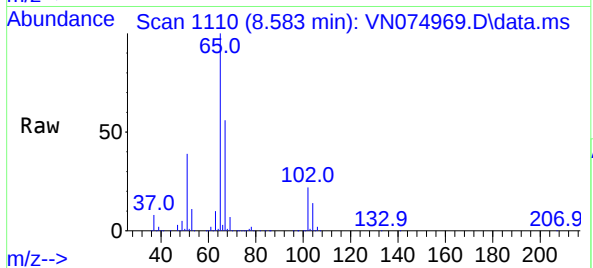

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion:114 Resp: 1341837
Ion Ratio Lower Upper
114 100
63 18.9 0.0 39.8
88 14.8 0.0 30.4


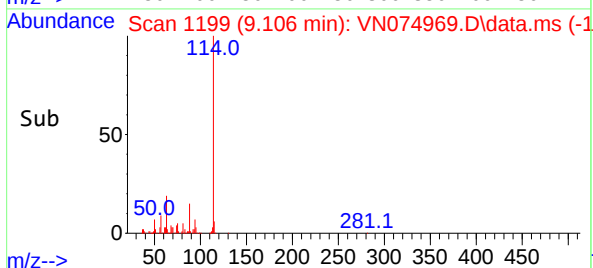






#35
Dibromofluoromethane
Concen: 43.483 ug/l
RT: 8.177 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion:113 Resp: 694475
Ion Ratio Lower Upper
113 100
111 102.2 83.4 125.2
192 16.4 13.3 19.9

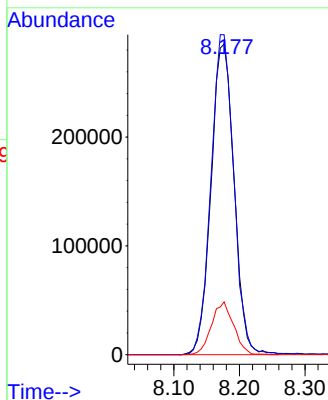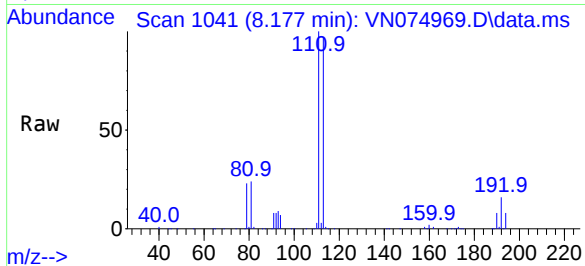

#36
1,1-Dichloropropene
Concen: 3.634 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.141 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 75 Resp: 73096
Ion Ratio Lower Upper
75 100
110 9.6 18.1 54.4#
77 0.0 25.0 37.4#


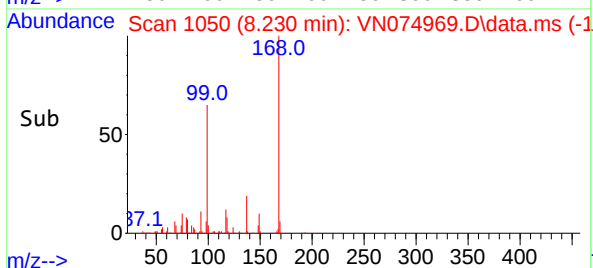
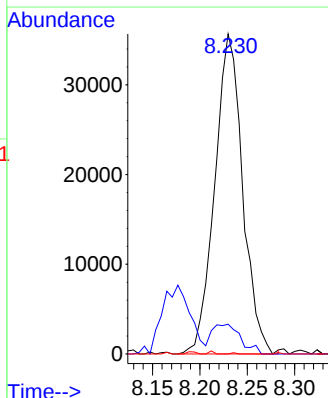
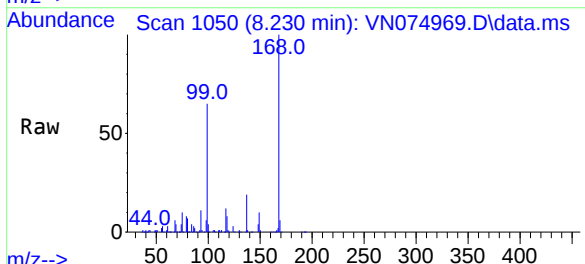




#38
Carbon Tetrachloride
Concen: 4.060 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.129 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion:117 Resp: 88907
Ion Ratio Lower Upper
117 100
119 3.3 75.2 112.8#
121 0.0 27.0 40.6#



#39
Methylcyclohexane
Concen: 0.306 ug/l
RT: 9.606 min Scan# 1284
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 83 Resp: 7296
Ion Ratio Lower Upper
83 100
55 43.2 50.8 76.2#
98 15.3 38.8 58.2#


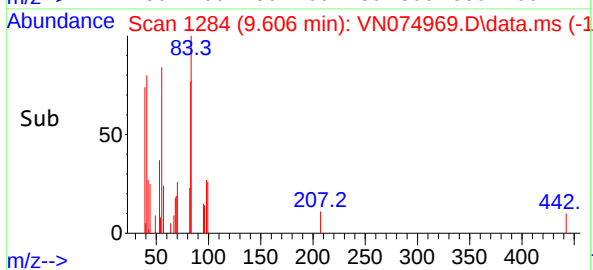






#40
Benzene
Concen: 2.122 ug/l
RT: 8.612 min Scan# 1115
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 78 Resp: 131606
Ion Ratio Lower Upper
78 100
77 24.3 19.6 29.4

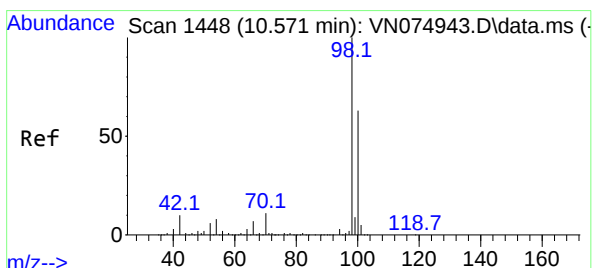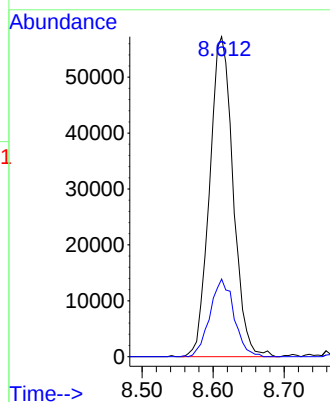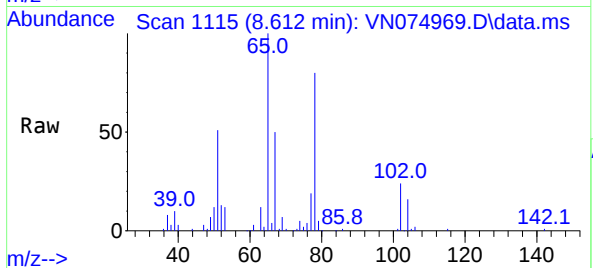

#50
Toluene-d8
Concen: 46.604 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 98 Resp: 2855773
Ion Ratio Lower Upper
98 100
100 64.6 51.4 77.2


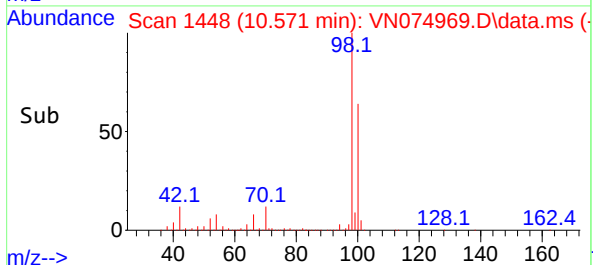

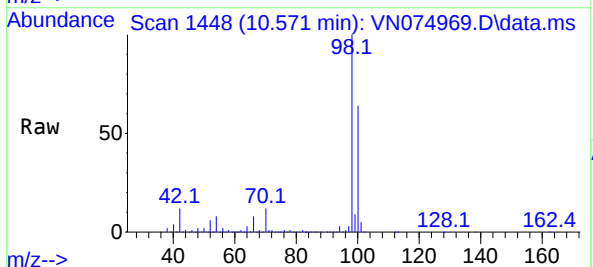




#51
4-Methyl-2-Pentanone
Concen: 0.703 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 43 Resp: 17097
Ion Ratio Lower Upper
43 100
58 46.4 33.6 50.4

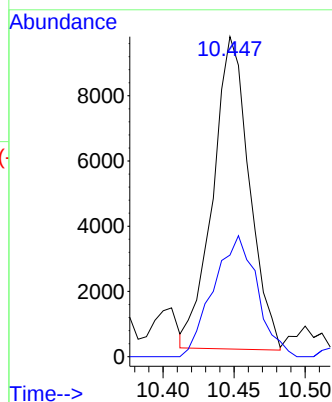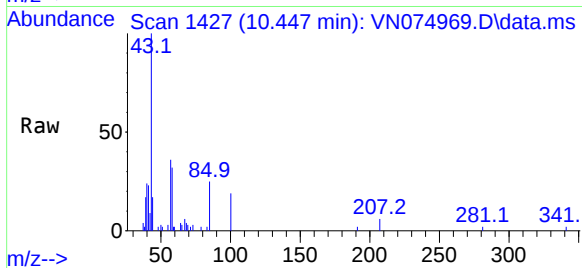

#52
Toluene
Concen: 2.878 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 92 Resp: 116440
Ion Ratio Lower Upper
92 100
91 172.5 139.2 208.8


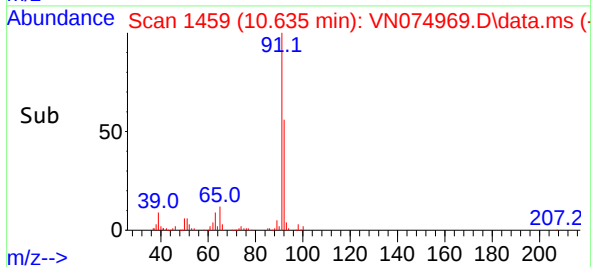
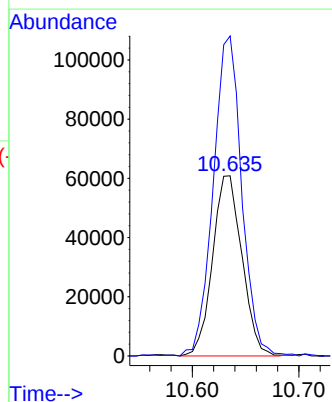
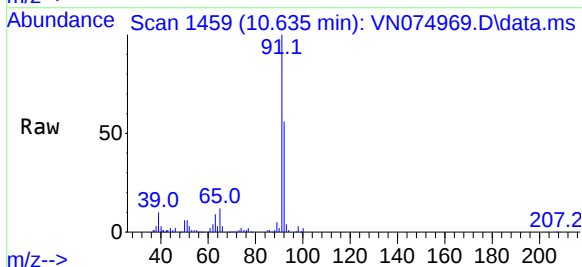




#58
2-Chloroethyl Vinyl ether
Concen: 3.616 ug/l
RT: 10.159 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 63 Resp: 85
Ion Ratio Lower Upper
63 100
106 0.0 24.1 36.1#

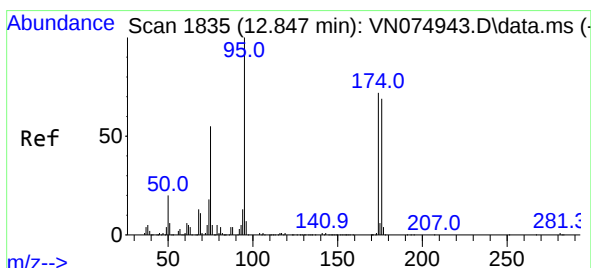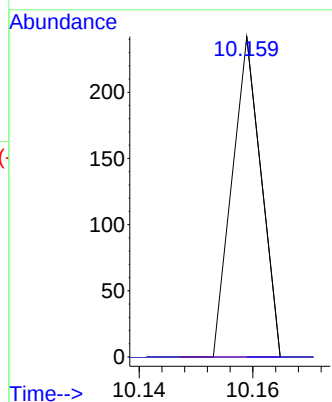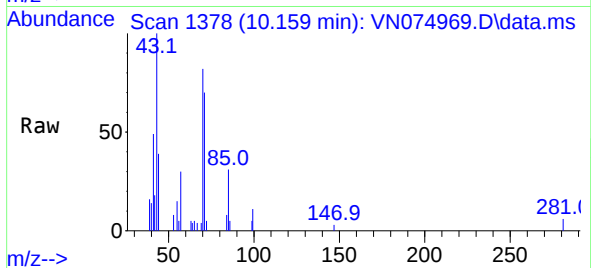

#62
4-Bromofluorobenzene
Concen: 41.420 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 95 Resp: 895297
Ion Ratio Lower Upper
95 100
174 73.2 0.0 143.0
176 70.3 0.0 138.2


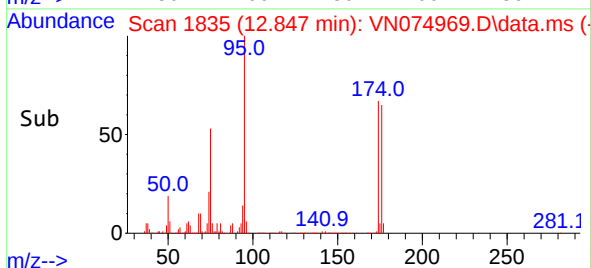






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion:117 Resp: 1319102
Ion Ratio Lower Upper
117 100
82 56.3 45.6 68.4
119 32.3 25.1 37.7

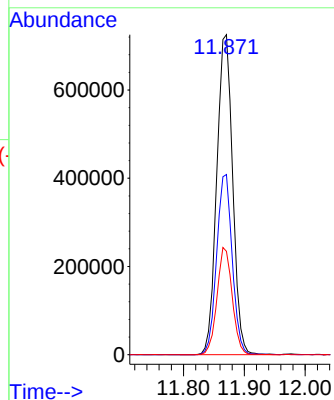

#67
Ethyl Benzene
Concen: 0.741 ug/l
RT: 11.965 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 91 Resp: 52462
Ion Ratio Lower Upper
91 100
106 24.8 25.4 38.2#


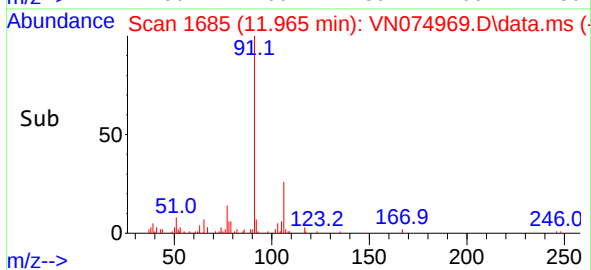
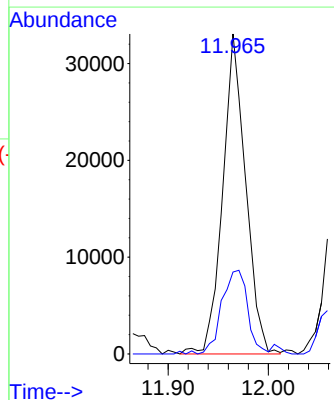





#68
m/p-Xylenes
Concen: 1.020 ug/l
RT: 12.071 min Scan# 1703
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion:106 Resp: 28166
Ion Ratio Lower Upper
106 100
91 179.5 159.7 239.5

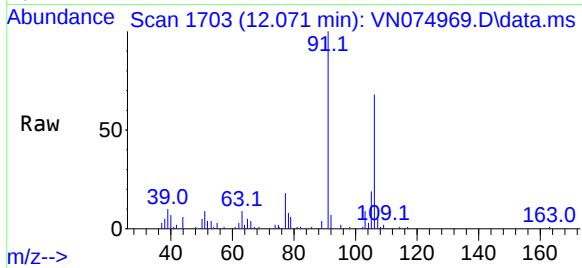

#69
o-Xylene
Concen: 0.205 ug/l
RT: 12.394 min Scan# 1758
Delta R.T. -0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion:106 Resp: 5662
Ion Ratio Lower Upper
106 100
91 222.6 103.6 310.7


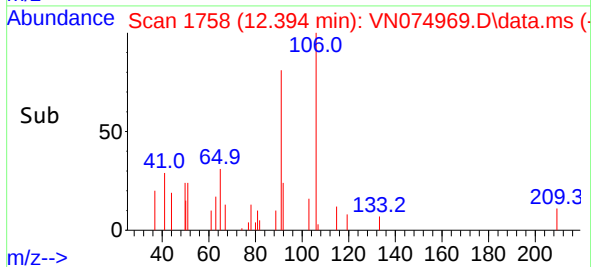

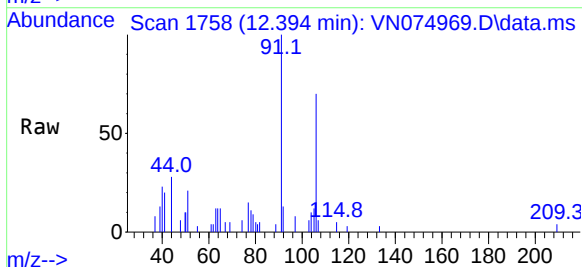




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion:152 Resp: 634513
Ion Ratio Lower Upper
152 100
115 60.7 31.3 93.8
150 155.8 0.0 349.6



#76
1,2,3-Trichloropropane
Concen: 28.996 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 75 Resp: 498935
Ion Ratio Lower Upper
75 100
77 1.2 81.0 243.0#


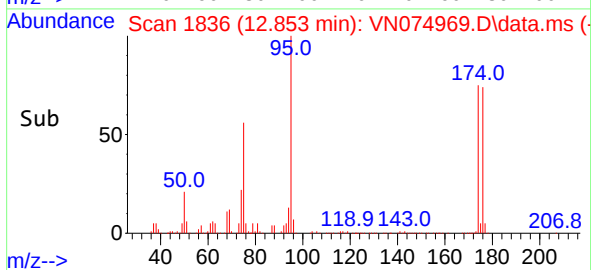






#81
trans-1,4-Dichloro-2-butene
Concen: 92.966 ug/l
RT: 12.853 min Scan# 1816
Delta R.T. 0.118 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12




Instrument :
MSVOA_N
ClientSampleId :
MW-1A


Tgt Ion: 75 Resp: 498935
Ion Ratio Lower Upper
75 100
53 0.1 79.2 118.8#
89 0.0 37.9 56.9#

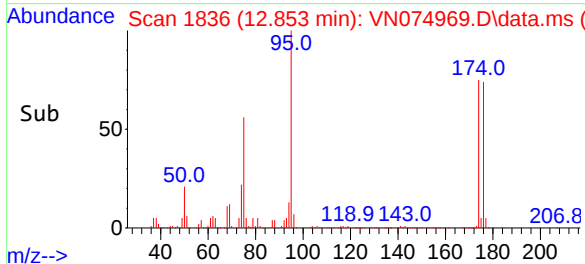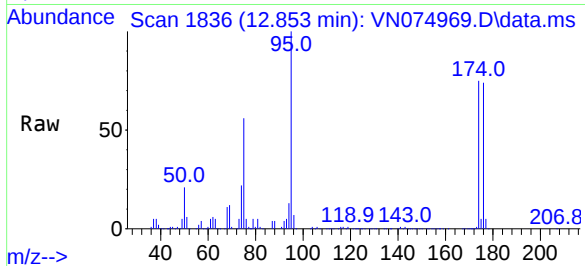

#84
1,2,4-Trimethylbenzene
Concen: 1.081 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion: 105 Resp: 48884
Ion Ratio Lower Upper
105 100
120 45.7 22.9 68.5


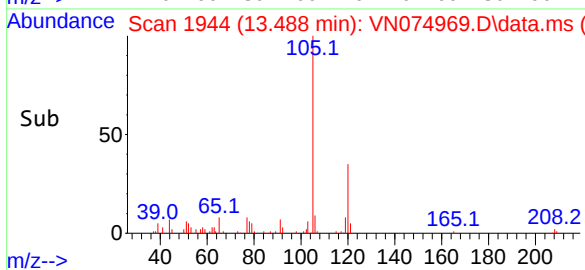

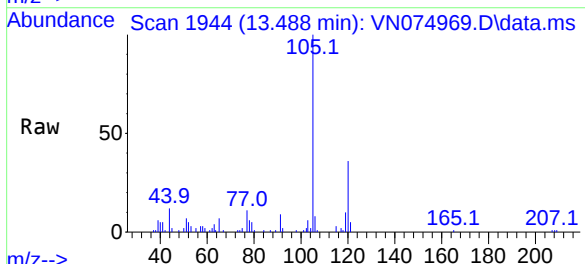




#90
Hexachloroethane
Concen: 0.232 ug/l
RT: 14.335 min Scan# 2088
Delta R.T. 0.000 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Instrument :
MSVOA_N
ClientSampleId :
MW-1A

Tgt Ion:117 Resp: 2060
Ion Ratio Lower Upper
117 100
201 0.0 30.6 91.6#



#95
Naphthalene
Concen: 2.853 ug/l
RT: 15.647 min Scan# 2311
Delta R.T. 0.006 min
Lab File: VN074969.D
Acq: 21 Oct 2022 18:12

Tgt Ion:128 Resp: 109990
Ion Ratio Lower Upper
128 100
127 14.2 10.4 15.6
129 10.0 8.6 12.8

