
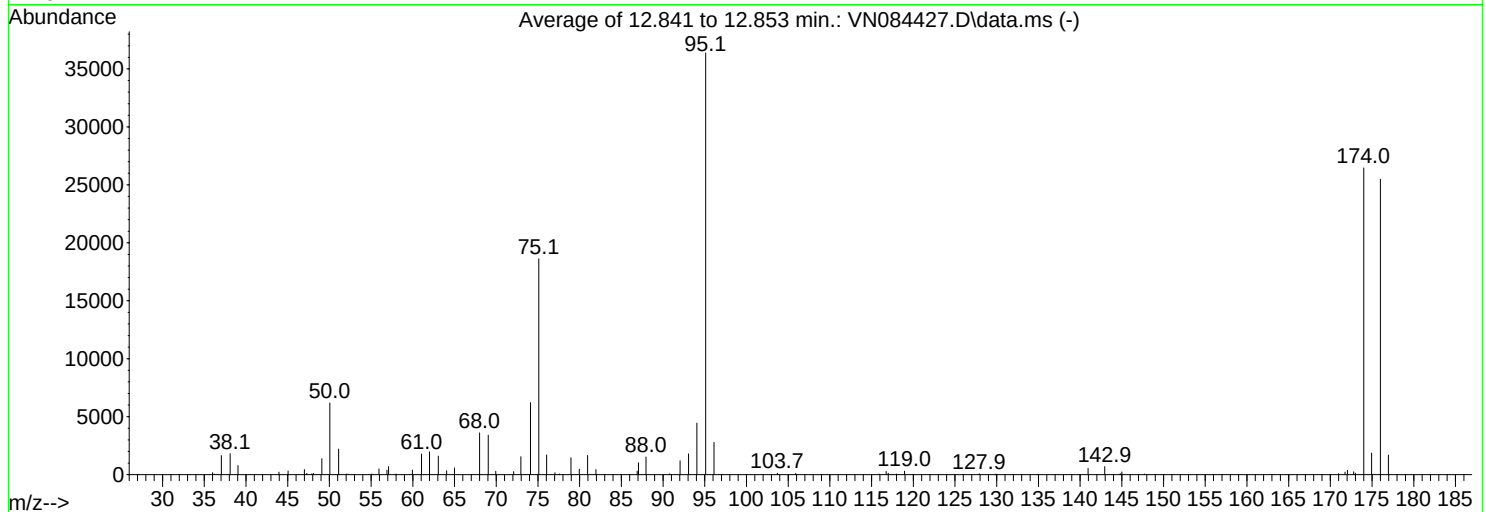


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102124\
Data File : VN084427.D
Acq On : 21 Oct 2024 11:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

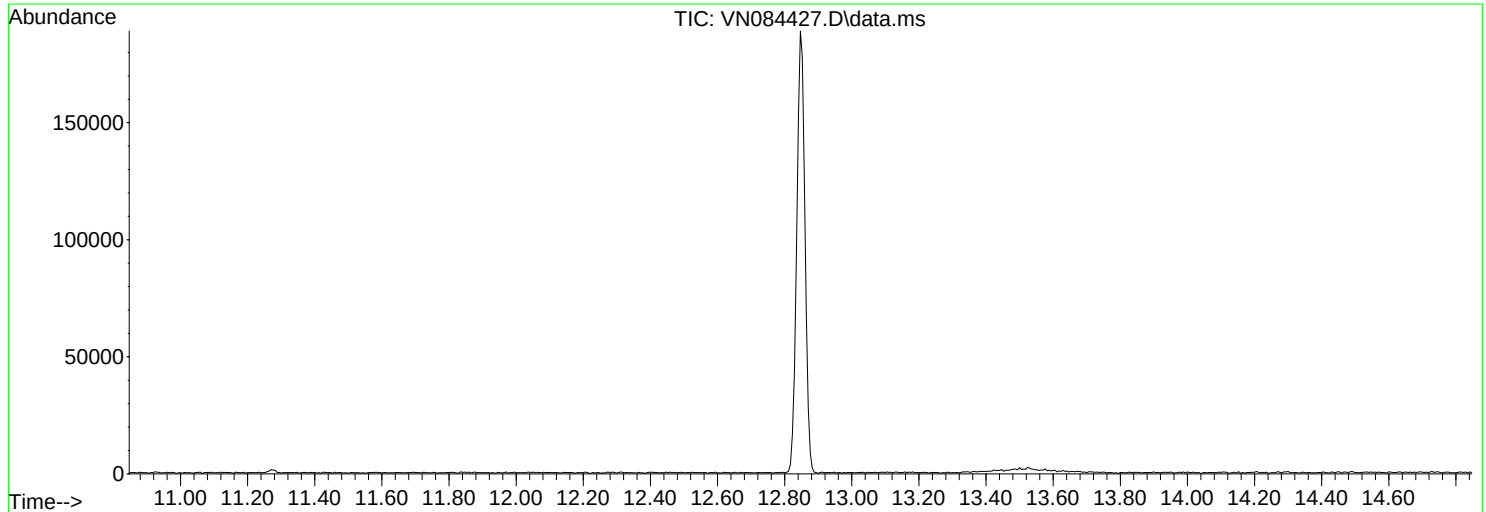

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	6183	PASS
75	95	30	60	51.2	18619	PASS
95	95	100	100	100.0	36389	PASS
96	95	5	9	7.6	2782	PASS
173	174	0.00	2	0.9	244	PASS
174	95	50	100	72.7	26461	PASS
175	174	5	9	7.0	1860	PASS
176	174	95	101	96.3	25488	PASS
177	176	5	9	6.6	1686	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	173	49.10	1383	62.00	1954	76.05	1691
36.20	62	50.05	6183	63.05	1600	77.05	1601
37.05	1646	51.10	2214	64.05	334	77.60	515
38.10	1802	52.10	76	65.00	574	78.95	1471
39.05	782	55.10	60	68.00	3606	79.95	469
43.95	224	55.95	502	69.05	3408	80.95	1651
45.05	325	56.90	392	69.95	285	81.95	446
47.00	441	57.10	689	72.10	256	86.90	298
47.30	116	58.00	55	72.95	1542	87.05	1021
47.90	81	59.95	405	74.10	6211	87.95	1521
48.10	92	61.05	1781	75.10	18619	90.80	69

Average of 12.841 to 12.853 min.: VN084427.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	1209	118.95	300	172.80	244		
93.05	1790	127.90	64	173.00	128		
94.05	4443	129.90	52	174.00	26461		
95.10	36389	140.95	536	174.95	1860		
96.10	2782	142.95	694	176.00	25488		
103.70	131	144.80	80	176.95	1686		
105.90	112	145.00	233				
115.90	53	147.70	52				
116.75	276	171.00	81				
117.00	118	171.75	218				
118.00	55	172.05	376				

Instrument :

MSVOA_N

ClientSampleId :

BFB