

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102219\
 Data File : VN058900.D
 Acq On : 22 Oct 2019 11:16
 Operator : JC/SP
 Sample : VN1022WBS01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1022WBS01

Quant Time: Oct 23 04:53:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100819SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 09 04:07:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	1711129	5.00	ug/l	-0.02
4) 1,4-Difluorobenzene	8.56	114	2353896	5.00	ug/l	0.00
8) Chlorobenzene-d5	11.41	117	2123186	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	656652	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.00	65	1100582	5.38	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	107.60%
5) Dibromofluoromethane	7.57	113	861817	5.81	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	116.20%
6) Toluene-d8	10.08	98	1810596	5.40	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	108.00%
7) 4-Bromofluorobenzene	12.40	95	716749	4.37	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	87.40%


Target Compounds					Qvalue
2) Vinyl Chloride	2.16	62	1017693	5.853 ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102219\
Data File : VN058900.D
Acq On : 22 Oct 2019 11:16
Operator : JC/SP
Sample : VN1022WBS01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1022WBS01

Quant Time: Oct 23 04:53:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N100819SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Wed Oct 09 04:07:23 2019
Response via : Initial Calibration

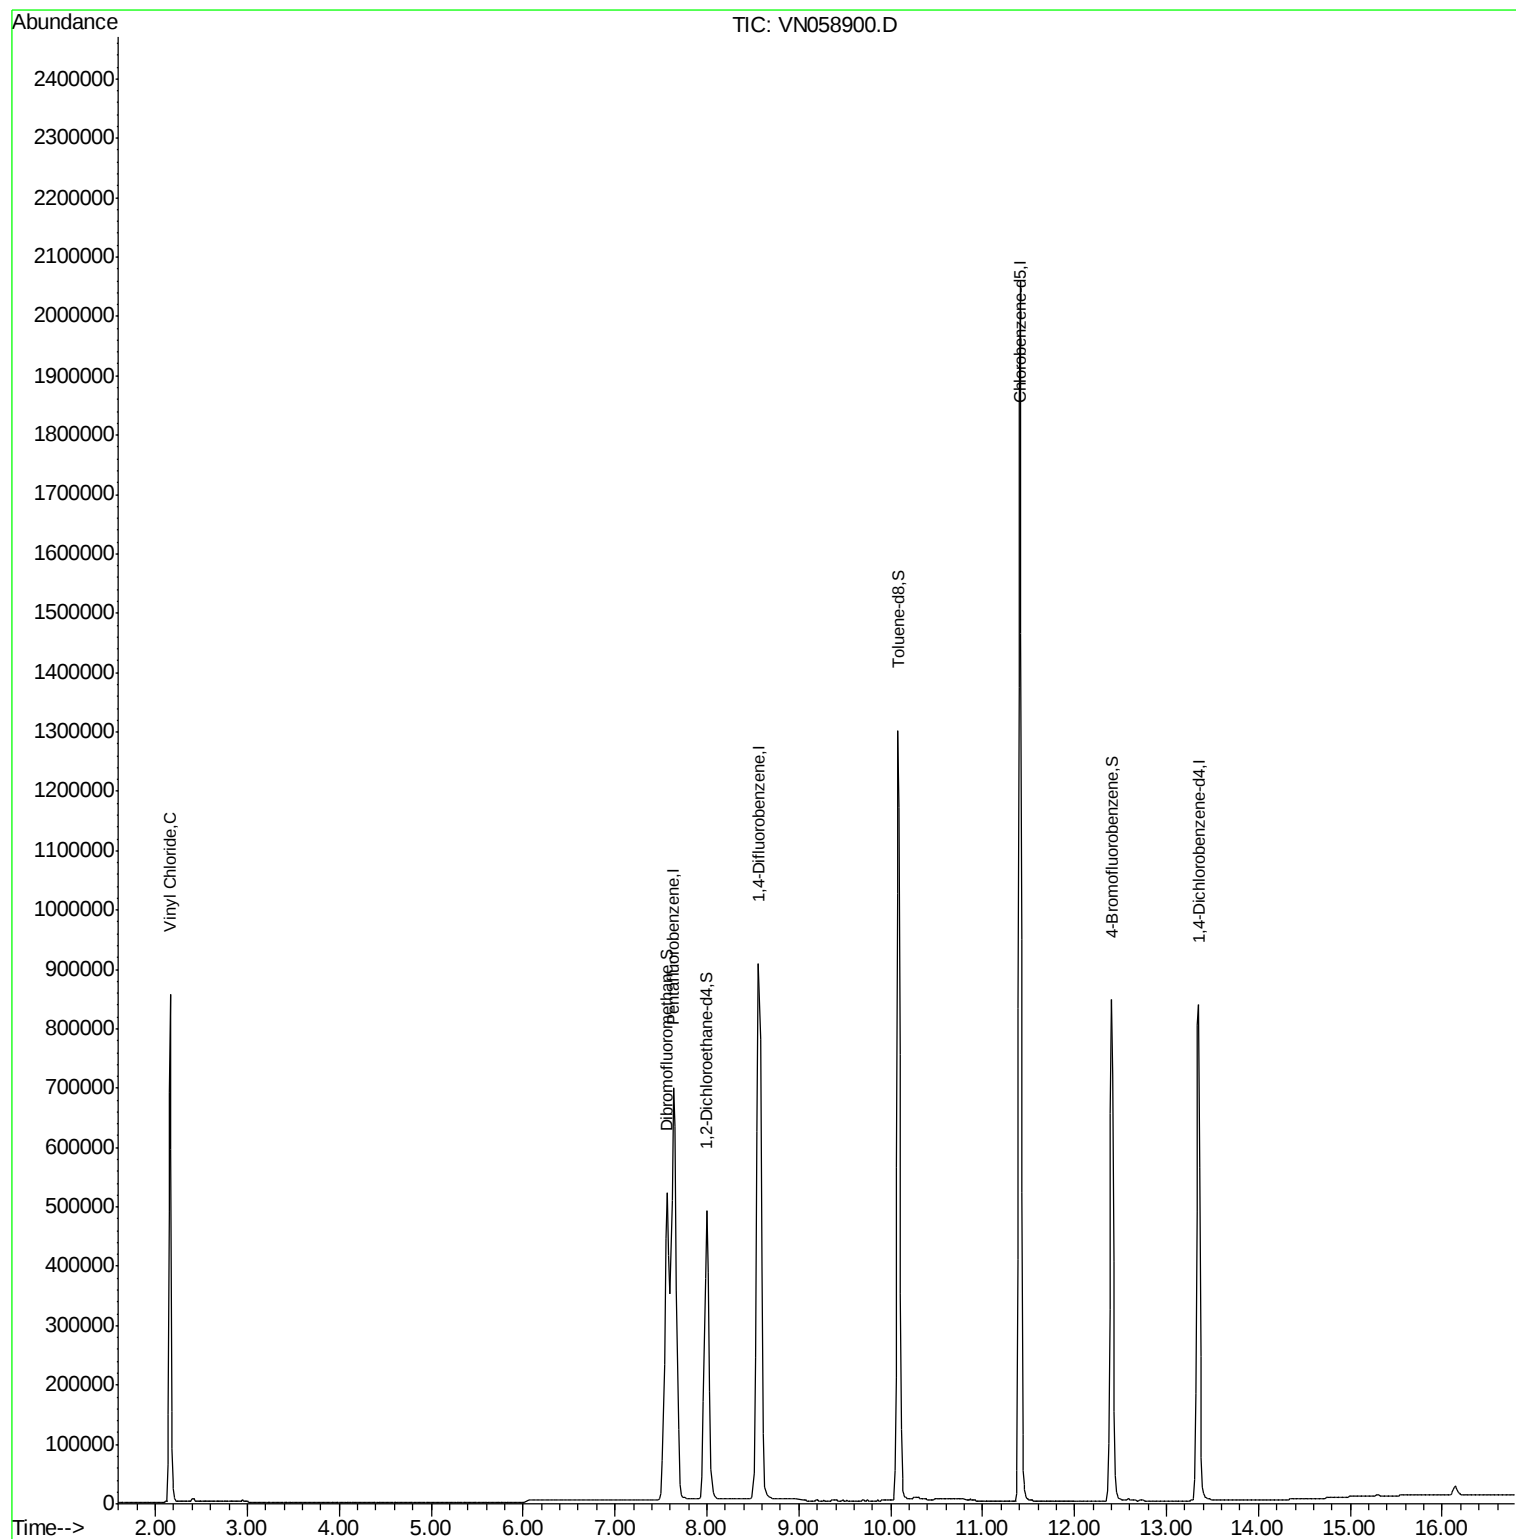



#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.64 min Scan# 1242

Delta R.T. -0.02 min

Lab File: VN058900.D

Acq: 22 Oct 2019 11:16

Instrument :

MSVOA_N

ClientSampleId :


VN1022WBS01

Tot Ion:168 Resp: 1711129

Ion Ratio Lower Upper




168 100

99 51.7 36.8 55.2

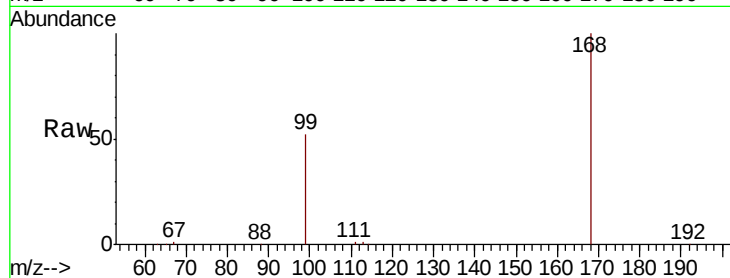

Abundance Ion 168.00 (167.70 to 168.70): VN058900.D (-1225) (-)

Ion 99.00 (98.70 to 99.70): VN058900.D (-1225) (-)

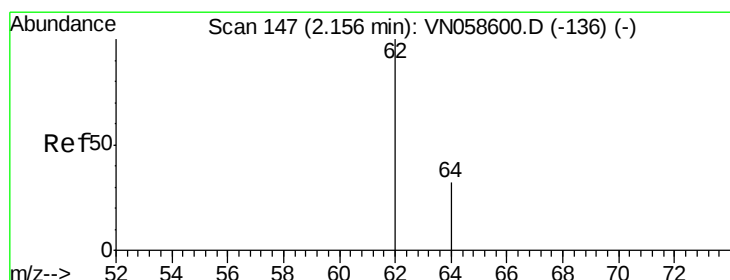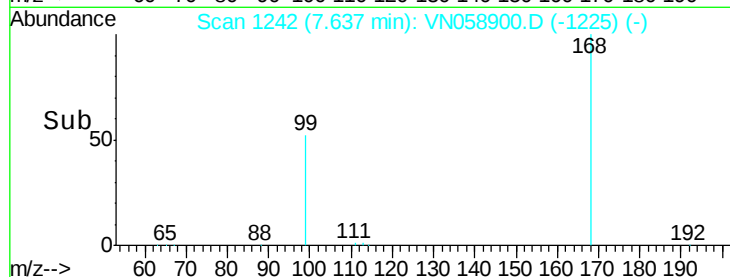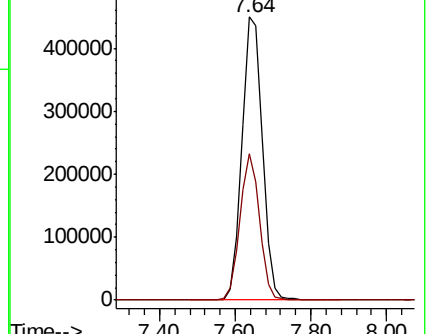

#2

Vinyl Chloride

Concen: 5.853 ug/l

RT: 2.16 min Scan# 148

Delta R.T. 0.00 min

Lab File: VN058900.D


Acq: 22 Oct 2019 11:16

Tgt Ion: 62 Resp: 1017693

Ion Ratio Lower Upper



62 100


64 32.7 25.8 38.6

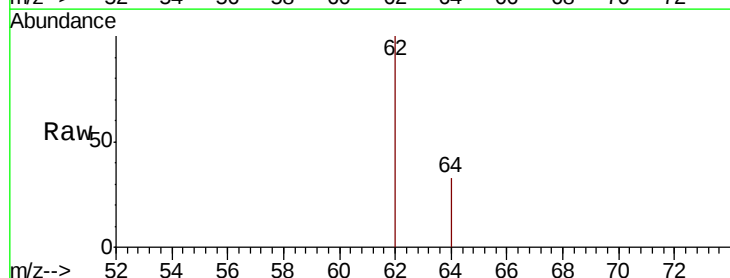

Abundance Ion 62.00 (61.70 to 62.70): VN058900.D (-95) (-)

Ion 64.00 (63.70 to 64.70): VN058900.D (-95) (-)

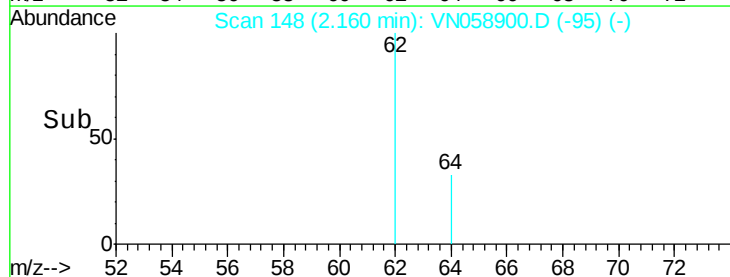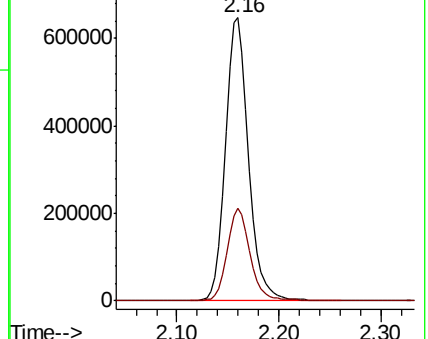

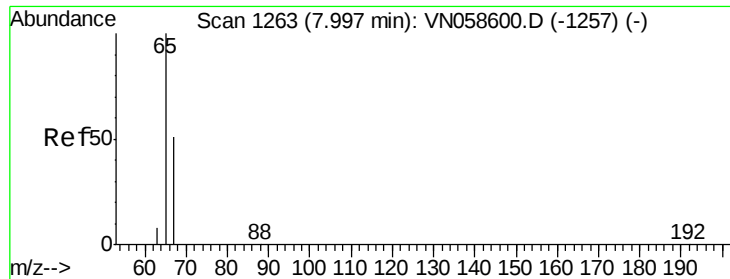

#3

1,2-Dichloroethane-d4

Concen: 5.384 ug/l

RT: 8.00 min Scan# 1263

Delta R.T. 0.00 min

Lab File: VN058900.D

Acq: 22 Oct 2019 11:16

Instrument :

MSVOA_N

ClientSampleId :





VN1022WBS01

Tot Ion: 65 Resp: 1100582

Ion Ratio Lower Upper

65 100

67 52.0 0.0 103.4

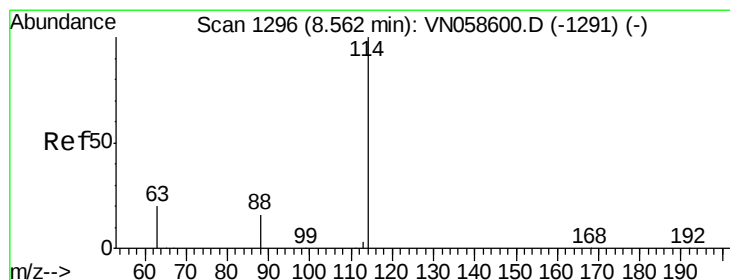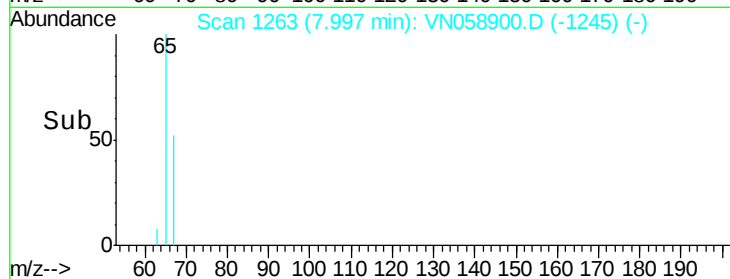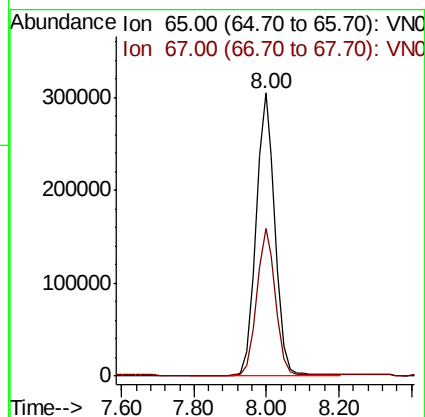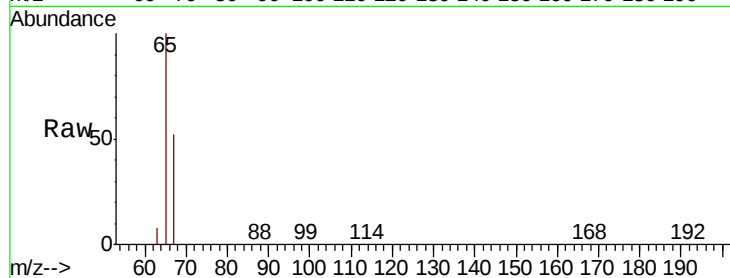

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.56 min Scan# 1296

Delta R.T. 0.00 min

Lab File: VN058900.D

Acq: 22 Oct 2019 11:16




Tgt Ion: 114 Resp: 2353896

Ion Ratio Lower Upper

114 100

63 19.1 0.0 40.6

88 15.2 0.0 32.4


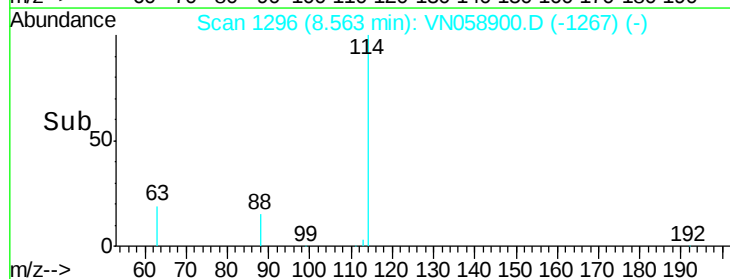
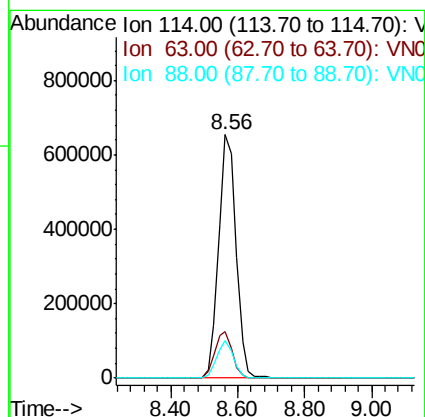
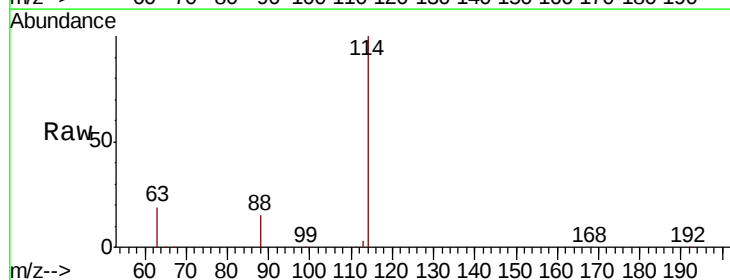




#5
 Dibromofluoromethane
 Concen: 5.812 ug/l
 RT: 7.57 min Scan# 1238
 Delta R.T. 0.00 min
 Lab File: VN058900.D
 Acq: 22 Oct 2019 11:16




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1022WBS01


Tot Ion	Ratio	Lower	Upper
113	100		
111	101.4	82.5	123.7
192	20.1	14.9	22.3

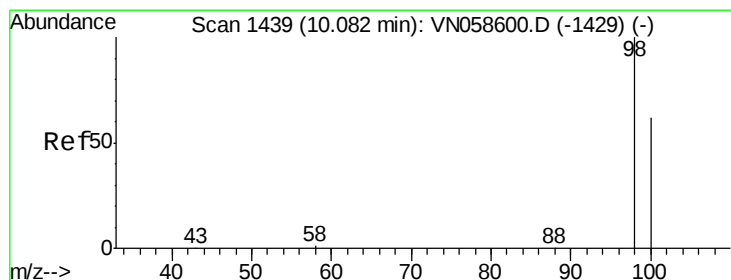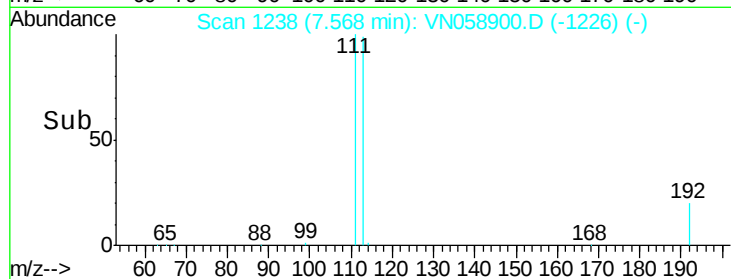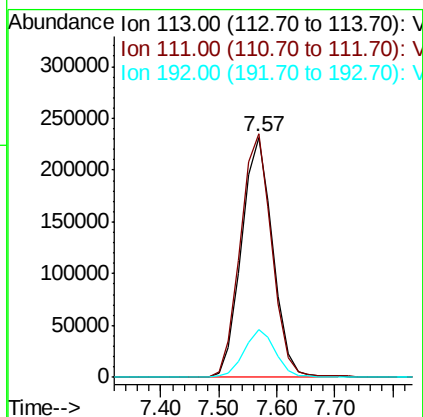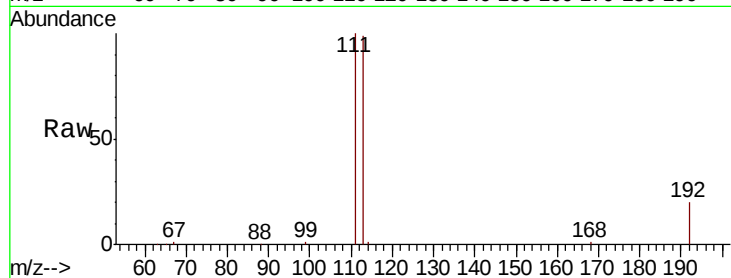

#6
 Toluene-d8
 Concen: 5.404 ug/l
 RT: 10.08 min Scan# 1439
 Delta R.T. 0.00 min
 Lab File: VN058900.D
 Acq: 22 Oct 2019 11:16

Tgt Ion	Ratio	Lower	Upper
98	100		
100	61.3	49.4	74.2

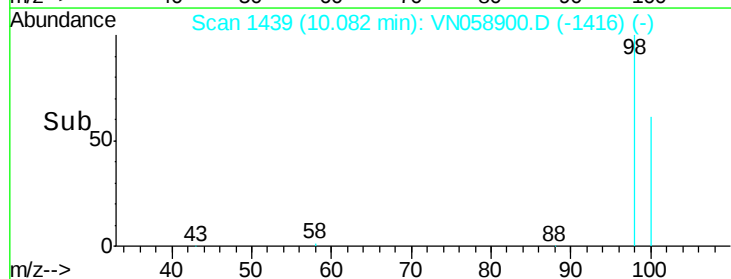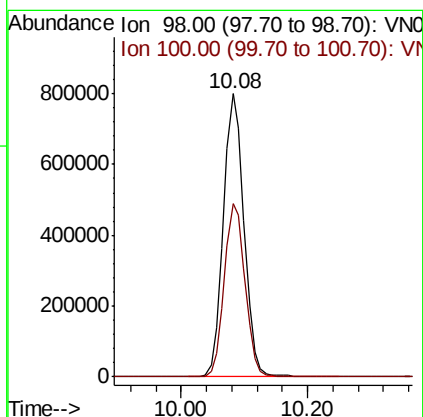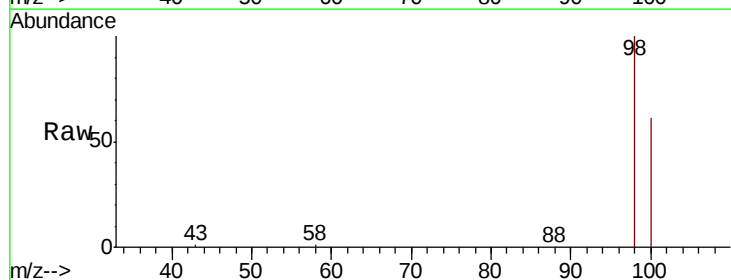

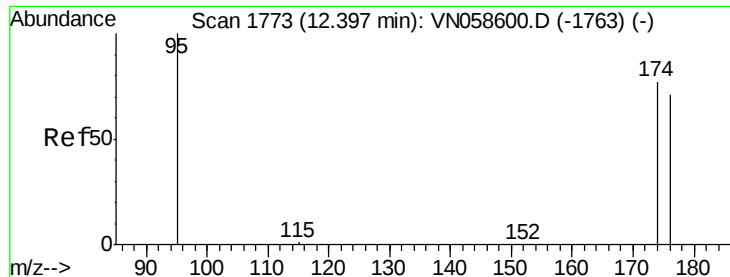

#7

4-Bromofluorobenzene

Concen: 4.366 ug/l

RT: 12.40 min Scan# 1773

Delta R.T. 0.01 min

Lab File: VN058900.D

Acq: 22 Oct 2019 11:16

Instrument :

MSVOA_N

ClientSampleId :

VN1022WBS01


Tot Ion: 95 Resp: 716749

Ion Ratio Lower Upper

95 100

174 96.4 0.0 153.4




176 90.5 0.0 142.2

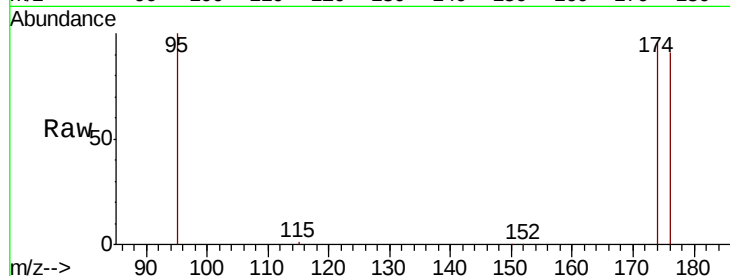

Abundance Ion 95.00 (94.70 to 95.70): VN058600.D (-1763) (-)

Ion 174.00 (173.70 to 174.70): VN058600.D (-1763) (-)

Ion 176.00 (175.70 to 176.70): VN058600.D (-1763) (-)

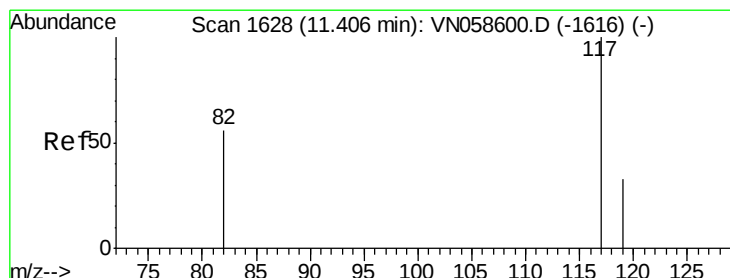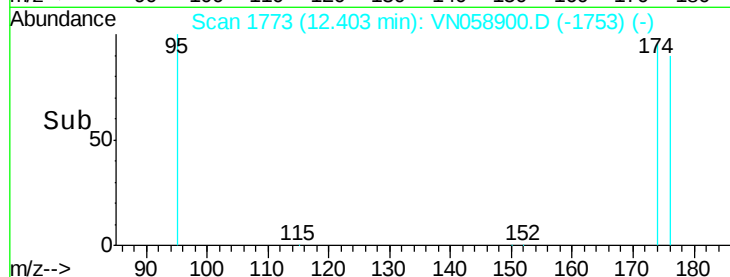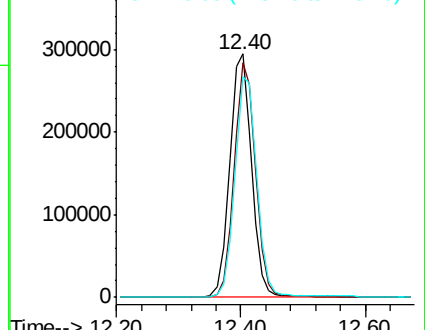

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.41 min Scan# 1628

Delta R.T. 0.00 min

Lab File: VN058900.D

Acq: 22 Oct 2019 11:16


Tgt Ion: 117 Resp: 2123186

Ion Ratio Lower Upper

117 100

82 52.1 44.7 67.1



119 32.1 27.0 40.4

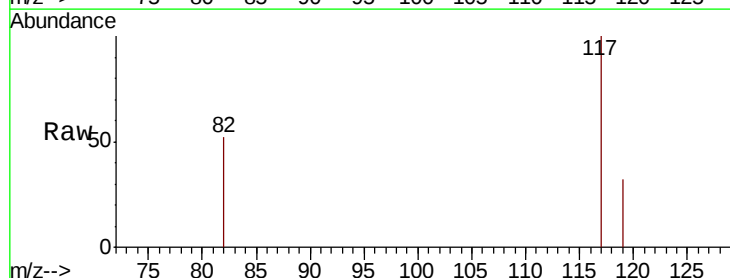


Abundance Ion 117.00 (116.70 to 117.70): VN058600.D (-1616) (-)

Ion 82.00 (81.70 to 82.70): VN058600.D (-1616) (-)

Ion 119.00 (118.70 to 119.70): VN058600.D (-1616) (-)

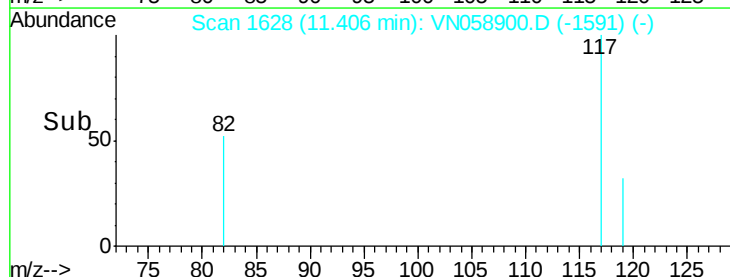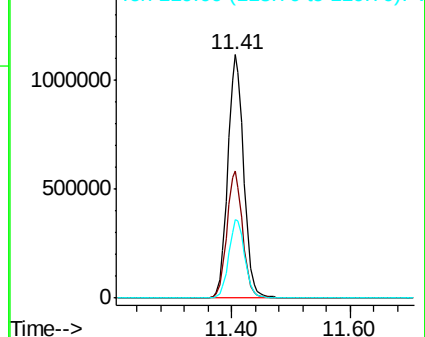


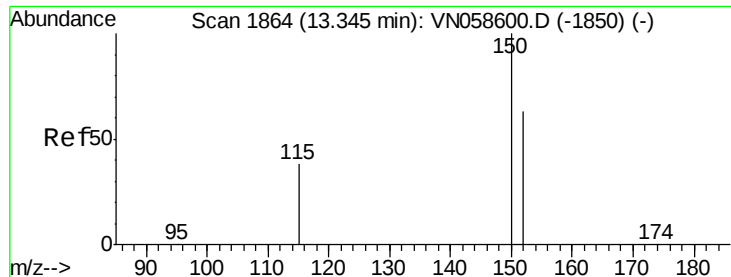

#9
 1,4-Dichlorobenzene-d4
 Concen: 5.000 ug/l
 RT: 13.35 min Scan# 1864
 Delta R.T. 0.01 min
 Lab File: VN058900.D
 Acq: 22 Oct 2019 11:16

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1022WBS01

Tot Ion:152 Resp: 656652
 Ion Ratio Lower Upper
 152 100
 115 52.6 29.9 89.8
 150 153.7 0.0 315.8

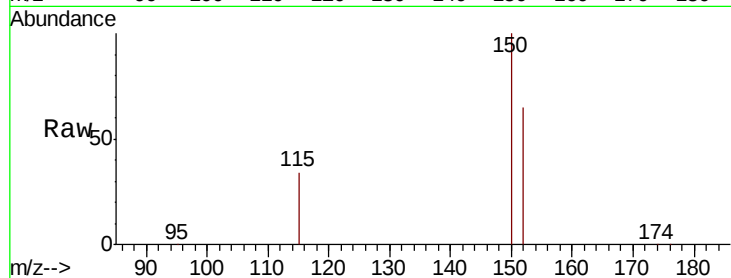

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

