


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102220\
Data File : VN064251.D
Acq On : 22 Oct 2020 14:06
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102120W.M
Title : SW846 8260
Last Update : Wed Oct 21 12:48:40 2020

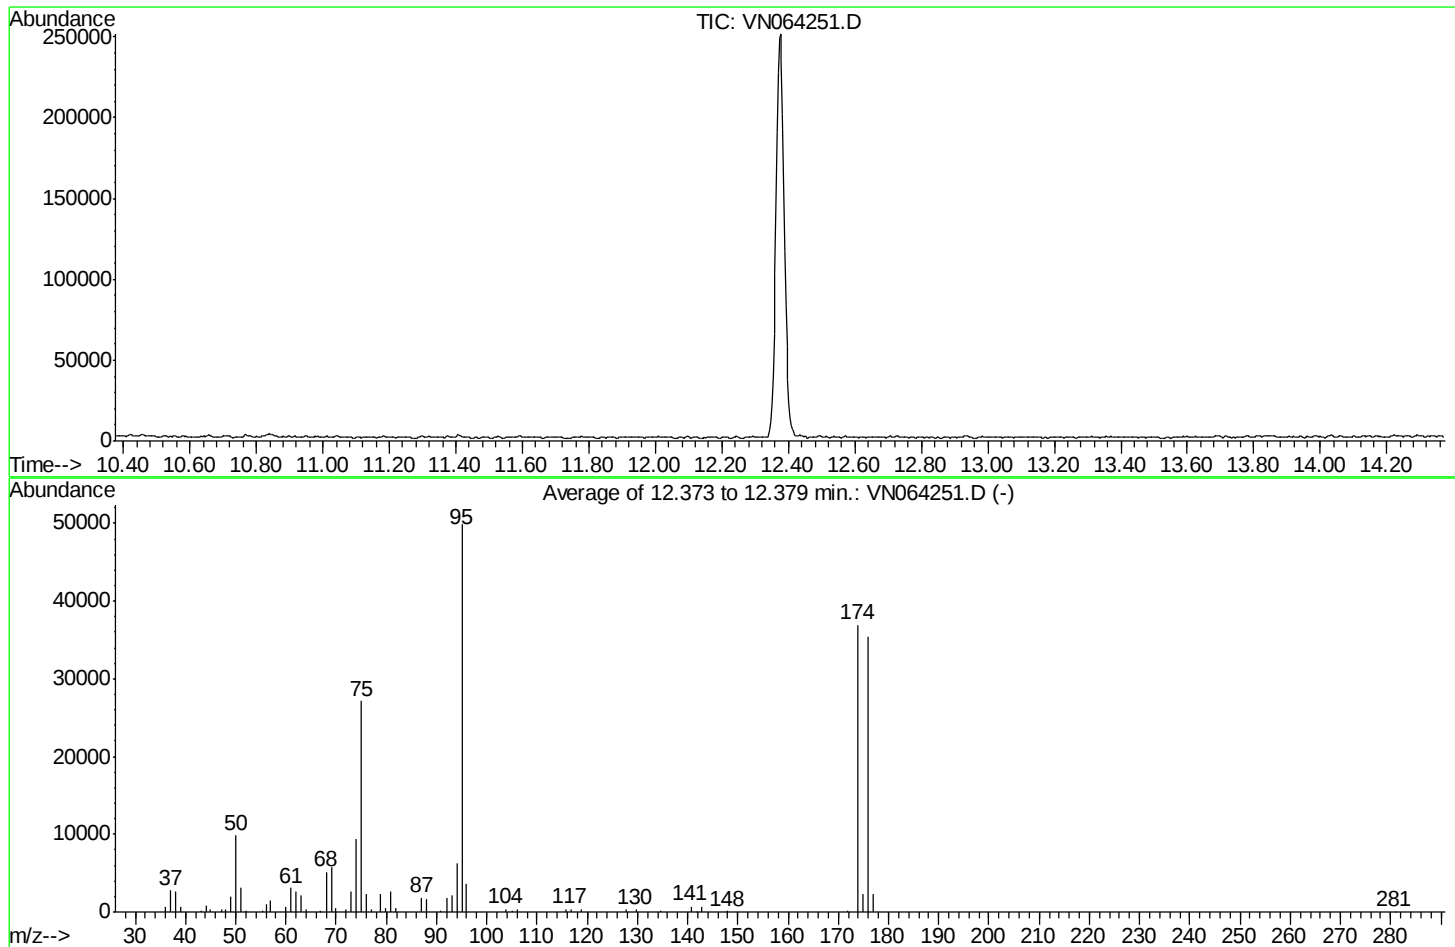

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	9859	PASS
75	95	30	60	54.5	27176	PASS
95	95	100	100	100.0	49885	PASS
96	95	5	9	7.1	3564	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.1	36970	PASS
175	174	5	9	6.3	2346	PASS
176	174	95	101	95.6	35338	PASS
177	176	5	9	6.5	2281	PASS