


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102221\
 Data File : VN069125.D
 Acq On : 22 Oct 2021 9:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N102221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Oct 22 13:15:19 2021

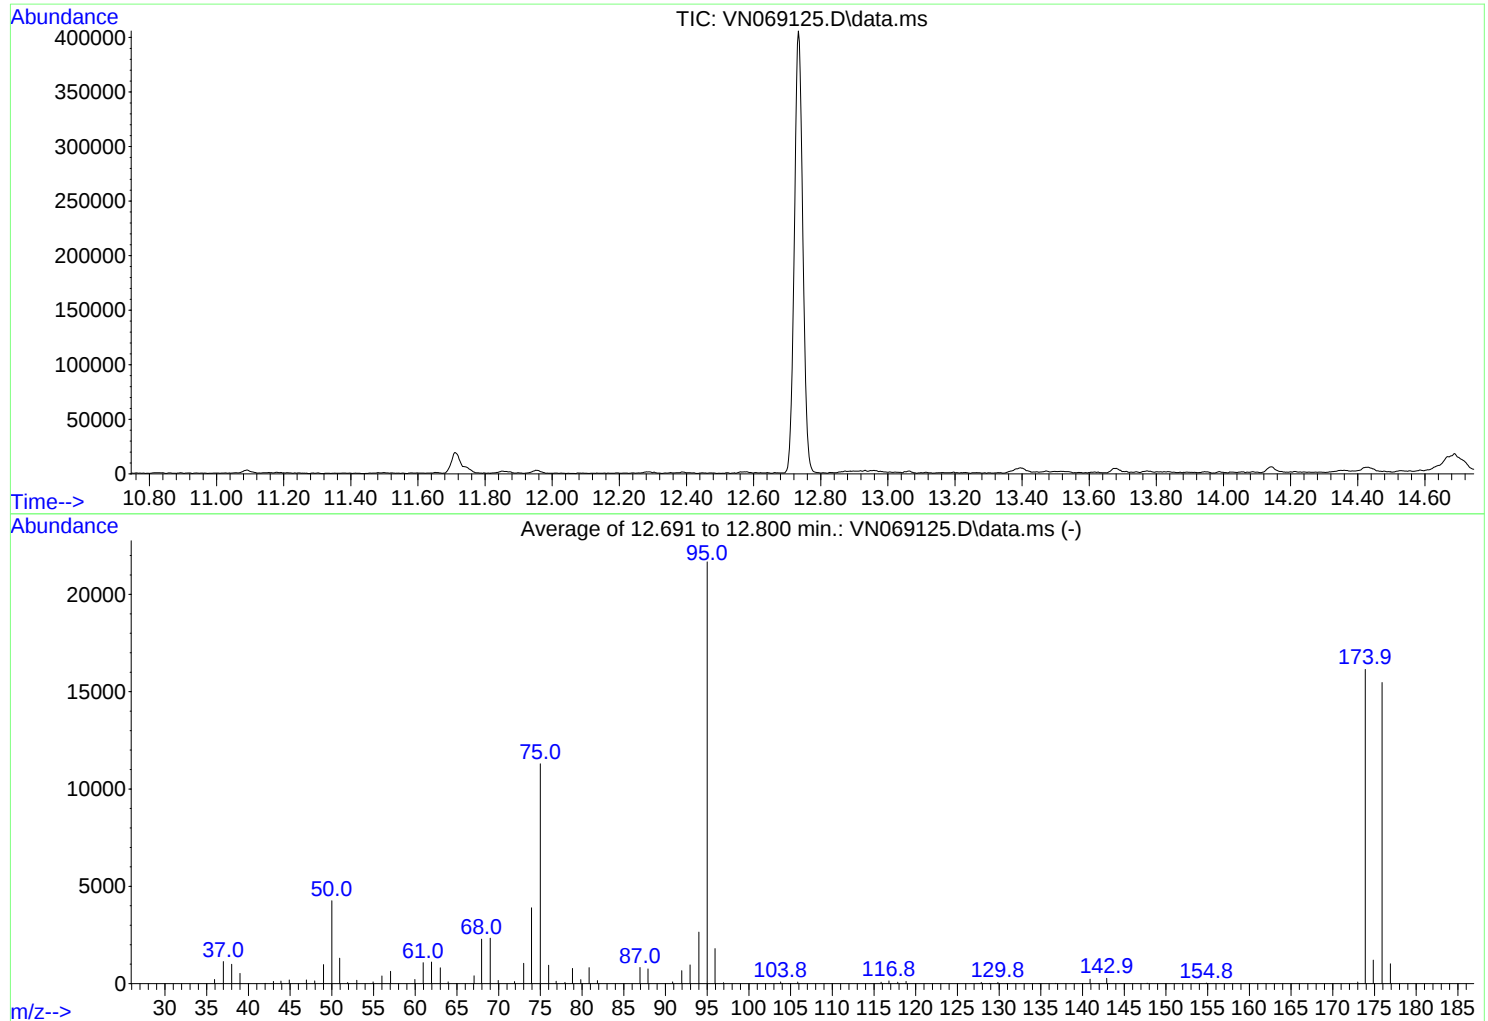

AutoFind: Averaged scan 3990 to 4031; Bkg corrected with scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	4256	PASS
75	95	30	60	52.1	11295	PASS
95	95	100	100	100.0	21671	PASS
96	95	5	9	8.3	1801	PASS
173	174	0.00	2	0.5	83	PASS
174	95	50	100	74.5	16147	PASS
175	174	5	9	7.5	1205	PASS
176	174	95	101	95.8	15469	PASS
177	176	5	9	6.6	1017	PASS