

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102224\
 Data File : VN084451.D
 Acq On : 22 Oct 2024 13:14
 Operator : JC\MD
 Sample : VN1022MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1022MBL01

Quant Time: Oct 23 01:26:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 01 07:11:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	164625	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	278457	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	235344	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	89956	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	113874	46.653	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	93.300%
35) Dibromofluoromethane	8.171	113	91902	50.062	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.120%
50) Toluene-d8	10.565	98	328010	48.566	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.140%
62) 4-Bromofluorobenzene	12.847	95	102137	41.510	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	83.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102224\
Data File : VN084451.D
Acq On : 22 Oct 2024 13:14
Operator : JC\MD
Sample : VN1022MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1022MBL01

Quant Time: Oct 23 01:26:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 01 07:11:01 2024
Response via : Initial Calibration




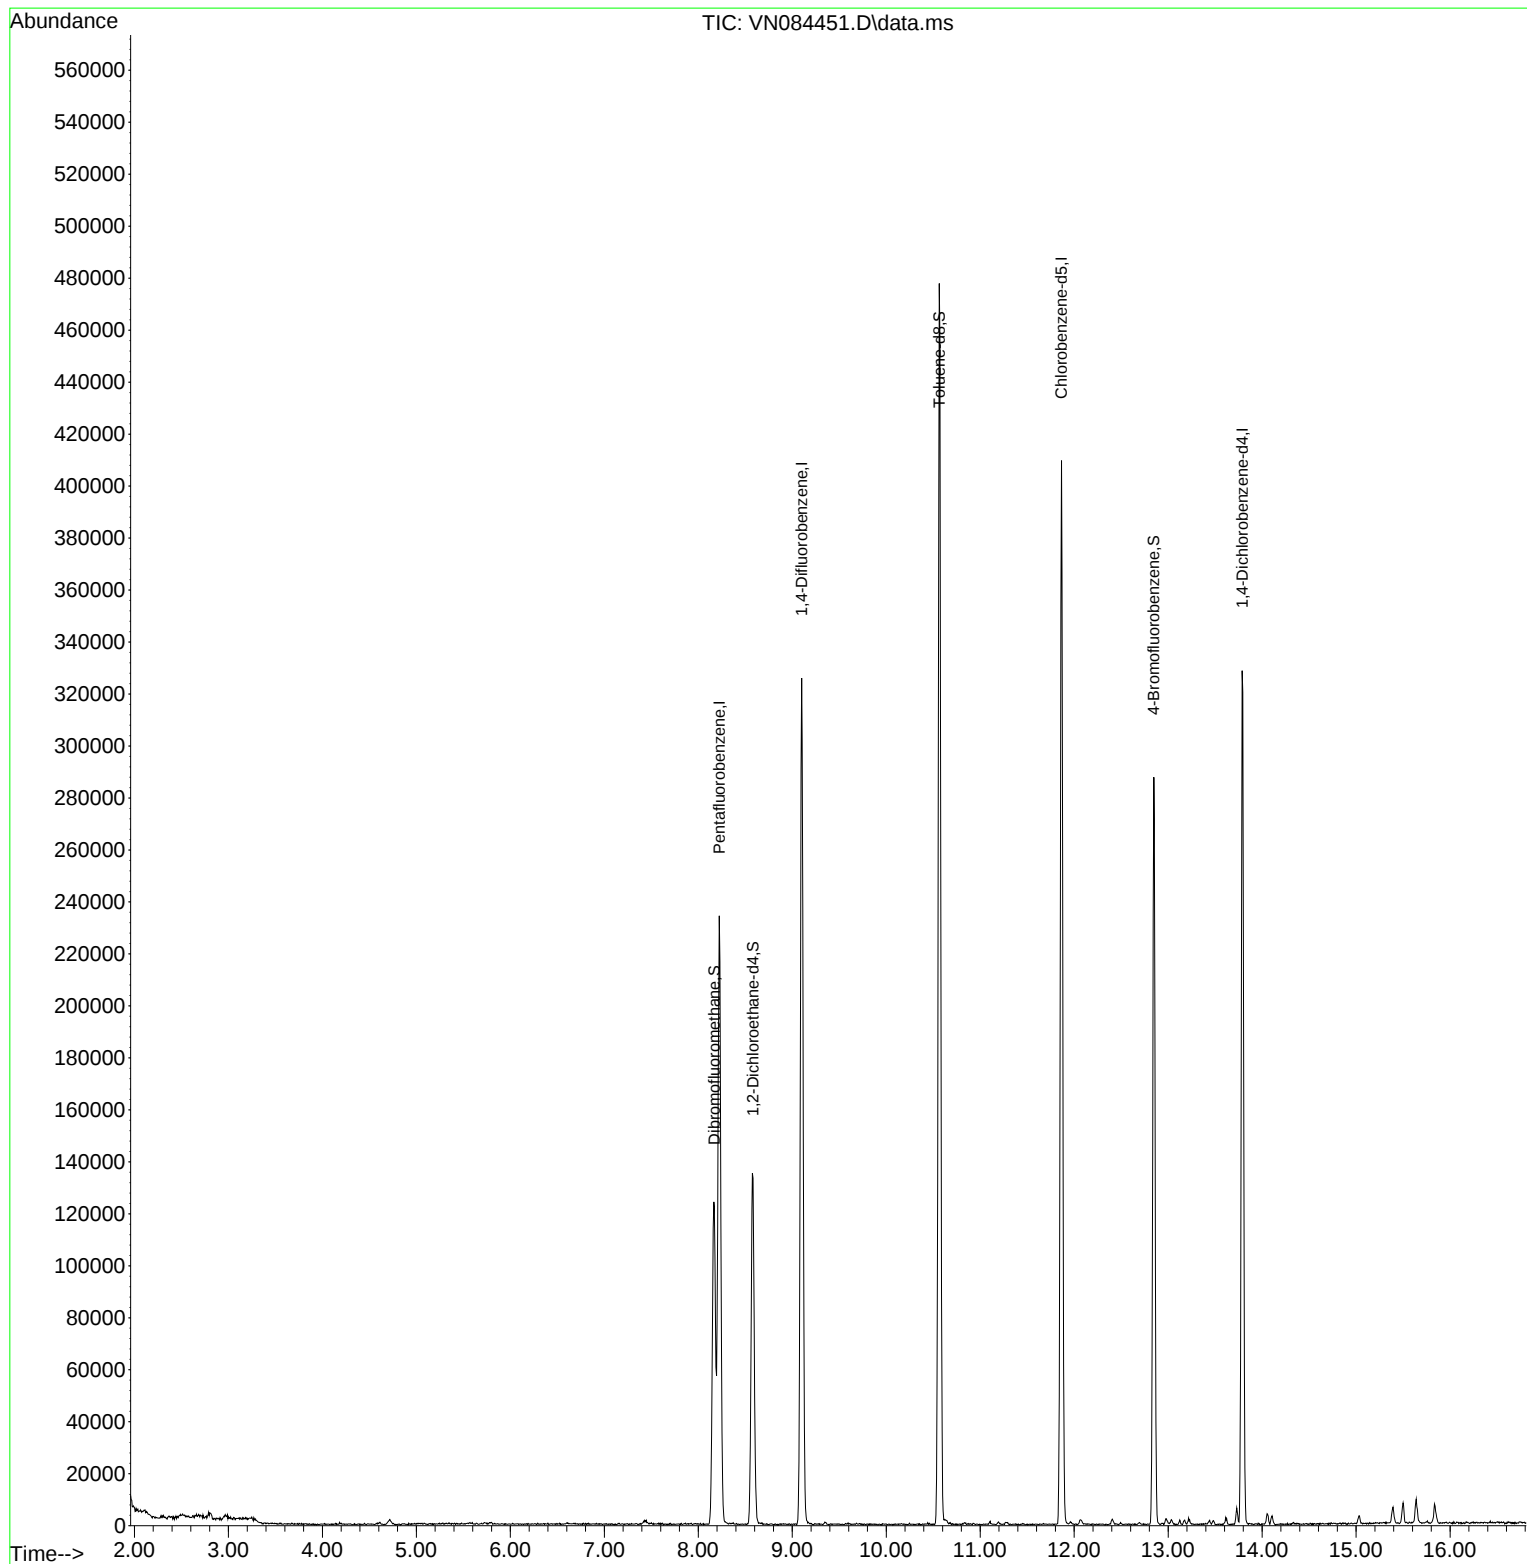


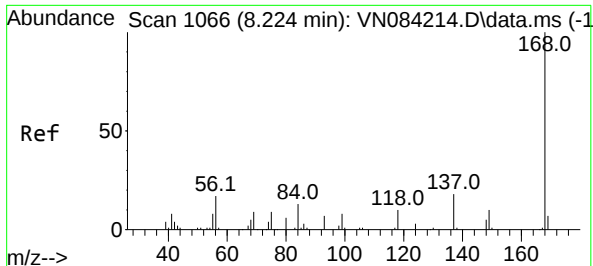

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN084451.D
Acq: 22 Oct 2024 13:14




Instrument :
MSVOA_N
ClientSampleId :
VN1022MBL01


Tgt Ion:168 Resp: 164625
Ion Ratio Lower Upper
168 100
99 62.4 54.2 81.2

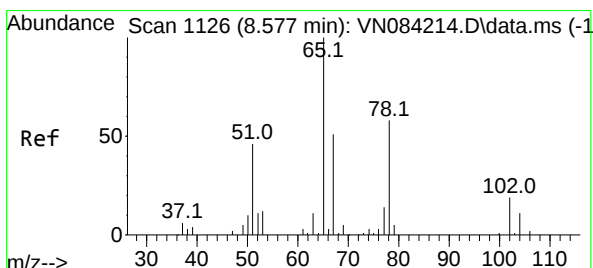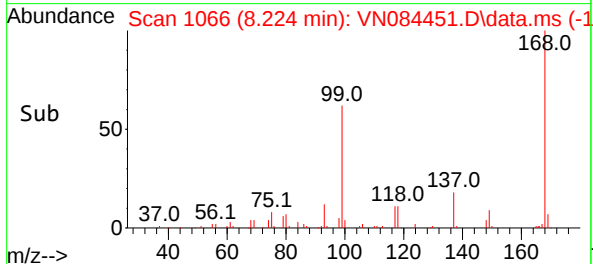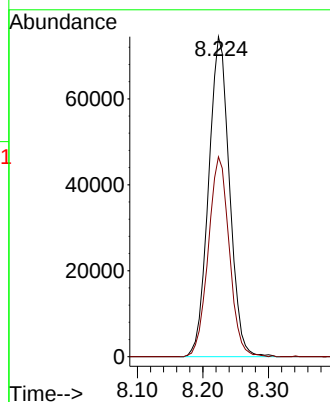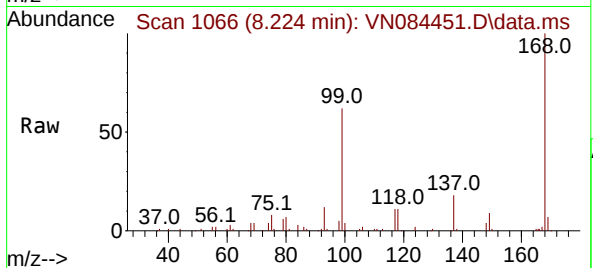

#33
1,2-Dichloroethane-d4
Concen: 46.653 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN084451.D
Acq: 22 Oct 2024 13:14

Tgt Ion: 65 Resp: 113874
Ion Ratio Lower Upper
65 100
67 53.2 0.0 102.0

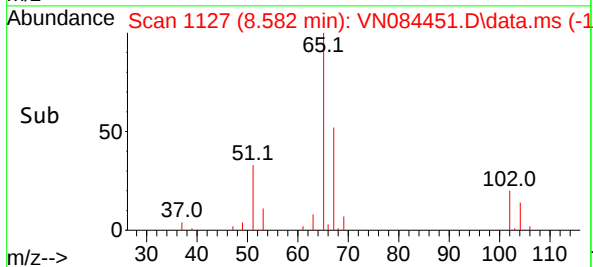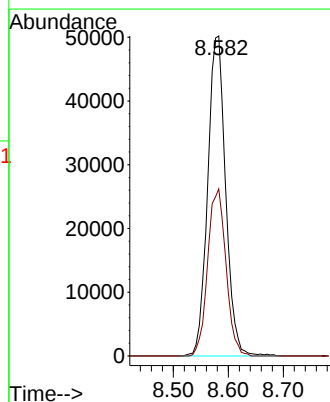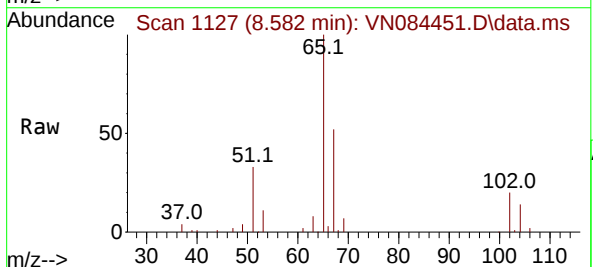

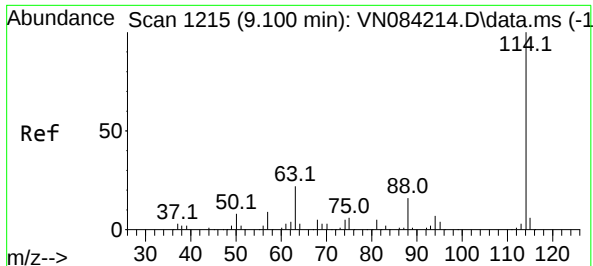

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN084451.D

Acq: 22 Oct 2024 13:14

Instrument :

MSVOA_N

ClientSampleId :

VN1022MBL01





Tgt Ion:114 Resp: 278457

Ion Ratio Lower Upper

114 100

63 21.2 0.0 43.8

88 17.4 0.0 31.6

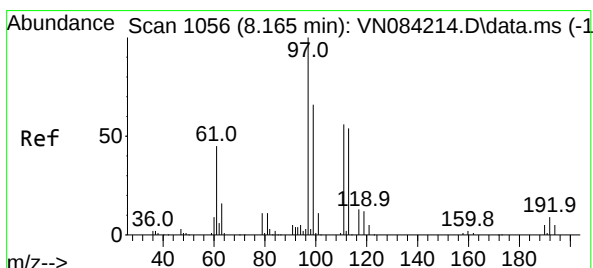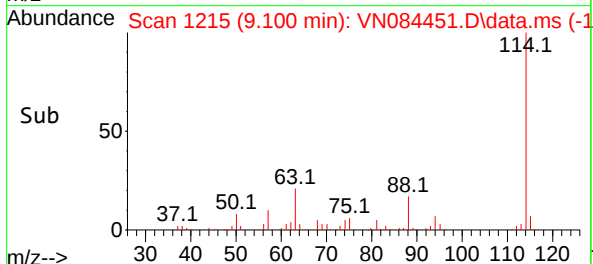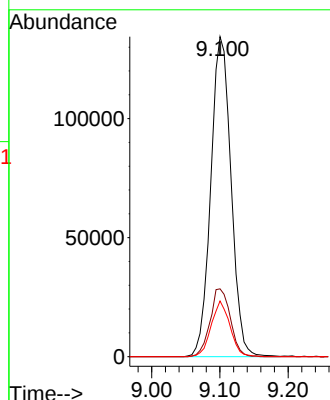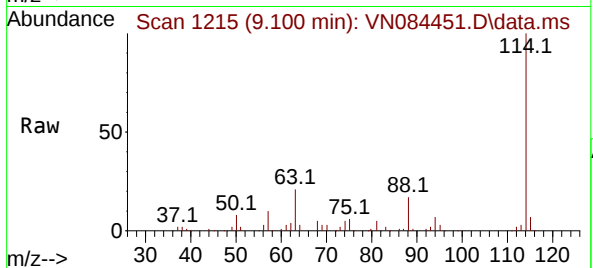

#35

Dibromofluoromethane

Concen: 50.062 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN084451.D

Acq: 22 Oct 2024 13:14




Tgt Ion:113 Resp: 91902


Ion Ratio Lower Upper

113 100

111 102.7 83.3 124.9

192 18.5 13.5 20.3


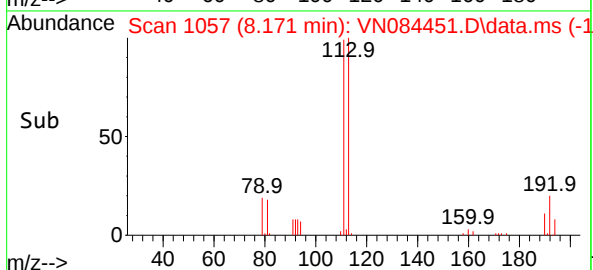
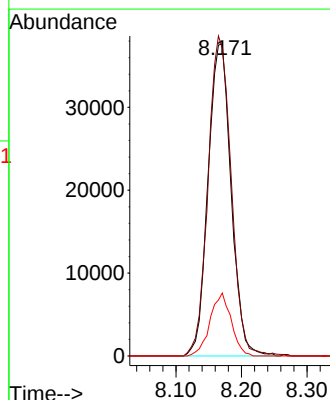
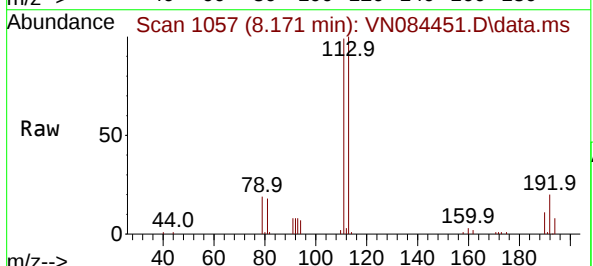


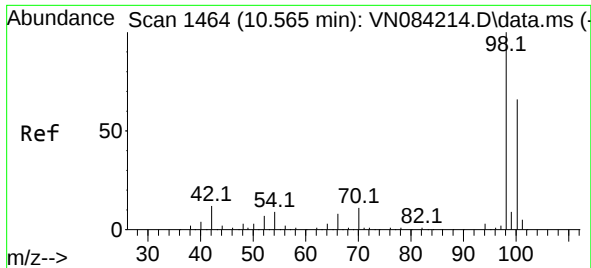

#50
Toluene-d8
Concen: 48.566 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN084451.D
Acq: 22 Oct 2024 13:14




Instrument :
MSVOA_N
ClientSampleId :
VN1022MBL01


Tgt Ion: 98 Resp: 328010
Ion Ratio Lower Upper
98 100
100 65.4 52.7 79.1

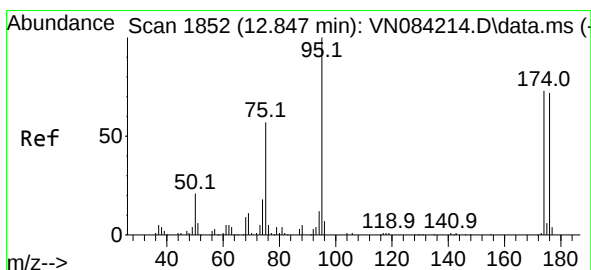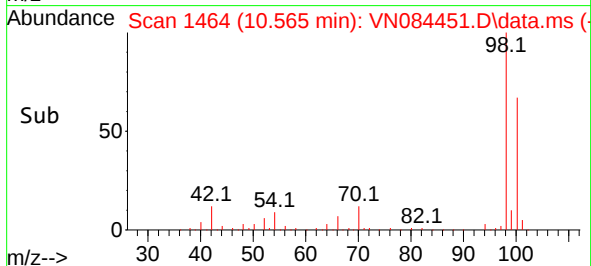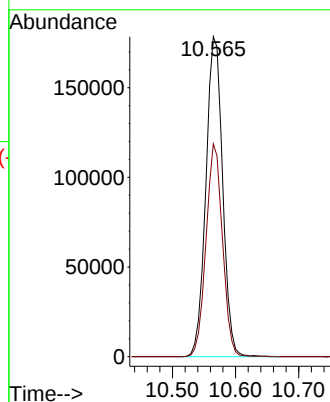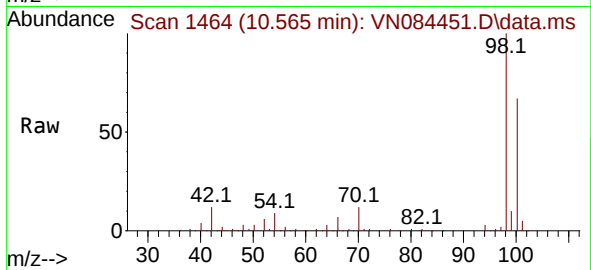

#62
4-Bromofluorobenzene
Concen: 41.510 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN084451.D
Acq: 22 Oct 2024 13:14

Tgt Ion: 95 Resp: 102137
Ion Ratio Lower Upper
95 100
174 75.6 0.0 145.2
176 70.4 0.0 140.0

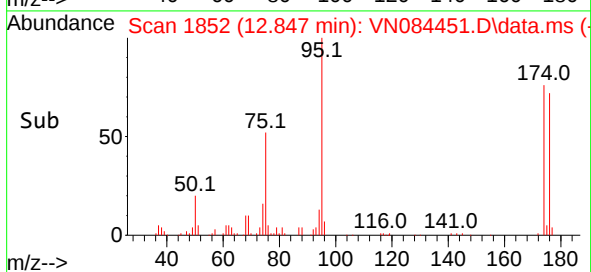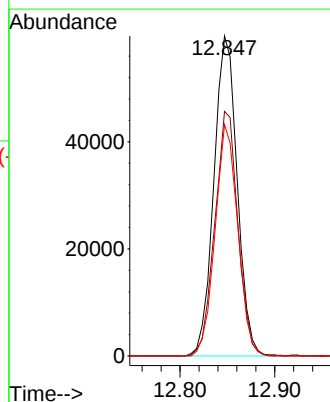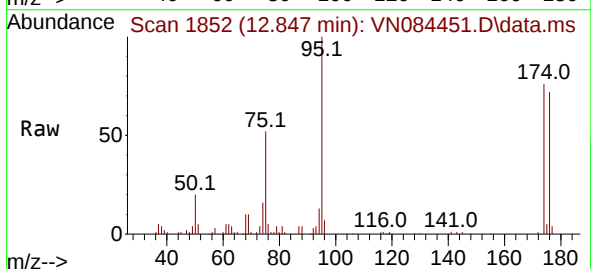

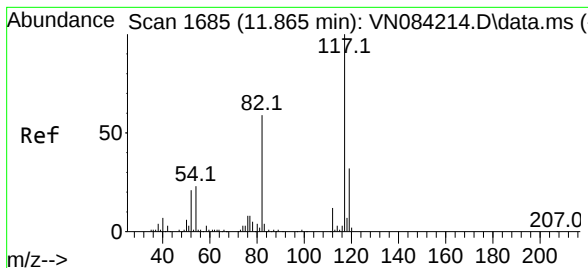

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN084451.D

Acq: 22 Oct 2024 13:14

Instrument :

MSVOA_N

ClientSampleId :

VN1022MBL01





Tgt Ion:117 Resp: 235344

Ion Ratio Lower Upper

117 100

82 56.9 47.2 70.8

119 31.3 25.4 38.0

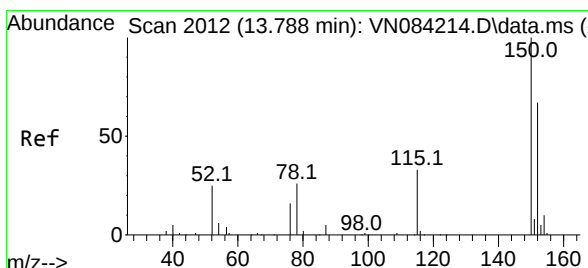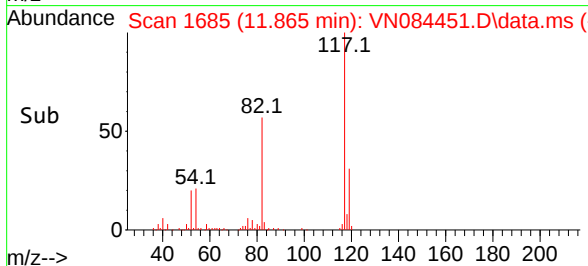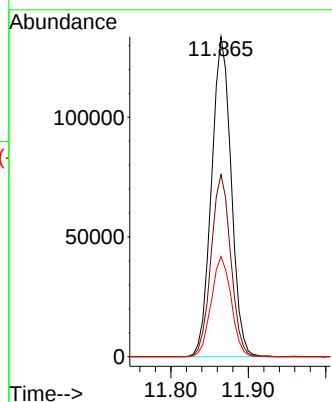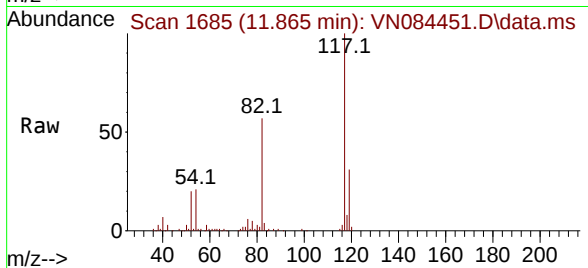

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 2012

Delta R.T. -0.000 min

Lab File: VN084451.D

Acq: 22 Oct 2024 13:14

Tgt Ion:152 Resp: 89956

Ion Ratio Lower Upper

152 100

115 62.8 31.3 93.9

150 158.3 0.0 349.8

