
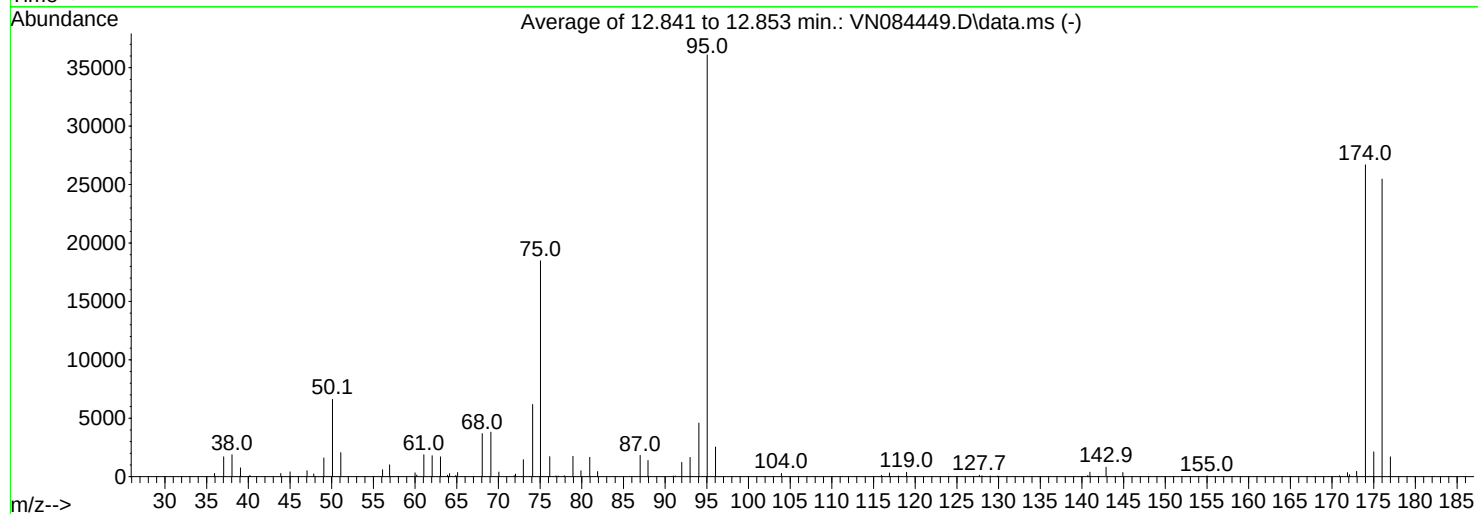


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102224\
Data File : VN084449.D
Acq On : 22 Oct 2024 08:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

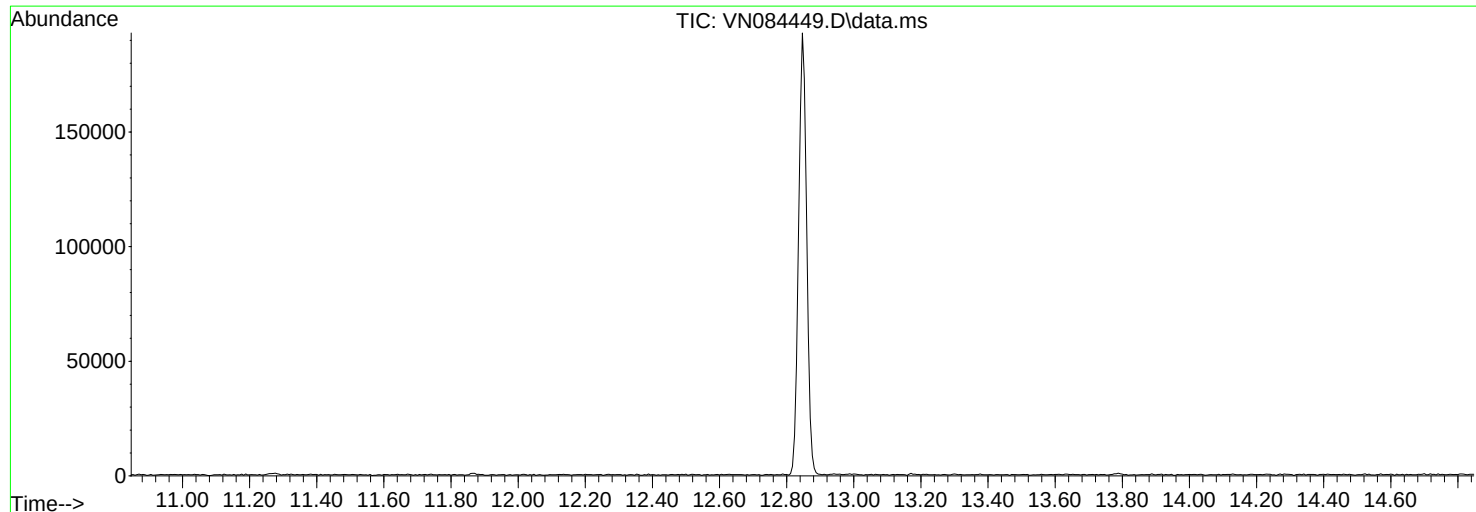

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	6621	PASS
75	95	30	60	51.2	18475	PASS
95	95	100	100	100.0	36101	PASS
96	95	5	9	7.0	2529	PASS
173	174	0.00	2	1.7	450	PASS
174	95	50	100	73.9	26696	PASS
175	174	5	9	7.9	2121	PASS
176	174	95	101	95.4	25467	PASS
177	176	5	9	6.7	1699	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	269	51.10	2048	65.10	358	77.20	61
37.05	1703	56.10	596	68.05	3681	77.90	81
38.05	1879	56.95	1016	69.10	3809	78.95	174
39.05	753	60.00	334	70.05	396	79.90	50
40.20	114	60.20	138	71.90	89	80.95	1659
43.90	270	61.05	1873	72.05	223	81.90	436
45.00	419	62.05	1793	73.00	1459	87.00	1816
47.05	510	63.05	1703	74.10	6180	87.95	1391
47.85	233	63.90	118	75.05	18475	91.00	54
49.05	1602	64.15	262	76.15	1707	91.20	56
50.10	6621	64.90	116	76.90	73	92.00	1224

Average of 12.841 to 12.853 min.: VN084449.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	1646	129.00	52	174.00	26696		
94.05	4594	129.90	60	175.00	2121		
95.05	36101	140.70	114	176.00	25467		
96.05	2529	140.95	391	177.00	1699		
103.95	278	142.90	812				
115.95	112	144.90	355				
116.90	314	155.00	51				
118.00	63	170.90	78				
118.95	376	171.85	349				
127.70	122	172.10	170				
128.00	74	172.95	450				

Instrument :
MSVOA_N
ClientSampleId :
BFB