




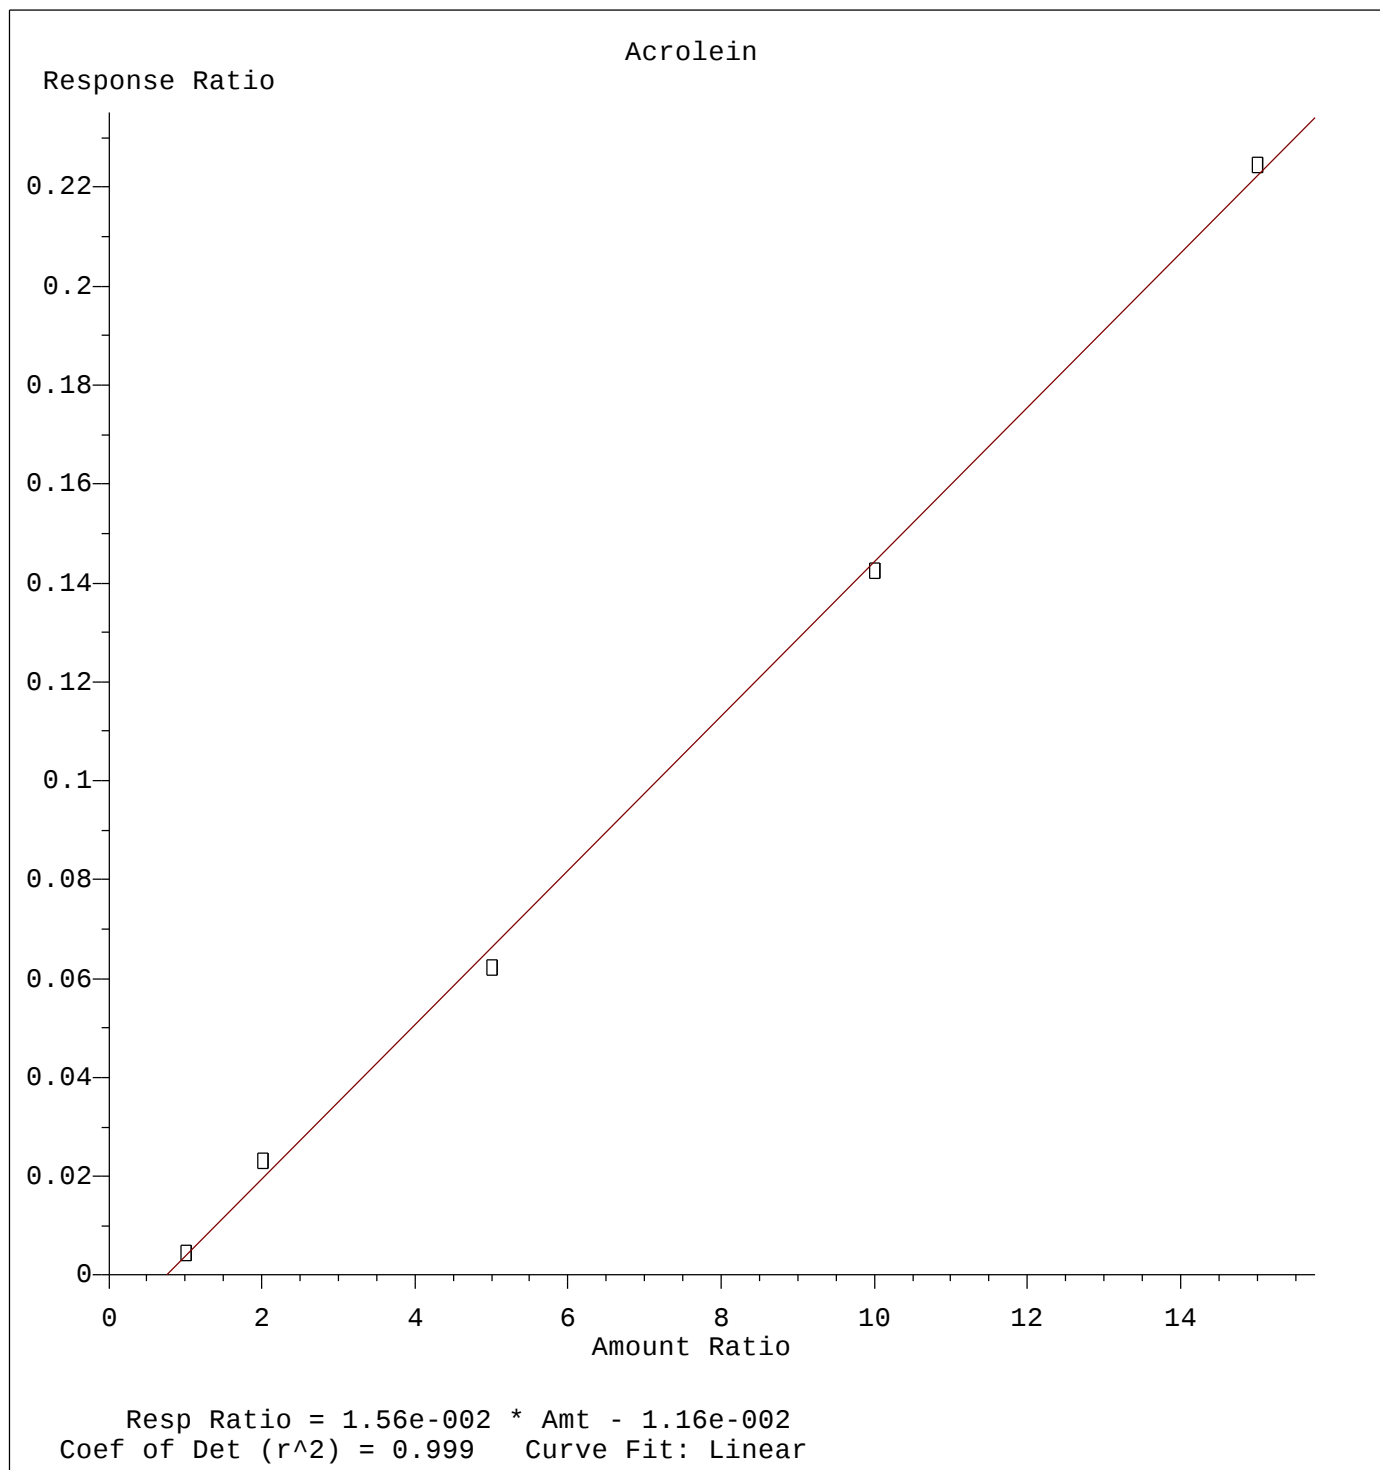


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

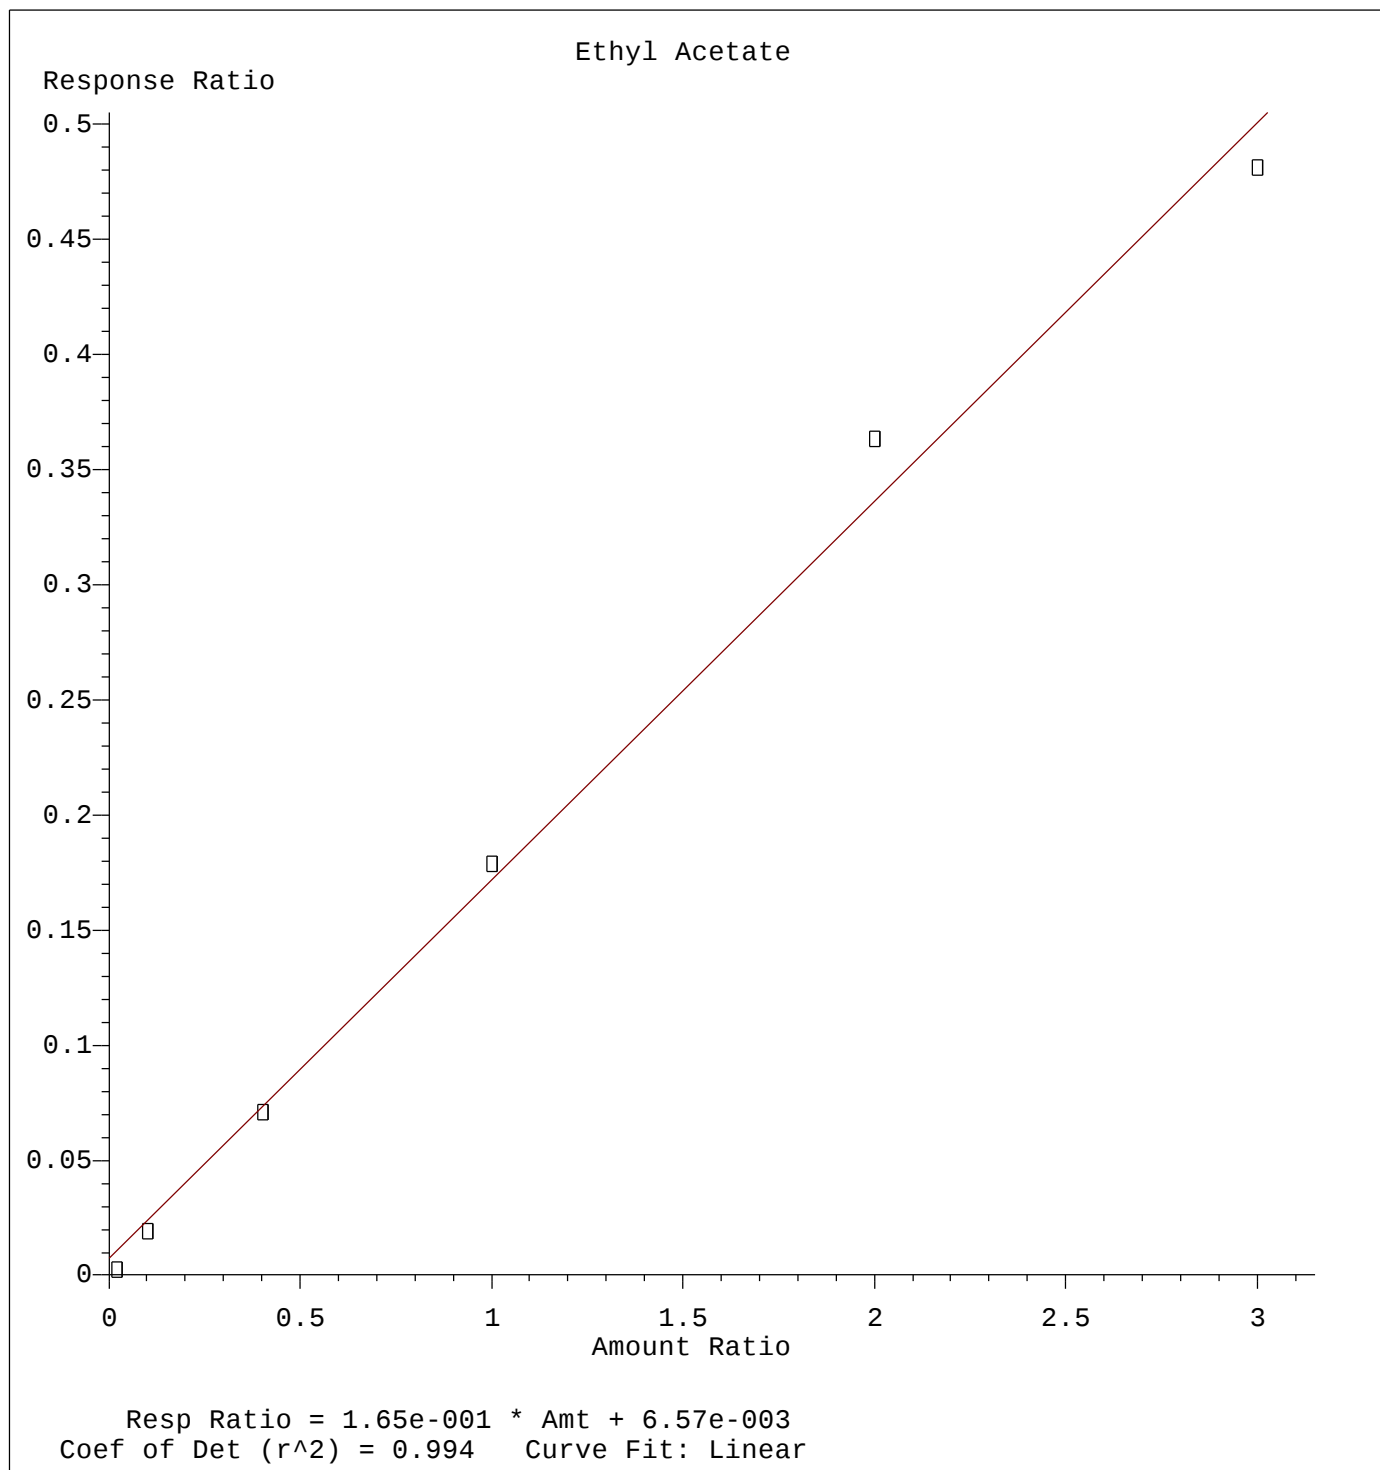

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

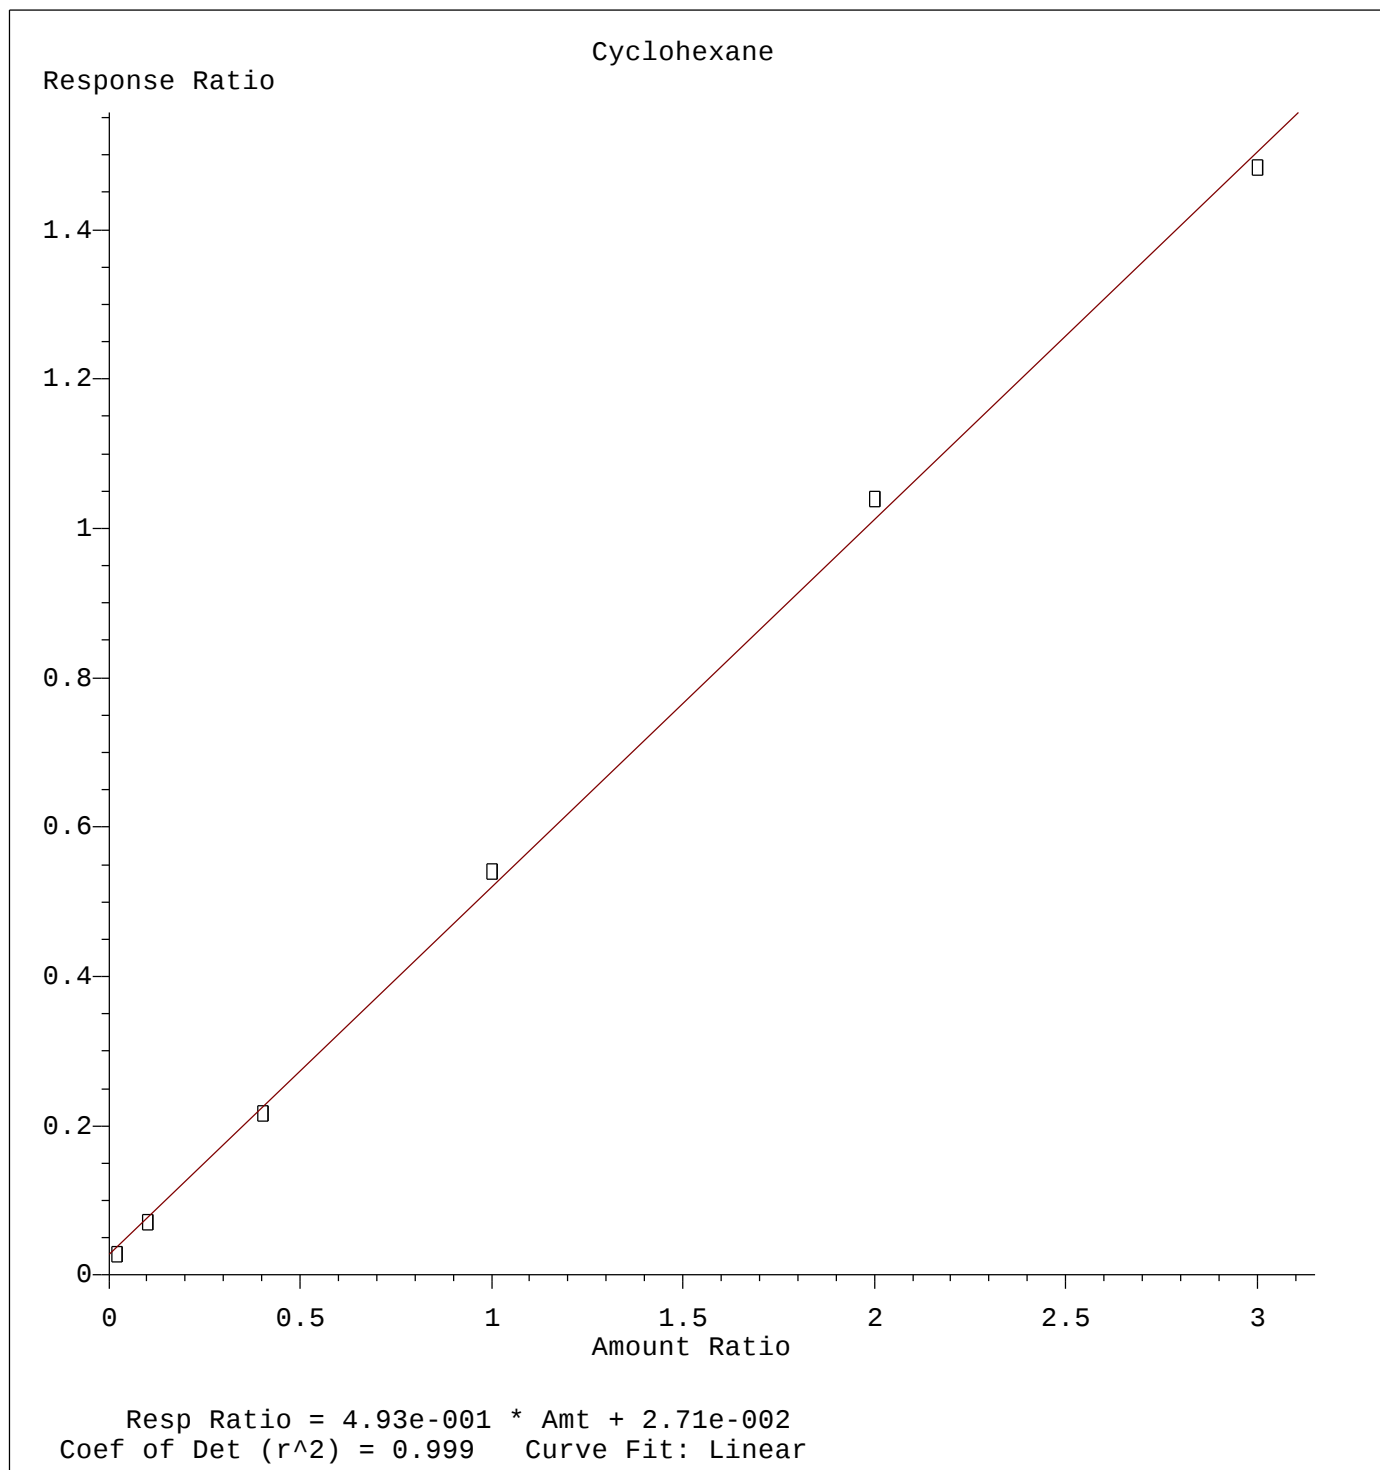


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

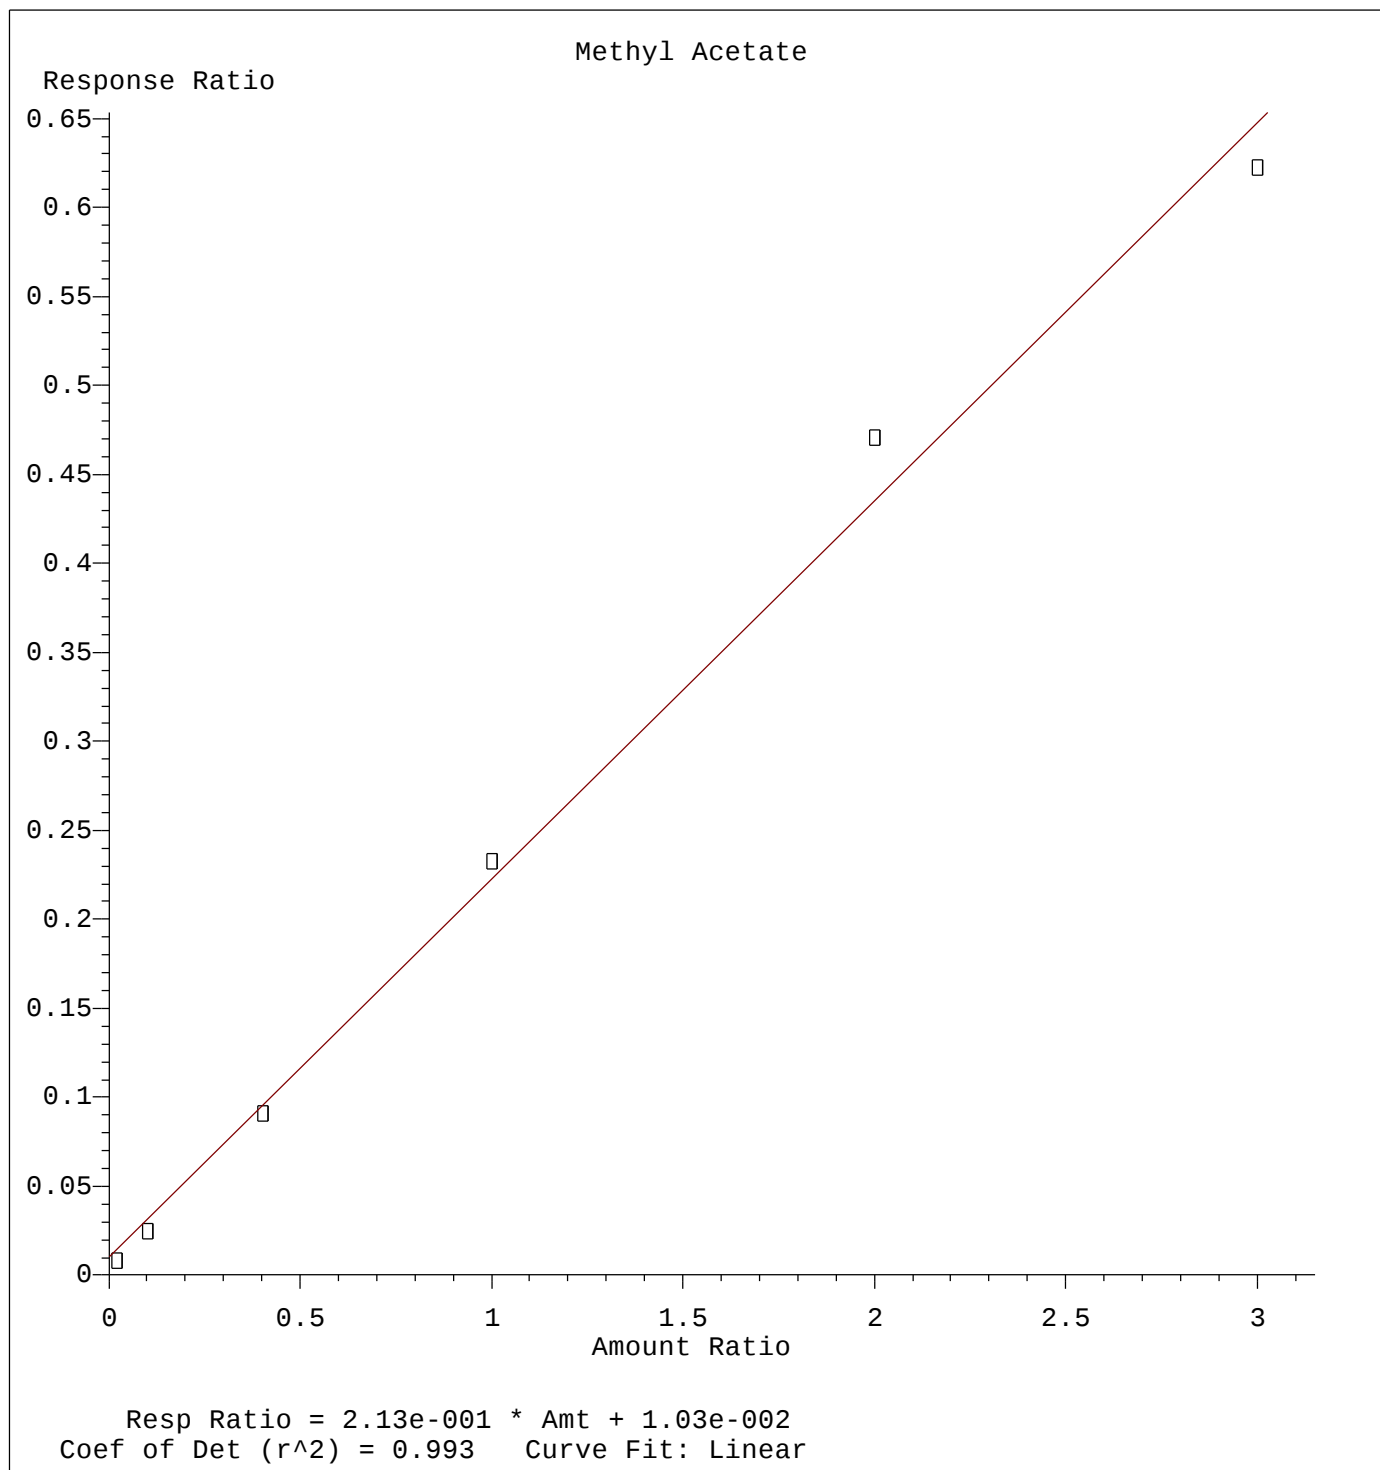


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

trans-1,4-Dichloro-2-butene

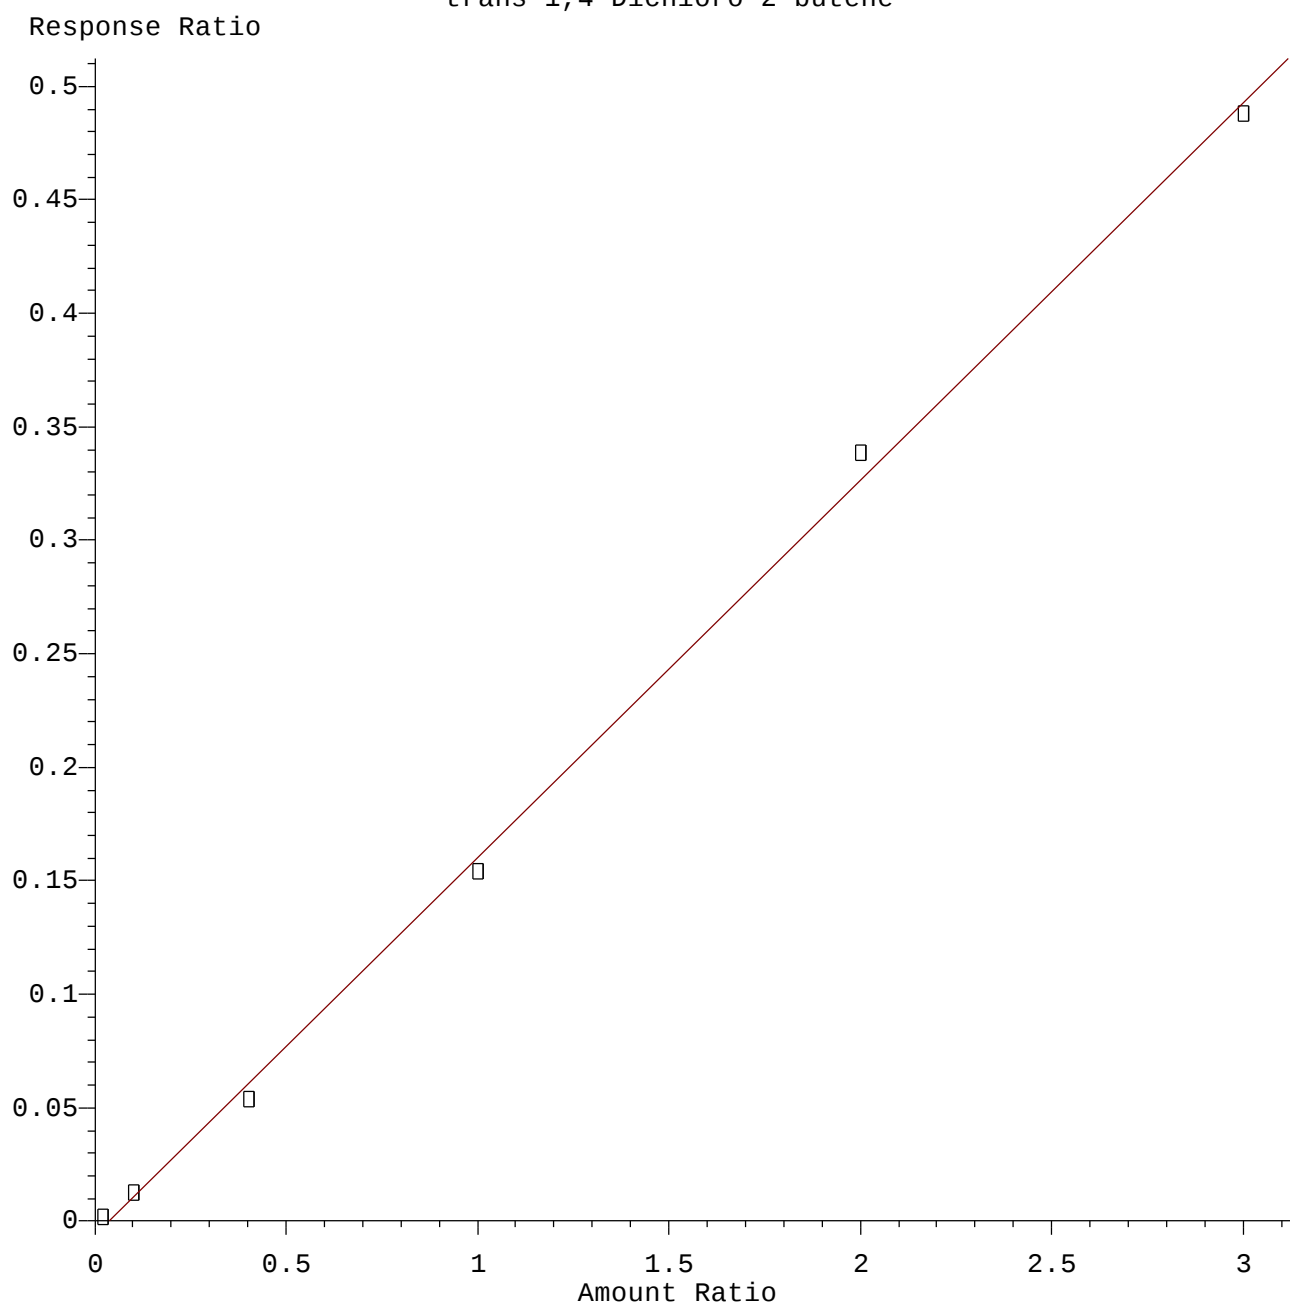


Resp Ratio = $1.66 \times 10^{-1} \times \text{Amt} - 5.99 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

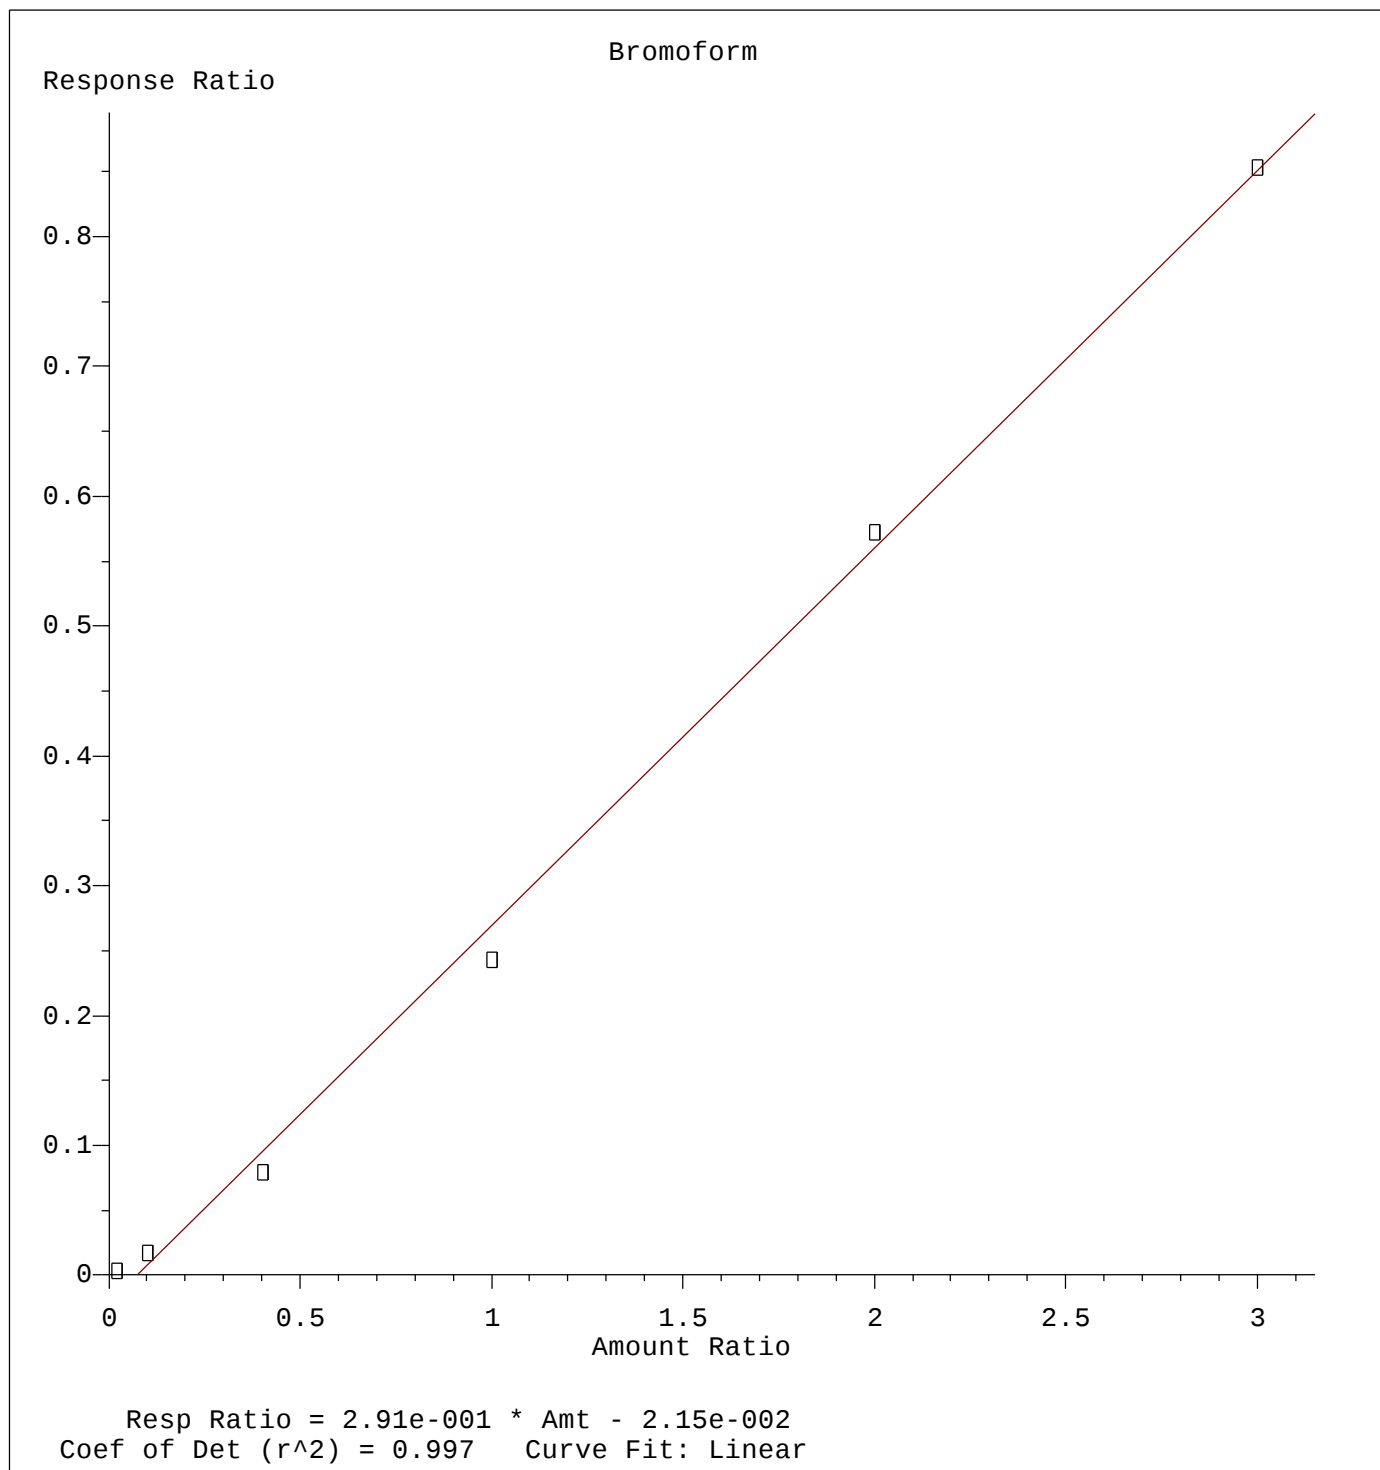


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

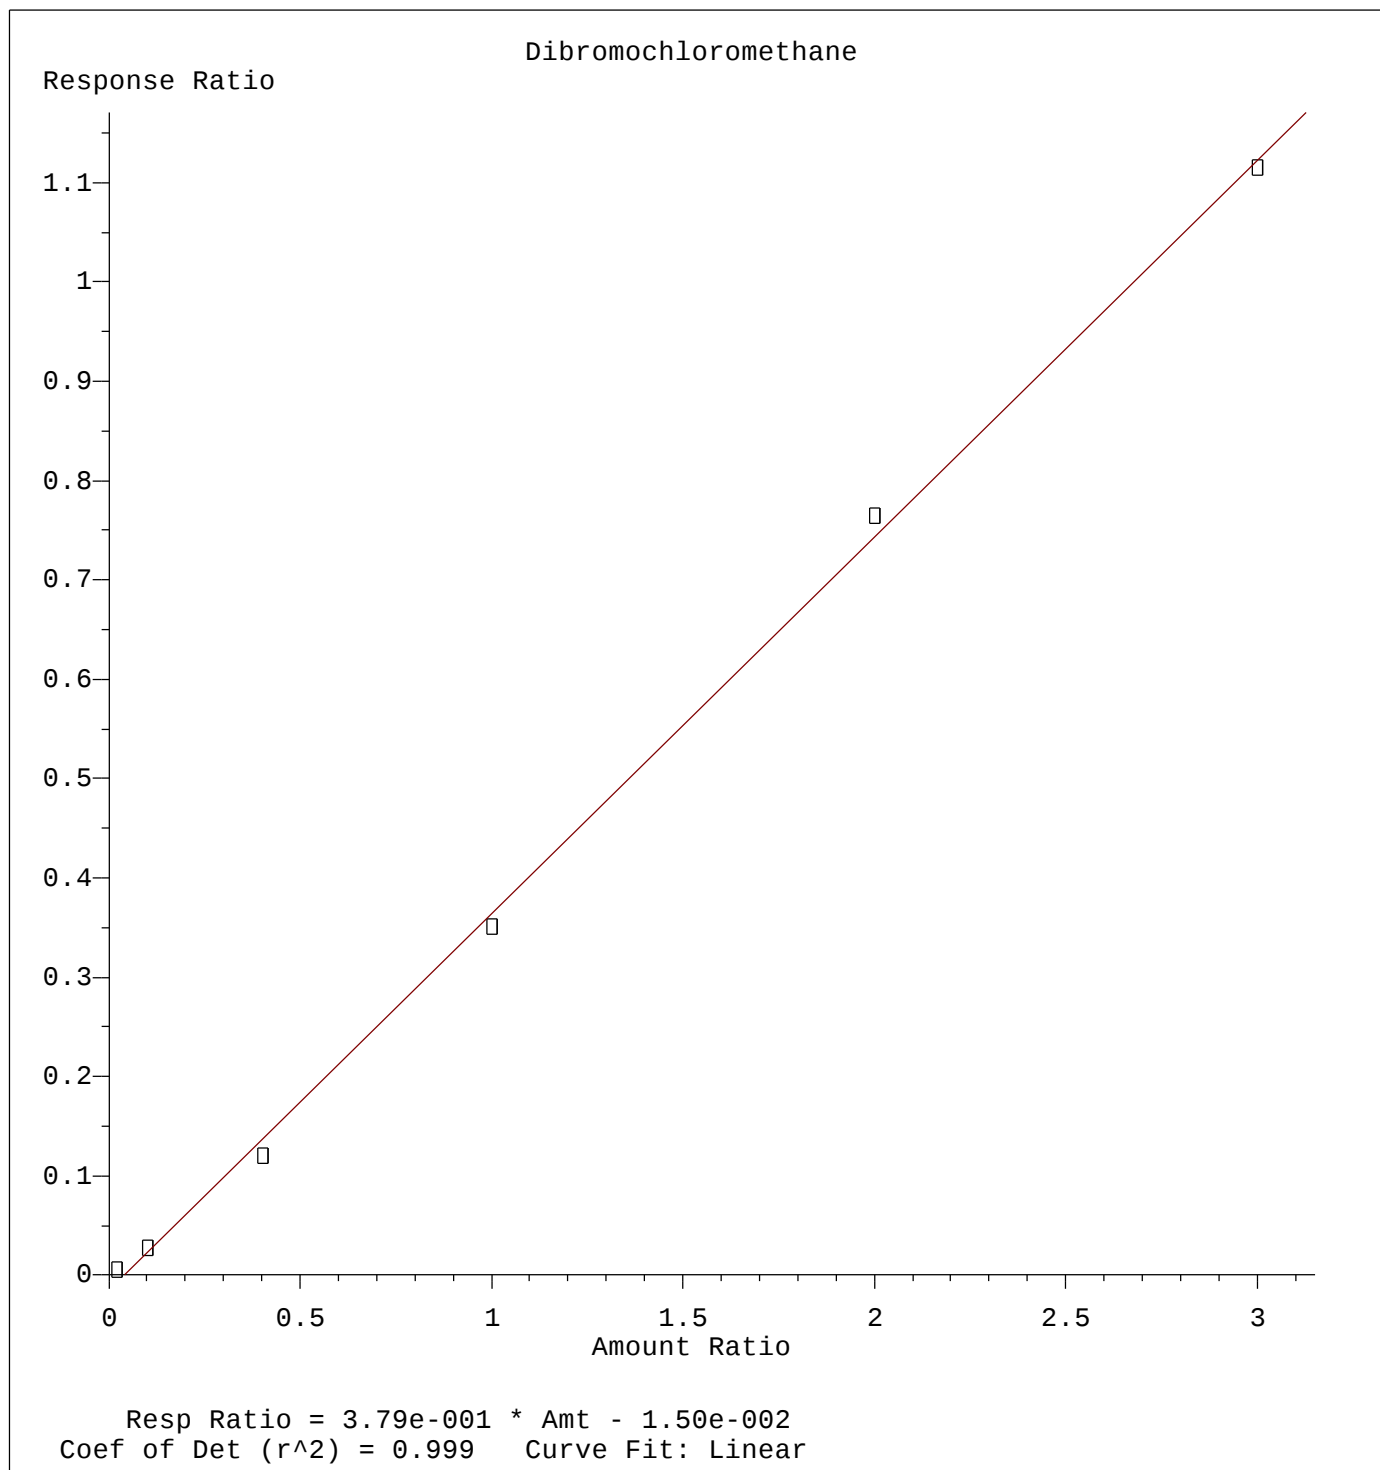

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018

t-1,3-Dichloropropene

Response Ratio

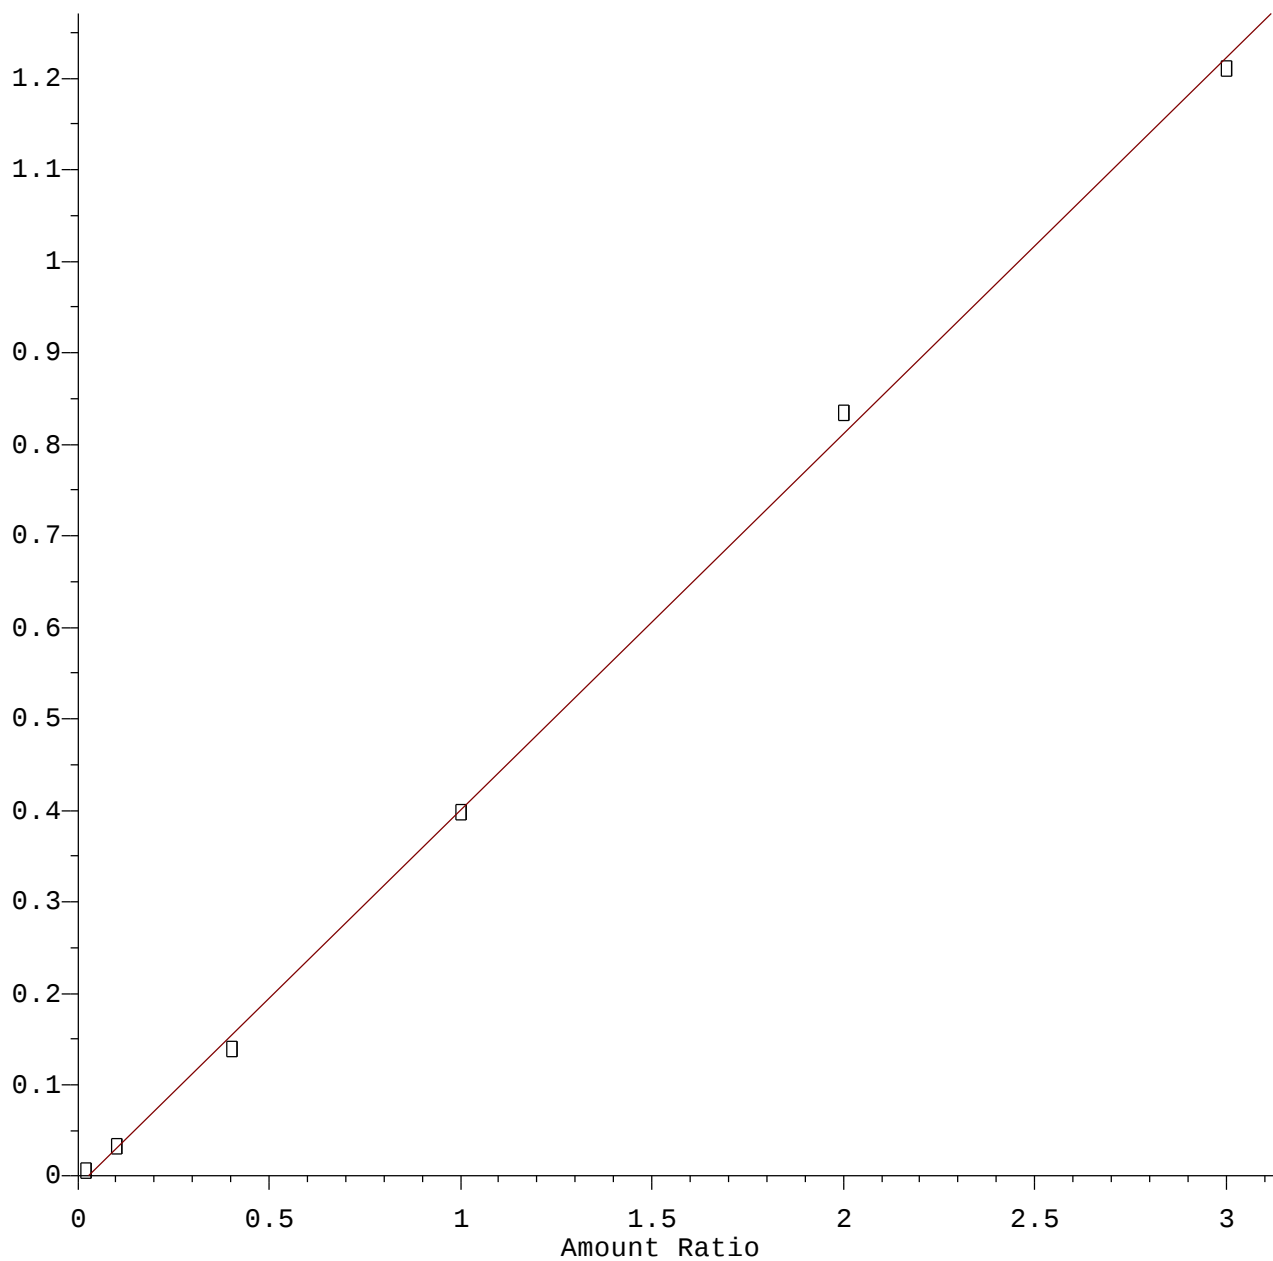

Resp Ratio = $4.11 \times 10^{-1} \times \text{Amt} - 1.02 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Calibration Table Last Updated: Wed Oct 24 10:12:55 2018