


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102318\
 Data File : VN051958.D
 Acq On : 23 Oct 2018 12:09
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
 Title : SW846 8260
 Last Update : Wed Oct 24 10:12:55 2018

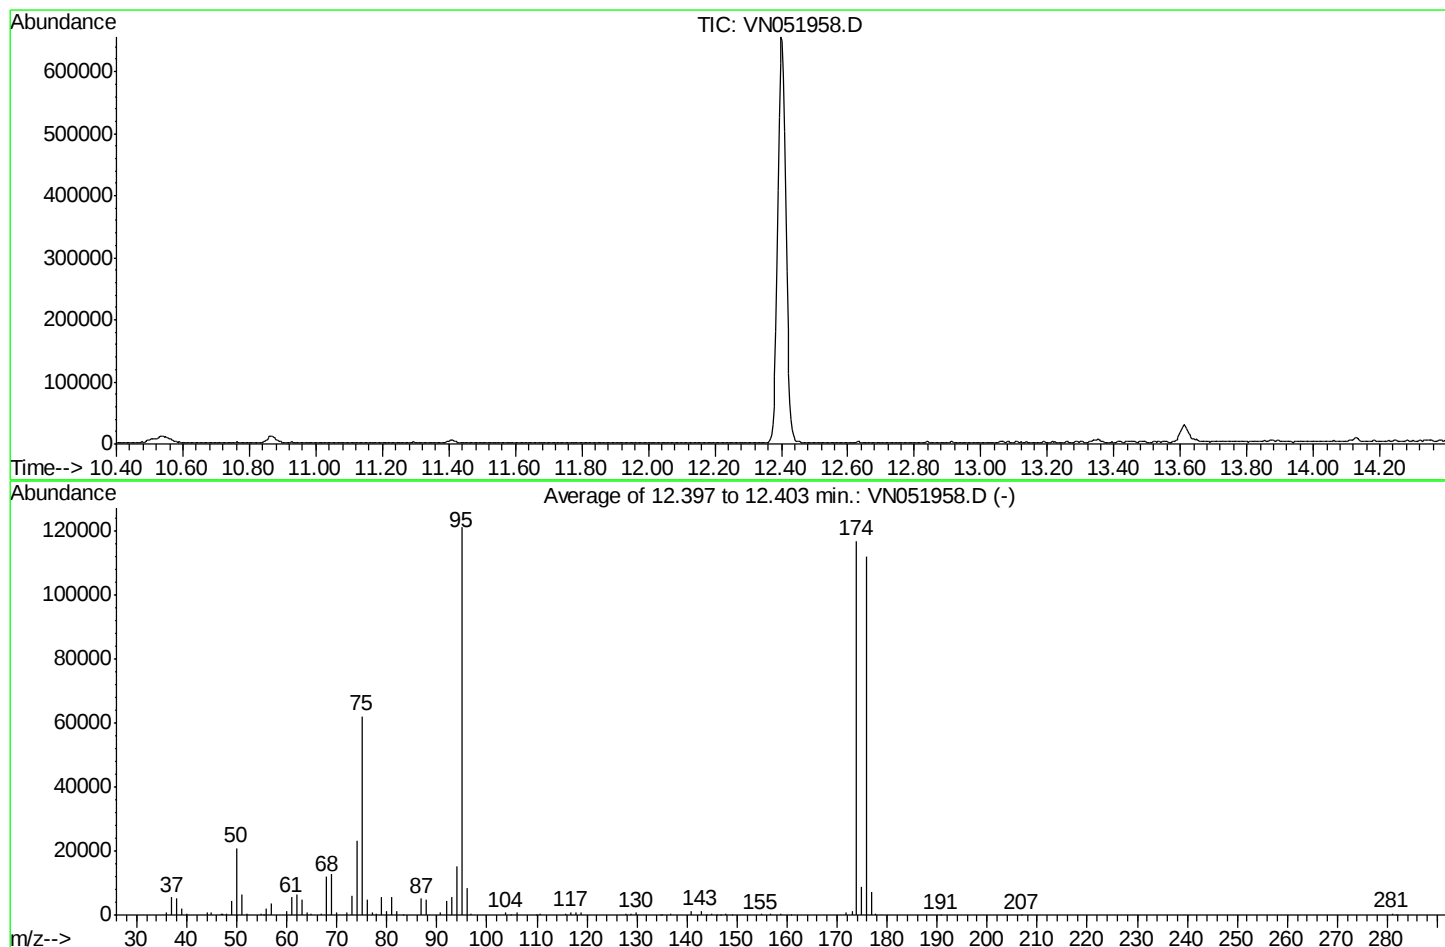

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	21013	PASS
75	95	30	60	51.2	62010	PASS
95	95	100	100	100.0	121152	PASS
96	95	5	9	7.1	8569	PASS
173	174	0.00	2	1.2	1384	PASS
174	95	50	100	96.5	116949	PASS
175	174	5	9	7.4	8678	PASS
176	174	95	101	95.7	111917	PASS
177	176	5	9	6.5	7315	PASS