


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102319\
Data File : VN058905.D
Acq On : 22 Oct 2019 13:41
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101119W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 11 04:26:47 2019

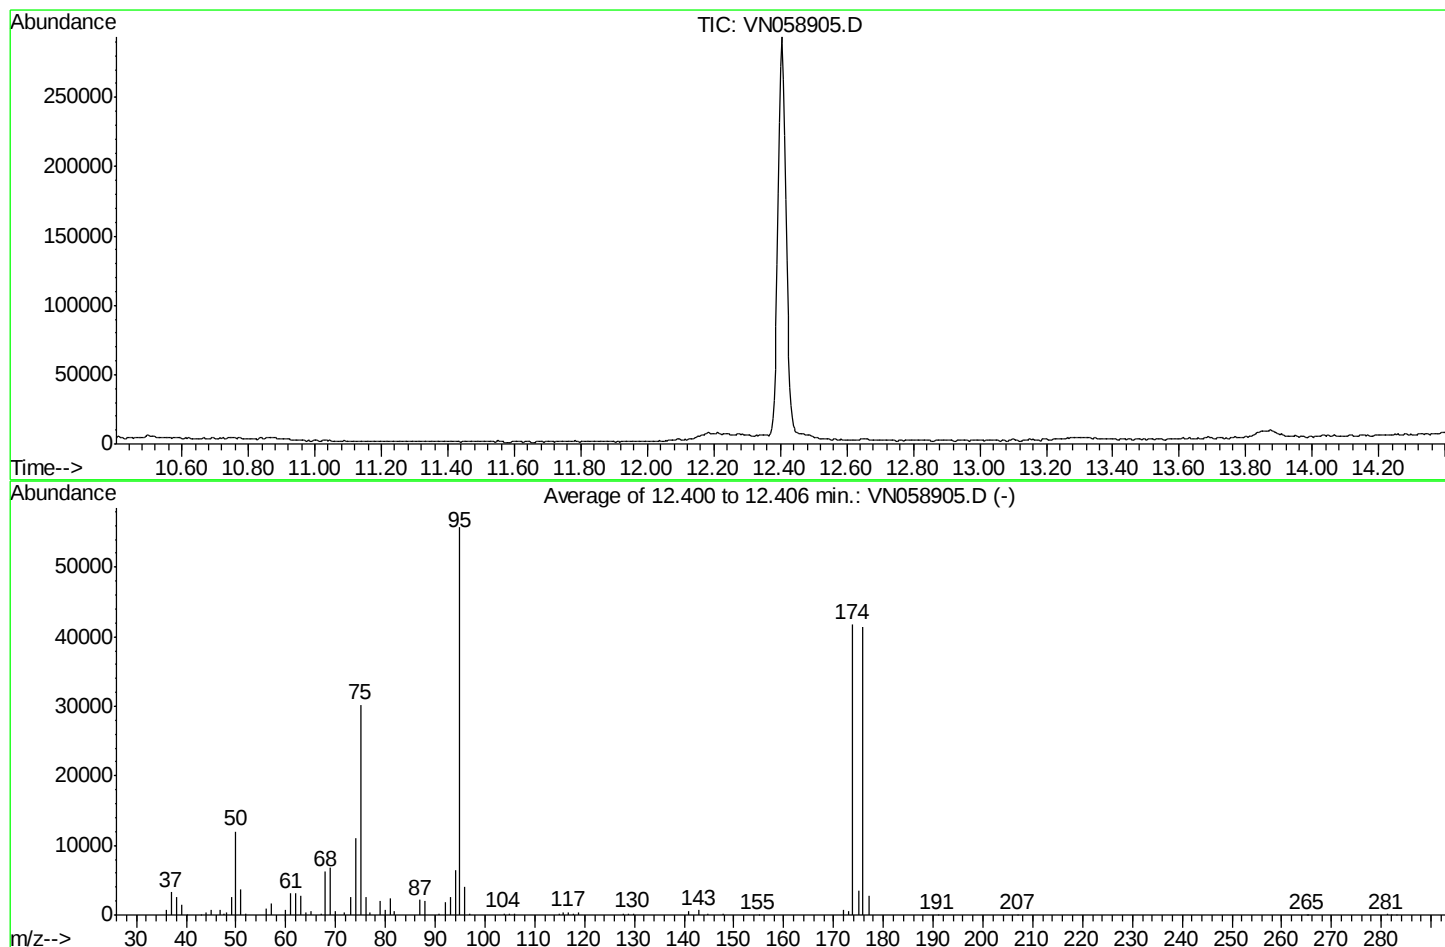

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	12007	PASS
75	95	30	60	54.2	30221	PASS
95	95	100	100	100.0	55725	PASS
96	95	5	9	7.2	4002	PASS
173	174	0.00	2	1.3	528	PASS
174	95	50	100	74.9	41717	PASS
175	174	5	9	8.4	3519	PASS
176	174	95	101	99.5	41488	PASS
177	176	5	9	6.7	2800	PASS