


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102320\
 Data File : VN064278.D
 Acq On : 23 Oct 2020 9:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N102320W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Oct 26 01:30:11 2020

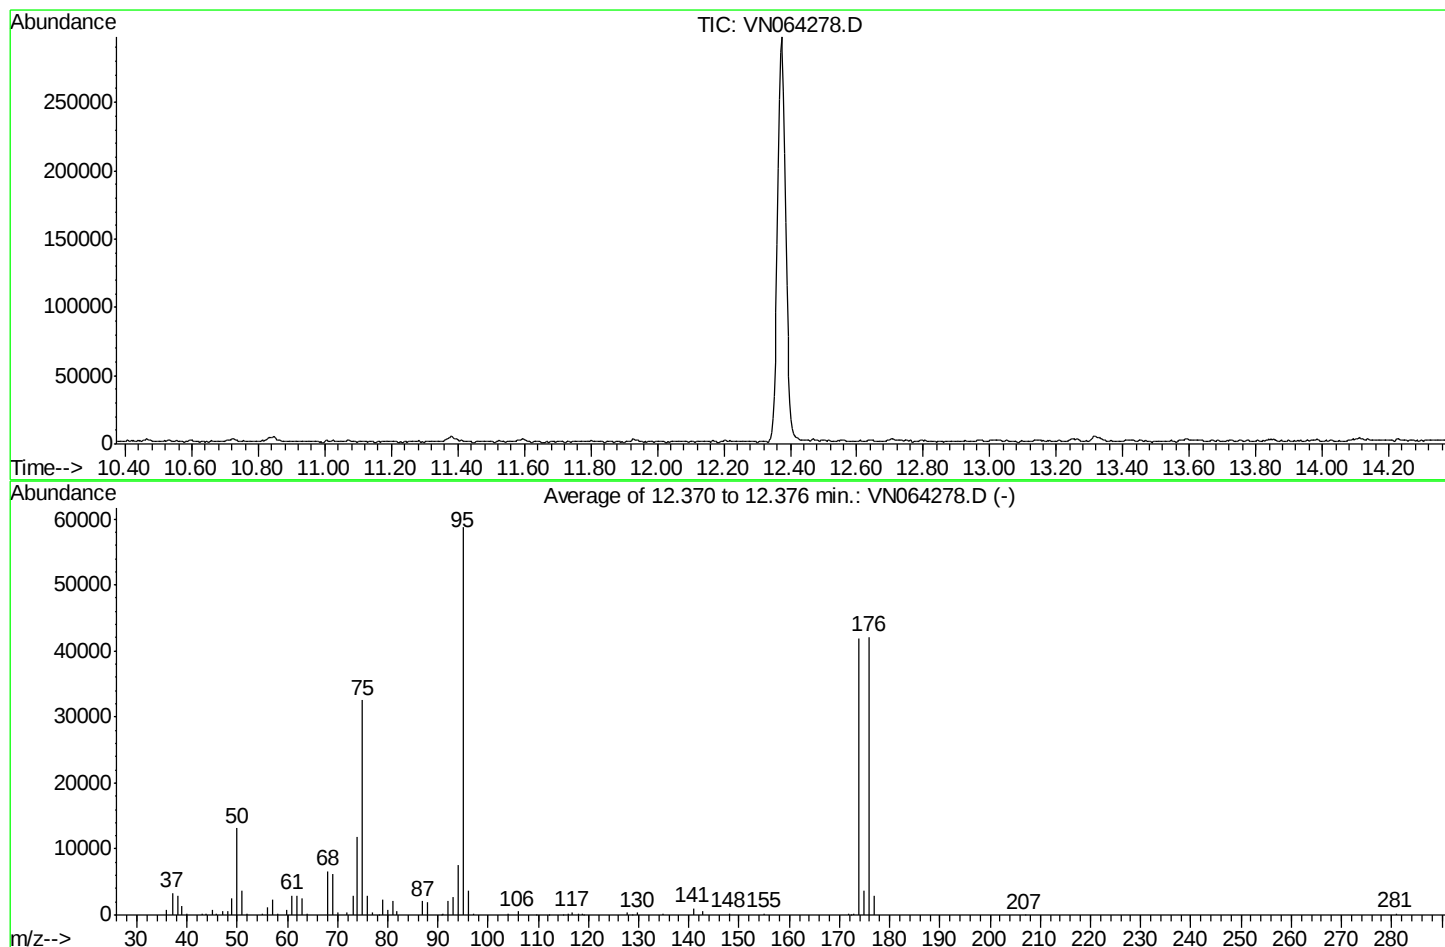

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	13111	PASS
75	95	30	60	55.3	32501	PASS
95	95	100	100	100.0	58725	PASS
96	95	5	9	6.1	3594	PASS
173	174	0.00	2	0.4	154	PASS
174	95	50	100	71.2	41834	PASS
175	174	5	9	8.7	3647	PASS
176	174	95	101	100.8	42176	PASS
177	176	5	9	6.8	2861	PASS