
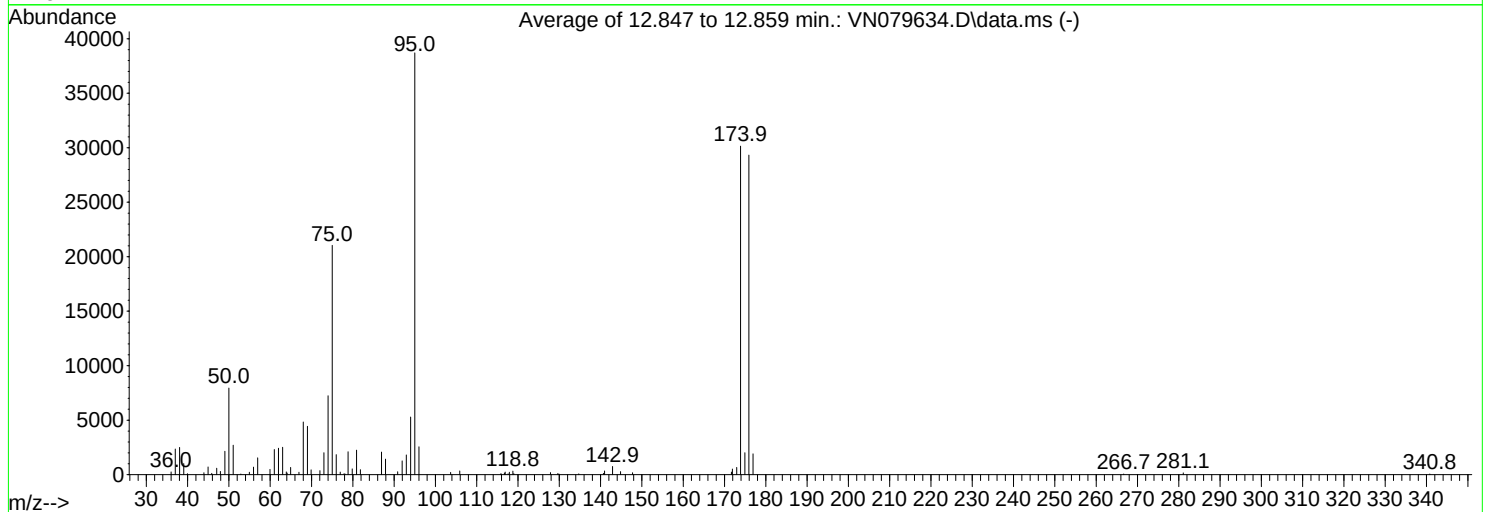


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102323\
Data File : VN079634.D
Acq On : 23 Oct 2023 08:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

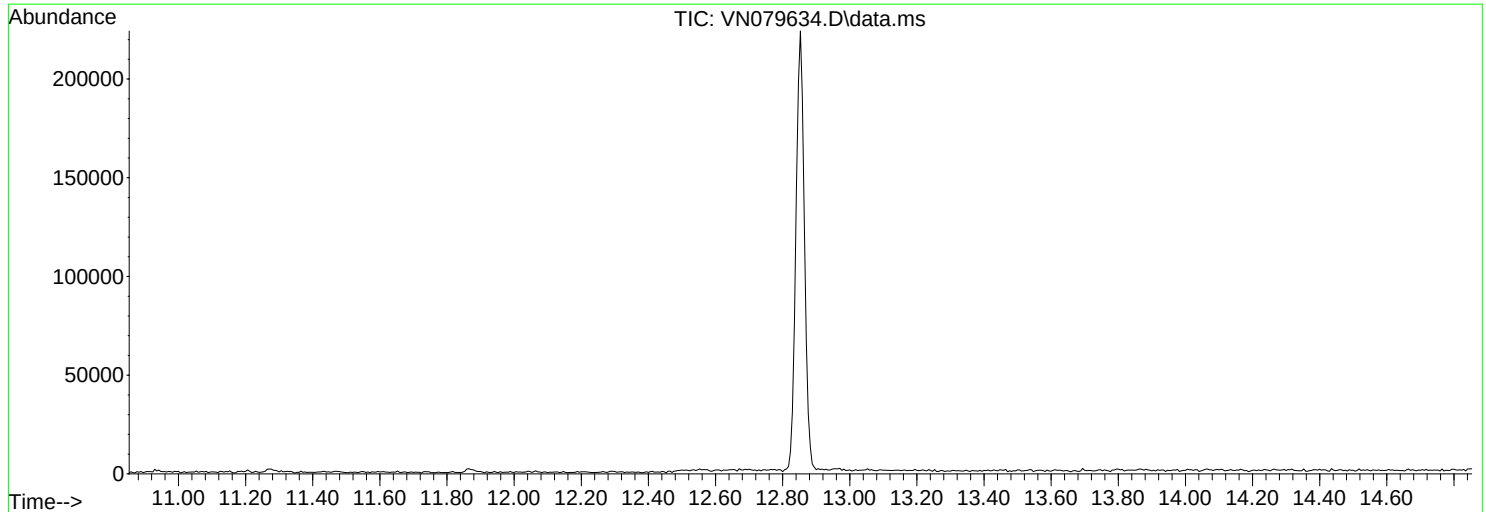

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	7948	PASS
75	95	30	60	54.4	21040	PASS
95	95	100	100	100.0	38709	PASS
96	95	5	9	6.6	2557	PASS
173	174	0.00	2	2.2	654	FAIL*
174	95	50	100	77.9	30141	PASS
175	174	5	9	6.7	2008	PASS
176	174	95	101	97.3	29325	PASS
177	176	5	9	6.5	1911	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	250	50.00	7948	64.10	154	76.95	230
37.00	2357	51.05	2698	64.95	667	77.90	81
38.05	2501	52.90	56	66.95	216	78.10	5
39.05	1008	54.95	222	68.00	4833	78.85	210
39.95	88	55.95	688	69.00	4436	79.85	535
43.95	178	56.95	1548	69.90	437	80.90	2243
44.95	710	59.95	487	72.05	371	81.85	460
45.85	112	61.00	2305	73.00	2014	86.95	2068
47.05	593	62.00	2427	74.00	7234	87.90	1431
47.95	297	63.00	2516	75.00	21040	90.85	267
49.00	2143	63.90	255	76.00	1836	91.95	1256

Average of 12.847 to 12.859 min.: VN079634.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1800	117.90	219	147.75	176		
94.00	5286	118.75	329	171.70	241		
95.00	38709	119.00	88	171.90	511		
96.00	2557	127.85	194	172.95	654		
103.70	211	129.65	107	173.90	30141		
105.90	342	129.90	57	174.95	2008		
115.80	73	134.70	74	175.90	29325		
116.00	55	140.70	116	176.90	1911		
116.70	151	140.95	344	266.70	55		
116.90	232	142.90	749	281.10	165		
117.60	72	144.85	276	340.80	66		

Instrument :

MSVOA_N

ClientSampleId :

BFB