


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102418\
Data File : VN051973.D
Acq On : 24 Oct 2018 7:34
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 12 10:23:44 2018

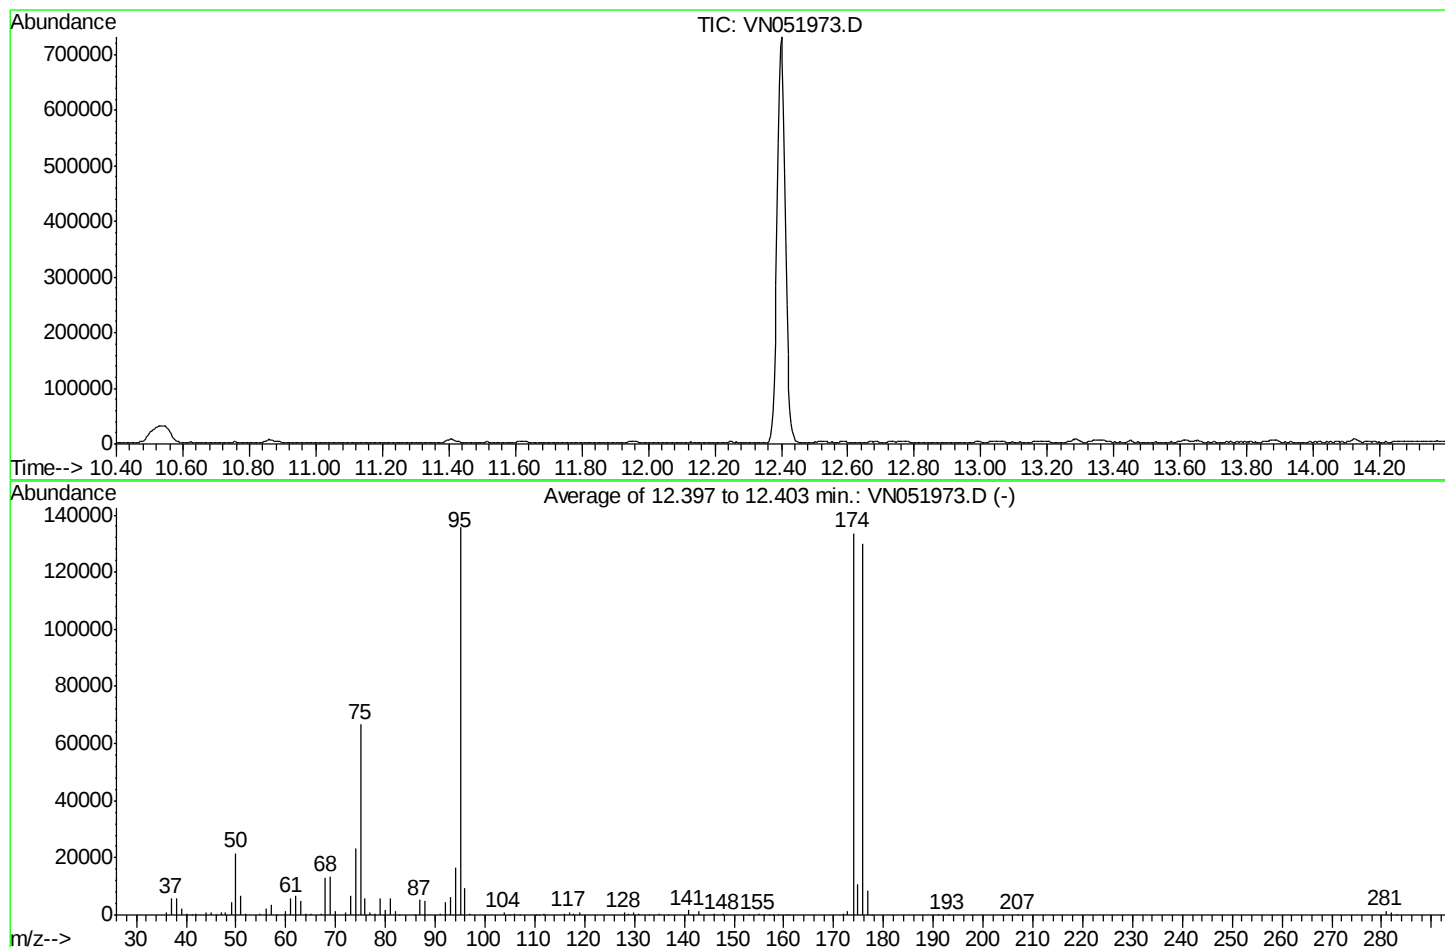

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	21642	PASS
75	95	30	60	49.1	66600	PASS
95	95	100	100	100.0	135680	PASS
96	95	5	9	7.0	9549	PASS
173	174	0.00	2	1.0	1285	PASS
174	95	50	100	98.5	133653	PASS
175	174	5	9	8.0	10633	PASS
176	174	95	101	97.1	129792	PASS
177	176	5	9	6.5	8420	PASS