

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102419\
 Data File : VN058935.D
 Acq On : 23 Oct 2019 17:14
 Operator : JC/SP
 Sample : K5507-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S81-0107

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.011	64	74	82	rBV	30661	46083	1.04%	0.129%
2	2.786	303	315	334	rVB2	142908	287808	6.52%	0.808%
3	3.117	404	418	436	rVB	99908	215200	4.87%	0.604%
4	3.786	604	626	646	rBV5	21623	75362	1.71%	0.212%
5	4.040	689	705	727	rBV	24115	74052	1.68%	0.208%
6	4.506	832	850	853	rBV2	34846	73708	1.67%	0.207%
7	4.571	859	870	911	rVB5	108387	513773	11.64%	1.442%
8	5.030	988	1013	1041	rVB3	93309	334525	7.58%	0.939%
9	5.548	1152	1174	1200	rVB3	72617	229796	5.20%	0.645%
10	6.606	1483	1503	1524	rVV2	203907	633040	14.34%	1.777%
11	6.809	1547	1566	1585	rVB4	21108	61953	1.40%	0.174%
12	7.368	1722	1740	1761	rVB5	18193	51756	1.17%	0.145%
13	7.574	1785	1804	1812	rBV	236534	591098	13.39%	1.659%
14	7.645	1813	1826	1842	rVV4	621268	1657431	37.54%	4.653%
15	7.728	1843	1852	1871	rVB3	58176	147261	3.34%	0.413%
16	7.860	1875	1893	1903	rBV3	78183	191710	4.34%	0.538%
17	8.011	1925	1940	1960	rBV2	326655	804555	18.22%	2.259%
18	8.143	1964	1981	1989	rBV4	60433	153446	3.48%	0.431%
19	8.284	2015	2025	2046	rVB4	79070	192865	4.37%	0.541%
20	8.574	2095	2115	2135	rBV	634345	1337212	30.29%	3.754%
21	9.069	2244	2269	2283	rBV	480077	1120008	25.37%	3.144%
22	9.259	2318	2328	2341	rVB2	47722	92484	2.09%	0.260%
23	9.358	2341	2359	2371	rVB6	20215	51354	1.16%	0.144%
24	9.506	2391	2405	2420	rVB4	61612	132285	3.00%	0.371%
25	9.644	2426	2448	2461	rBV3	77767	187439	4.25%	0.526%
26	9.837	2494	2508	2538	rBV5	29534	114068	2.58%	0.320%
27	10.082	2571	2584	2598	rBV	1055360	2041873	46.25%	5.732%
28	10.149	2600	2605	2617	rVB	93774	153318	3.47%	0.430%
29	10.255	2628	2638	2660	rVB8	55703	169817	3.85%	0.477%
30	10.426	2682	2691	2705	rVB	93326	175568	3.98%	0.493%
31	10.525	2707	2722	2735	rVB4	49697	108119	2.45%	0.304%
32	10.950	2847	2854	2862	rVB	72233	112758	2.55%	0.317%
33	11.001	2862	2870	2881	rVB	66998	116151	2.63%	0.326%
34	11.406	2983	2996	3013	rBV	886021	1554964	35.22%	4.365%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102419\
 Data File : VN058935.D
 Acq On : 23 Oct 2019 17:14
 Operator : JC/SP
 Sample : K5507-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S81-0107

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
 Title : SW846 8260

35	11.509	3014	3028	3046	rVV	1179494	2056753	46.59%	5.774%
36	11.625	3047	3064	3096	rVB	704944	1474982	33.41%	4.141%
37	11.950	3143	3165	3189	rBV	2600888	4414928	100.00%	12.394%
38	12.120	3210	3218	3227	rBV2	39444	60688	1.37%	0.170%
39	12.252	3249	3259	3270	rVB	110602	179521	4.07%	0.504%
40	12.403	3294	3306	3320	rBV	692856	1184275	26.82%	3.325%
41	12.593	3350	3365	3375	rVB	111576	215854	4.89%	0.606%
42	12.660	3376	3386	3390	rVV	141484	222251	5.03%	0.624%
43	12.693	3391	3396	3403	rVV	151253	232550	5.27%	0.653%
44	12.738	3403	3410	3421	rVB	112797	177979	4.03%	0.500%
45	12.895	3445	3459	3472	rBV	1041429	1667017	37.76%	4.680%
46	12.966	3473	3481	3493	rVV7	23032	44678	1.01%	0.125%
47	13.043	3494	3505	3517	rVV	748489	1193233	27.03%	3.350%
48	13.175	3535	3546	3554	rBV4	35750	66484	1.51%	0.187%
49	13.239	3556	3566	3575	rVV	124282	207088	4.69%	0.581%
50	13.294	3576	3583	3589	rVV2	32751	47155	1.07%	0.132%
51	13.348	3589	3600	3604	rVV	849259	1339422	30.34%	3.760%
52	13.377	3605	3609	3623	rVV	1023813	1513071	34.27%	4.248%
53	13.448	3623	3631	3640	rVV2	36082	55717	1.26%	0.156%
54	13.548	3655	3662	3671	rVB	340855	508948	11.53%	1.429%
55	13.593	3671	3676	3691	rVB5	95501	175670	3.98%	0.493%
56	13.676	3691	3702	3711	rBV4	114254	195034	4.42%	0.548%
57	13.747	3712	3724	3734	rBV	242191	390451	8.84%	1.096%
58	13.808	3734	3743	3748	rBV	101267	163836	3.71%	0.460%
59	13.837	3748	3752	3761	rVB2	93382	127491	2.89%	0.358%
60	13.895	3761	3770	3779	rVB	144226	218466	4.95%	0.613%
61	13.953	3780	3788	3793	rBV2	49975	73911	1.67%	0.207%
62	14.001	3793	3803	3813	rVB2	290319	462132	10.47%	1.297%
63	14.053	3813	3819	3834	rVB5	34885	77503	1.76%	0.218%
64	14.136	3835	3845	3854	rBV2	200624	319915	7.25%	0.898%
65	14.217	3862	3870	3876	rBV	142145	210608	4.77%	0.591%
66	14.255	3876	3882	3890	rVB	149325	216895	4.91%	0.609%
67	14.300	3890	3896	3902	rBV2	42180	56191	1.27%	0.158%
68	14.435	3927	3938	3946	rBV5	49334	101916	2.31%	0.286%
69	14.483	3946	3953	3962	rBV2	60307	100832	2.28%	0.283%
70	14.532	3962	3968	3975	rVB	55124	74724	1.69%	0.210%
71	14.593	3976	3987	4002	rBV4	507189	1039029	23.53%	2.917%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102419\
Data File : VN058935.D
Acq On : 23 Oct 2019 17:14
Operator : JC/SP
Sample : K5507-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S81-0107

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Title : SW846 8260

72	14.750	4027	4036	4044	rBV	161660	247069	5.60%	0.694%
73	14.860	4062	4070	4075	rBV3	82801	132812	3.01%	0.373%
74	14.963	4094	4102	4117	rVB4	97943	210423	4.77%	0.591%
75	15.094	4136	4143	4147	rBV	34157	50277	1.14%	0.141%
76	15.133	4149	4155	4164	rVB	81526	125428	2.84%	0.352%
77	15.184	4165	4171	4178	rBV3	34514	47077	1.07%	0.132%
78	15.834	4366	4373	4385	rVB4	78649	139119	3.15%	0.391%


Sum of corrected areas: 35622243

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102419\
Data File : VN058935.D
Acq On : 23 Oct 2019 17:14
Operator : JC/SP
Sample : K5507-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S81-0107

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

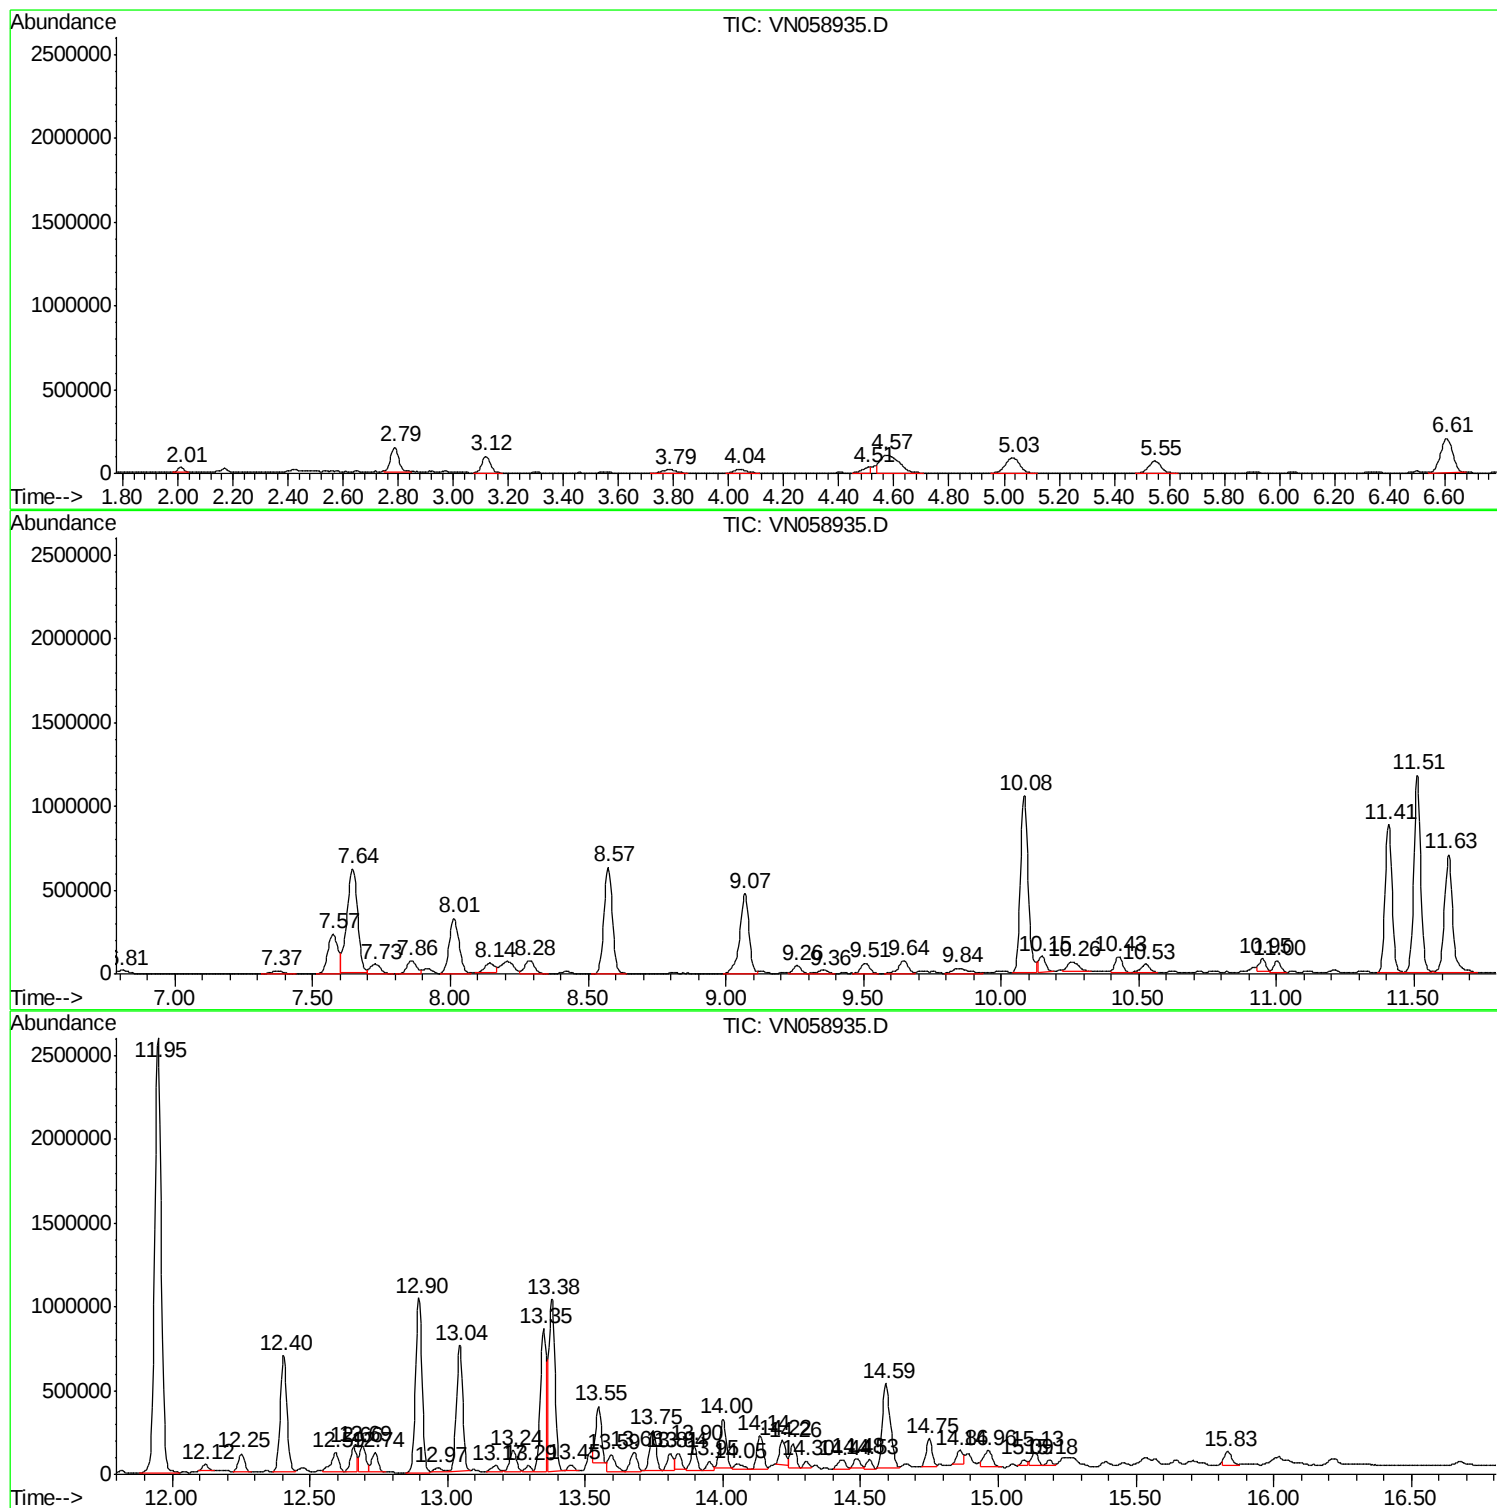

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN102419\
Data File : VN058935.D
Acq On : 23 Oct 2019 17:14
Operator : JC/SP
Sample : K5507-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S81-0107

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN102419\
Data File : VN058935.D
Acq On : 23 Oct 2019 17:14
Operator : JC/SP
Sample : K5507-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S81-0107

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc