

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102419\
 Data File : VN058940.D
 Acq On : 23 Oct 2019 19:04
 Operator : JC/SP
 Sample : K5508-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S32-0669

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	109	123	141	rBV	452903	702946	41.19%	6.114%
2	2.429	195	204	214	rVB6	10514	18856	1.10%	0.164%
3	3.876	642	654	668	rVB4	8323	21738	1.27%	0.189%
4	4.037	681	704	729	rBV	54072	158505	9.29%	1.379%
5	5.021	991	1010	1035	rVB3	21825	71069	4.16%	0.618%
6	6.809	1545	1566	1591	rBV	297773	864600	50.67%	7.521%
7	7.574	1783	1804	1815	rBV	238511	588471	34.48%	5.119%
8	7.648	1815	1827	1850	rVB	387599	919983	53.91%	8.002%
9	8.011	1918	1940	1963	rBV	291702	675259	39.57%	5.874%
10	8.574	2097	2115	2135	rBV	590238	1235281	72.39%	10.745%
11	8.812	2170	2189	2208	rBV4	133026	334312	19.59%	2.908%
12	9.059	2249	2266	2284	rVB3	56570	122167	7.16%	1.063%
13	9.921	2523	2534	2544	rBV3	14635	26992	1.58%	0.235%
14	10.085	2571	2585	2605	rBV	922645	1706489	100.00%	14.844%
15	10.278	2633	2645	2647	rBV2	14411	27500	1.61%	0.239%
16	11.406	2981	2996	3019	rBV	821416	1448136	84.86%	12.596%
17	12.403	3294	3306	3326	rBV	607173	1034197	60.60%	8.996%
18	12.593	3357	3365	3375	rVB2	14427	23337	1.37%	0.203%
19	12.895	3450	3459	3469	rBV3	29501	45888	2.69%	0.399%
20	13.172	3534	3545	3556	rVB4	13103	26370	1.55%	0.229%
21	13.349	3587	3600	3621	rBV	685685	1202968	70.49%	10.464%
22	13.455	3624	3633	3646	rBV3	30606	52027	3.05%	0.453%
23	13.548	3654	3662	3671	rBV3	11743	19464	1.14%	0.169%
24	13.747	3716	3724	3732	rVV2	13499	20569	1.21%	0.179%
25	14.001	3795	3803	3812	rVV3	34235	55709	3.26%	0.485%
26	14.136	3837	3845	3854	rVB3	20739	31134	1.82%	0.271%
27	14.593	3978	3987	3998	rBV4	33035	62556	3.67%	0.544%


Sum of corrected areas: 11496523

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102419\
Data File : VN058940.D
Acq On : 23 Oct 2019 19:04
Operator : JC/SP
Sample : K5508-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S32-0669

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

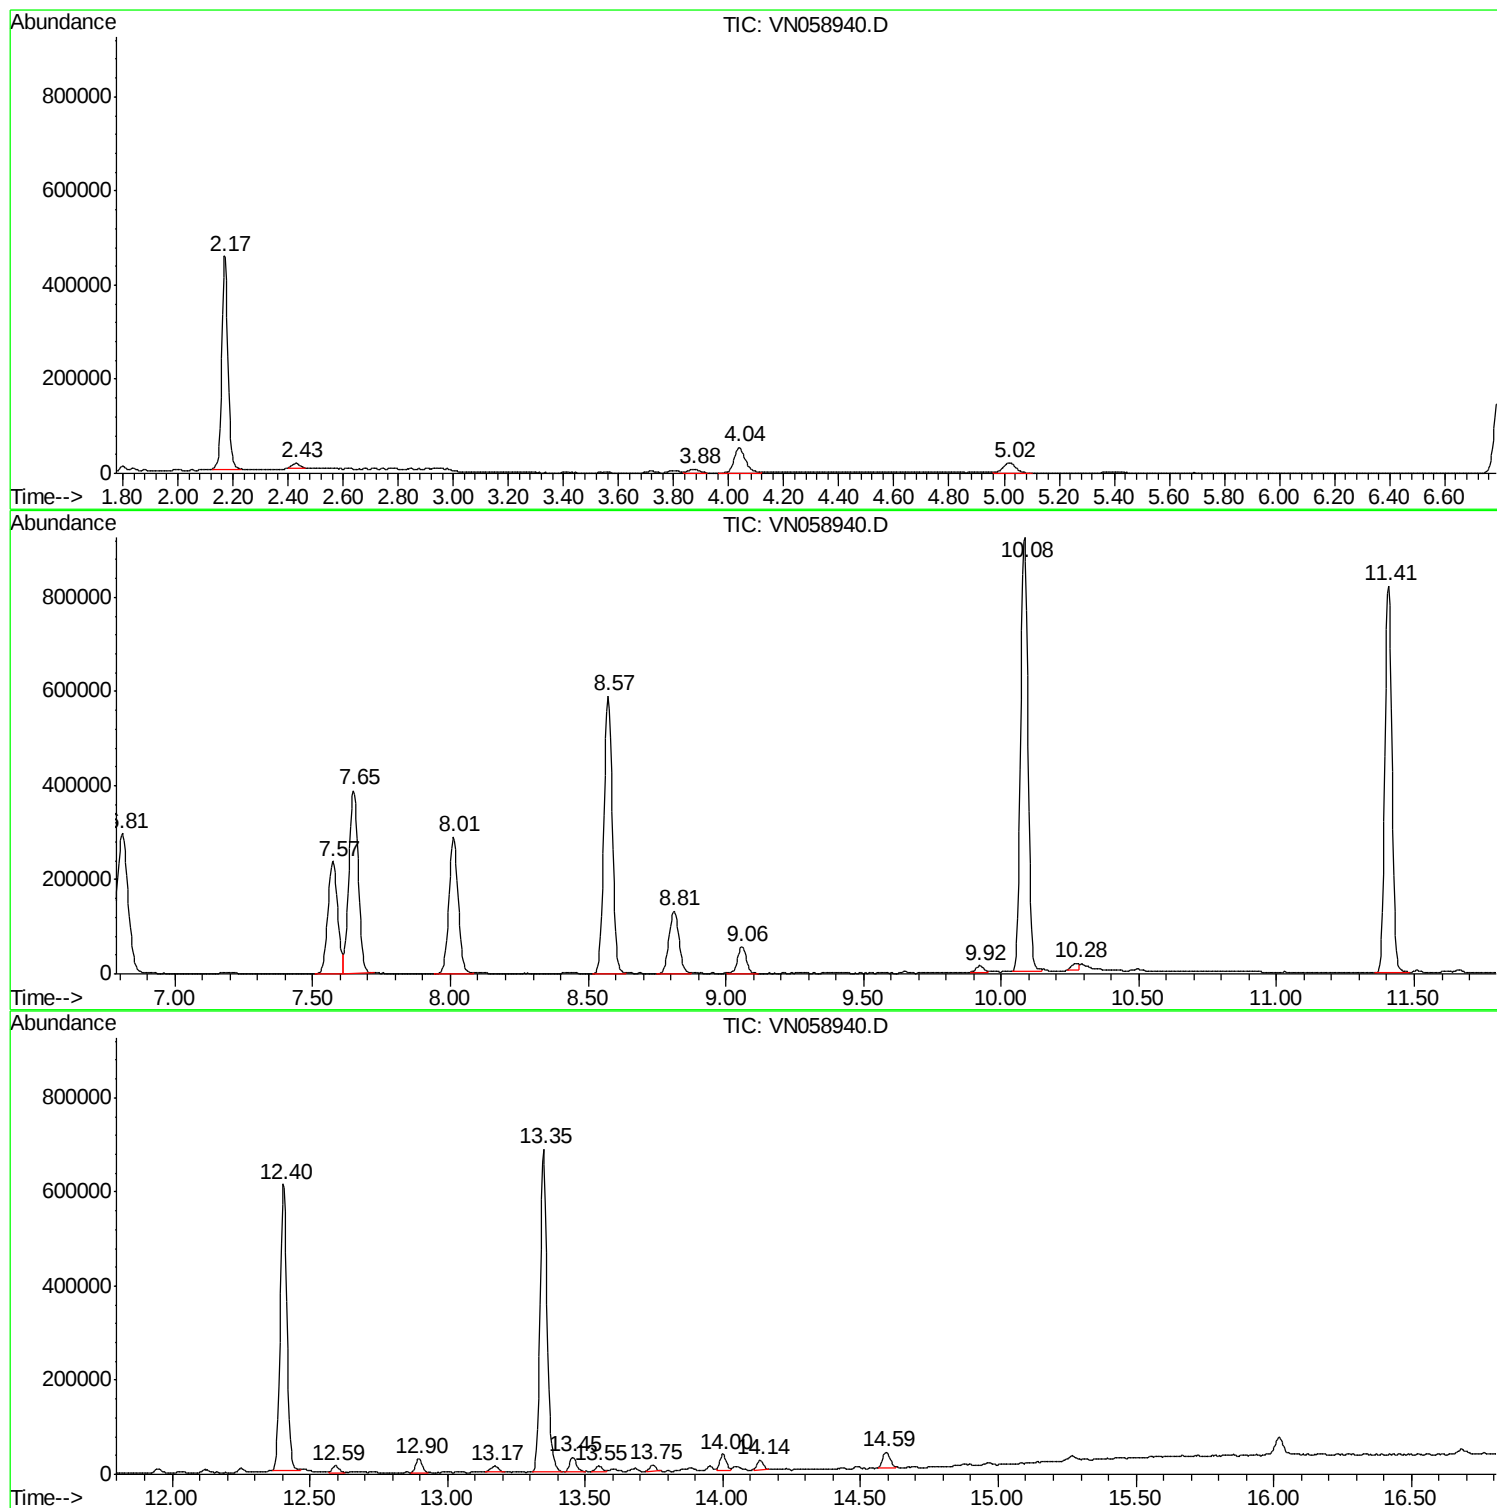

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN102419\
Data File : VN058940.D
Acq On : 23 Oct 2019 19:04
Operator : JC/SP
Sample : K5508-06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S32-0669

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN102419\
Data File : VN058940.D
Acq On : 23 Oct 2019 19:04
Operator : JC/SP
Sample : K5508-06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S32-0669

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc