
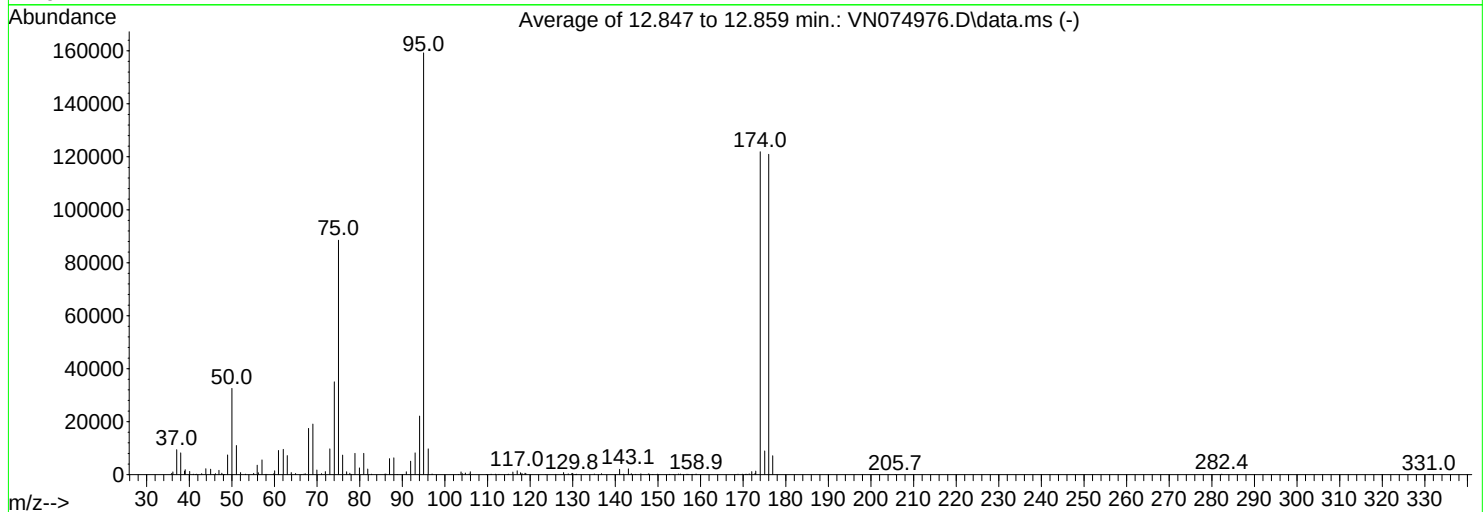


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102422\
Data File : VN074976.D
Acq On : 24 Oct 2022 11:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
Title : SW846 8260
Last Update : Fri Oct 21 09:37:47 2022

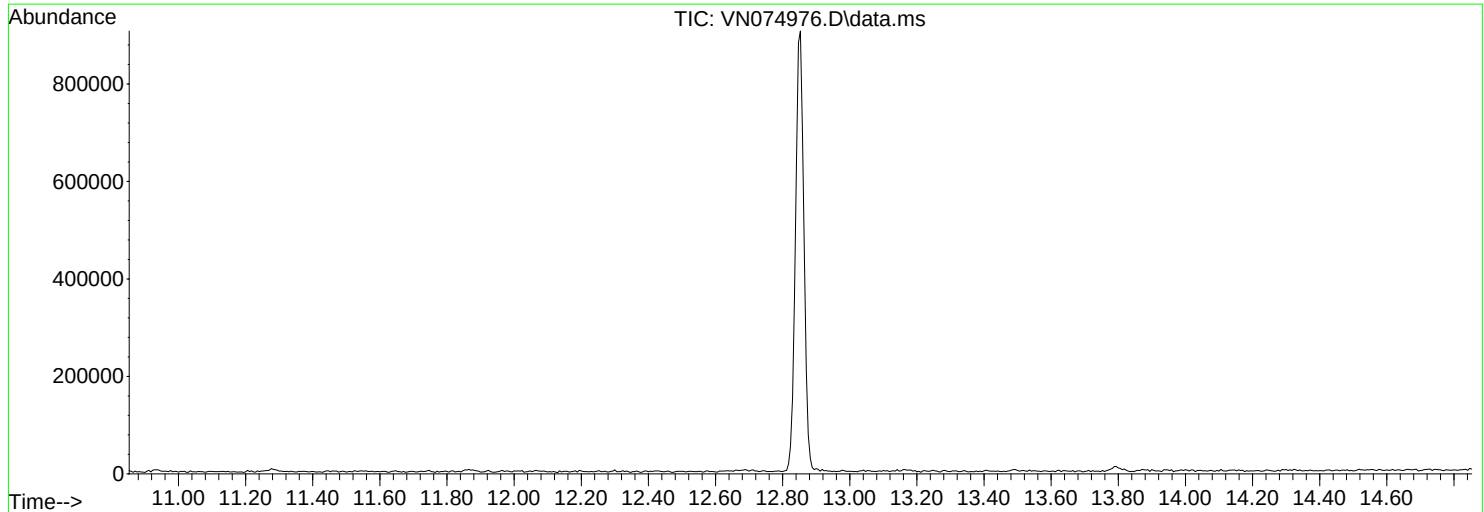

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	32557	PASS
75	95	30	60	55.6	88507	PASS
95	95	100	100	100.0	159240	PASS
96	95	5	9	6.1	9708	PASS
173	174	0.00	2	1.1	1334	PASS
174	95	50	100	76.5	121885	PASS
175	174	5	9	7.4	8965	PASS
176	174	95	101	99.2	120963	PASS
177	176	5	9	5.9	7146	PASS

Average of 12.847 to 12.859 min.: VN074976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	502	43.90	2227	53.20	173	63.00	716
36.15	1047	45.00	2045	55.10	516	63.95	811
37.05	9417	45.80	73	55.95	3570	64.95	43
38.00	8193	46.15	375	56.20	739	66.40	7
38.90	1349	46.95	1658	57.05	5582	66.90	209
39.05	1873	47.65	564	57.80	130	67.20	347
40.10	1210	48.00	36	58.20	98	68.00	17449
40.95	194	49.00	7419	59.80	333	69.00	19072
41.50	56	50.00	32557	60.05	1471	69.95	1748
41.75	181	51.05	10969	60.95	9144	71.05	368
42.90	362	52.05	799	62.05	9565	71.95	1167

Average of 12.847 to 12.859 min.: VN074976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.00	9743	82.80	171	96.10	9708	112.70	111
74.05	35037	85.90	165	97.00	267	114.70	69
75.00	88507	86.15	260	103.20	83	114.95	201
76.00	7388	87.00	6016	103.80	1057	115.95	996
76.95	1114	88.00	6362	104.10	357	116.95	1477
77.70	533	88.80	54	104.80	636	117.75	730
78.00	153	90.95	1098	105.70	230	118.10	430
78.90	8064	91.95	5085	105.95	1090	118.80	574
79.95	2530	93.00	8195	109.70	80	119.00	442
80.95	8019	94.05	22141	110.85	174	123.70	57
81.90	2113	95.00	159240	111.90	203	126.00	123

Average of 12.847 to 12.859 min.: VN074976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.85	786	143.05	2162	155.25	238	171.40	312
128.95	326	143.75	359	156.80	202	172.00	1146
129.80	485	144.80	152	157.05	148	172.80	479
130.00	472	146.00	325	158.00	129	172.95	1334
130.60	74	147.75	288	158.95	238	174.00	121885
130.85	213	148.00	190	168.30	62	175.05	8965
135.05	232	148.80	62	168.80	160	176.00	120963
136.75	358	149.90	163	169.80	203	176.95	7146
140.00	95	152.70	151	170.50	111	205.70	54
141.00	2026	153.60	57	170.70	186	282.35	160
141.90	191	154.80	257	171.00	94	331.00	58

Instrument :

MSVOA_N

ClientSampleId :

BFB