
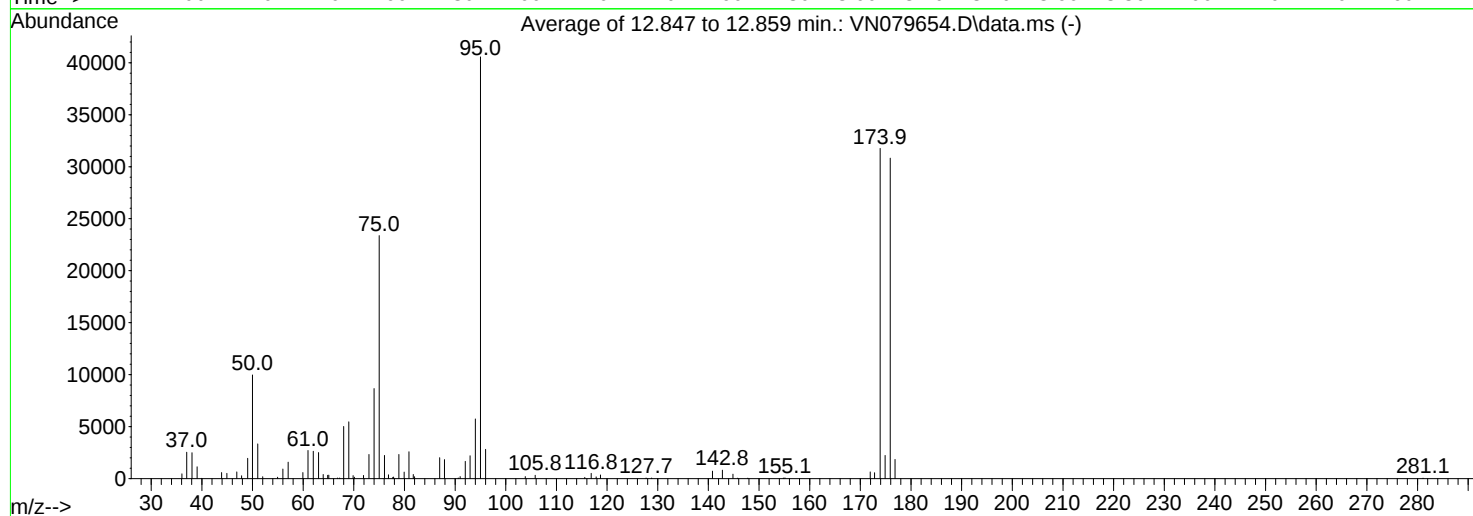


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102423\
Data File : VN079654.D
Acq On : 24 Oct 2023 09:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

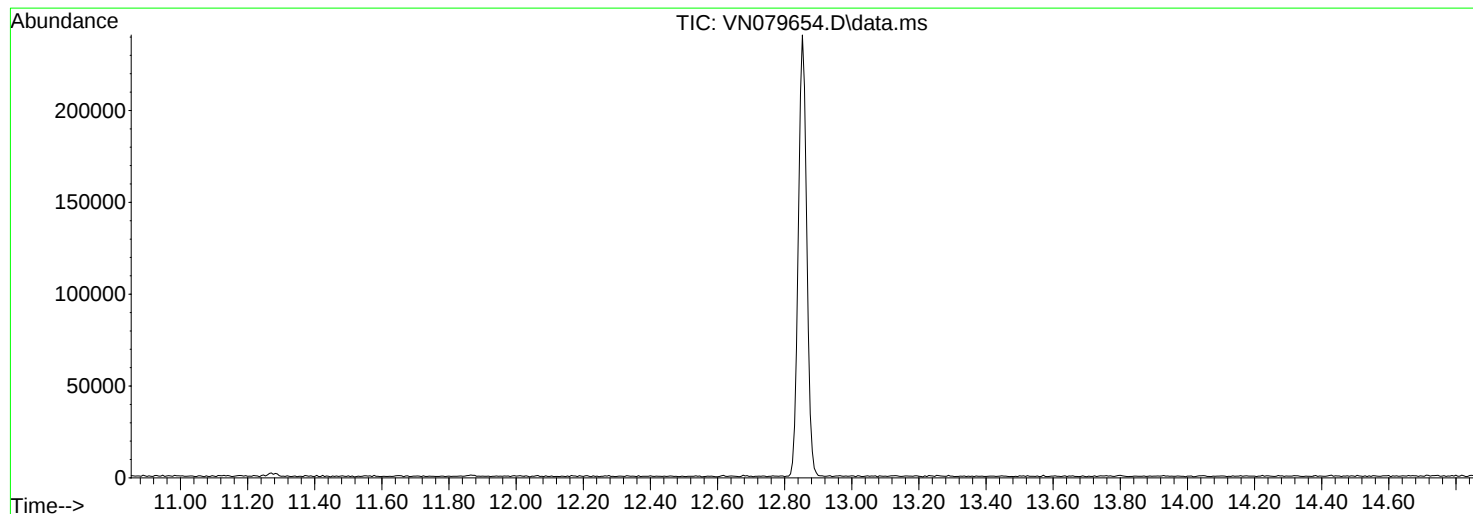

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	9974	PASS
75	95	30	60	57.6	23371	PASS
95	95	100	100	100.0	40568	PASS
96	95	5	9	6.9	2815	PASS
173	174	0.00	2	1.8	573	PASS
174	95	50	100	78.3	31760	PASS
175	174	5	9	7.0	2239	PASS
176	174	95	101	97.1	30824	PASS
177	176	5	9	6.0	1847	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	457	51.05	3338	65.05	344	76.05	2231
37.00	2533	52.00	190	66.80	64	76.85	371
38.05	2499	54.95	137	67.20	63	77.70	111
39.05	1146	56.00	923	68.00	5025	77.85	150
39.95	26	57.05	1588	69.00	5461	78.90	2328
43.90	585	59.95	585	69.85	299	79.95	632
44.95	502	60.95	2717	70.10	137	80.90	2580
46.90	645	62.00	2636	71.90	311	81.75	394
47.85	279	63.05	2510	73.00	2328	82.00	191
49.05	1954	63.95	397	74.00	8671	86.95	2022
50.00	9974	64.85	330	75.00	23371	87.90	1839

Average of 12.847 to 12.859 min.: VN079654.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.60	67	117.85	164	171.95	641		
91.00	209	118.70	356	172.80	573		
92.00	1665	127.70	66	173.90	31760		
92.95	2204	128.80	56	174.90	2239		
94.00	5747	140.80	728	175.90	30824		
95.00	40568	142.75	822	176.85	1847		
96.00	2815	144.85	433	281.10	52		
103.85	201	145.80	51				
105.80	327	147.80	54				
115.60	125	154.80	59				
116.85	503	155.10	72				

Instrument :

MSVOA_N

ClientSampleId :

BFB