

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102425\
 Data File : VN088088.D
 Acq On : 24 Oct 2025 13:01
 Operator : JC\MD
 Sample : VN1024MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1024MBL01

Quant Time: Oct 25 01:01:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 25 00:15:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	224317	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.083	114	483912	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	460634	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.771	152	217876	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	222975	57.484	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	114.960%
35) Dibromofluoromethane	8.153	113	167888	51.643	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.280%
50) Toluene-d8	10.547	98	625594	49.942	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.880%
62) 4-Bromofluorobenzene	12.829	95	231751	52.386	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	104.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102425\
Data File : VN088088.D
Acq On : 24 Oct 2025 13:01
Operator : JC\MD
Sample : VN1024MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1024MBL01

Quant Time: Oct 25 01:01:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 25 00:15:22 2025
Response via : Initial Calibration




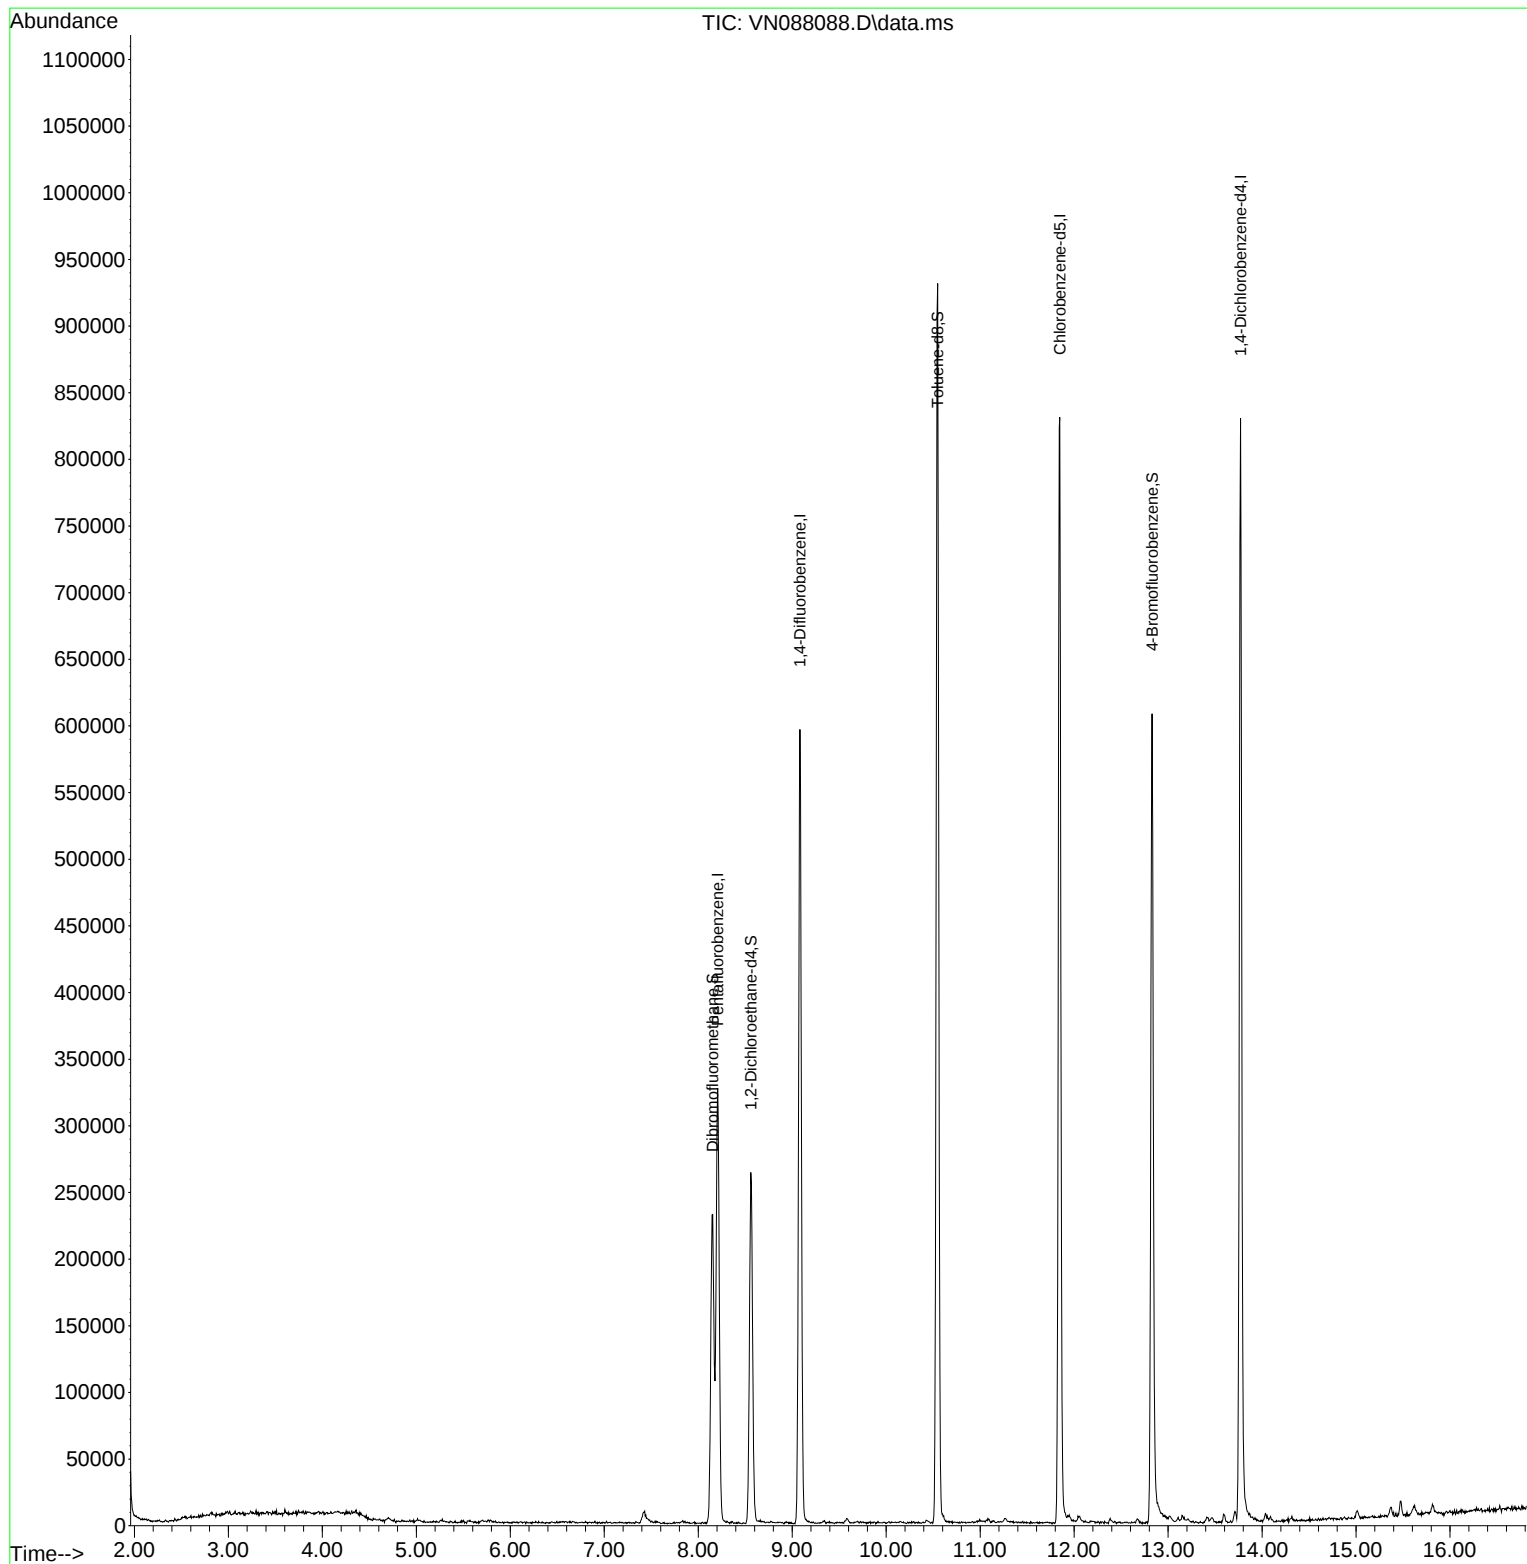


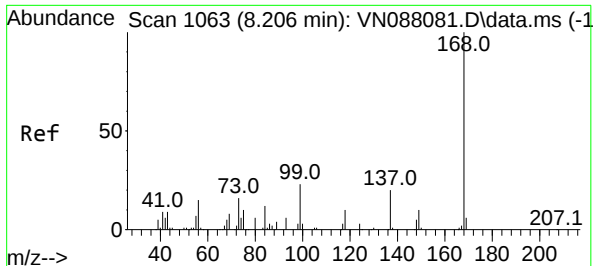

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. 0.000 min
Lab File: VN088088.D
Acq: 24 Oct 2025 13:01




Instrument :
MSVOA_N
ClientSampleId :
VN1024MBL01


Tgt Ion:168 Resp: 224317
Ion Ratio Lower Upper
168 100
99 67.8 57.2 85.8

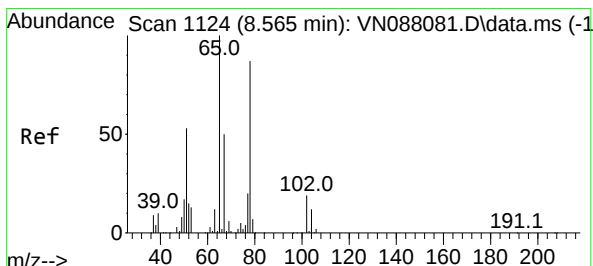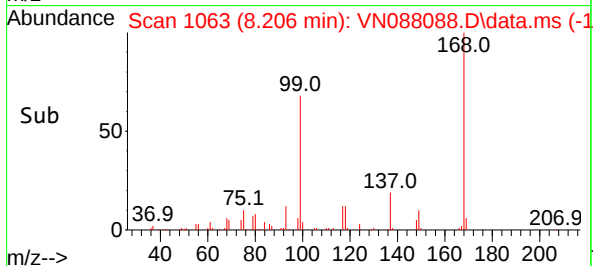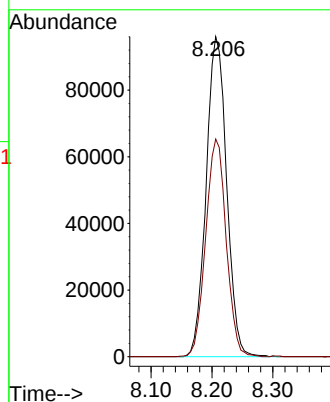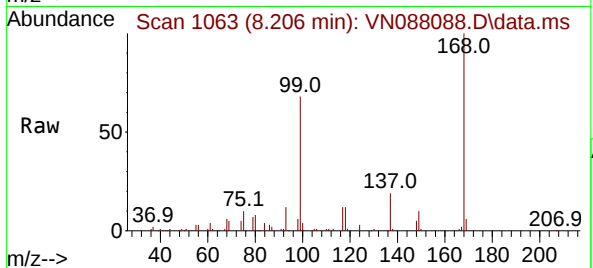

#33
1,2-Dichloroethane-d4
Concen: 57.484 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. 0.000 min
Lab File: VN088088.D
Acq: 24 Oct 2025 13:01

Tgt Ion: 65 Resp: 222975
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.0

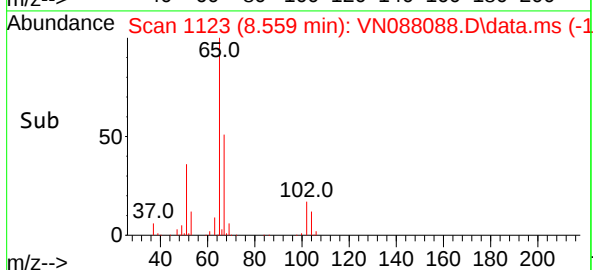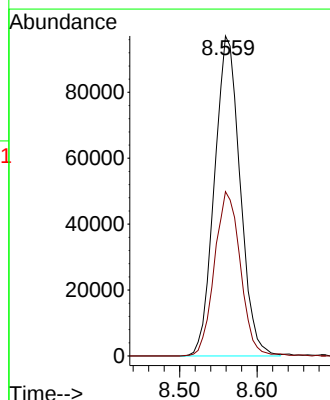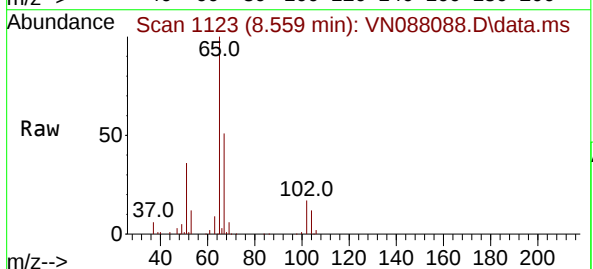

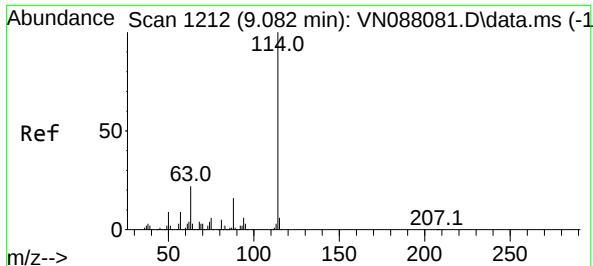

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.083 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN088088.D

Acq: 24 Oct 2025 13:01

Instrument :

MSVOA_N

ClientSampleId :

VN1024MBL01





Tgt Ion:114 Resp: 483912

Ion Ratio Lower Upper

114 100

63 23.5 0.0 45.2

88 17.1 0.0 33.4

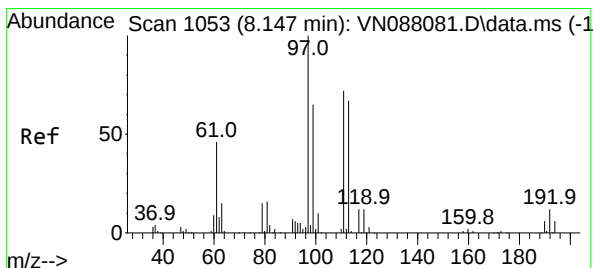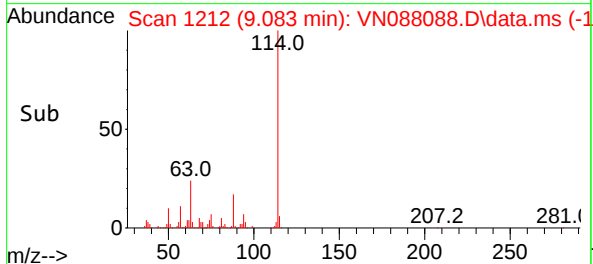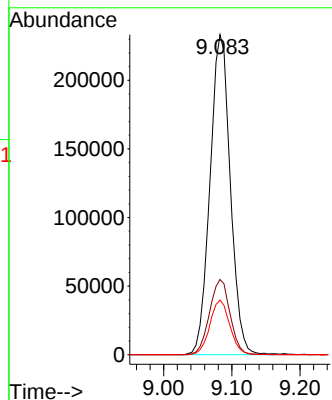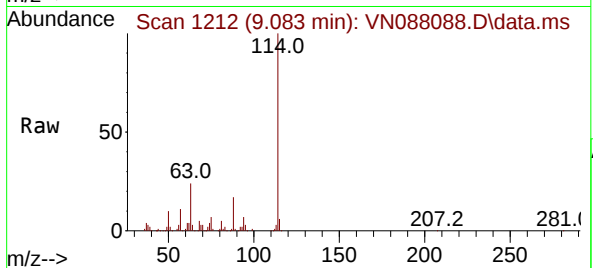

#35

Dibromofluoromethane

Concen: 51.643 ug/l

RT: 8.153 min Scan# 1054

Delta R.T. 0.000 min

Lab File: VN088088.D

Acq: 24 Oct 2025 13:01




Tgt Ion:113 Resp: 167888


Ion Ratio Lower Upper

113 100

111 103.9 82.8 124.2

192 16.3 12.8 19.2


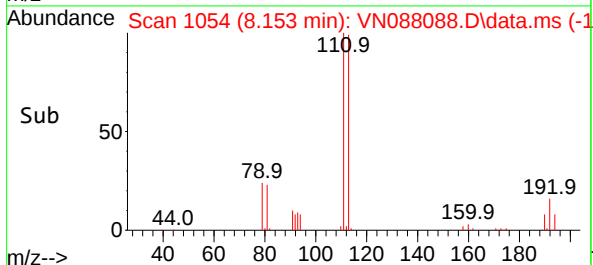
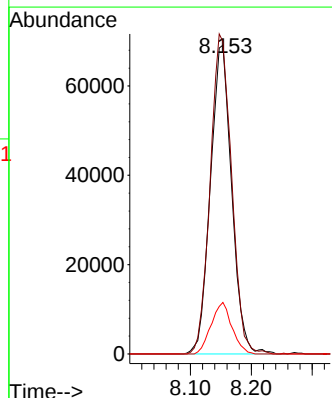
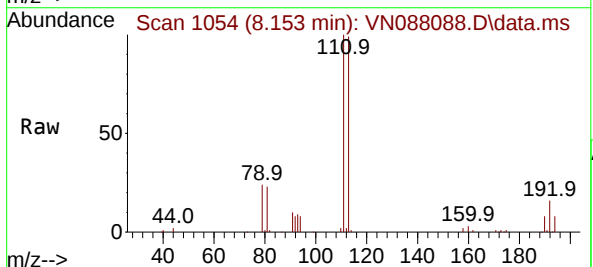


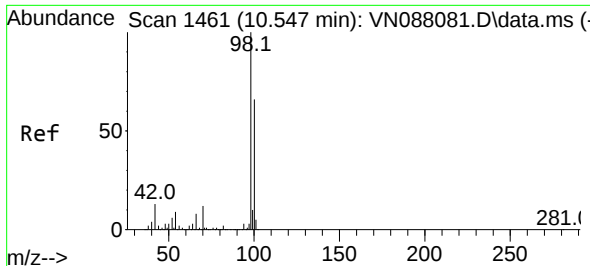

#50
Toluene-d8
Concen: 49.942 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. 0.000 min
Lab File: VN088088.D
Acq: 24 Oct 2025 13:01




Instrument :
MSVOA_N
ClientSampleId :
VN1024MBL01


Tgt Ion: 98 Resp: 625594
Ion Ratio Lower Upper
98 100
100 64.8 52.8 79.2

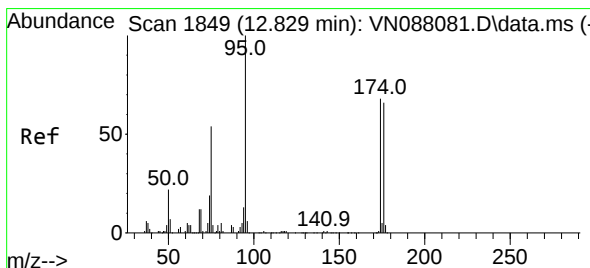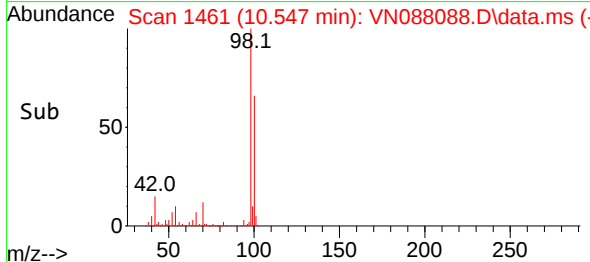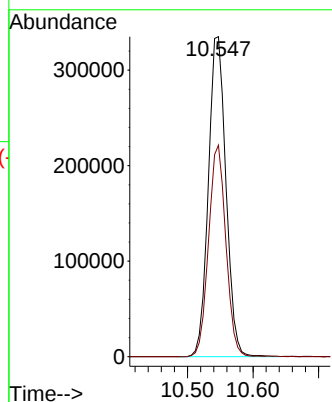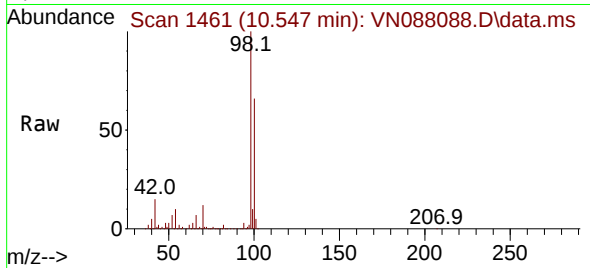

#62
4-Bromofluorobenzene
Concen: 52.386 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088088.D
Acq: 24 Oct 2025 13:01

Tgt Ion: 95 Resp: 231751
Ion Ratio Lower Upper
95 100
174 69.7 0.0 138.4
176 65.5 0.0 132.6


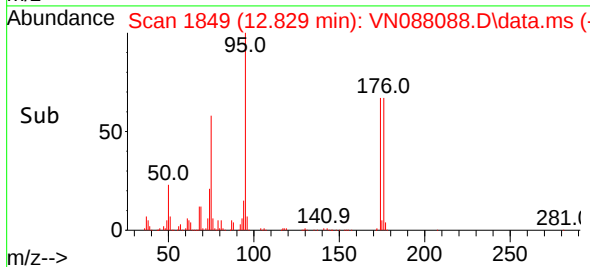
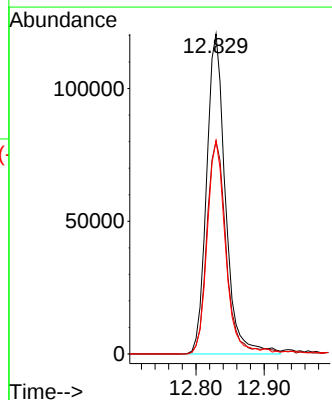
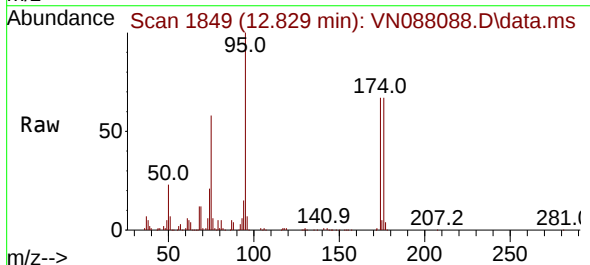


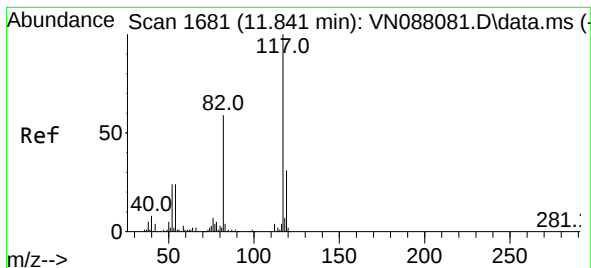

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN088088.D
Acq: 24 Oct 2025 13:01

Instrument :
MSVOA_N
ClientSampleId :
VN1024MBL01

Tgt Ion:117 Resp: 460634
Ion Ratio Lower Upper
117 100
82 58.7 47.4 71.2
119 32.1 24.3 36.5

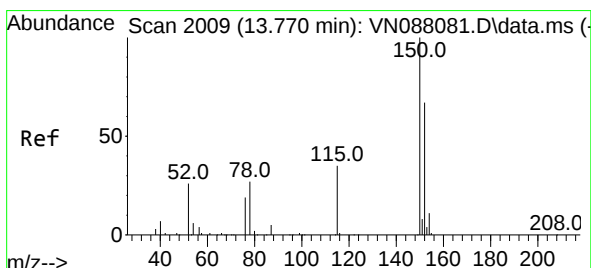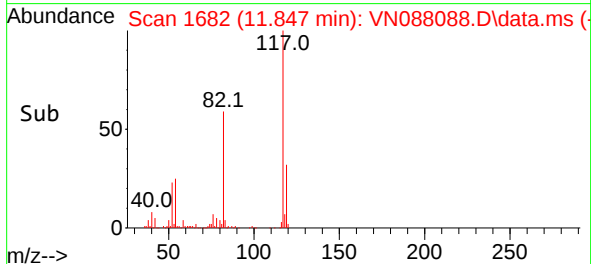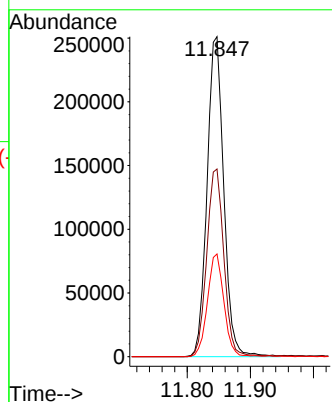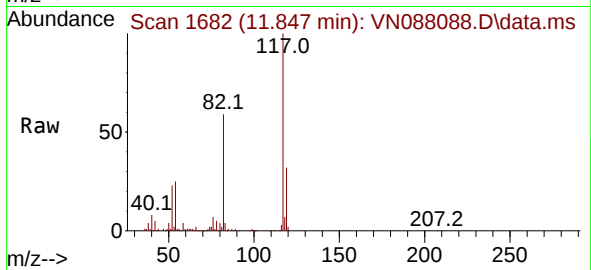

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.771 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN088088.D
Acq: 24 Oct 2025 13:01

Tgt Ion:152 Resp: 217876
Ion Ratio Lower Upper
152 100
115 64.8 32.3 96.8
150 158.6 0.0 351.0

