


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102518\
Data File : VN051998.D
Acq On : 25 Oct 2018 7:40
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102318W.M
Title : SW846 8260
Last Update : Wed Oct 24 10:12:55 2018

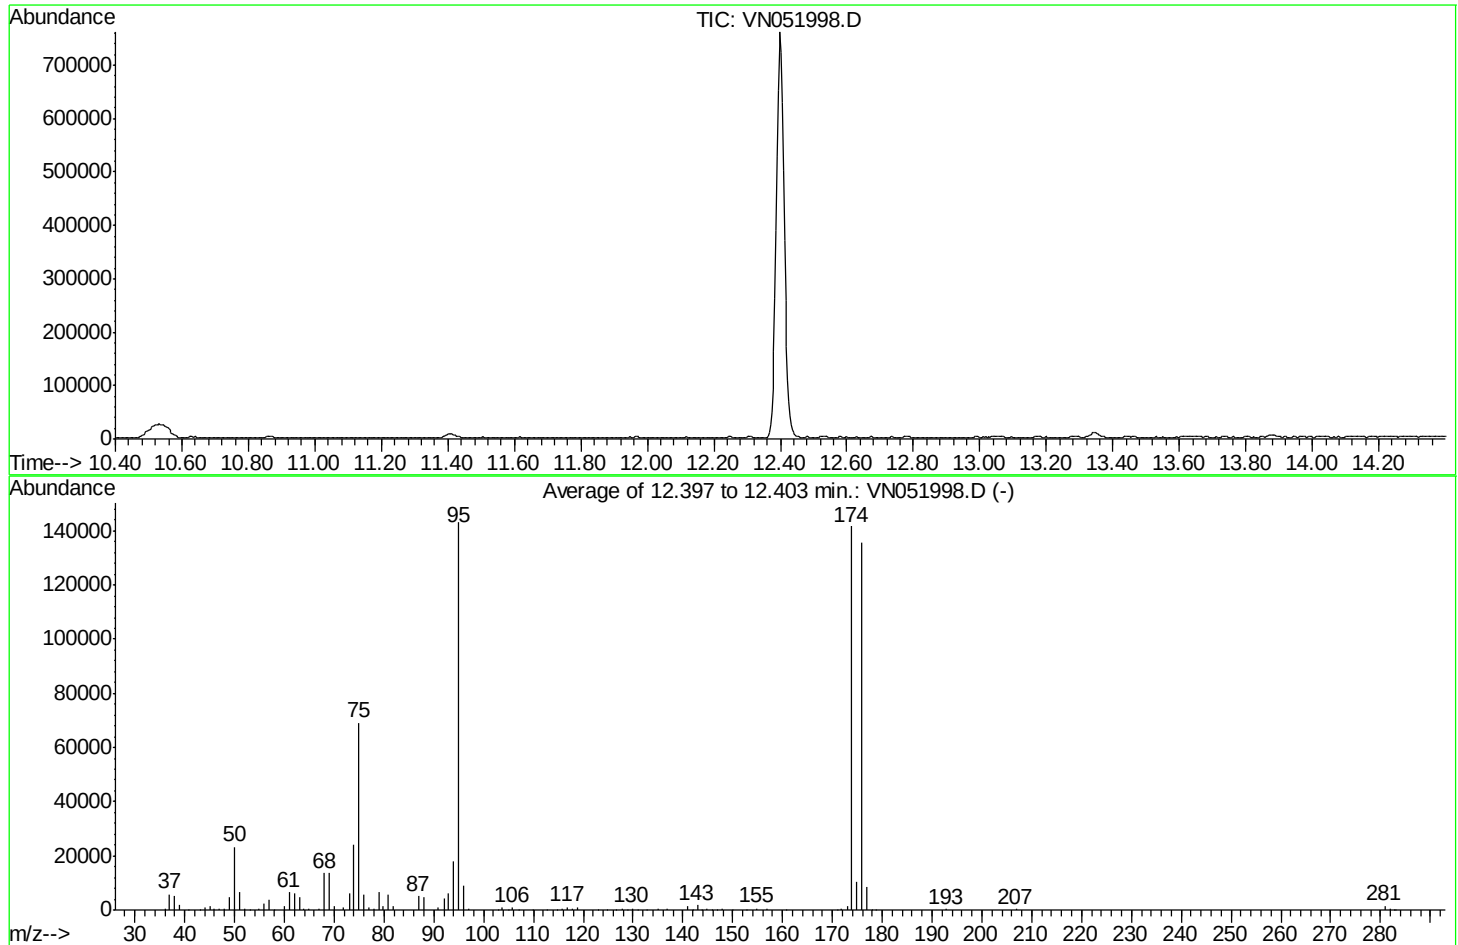

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	23341	PASS
75	95	30	60	48.2	69040	PASS
95	95	100	100	100.0	143168	PASS
96	95	5	9	6.4	9209	PASS
173	174	0.00	2	1.0	1355	PASS
174	95	50	100	99.2	142016	PASS
175	174	5	9	7.5	10631	PASS
176	174	95	101	95.4	135552	PASS
177	176	5	9	6.1	8332	PASS