

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102521\
 Data File : VN069147.D
 Acq On : 25 Oct 2021 12:11
 Operator : JC/MD
 Sample : VN1025WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1025WBL01

Quant Time: Oct 26 03:34:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N102221W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Oct 22 13:15:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.662	128	52306	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	8.971	114	314308	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.747	117	269826	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.440	65	127293	31.245	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	104.133%
60) 4-Bromofluorobenzene	12.734	95	116823	25.250	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	84.167%
63) Toluene-d8	10.443	98	377523	30.968	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	103.233%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102521\
Data File : VN069147.D
Acq On : 25 Oct 2021 12:11
Operator : JC/MD
Sample : VN1025WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01

Quant Time: Oct 26 03:34:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N102221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Oct 22 13:15:19 2021
Response via : Initial Calibration




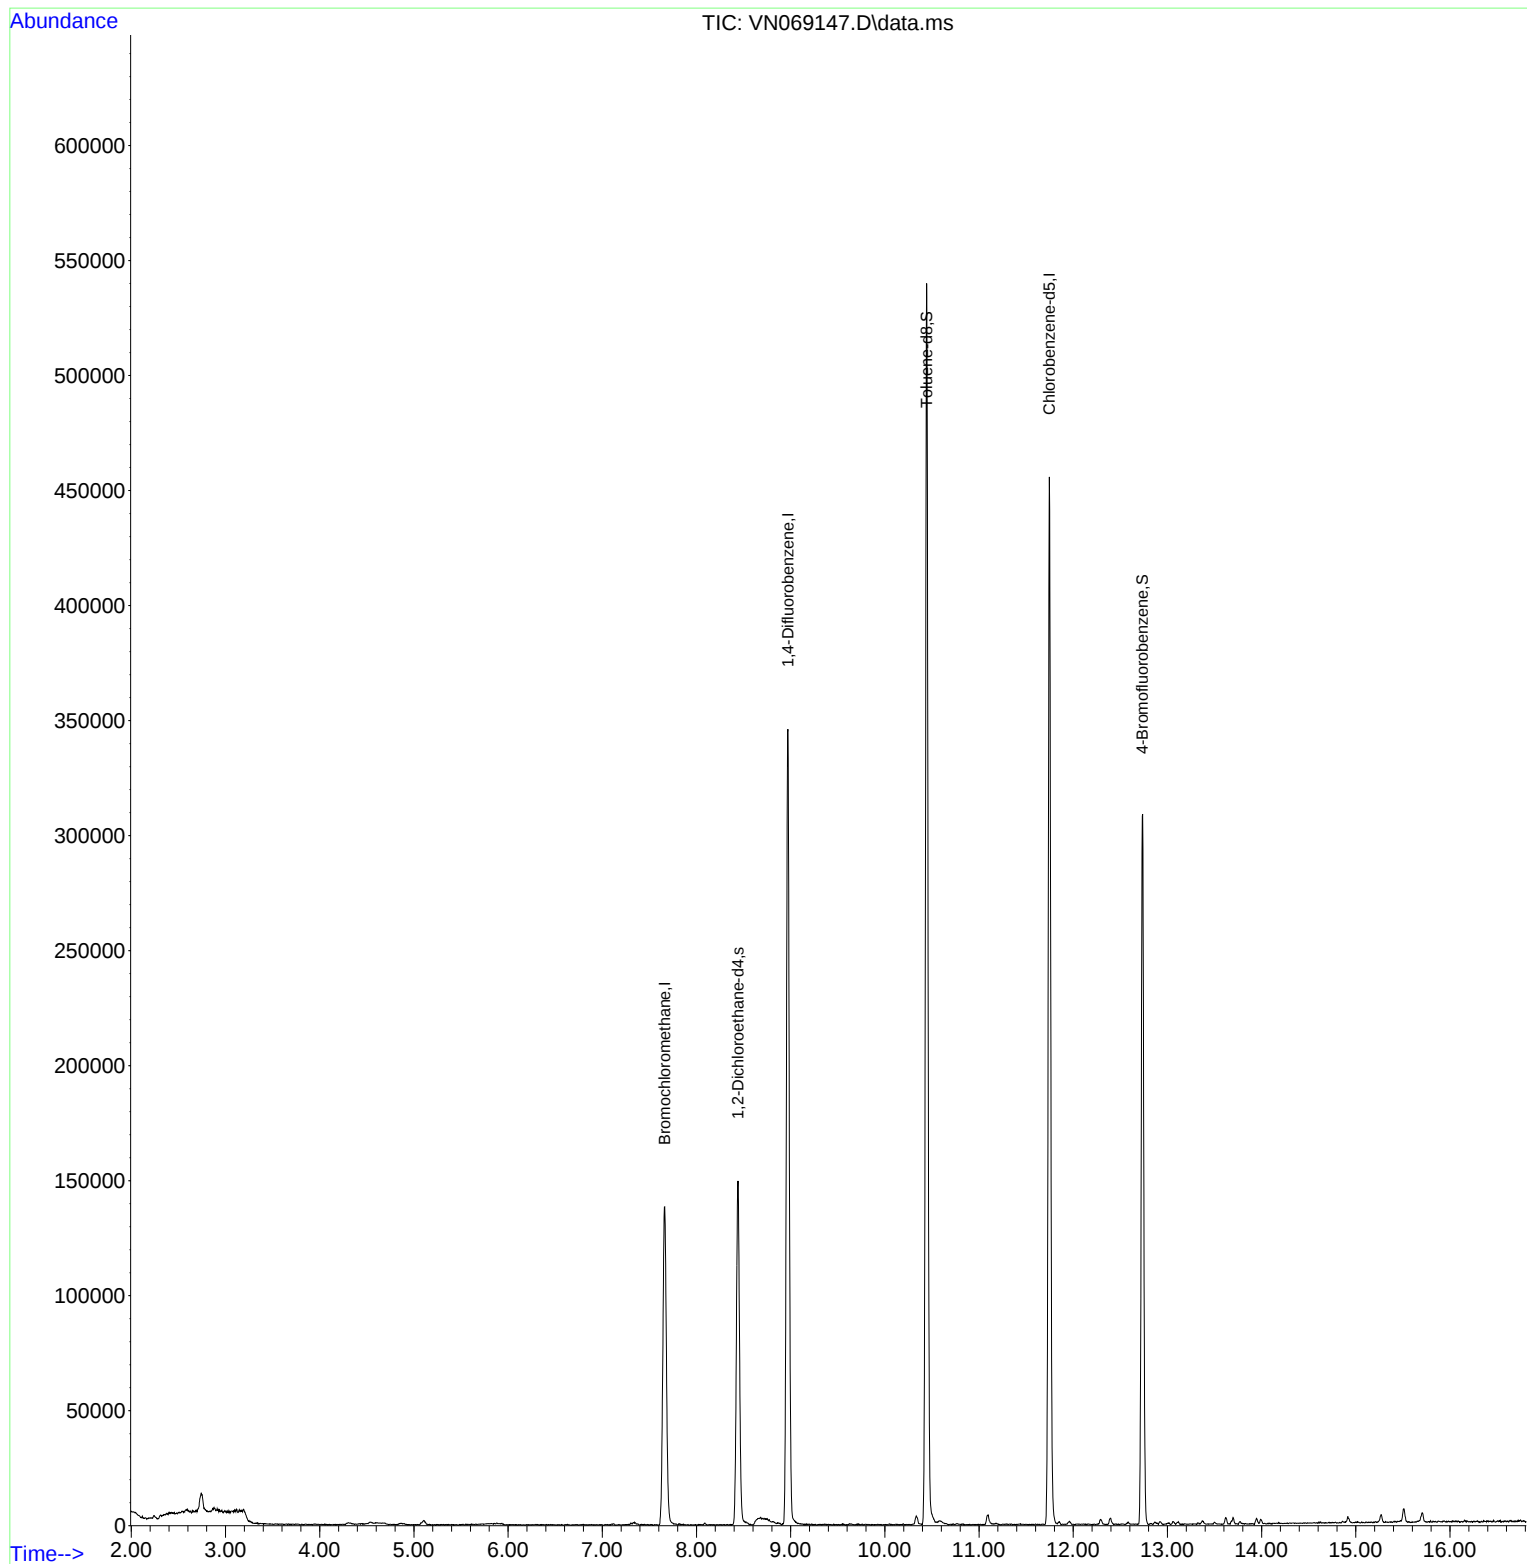


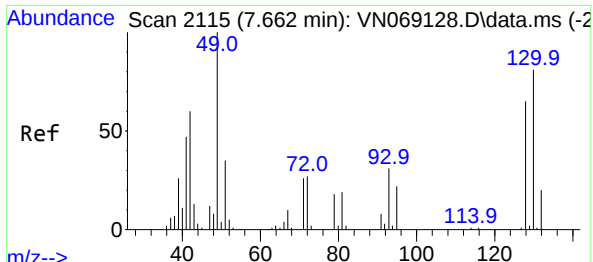

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.662 min Scan# 2115
Delta R.T. -0.000 min
Lab File: VN069147.D
Acq: 25 Oct 2021 12:11




Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01


Tgt Ion:128 Resp: 52306
Ion Ratio Lower Upper
128 100
49 160.0 0.0 392.3
130 129.5 0.0 320.2

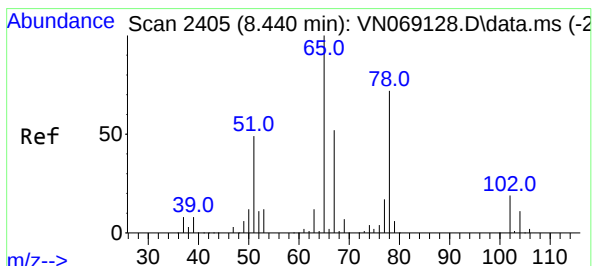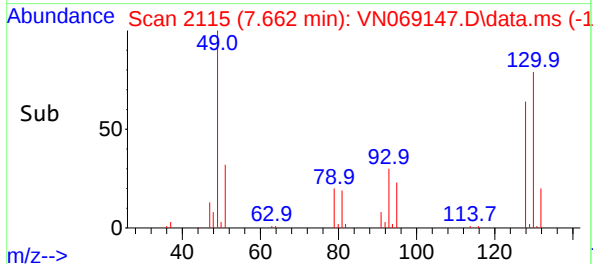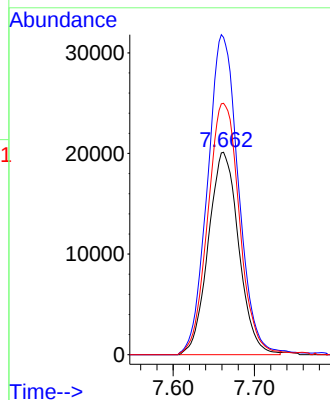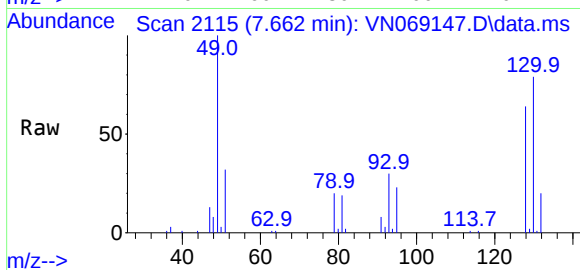

#27
1,2-Dichloroethane-d4
Concen: 31.245 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN069147.D
Acq: 25 Oct 2021 12:11

Tgt Ion: 65 Resp: 127293
Ion Ratio Lower Upper
65 100
67 52.2 40.2 60.2

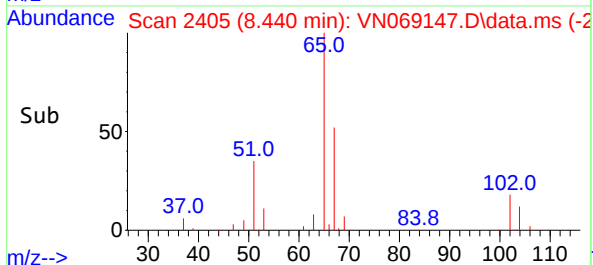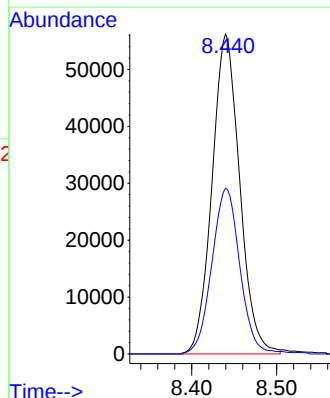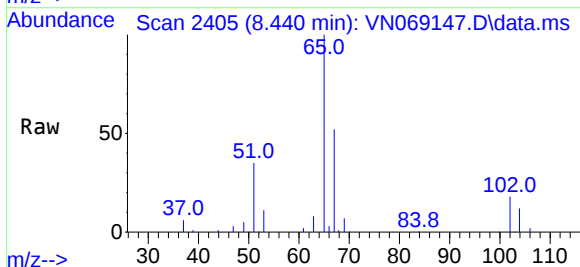




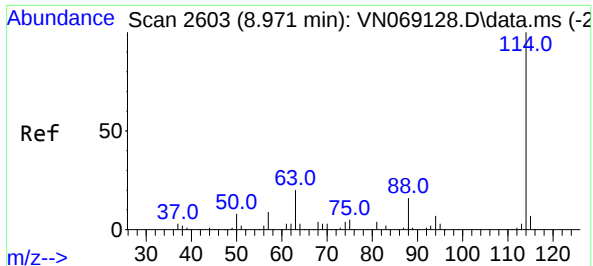


#28

1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.000 min
Lab File: VN069147.D
Acq: 25 Oct 2021 12:11

Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01




Tgt Ion:114 Resp: 314308
Ion Ratio Lower Upper
114 100
63 20.5 15.8 23.6
88 15.8 11.6 17.4

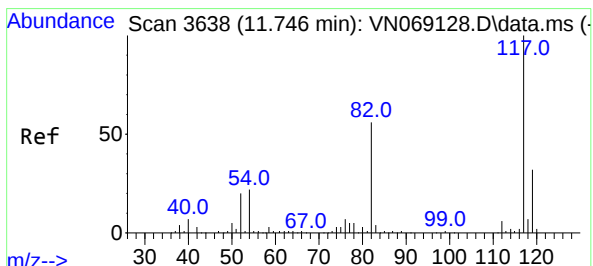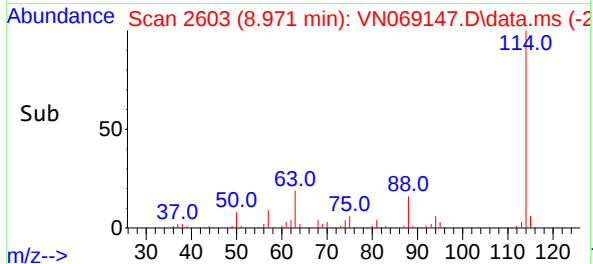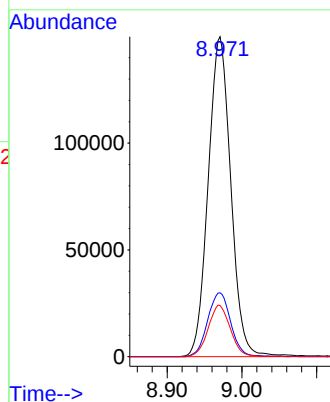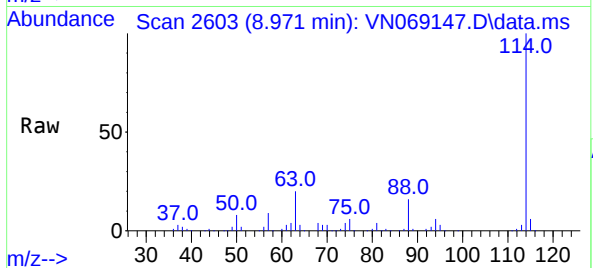


#57

Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069147.D
Acq: 25 Oct 2021 12:11

Tgt Ion:117 Resp: 269826
Ion Ratio Lower Upper
117 100
82 56.1 43.6 65.4
119 31.6 25.8 38.6


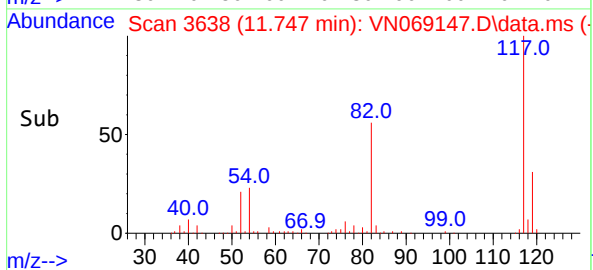
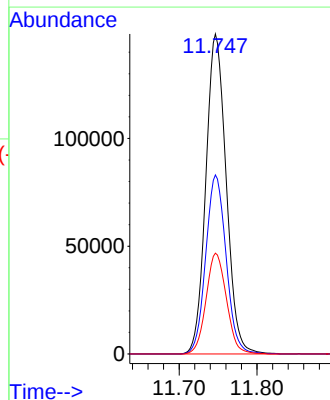
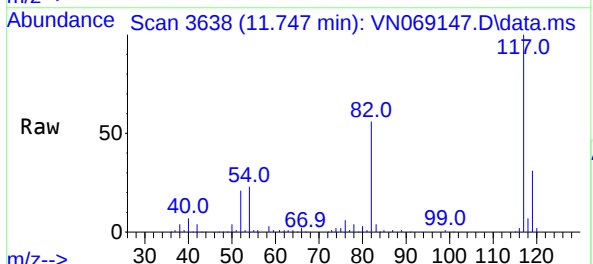


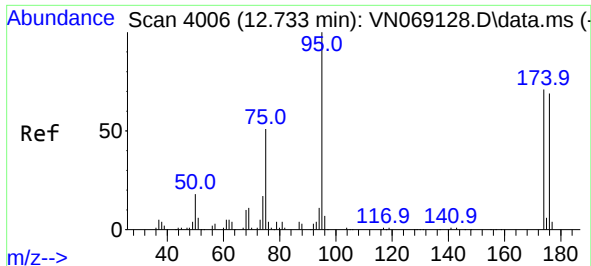

#60
4-Bromofluorobenzene
Concen: 25.250 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069147.D
Acq: 25 Oct 2021 12:11

Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01

Tgt Ion: 95 Resp: 116823
Ion Ratio Lower Upper
95 100
174 72.4 62.9 94.3
176 70.4 61.0 91.4

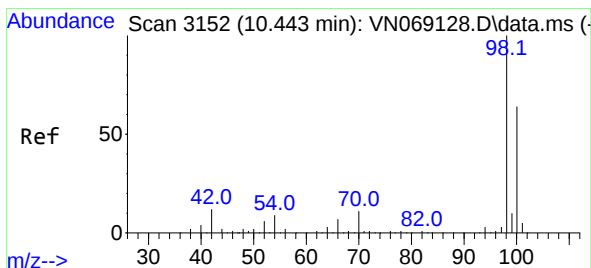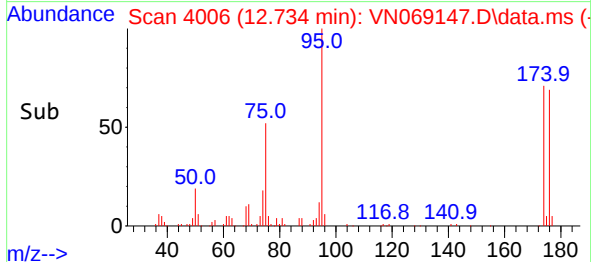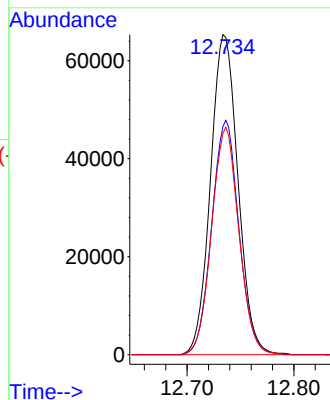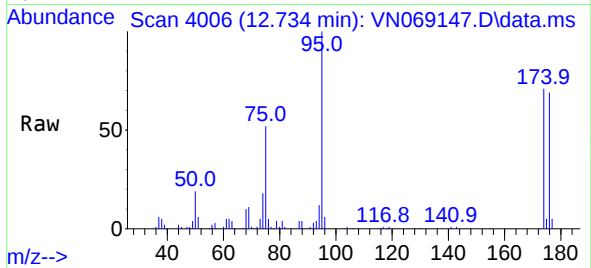

#63
Toluene-d8
Concen: 30.968 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069147.D
Acq: 25 Oct 2021 12:11

Tgt Ion: 98 Resp: 377523
Ion Ratio Lower Upper
98 100
100 64.4 50.6 76.0

