
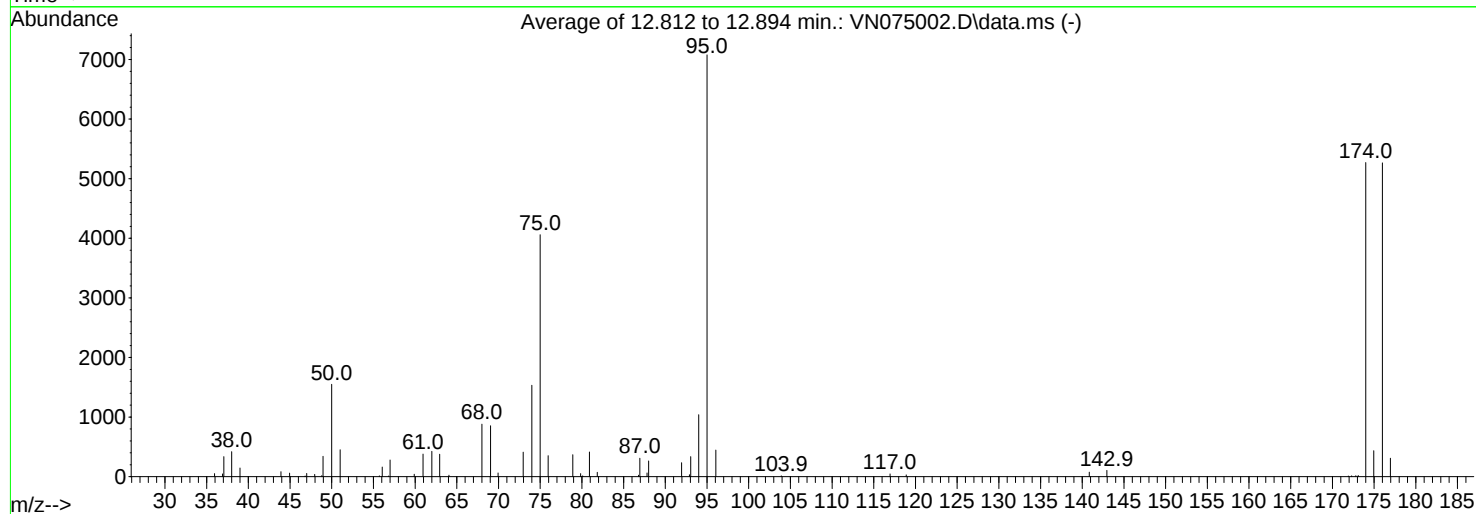


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102522\
Data File : VN075002.D
Acq On : 25 Oct 2022 09:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N102522W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 27 10:19:47 2022

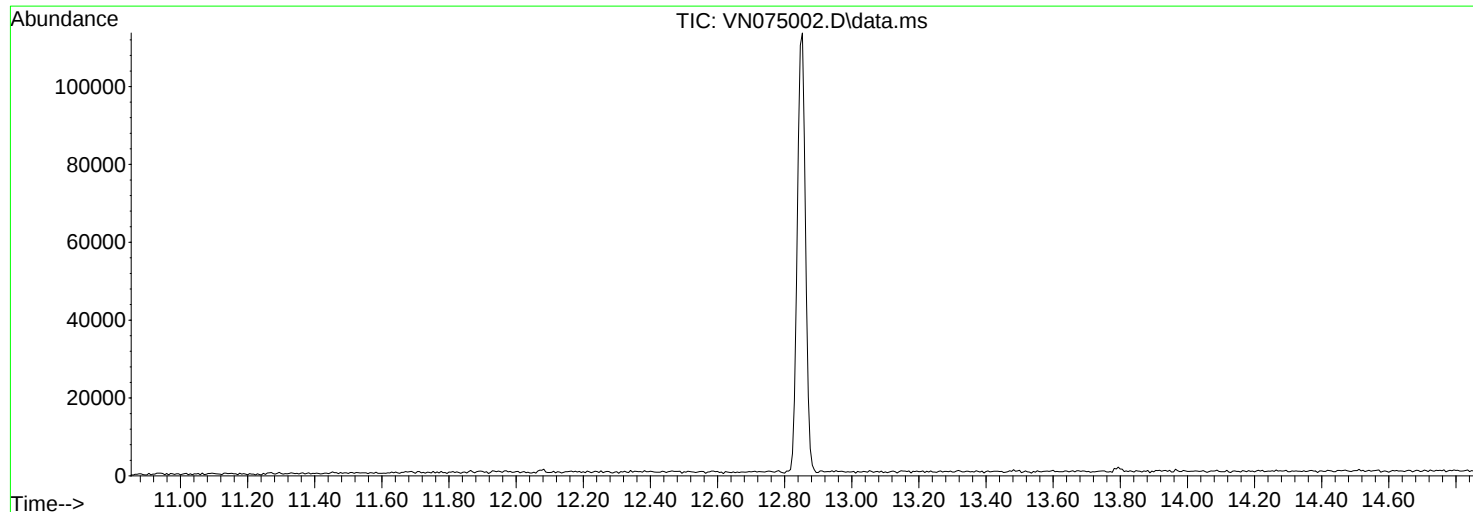

Spectrum Information: Average of 12.812 to 12.894 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	1549	PASS
75	95	30	60	57.3	4059	PASS
95	95	100	100	100.0	7078	PASS
96	95	5	9	6.3	447	PASS
173	174	0.00	2	0.3	18	PASS
174	95	50	100	74.5	5271	PASS
175	174	5	9	8.2	434	PASS
176	174	95	101	99.9	5265	PASS
177	176	5	9	5.9	309	PASS