

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102523\
 Data File : VN079687.D
 Acq On : 25 Oct 2023 17:25
 Operator : JC\MD
 Sample : 05054-01RE 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 14B-1RE

Quant Time: Oct 26 01:38:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N101723W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Oct 18 02:19:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.824	128	18041	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.106	114	112470	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.871	117	131662	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.583	65	79080	30.830	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	102.767%
60) 4-Bromofluorobenzene	12.853	95	52473	21.794	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	72.633%
63) Toluene-d8	10.571	98	162993	28.890	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	96.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102523\
Data File : VN079687.D
Acq On : 25 Oct 2023 17:25
Operator : JC\MD
Sample : 05054-01RE 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
14B-1RE

Quant Time: Oct 26 01:38:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N101723W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Oct 18 02:19:15 2023
Response via : Initial Calibration




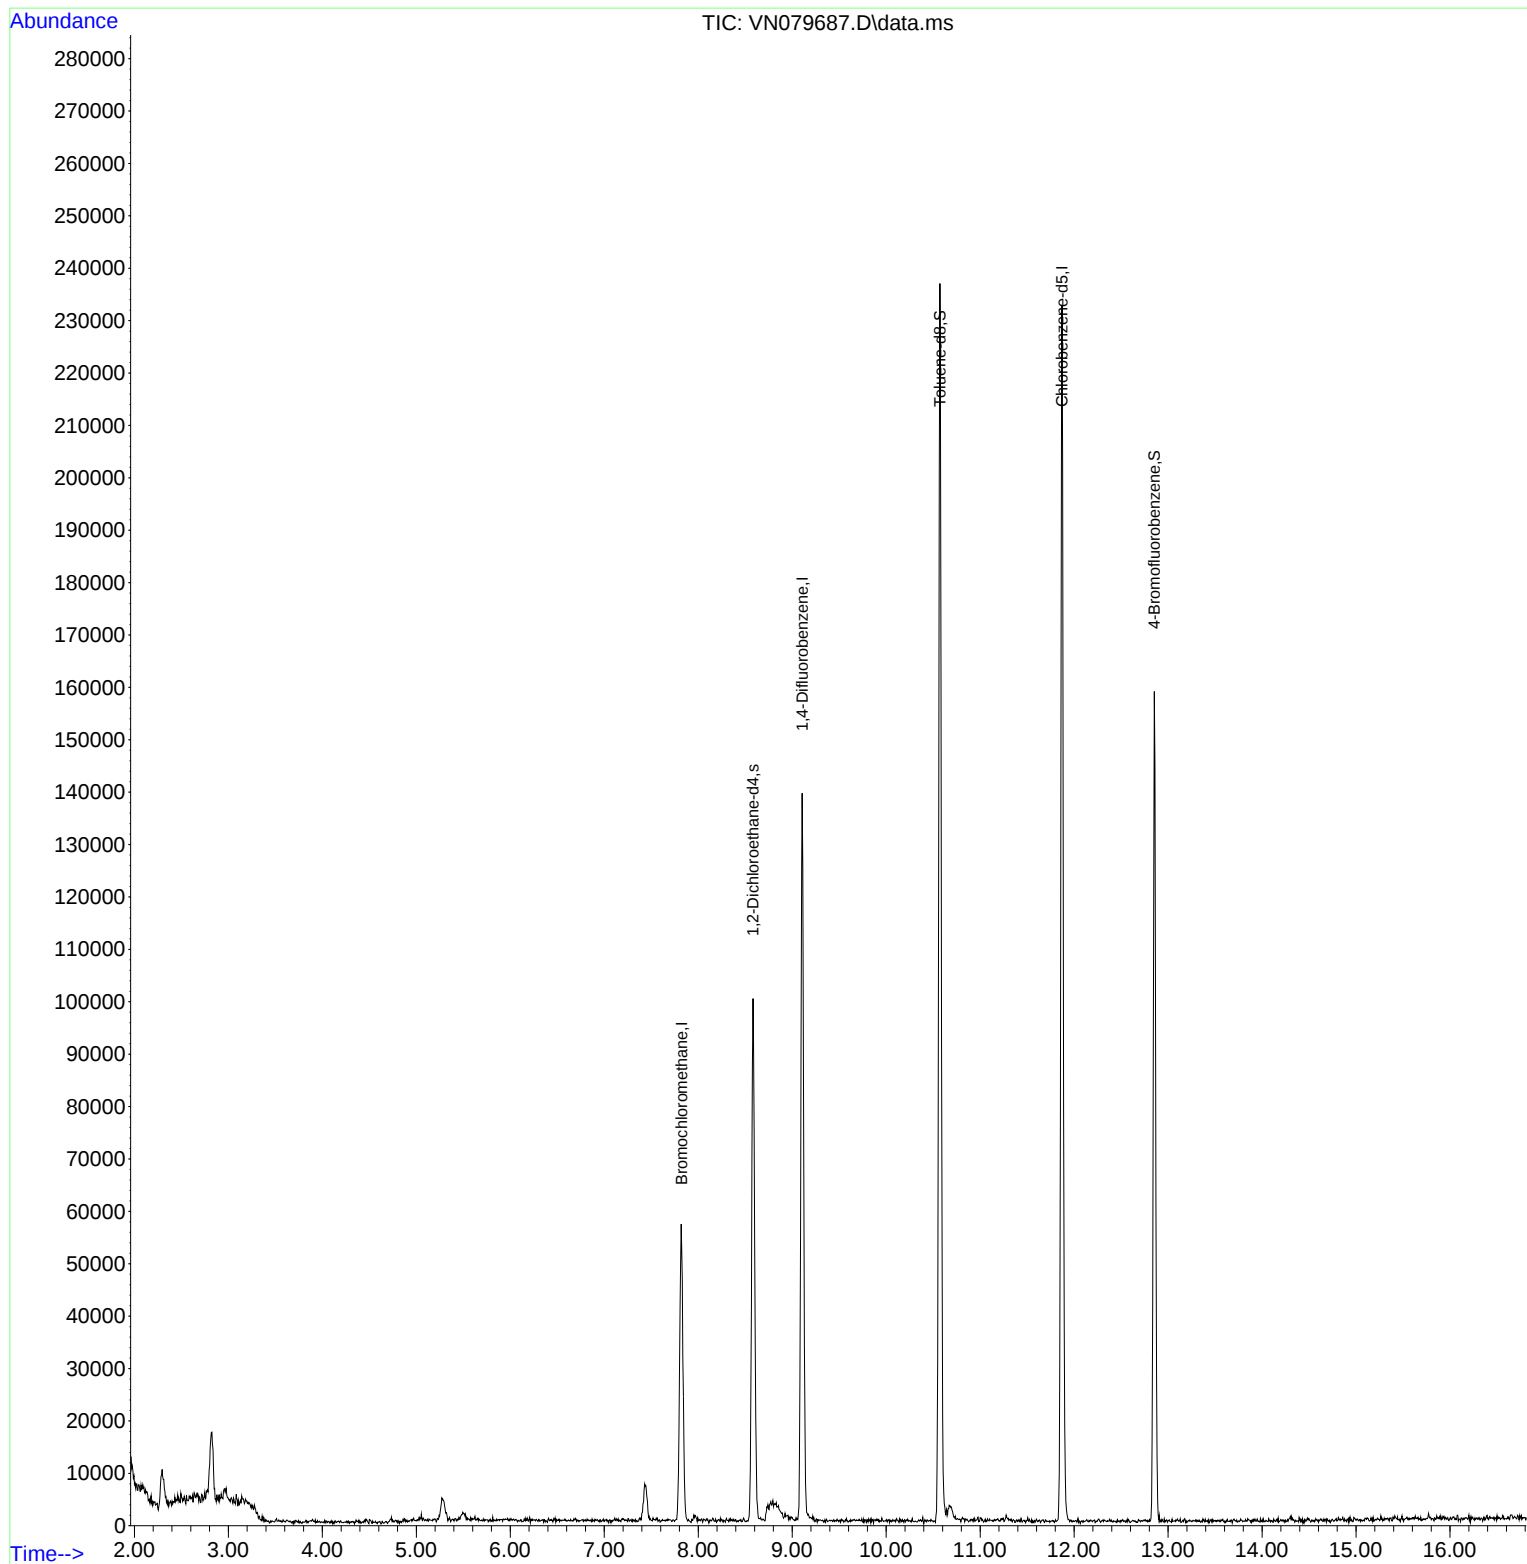


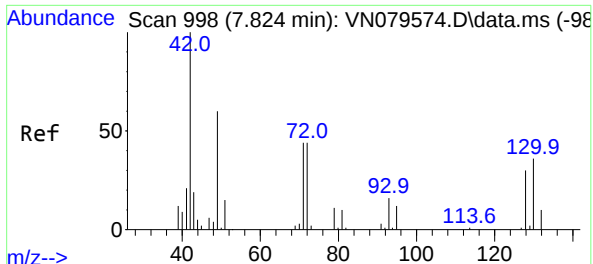

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.824 min Scan# 998
Delta R.T. -0.000 min
Lab File: VN079687.D
Acq: 25 Oct 2023 17:25




Instrument :
MSVOA_N
ClientSampleId :
14B-1RE


Tgt Ion:128 Resp: 18041
Ion Ratio Lower Upper
128 100
49 190.7 0.0 468.5
130 129.7 0.0 320.7

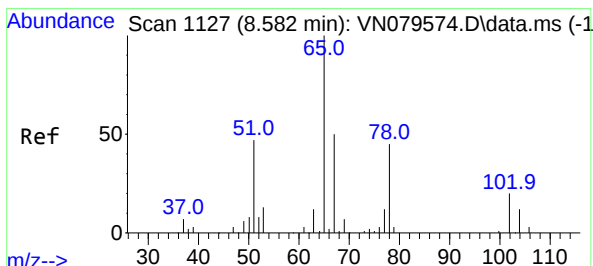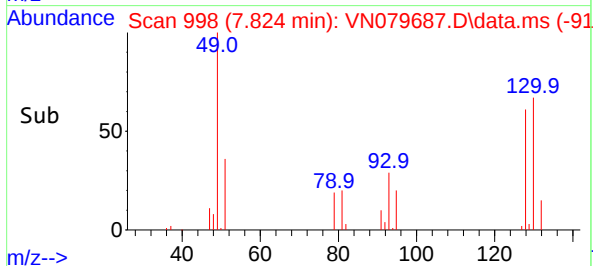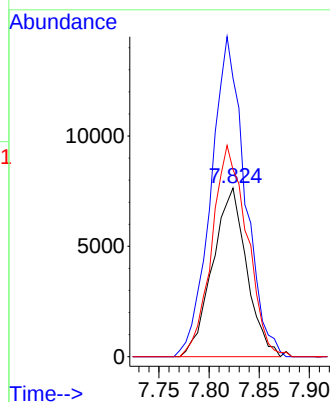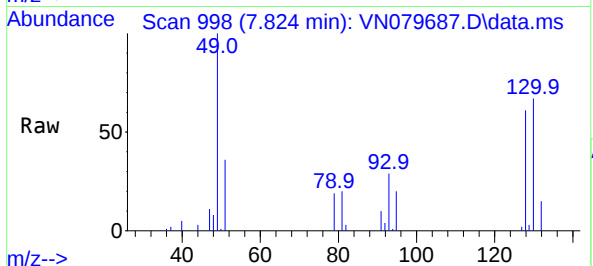

#27
1,2-Dichloroethane-d4
Concen: 30.830 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN079687.D
Acq: 25 Oct 2023 17:25

Tgt Ion: 65 Resp: 79080
Ion Ratio Lower Upper
65 100
67 51.4 42.1 63.1

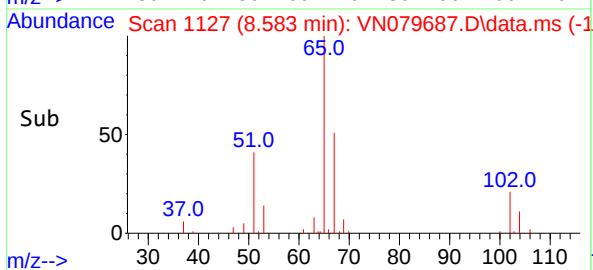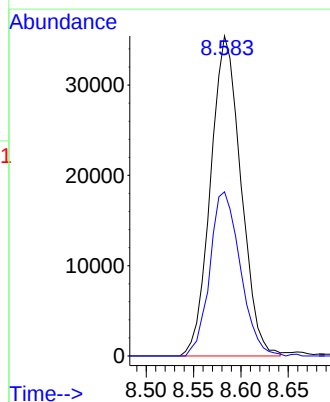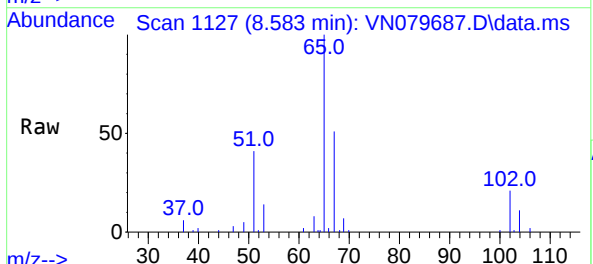

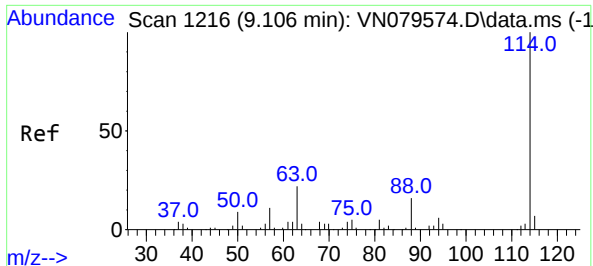

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN079687.D

Acq: 25 Oct 2023 17:25

Instrument :

MSVOA_N

ClientSampleId :

14B-1RE





Tgt Ion:114 Resp: 112470

Ion Ratio Lower Upper

114 100

63 22.8 18.1 27.1

88 14.8 12.2 18.2

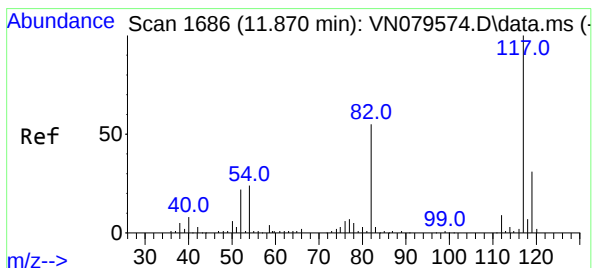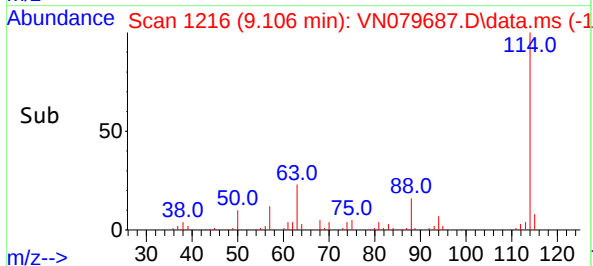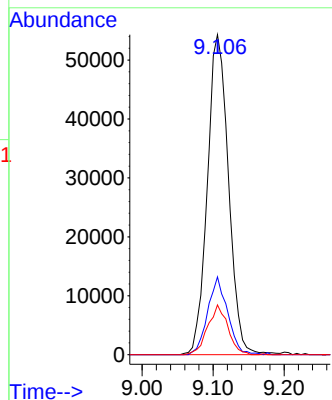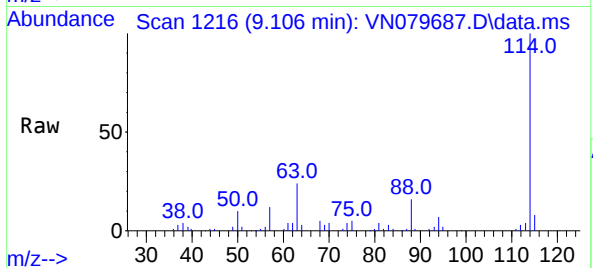

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.871 min Scan# 1686

Delta R.T. 0.000 min

Lab File: VN079687.D

Acq: 25 Oct 2023 17:25




Tgt Ion:117 Resp: 131662


Ion Ratio Lower Upper

117 100

82 58.8 46.2 69.2

119 33.6 25.2 37.8


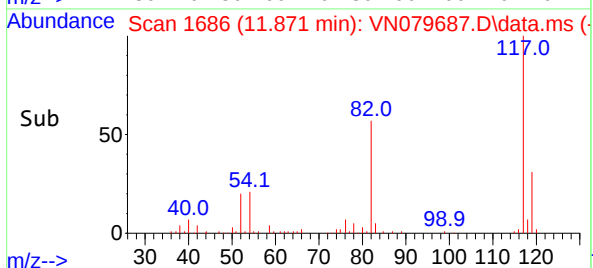
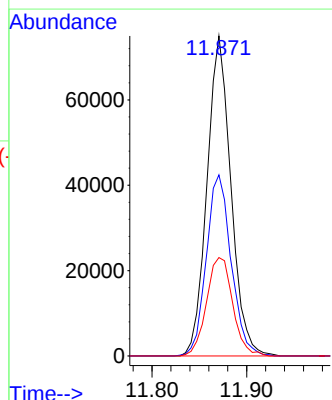
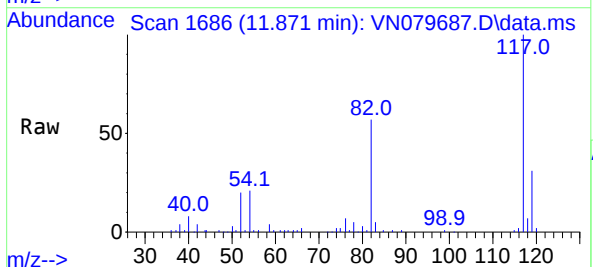


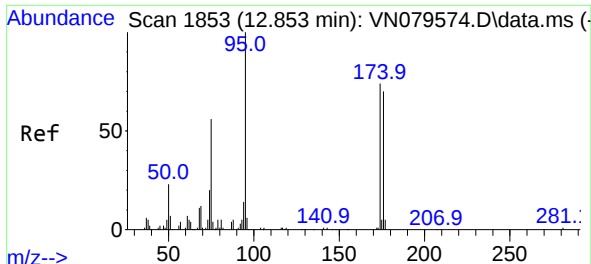

#60
4-Bromofluorobenzene
Concen: 21.794 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079687.D
Acq: 25 Oct 2023 17:25

Instrument :
MSVOA_N
ClientSampleId :
14B-1RE

Tgt Ion: 95 Resp: 52473
Ion Ratio Lower Upper
95 100
174 78.0 60.5 90.7
176 74.0 57.2 85.8

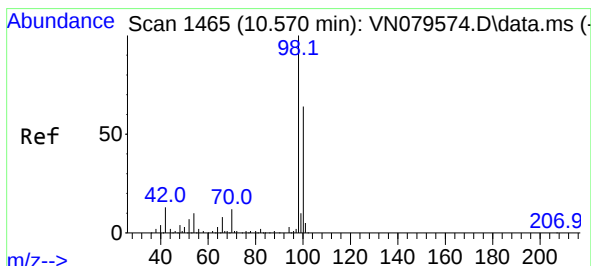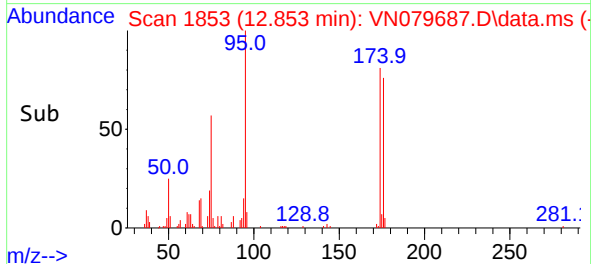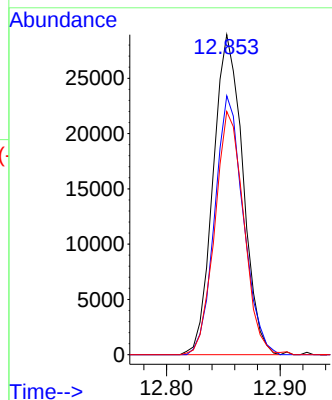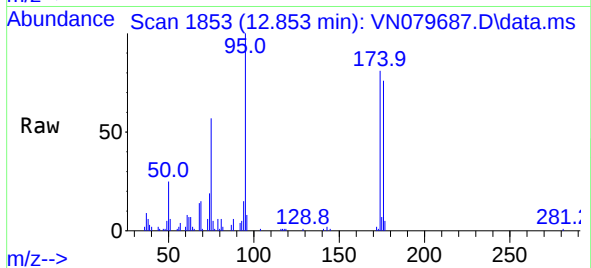

#63
Toluene-d8
Concen: 28.890 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079687.D
Acq: 25 Oct 2023 17:25

Tgt Ion: 98 Resp: 162993
Ion Ratio Lower Upper
98 100
100 63.4 51.6 77.4

