


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102523\
Data File : VN079671.D
Acq On : 25 Oct 2023 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N101723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Oct 18 02:19:15 2023

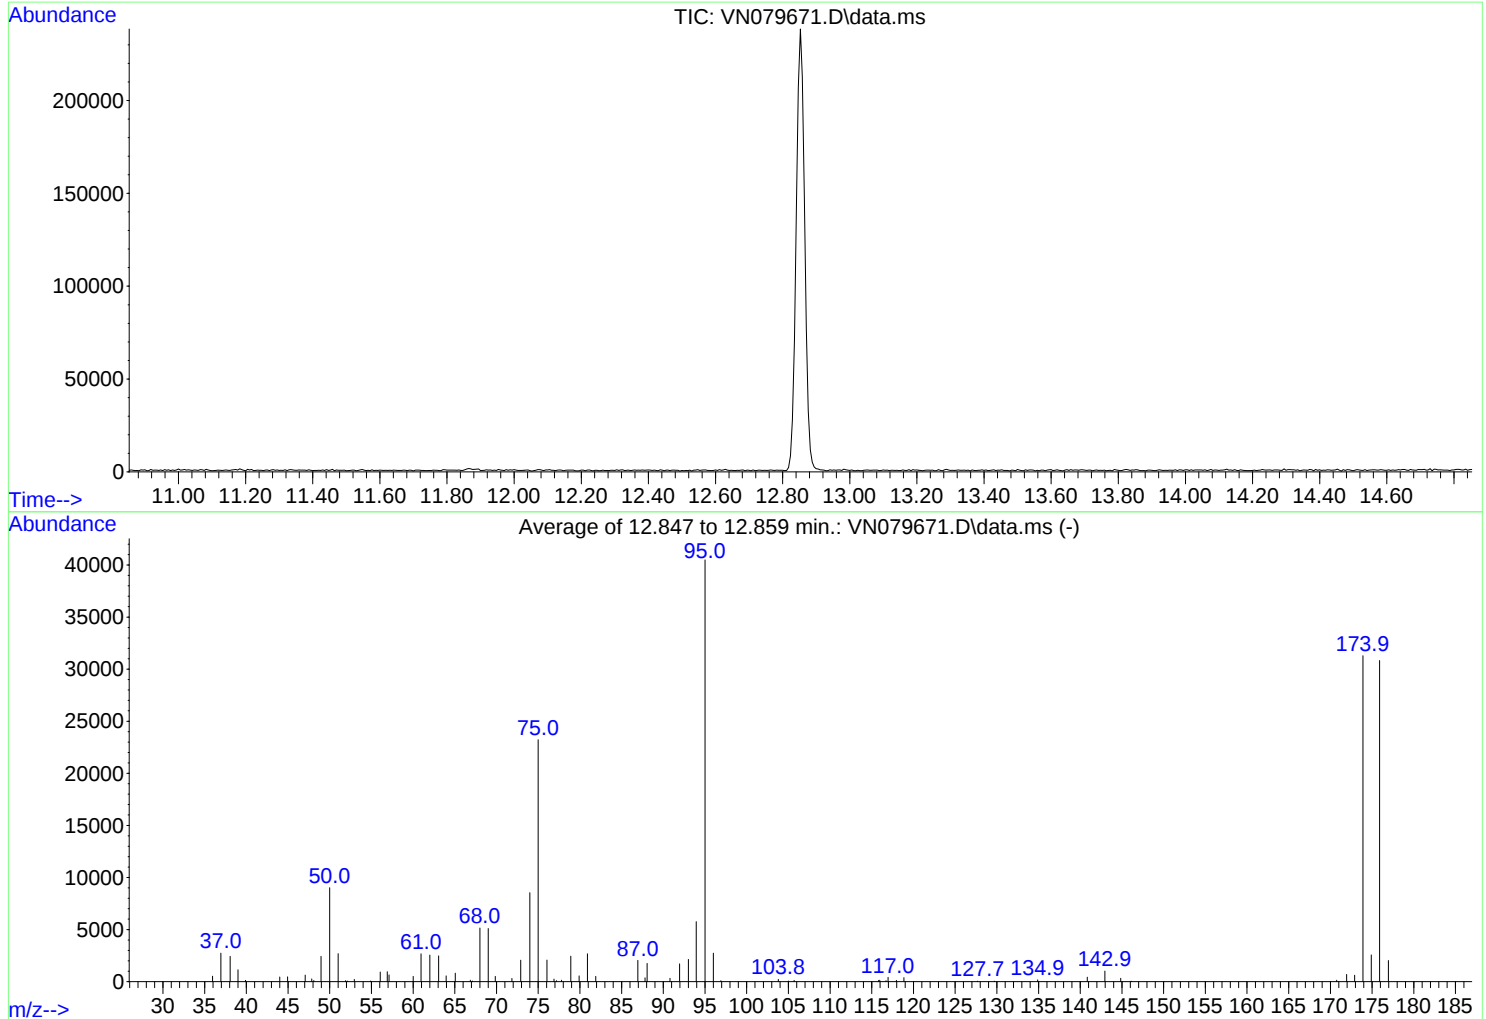

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	9013	PASS
75	95	30	60	57.4	23227	PASS
95	95	100	100	100.0	40496	PASS
96	95	5	9	6.8	2734	PASS
173	174	0.00	2	2.0	611	PASS
174	95	50	100	77.3	31299	PASS
175	174	5	9	8.2	2570	PASS
176	174	95	101	98.5	30832	PASS
177	176	5	9	6.6	2030	PASS