


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102619\
 Data File : VN058972.D
 Acq On : 25 Oct 2019 8:05
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
 Title : SW846 8260
 Last Update : Sat Oct 19 00:16:20 2019

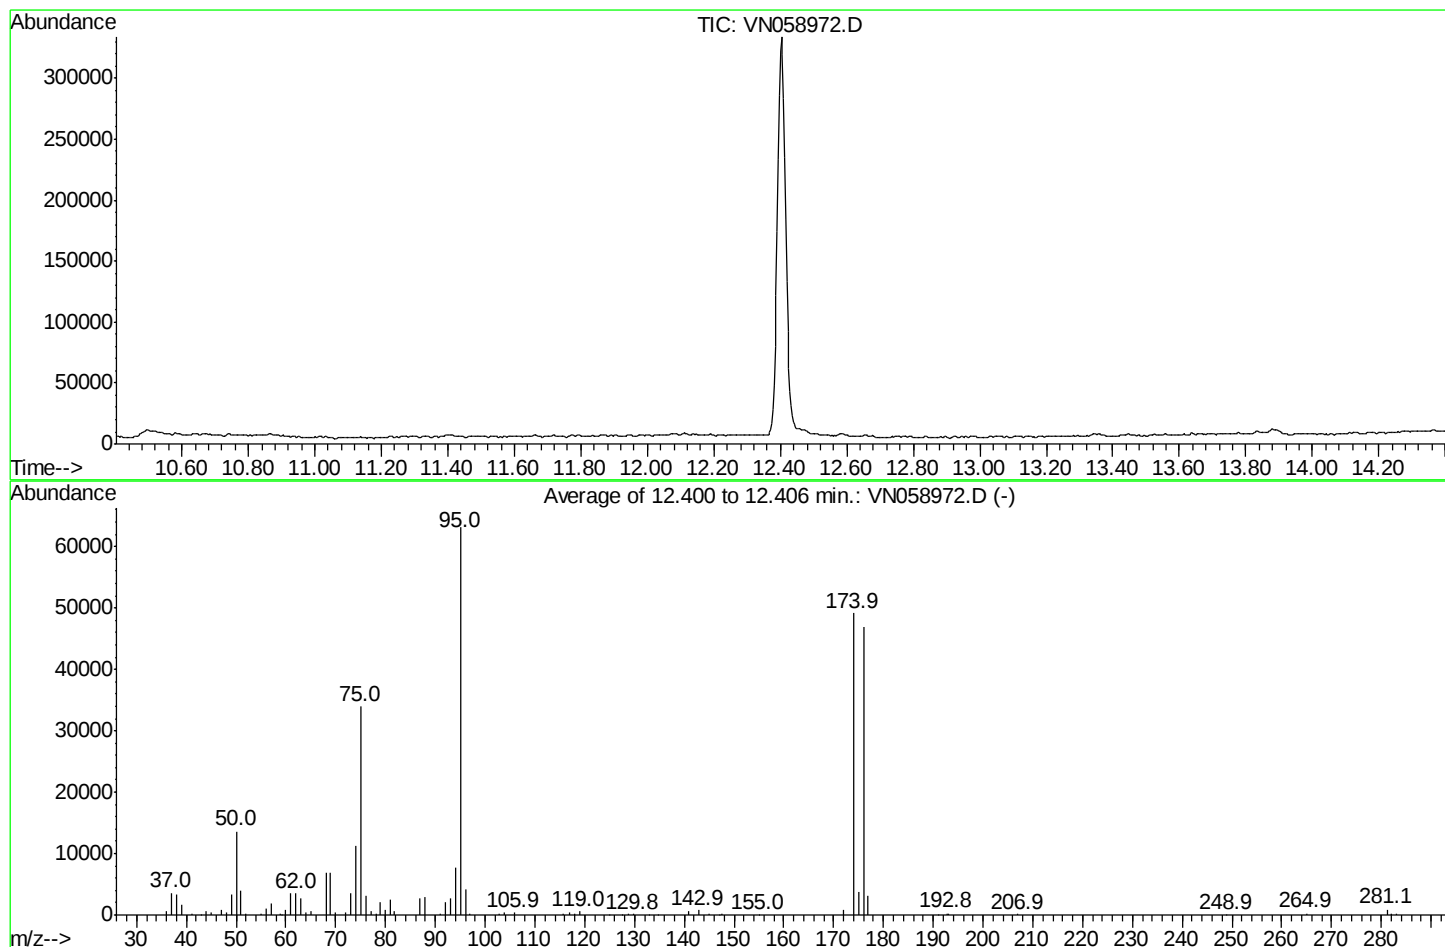

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	13601	PASS
75	95	30	60	53.8	33954	PASS
95	95	100	100	100.0	63130	PASS
96	95	5	9	6.8	4273	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.8	49106	PASS
175	174	5	9	7.5	3672	PASS
176	174	95	101	95.5	46917	PASS
177	176	5	9	6.6	3114	PASS