


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102620\
 Data File : VN064303.D
 Acq On : 26 Oct 2020 14:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N102620W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Oct 26 17:44:53 2020

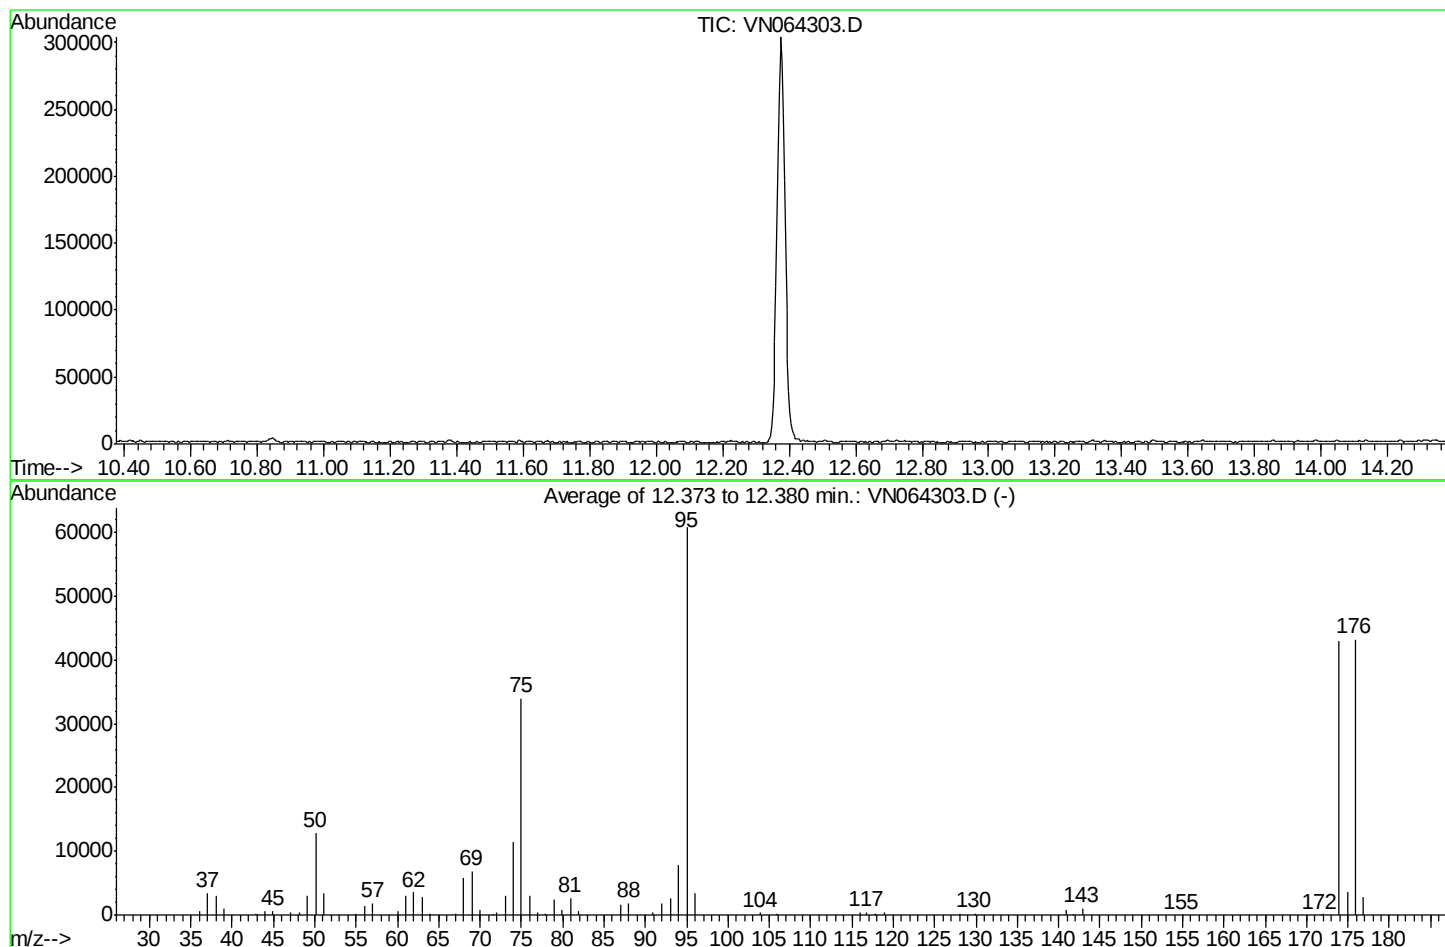

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	12901	PASS
75	95	30	60	55.8	33957	PASS
95	95	100	100	100.0	60840	PASS
96	95	5	9	5.6	3382	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.6	42952	PASS
175	174	5	9	8.3	3577	PASS
176	174	95	101	100.7	43234	PASS
177	176	5	9	6.7	2880	PASS