

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
 Data File : VN069163.D
 Acq On : 25 Oct 2021 20:15
 Operator : JC/MD
 Sample : M4307-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 26 01:36:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.088	168	344968	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	606871	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	580937	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	221003	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	225074	49.485	ug/l	0.00
Spiked Amount	50.000	Range 61 - 141	Recovery	=	98.980%	
35) Dibromofluoromethane	8.024	113	176834	50.083	ug/l	0.00
Spiked Amount	50.000	Range 69 - 133	Recovery	=	100.160%	
50) Toluene-d8	10.443	98	748575	52.987	ug/l	0.00
Spiked Amount	50.000	Range 65 - 126	Recovery	=	105.980%	
62) 4-Bromofluorobenzene	12.733	95	271895	51.011	ug/l	0.00
Spiked Amount	50.000	Range 58 - 135	Recovery	=	102.020%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.309	50	1224	0.290	ug/l	93
4) Vinyl Chloride	2.443	62	867	0.202	ug/l #	43
6) Chloroethane	3.030	64	5045	1.999	ug/l	100
11) Tert butyl alcohol	5.369	59	854	1.028	ug/l #	72
16) Acetone	4.299	43	8087	4.765	ug/l	95
20) Methylene Chloride	5.101	84	2585	0.662	ug/l	99
24) 1,1-Dichloroethane	6.393	63	2859	0.423	ug/l #	83
25) 2-Butanone	7.316	43	1209	0.471	ug/l #	48
29) Tetrahydrofuran	7.707	42	342	0.205	ug/l #	50
30) Chloroform	7.817	83	1464	0.206	ug/l	94
31) Cyclohexane	8.086	56	8234	1.164	ug/l #	29
36) 1,1-Dichloropropene	8.088	75	28822	5.560	ug/l #	50
38) Carbon Tetrachloride	8.088	117	36342	6.384	ug/l #	15
42) 1,2-Dichloroethane	8.536	62	3515	0.629	ug/l #	76
49) 1,4-Dioxane	9.577	88	27	35.935	ug/l #	68
51) 4-Methyl-2-Pentanone	10.336	43	2131	0.389	ug/l #	78
55) 1,1,2-Trichloroethane	10.896	97	1591	0.397	ug/l	93
57) 1,3-Dichloropropane	11.044	76	1740	0.264	ug/l #	78
59) 2-Hexanone	11.092	43	4594	1.170	ug/l	84
68) m/p-Xylenes	11.953	106	1706	0.220	ug/l	97
74) N-amyl acetate	12.393	43	2768	0.397	ug/l #	87
76) 1,2,3-Trichloropropane	12.733	75	144389	30.706	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	144389	73.462	ug/l #	12
87) 1,3-Dichlorobenzene	13.619	146	1546	0.220	ug/l	94
88) 1,4-Dichlorobenzene	13.619	146	1546	0.221	ug/l	93
89) n-Butylbenzene	13.946	91	3766	0.305	ug/l	91
91) 1,2-Dichlorobenzene	13.986	146	1805	0.264	ug/l	93
92) 1,2-Dibromo-3-Chloropr...	14.611	75	267	0.260	ug/l	76
93) 1,2,4-Trichlorobenzene	15.263	180	2937	3.352	ug/l #	81
95) Naphthalene	15.509	128	15557	5.213	ug/l	99
96) 1,2,3-Trichlorobenzene	15.708	180	3331	3.409	ug/l #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
Data File : VN069163.D
Acq On : 25 Oct 2021 20:15
Operator : JC/MD
Sample : M4307-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Oct 26 01:36:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration

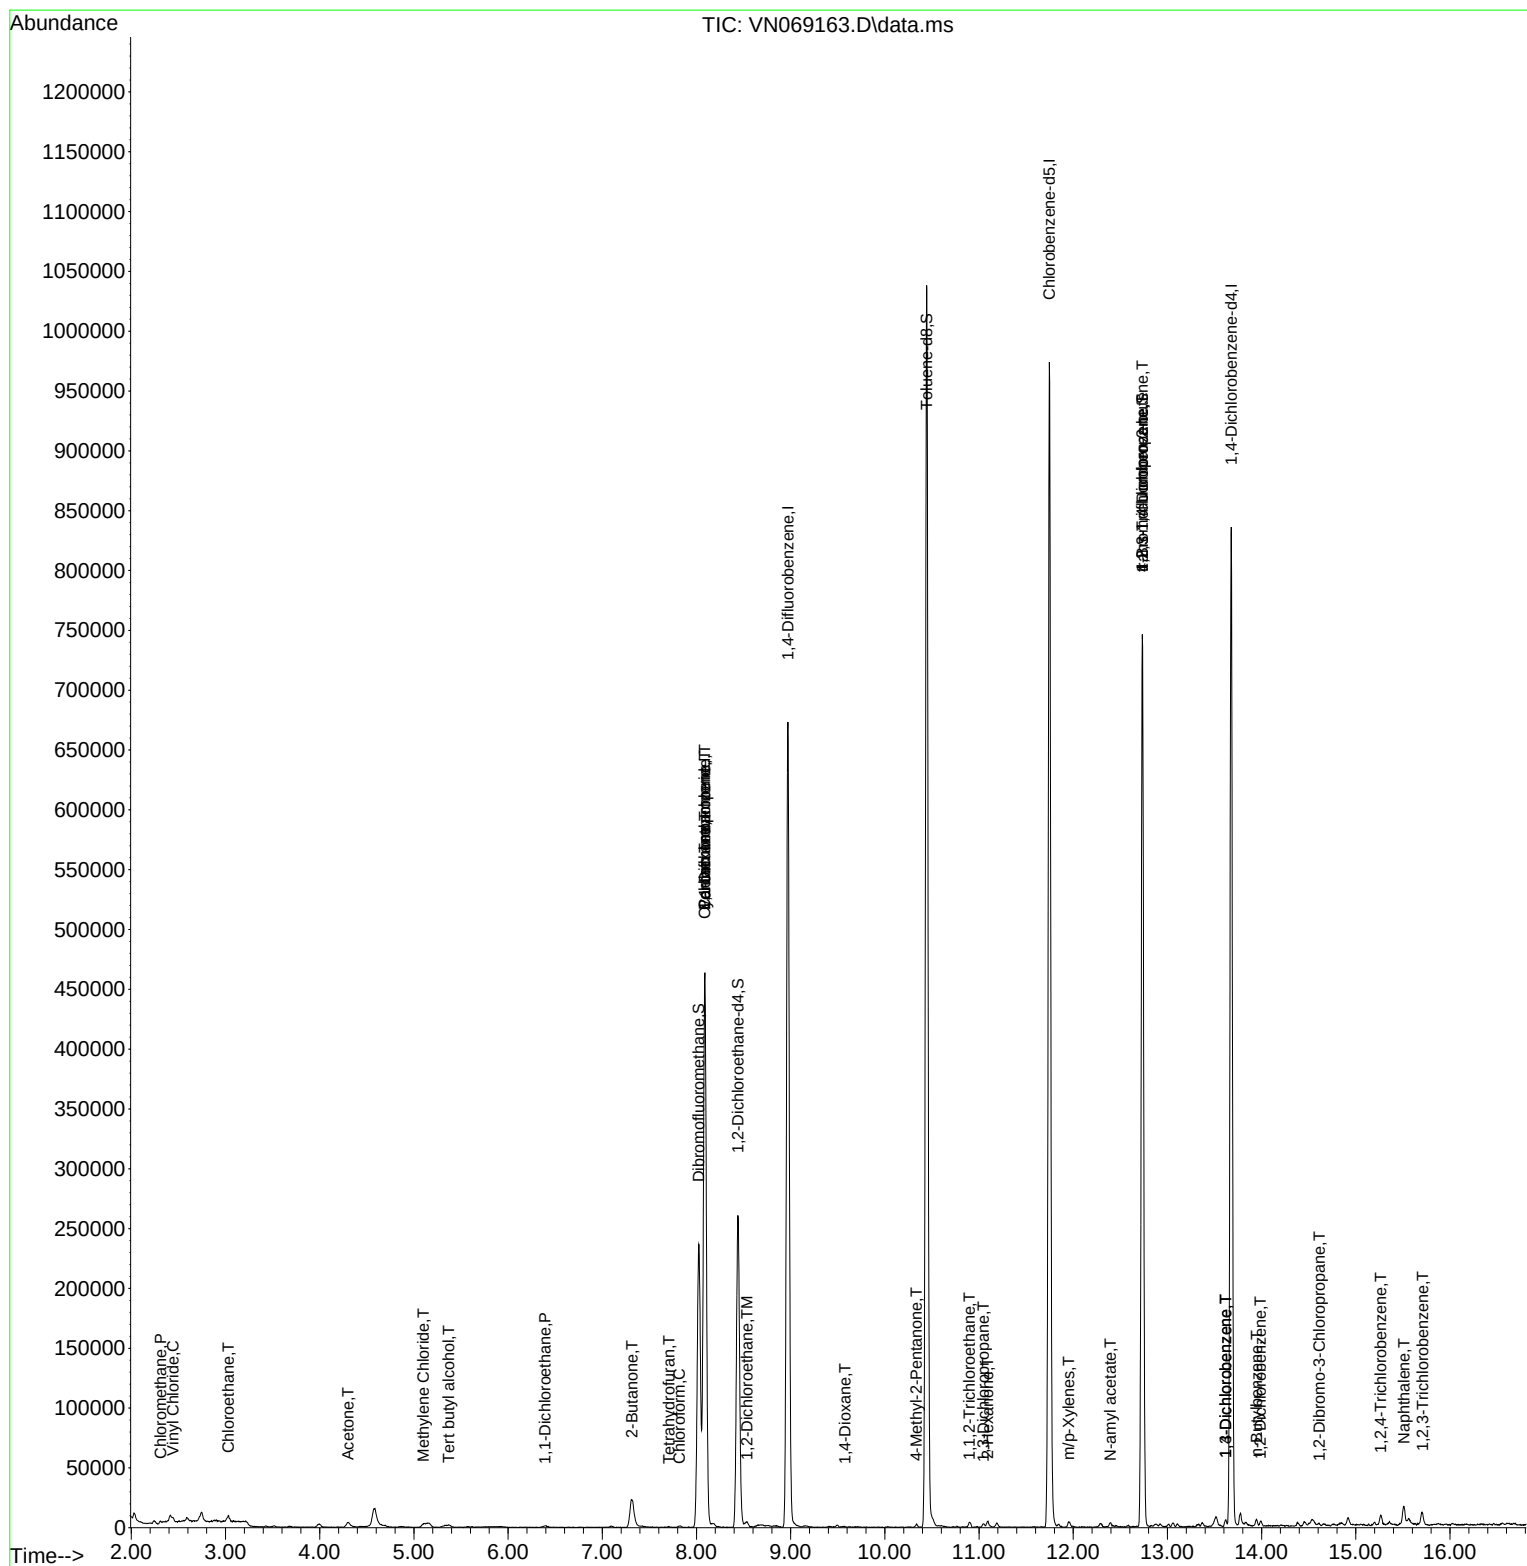



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN069163.D





Acq: 25 Oct 2021 20:15

Tgt Ion:168 Resp: 344968

Ion Ratio Lower Upper

168 100

99 62.6 48.9 73.3

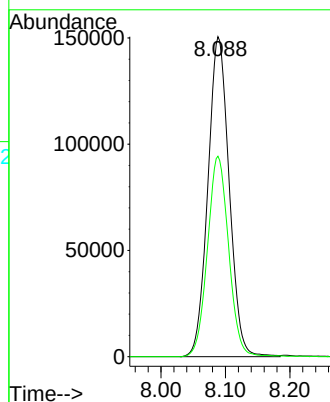

#3

Chloromethane

Concen: 0.290 ug/l

RT: 2.309 min Scan# 119

Delta R.T. 0.008 min

Lab File: VN069163.D




Acq: 25 Oct 2021 20:15


Tgt Ion: 50 Resp: 1224

Ion Ratio Lower Upper

50 100

52 28.8 26.3 39.5



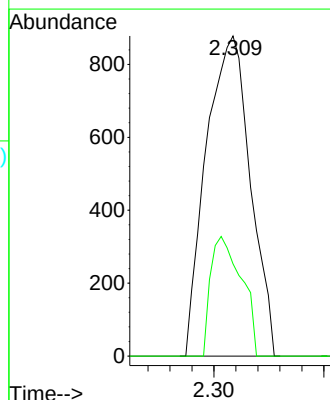
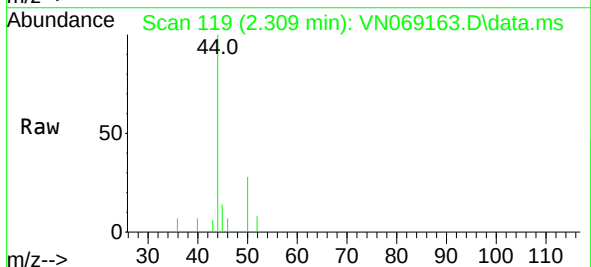


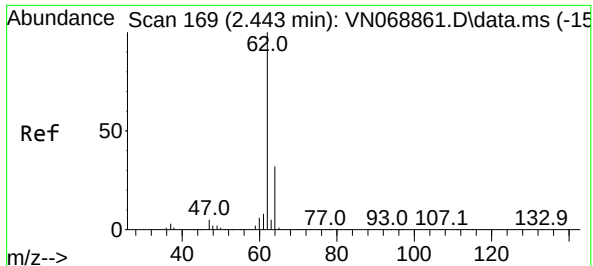

#4
 Vinyl Chloride
 Concen: 0.202 ug/l
 RT: 2.443 min Scan# 169
 Delta R.T. 0.000 min
 Lab File: VN069163.D
 Acq: 25 Oct 2021 20:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 62 Resp: 867
 Ion Ratio Lower Upper
 62 100
 64 0.0 25.7 38.5#

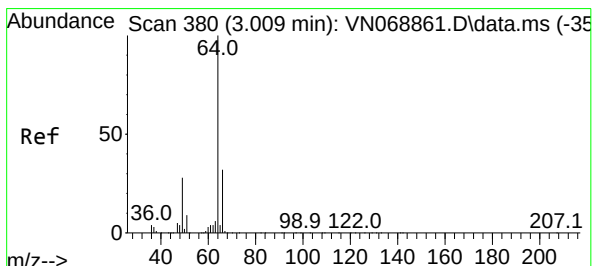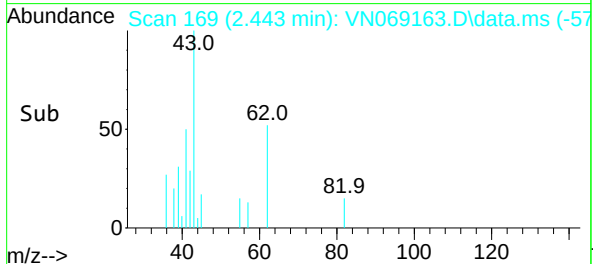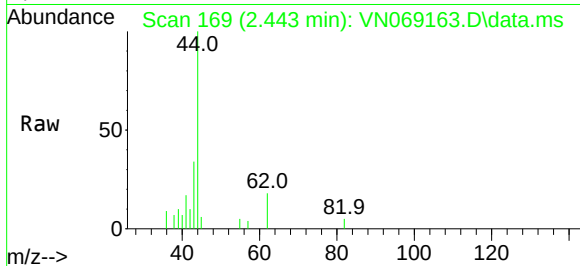

#6
 Chloroethane
 Concen: 1.999 ug/l
 RT: 3.030 min Scan# 388
 Delta R.T. 0.021 min
 Lab File: VN069163.D
 Acq: 25 Oct 2021 20:15

Tgt Ion: 64 Resp: 5045
 Ion Ratio Lower Upper
 64 100
 66 31.9 25.6 38.4

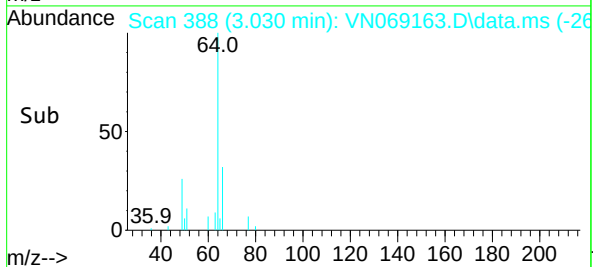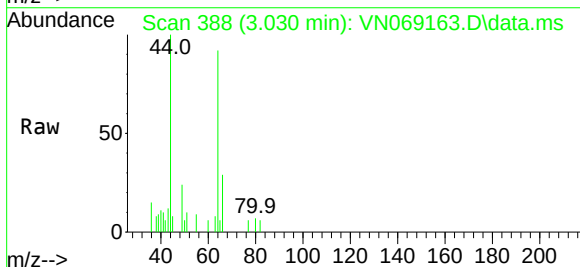




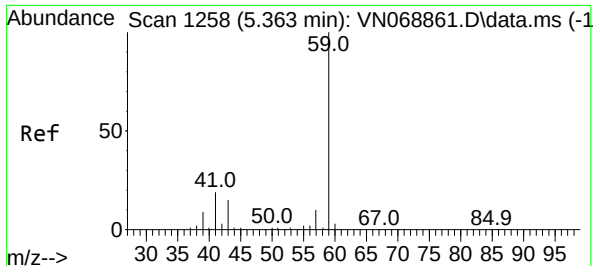


#11

Tert butyl alcohol
Concen: 1.028 ug/l
RT: 5.369 min Scan# 1260
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 854
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

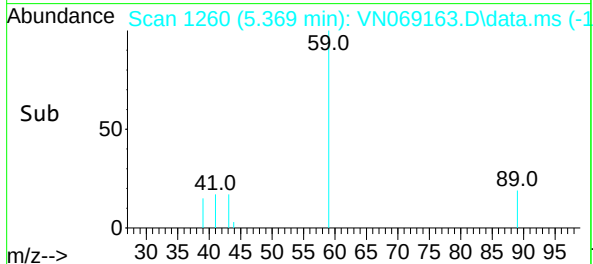


#16

Acetone
Concen: 4.765 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.013 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15


Tgt Ion: 43 Resp: 8087
Ion Ratio Lower Upper
43 100
58 33.6 24.5 36.7

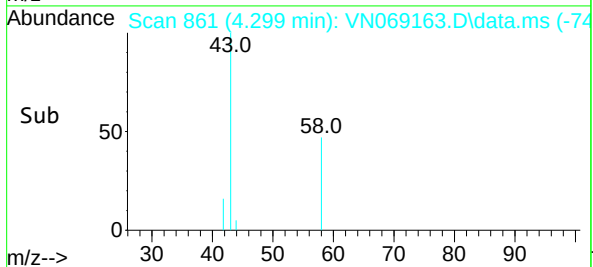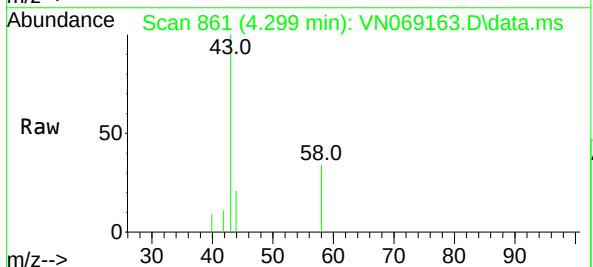






#20
Methylene Chloride
Concen: 0.662 ug/l
RT: 5.101 min Scan# 1160
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Instrument :
MSVOA_N
ClientSampled :



Tgt Ion: 84 Resp: 2585




Ion	Ratio	Lower	Upper
84	100		
49	122.3	97.6	146.4
51	36.1	30.3	45.5
86	64.7	51.8	77.6

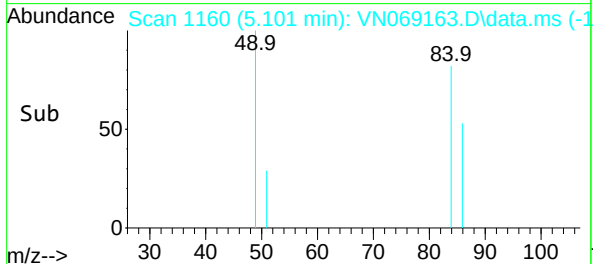


#24
1,1-Dichloroethane
Concen: 0.423 ug/l
RT: 6.393 min Scan# 1642
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 63 Resp: 2859

Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.5	10.4#
100	0.0	2.1	6.5#


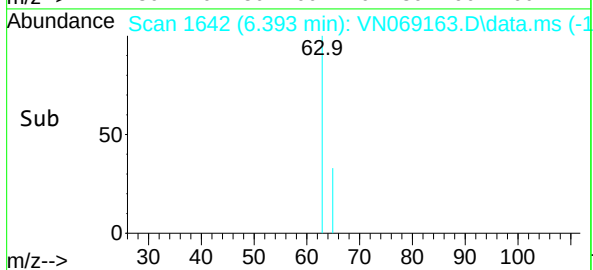

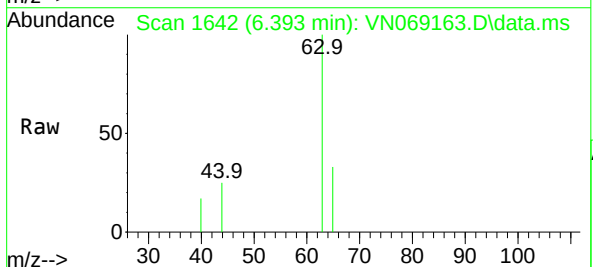




#25
2-Butanone
Concen: 0.471 ug/l
RT: 7.316 min Scan# 1986
Delta R.T. -0.016 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 1209
Ion Ratio Lower Upper
43 100
72 0.0 21.2 31.8#

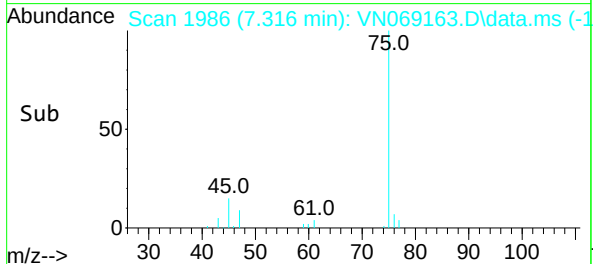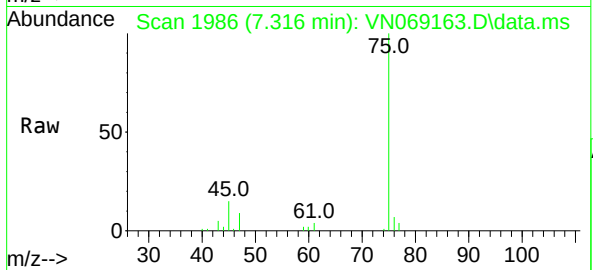

#29
Tetrahydrofuran
Concen: 0.205 ug/l
RT: 7.707 min Scan# 2132
Delta R.T. 0.024 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 42 Resp: 342
Ion Ratio Lower Upper
42 100
72 22.5 35.4 53.2#
71 0.0 33.8 50.6#

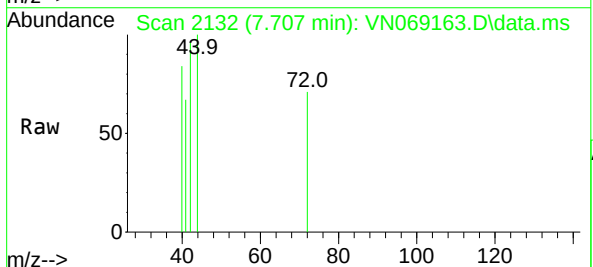



#30

Chloroform

Concen: 0.206 ug/l

RT: 7.817 min Scan# 2173

Delta R.T. 0.000 min

Lab File: VN069163.D

Acq: 25 Oct 2021 20:15

Tgt Ion: 83 Resp: 1464

Ion Ratio Lower Upper





83 100

85 58.9 51.1 76.7

Instrument :

MSVOA_N

ClientSampled :

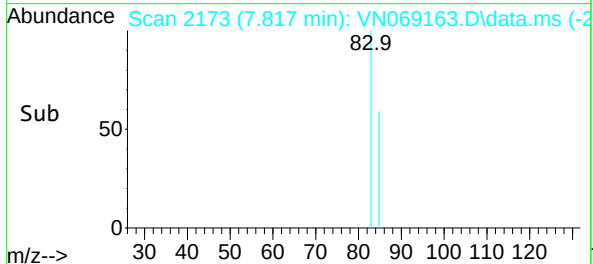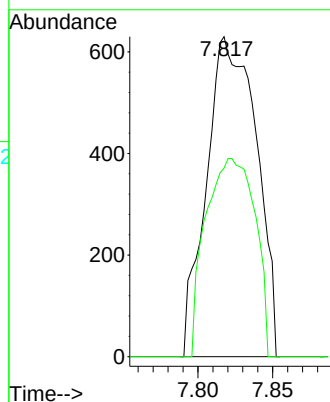

#31

Cyclohexane

Concen: 1.164 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.010 min

Lab File: VN069163.D

Acq: 25 Oct 2021 20:15




Tgt Ion: 56 Resp: 8234


Ion Ratio Lower Upper

56 100

69 142.5 26.9 40.3#

84 106.1 67.6 101.4#


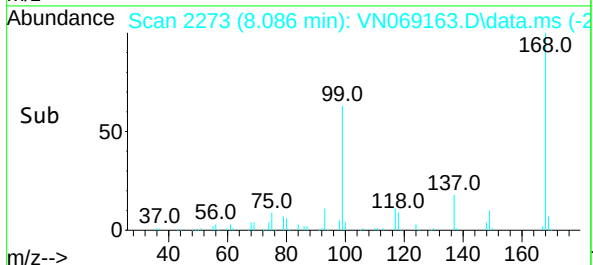
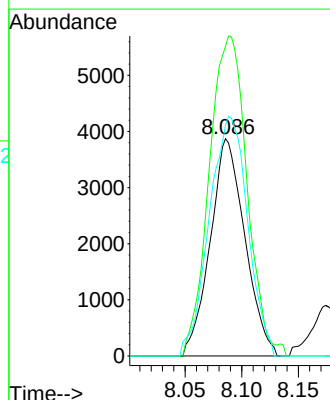
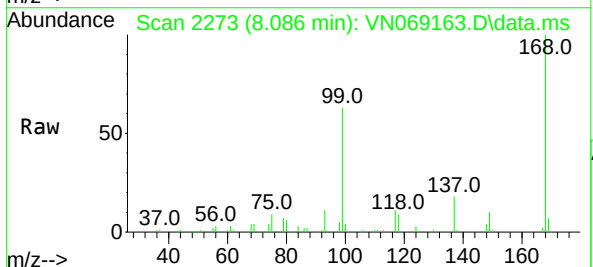




#33
 1,2-Dichloroethane-d4
 Concen: 49.485 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. 0.000 min
 Lab File: VN069163.D
 Acq: 25 Oct 2021 20:15




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 65 Resp: 225074
 Ion Ratio Lower Upper
 65 100
 67 52.2 0.0 103.8

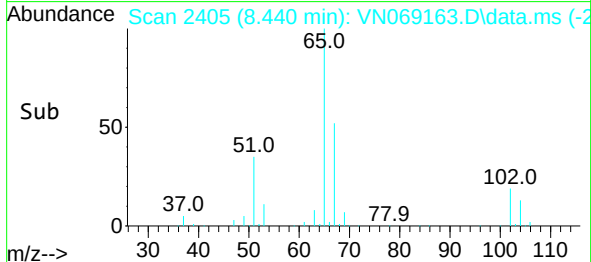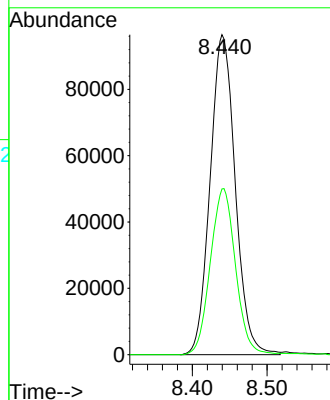

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.003 min
 Lab File: VN069163.D
 Acq: 25 Oct 2021 20:15

Tgt Ion: 114 Resp: 606871
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 42.6
 88 15.6 0.0 32.0



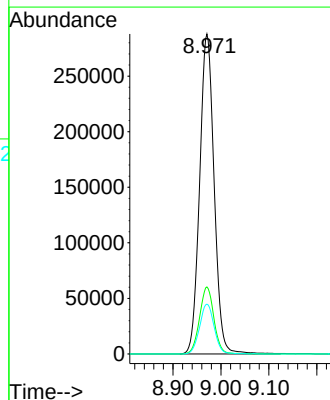





#35
Dibromofluoromethane
Concen: 50.083 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:113 Resp: 176834
Ion Ratio Lower Upper
113 100
111 102.6 83.2 124.8
192 17.9 15.0 22.4

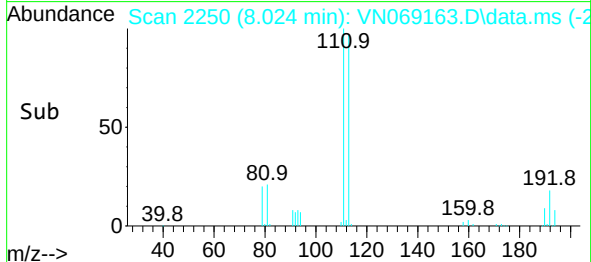

#36
1,1-Dichloropropene
Concen: 5.560 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15


Tgt Ion: 75 Resp: 28822
Ion Ratio Lower Upper
75 100
110 9.3 17.9 53.8#
77 0.0 24.7 37.1#

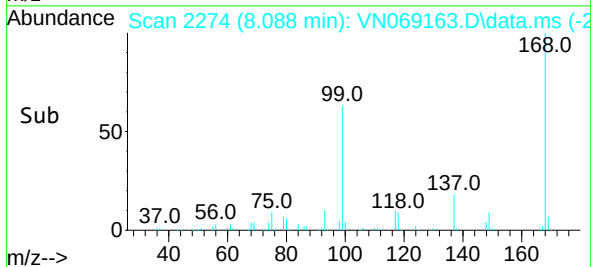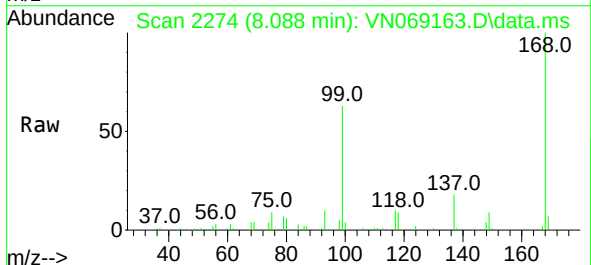






#38
Carbon Tetrachloride
Concen: 6.384 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:117 Resp: 36342
Ion Ratio Lower Upper
117 100
119 4.3 76.9 115.3#
121 0.0 24.6 37.0#



#42
1,2-Dichloroethane
Concen: 0.629 ug/l
RT: 8.536 min Scan# 2441
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 62 Resp: 3515
Ion Ratio Lower Upper
62 100
98 0.0 0.0 17.2


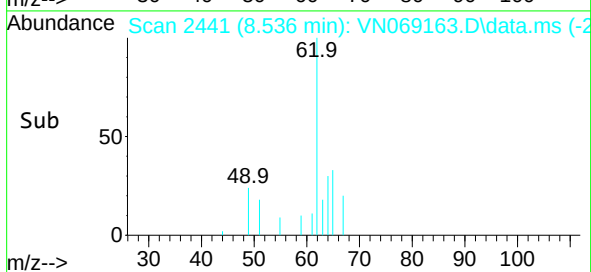






#49
1,4-Dioxane
Concen: 35.935 ug/l
RT: 9.577 min Scan# 2829
Delta R.T. 0.008 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 88 Resp: 27
Ion Ratio Lower Upper
88 100
43 0.0 24.9 37.3#
58 88.9 56.9 85.3#



#50
Toluene-d8
Concen: 52.987 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 98 Resp: 748575
Ion Ratio Lower Upper
98 100
100 64.3 51.5 77.3









#51
4-Methyl-2-Pentanone
Concen: 0.389 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2131
Ion Ratio Lower Upper
43 100
58 25.4 31.0 46.4#



#55
1,1,2-Trichloroethane
Concen: 0.397 ug/l
RT: 10.896 min Scan# 3321
Delta R.T. -0.003 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 97 Resp: 1591
Ion Ratio Lower Upper
97 100
83 80.0 70.5 105.7
85 50.2 45.3 67.9
99 60.8 50.7 76.1




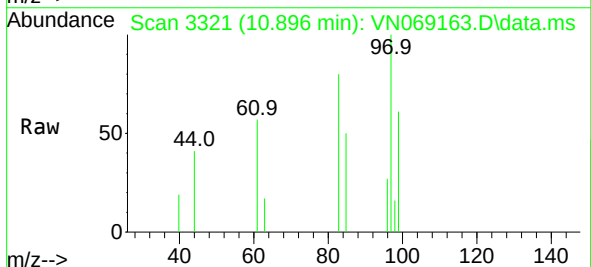




#57
1,3-Dichloropropane
Concen: 0.264 ug/l
RT: 11.044 min Scan# 3376
Delta R.T. -0.003 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 1740
Ion Ratio Lower Upper
76 100
78 19.8 25.8 38.8#

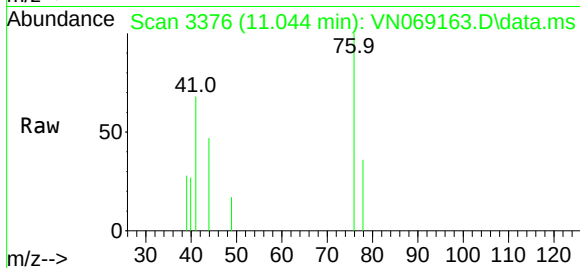

#59
2-Hexanone
Concen: 1.170 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 43 Resp: 4594
Ion Ratio Lower Upper
43 100
58 42.1 26.9 80.7




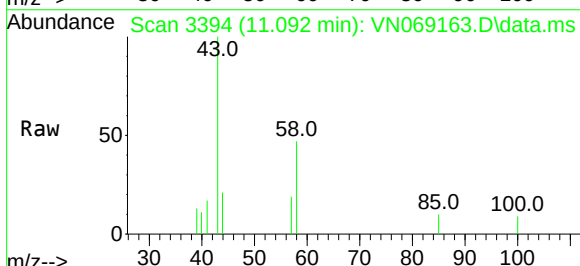




#62
4-Bromofluorobenzene
Concen: 51.011 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 271895
Ion Ratio Lower Upper
95 100
174 75.4 0.0 144.8
176 71.1 0.0 140.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 117 Resp: 580937
Ion Ratio Lower Upper
117 100
82 55.9 46.4 69.6
119 31.9 26.0 39.0




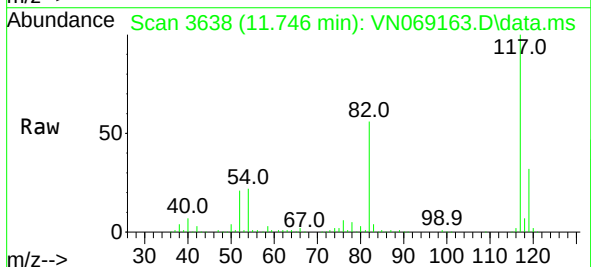




#68
m/p-Xylenes
Concen: 0.220 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. 0.000 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 1706
Ion Ratio Lower Upper
106 100
91 213.0 166.8 250.2



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion:152 Resp: 221003
Ion Ratio Lower Upper
152 100
115 64.1 31.4 94.3
150 159.1 0.0 351.0




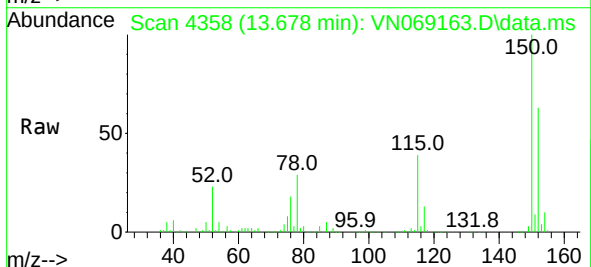




#74
N-amy1 acetate
Concen: 0.397 ug/l
RT: 12.393 min Scan# 3879
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43	Resp: 2768
Ion Ratio	Lower Upper
43 100	
70 38.0	32.2 48.2
55 31.4	18.0 27.0#
61 12.2	19.0 28.4#



#76
1,2,3-Trichloropropane
Concen: 30.706 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 75	Resp: 144389
Ion Ratio	Lower Upper
75 100	
77 1.1	96.2 288.4#




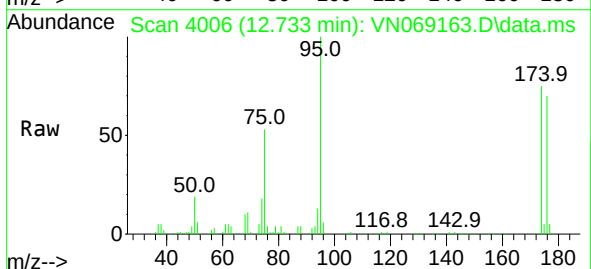




#81
trans-1,4-Dichloro-2-butene
Concen: 73.462 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 144389
Ion Ratio Lower Upper
75 100
53 0.0 75.4 113.2#
89 0.0 36.9 55.3#

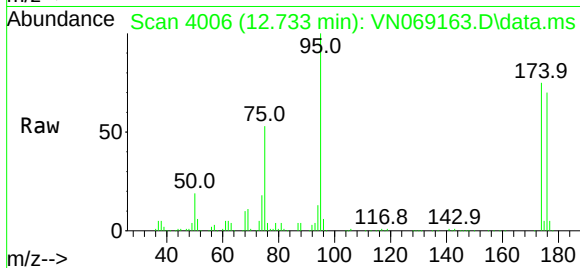

#87
1,3-Dichlorobenzene
Concen: 0.220 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. 0.000 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion:146 Resp: 1546
Ion Ratio Lower Upper
146 100
111 44.9 21.4 64.2
148 58.1 32.0 96.2


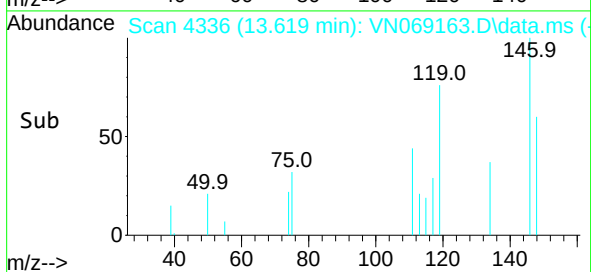

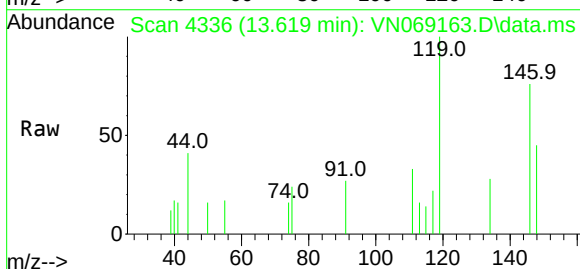




#88
1,4-Dichlorobenzene
Concen: 0.221 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. -0.078 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 1546
Ion Ratio Lower Upper
146 100
111 44.9 20.6 61.8
148 58.1 32.1 96.5



#89
n-Butylbenzene
Concen: 0.305 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.003 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 91 Resp: 3766
Ion Ratio Lower Upper
91 100
92 44.3 26.0 78.0
134 22.1 12.5 37.5









#91
1,2-Dichlorobenzene
Concen: 0.264 ug/l
RT: 13.986 min Scan# 4473
Delta R.T. -0.003 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 1805
Ion Ratio Lower Upper
146 100
111 53.4 22.0 66.0
148 65.3 32.1 96.5



#92
1,2-Dibromo-3-Chloropropane
Concen: 0.260 ug/l
RT: 14.611 min Scan# 4706
Delta R.T. 0.005 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15

Tgt Ion: 75 Resp: 267
Ion Ratio Lower Upper
75 100
155 41.6 38.8 116.4
157 89.9 50.2 150.6


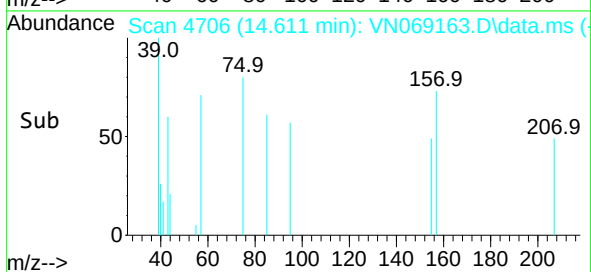




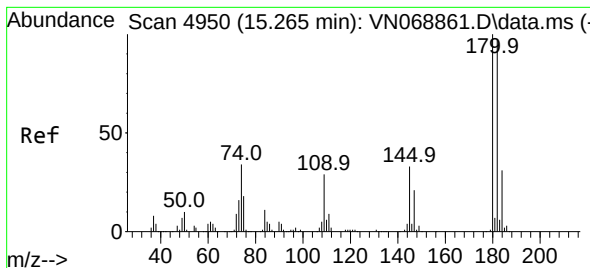

#93
1,2,4-Trichlorobenzene
Concen: 3.352 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.002 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:180 Resp: 2937
Ion Ratio Lower Upper
180 100
182 101.2 47.9 143.7
145 65.0 16.4 49.2#

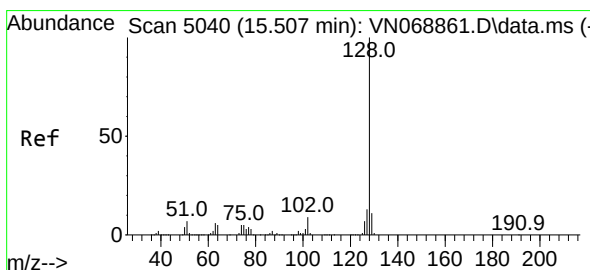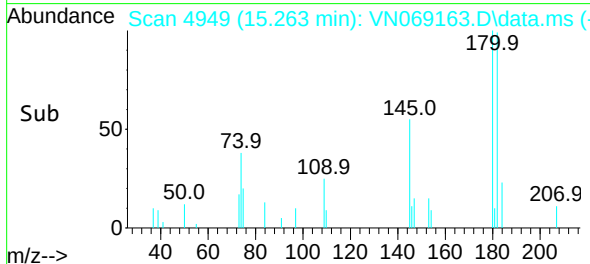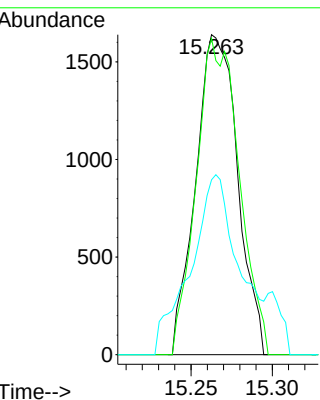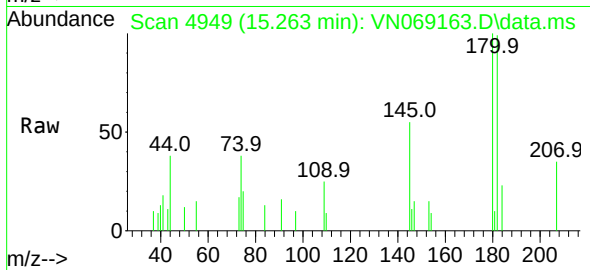

#95
Naphthalene
Concen: 5.213 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN069163.D
Acq: 25 Oct 2021 20:15


Tgt Ion:128 Resp: 15557
Ion Ratio Lower Upper
128 100
127 13.0 10.5 15.7
129 11.7 8.9 13.3

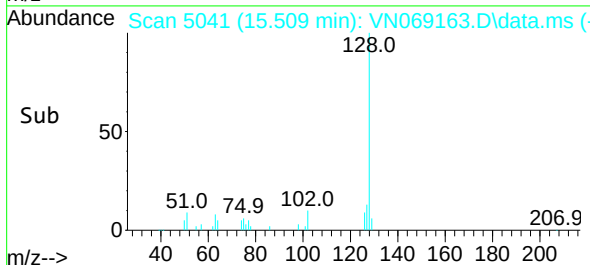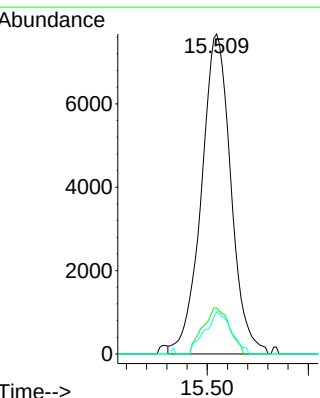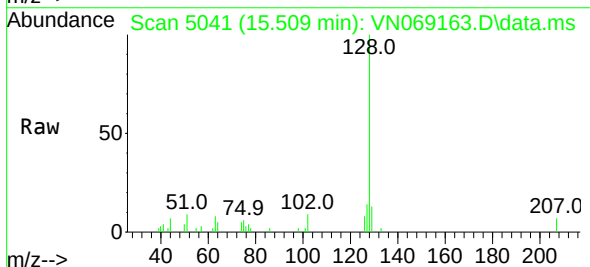



#96
 1,2,3-Trichlorobenzene
 Concen: 3.409 ug/l
 RT: 15.708 min Scan# 5115
 Delta R.T. 0.006 min
 Lab File: VN069163.D
 Acq: 25 Oct 2021 20:15

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:180 Resp: 3331
 Ion Ratio Lower Upper
 180 100
 182 98.7 48.1 144.3
 145 0.0 17.4 52.2#

