

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
 Data File : VN069155.D
 Acq On : 25 Oct 2021 16:45
 Operator : JC/MD
 Sample : VN1025WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1025WBL01

Quant Time: Oct 26 01:34:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.091	168	345560	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	601916	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	587235	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	212387	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	226038	49.612	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.220%
35) Dibromofluoromethane	8.024	113	176107	50.288	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.580%
50) Toluene-d8	10.443	98	756022	53.955	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.920%
62) 4-Bromofluorobenzene	12.733	95	263111	49.769	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	99.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
Data File : VN069155.D
Acq On : 25 Oct 2021 16:45
Operator : JC/MD
Sample : VN1025WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01

Quant Time: Oct 26 01:34:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration




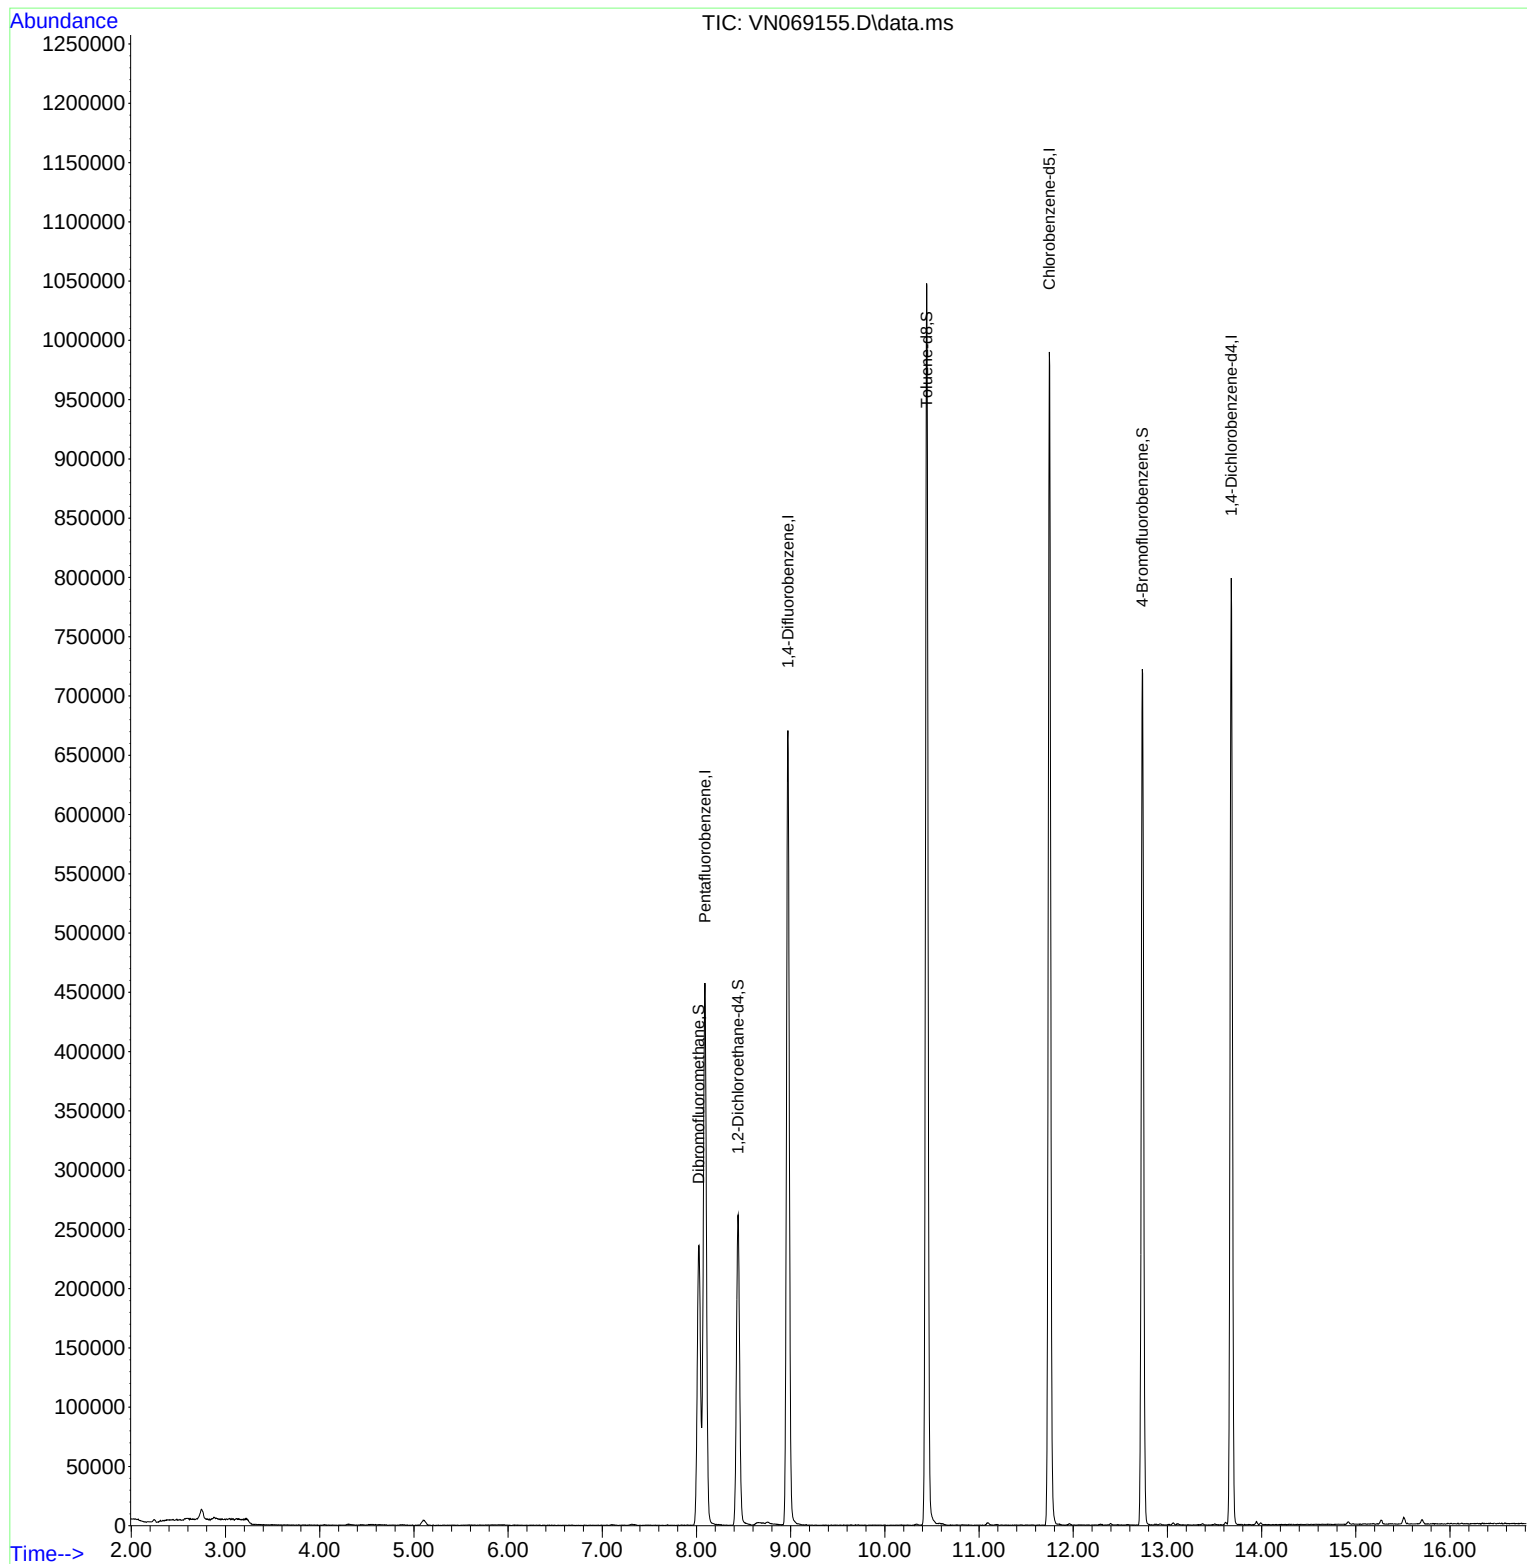


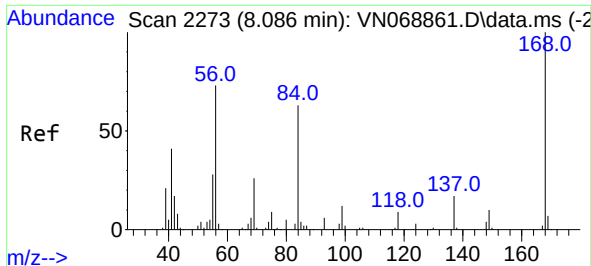

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. 0.005 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45




Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01


Tgt Ion:168 Resp: 345560
Ion Ratio Lower Upper
168 100
99 60.5 48.9 73.3

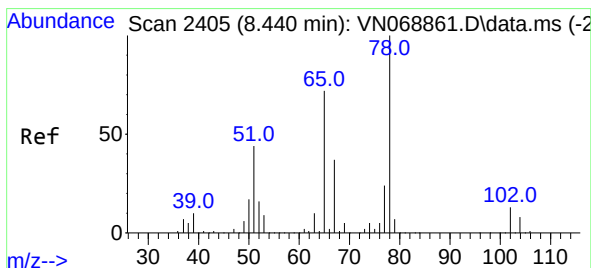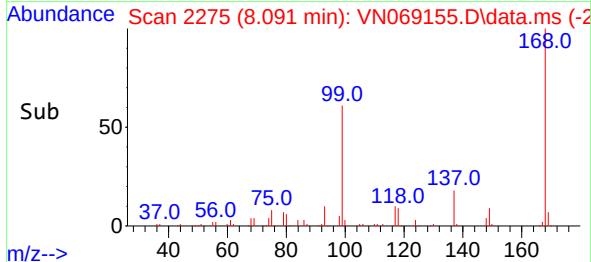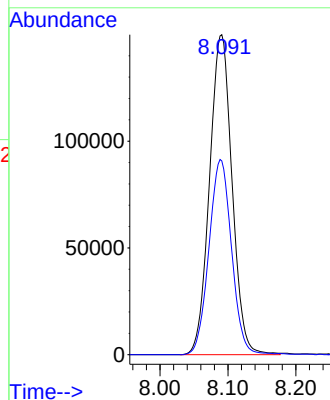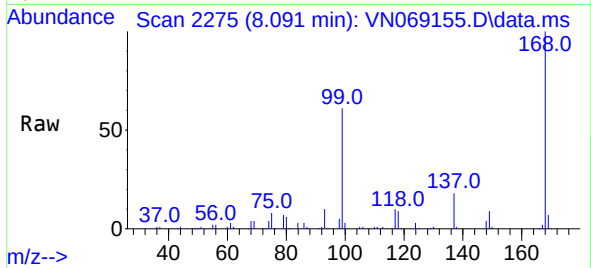

#33
1,2-Dichloroethane-d4
Concen: 49.612 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45

Tgt Ion: 65 Resp: 226038
Ion Ratio Lower Upper
65 100
67 51.6 0.0 103.8


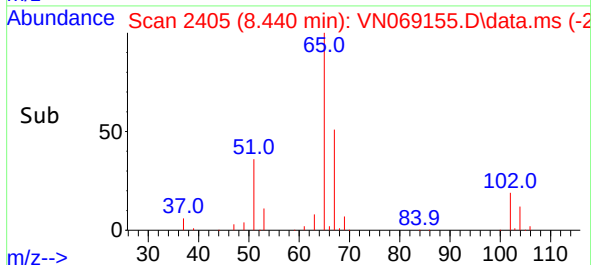
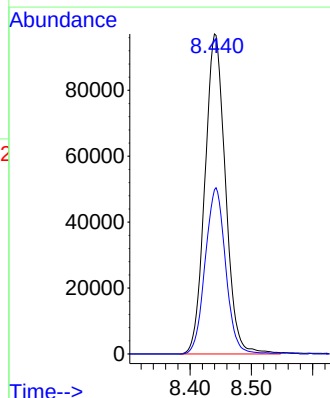
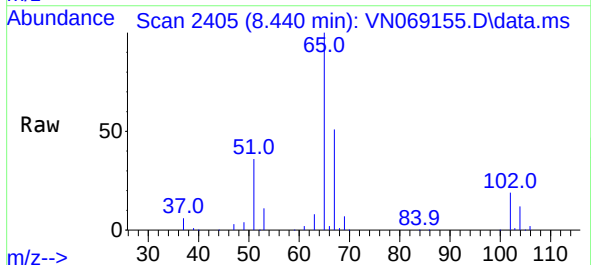


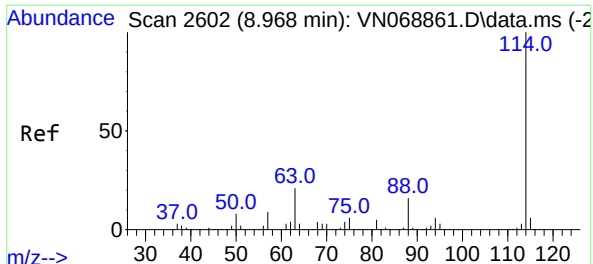

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45




Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01


Tgt Ion:114 Resp: 601916
Ion Ratio Lower Upper
114 100
63 20.9 0.0 42.6
88 15.8 0.0 32.0

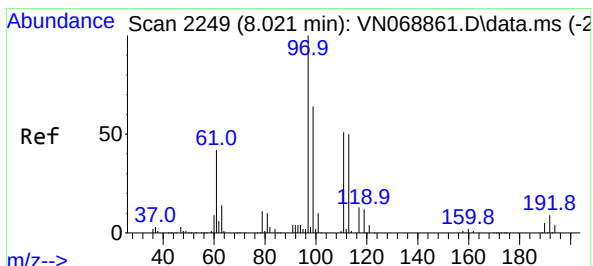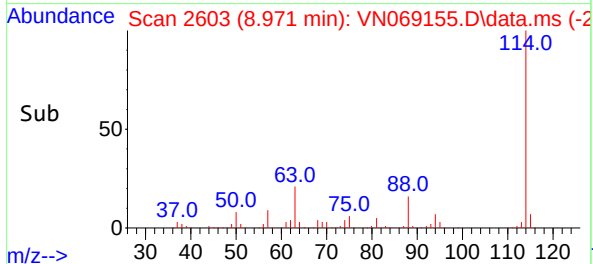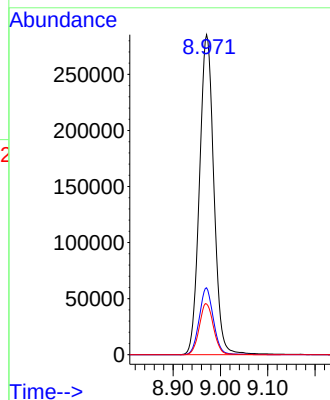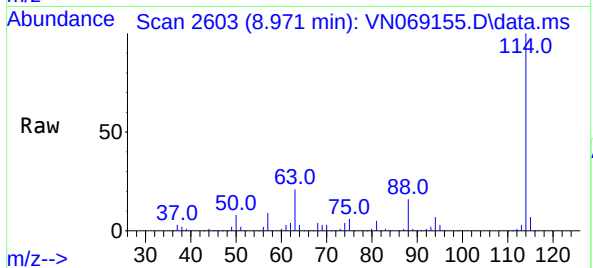

#35
Dibromofluoromethane
Concen: 50.288 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45

Tgt Ion:113 Resp: 176107
Ion Ratio Lower Upper
113 100
111 103.2 83.2 124.8
192 18.5 15.0 22.4


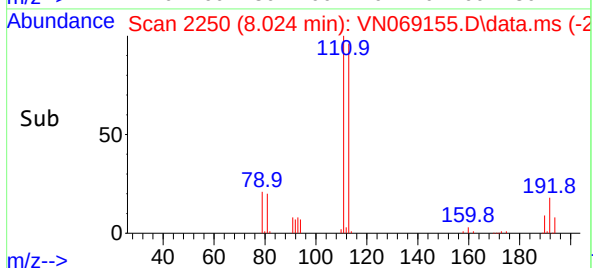
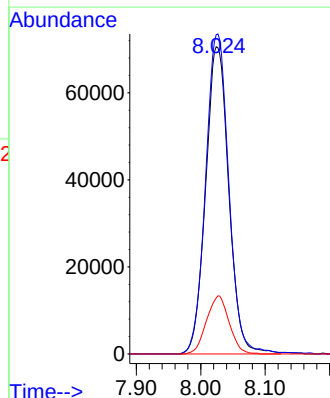
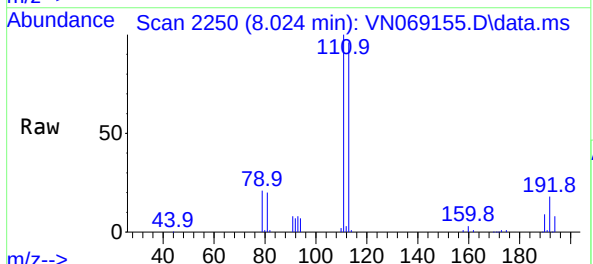


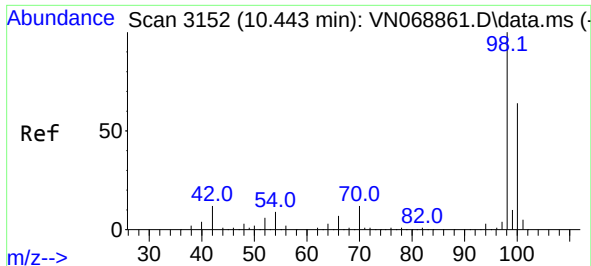

#50
Toluene-d8
Concen: 53.955 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45




Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01


Tgt Ion: 98 Resp: 756022
Ion Ratio Lower Upper
98 100
100 64.0 51.5 77.3

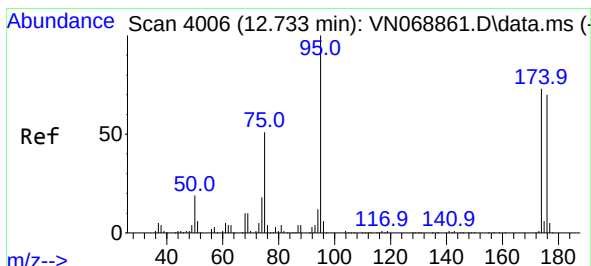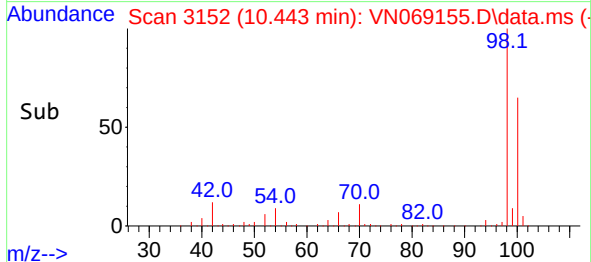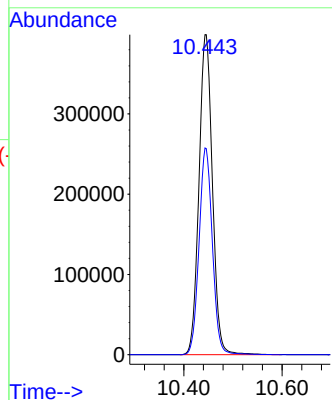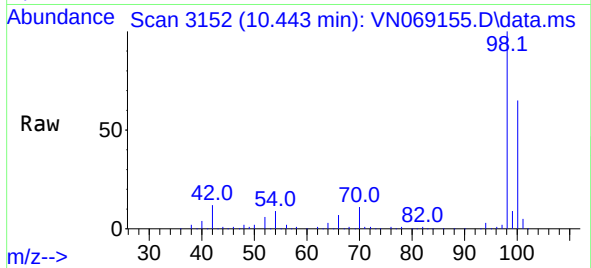

#62
4-Bromofluorobenzene
Concen: 49.769 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45

Tgt Ion: 95 Resp: 263111
Ion Ratio Lower Upper
95 100
174 74.7 0.0 144.8
176 72.0 0.0 140.0


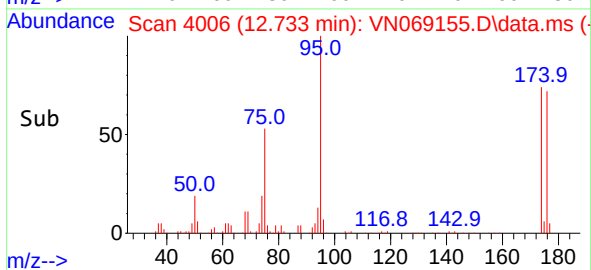
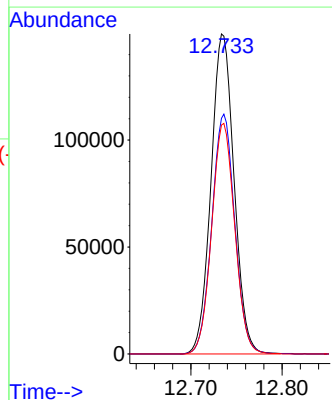
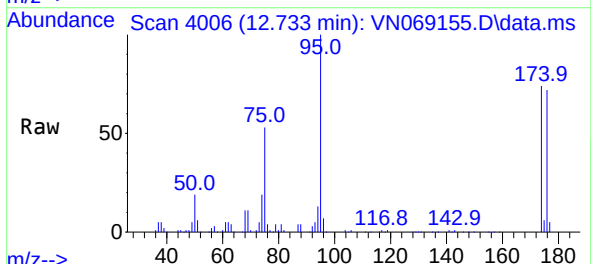


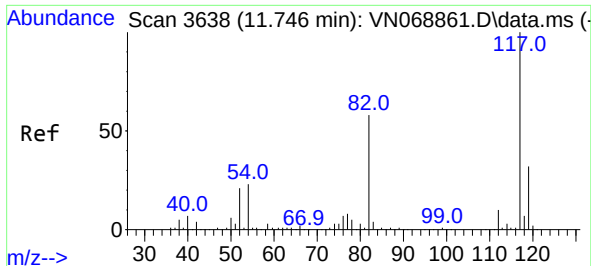

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45

Instrument :
MSVOA_N
ClientSampleId :
VN1025WBL01

Tgt Ion:117 Resp: 587235
Ion Ratio Lower Upper
117 100
82 56.2 46.4 69.6
119 32.4 26.0 39.0

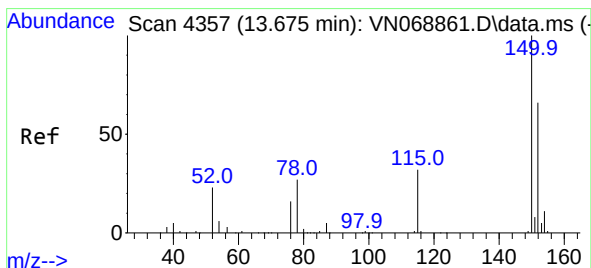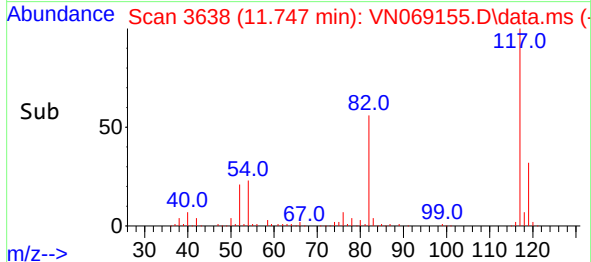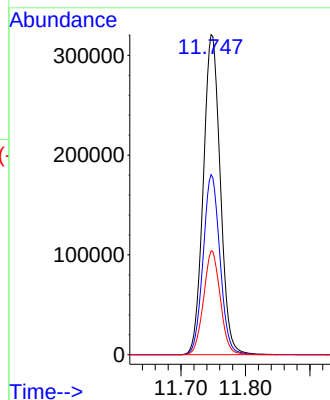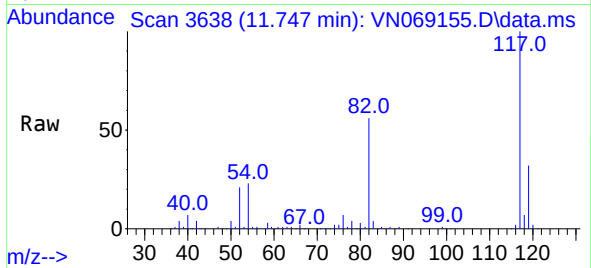

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN069155.D
Acq: 25 Oct 2021 16:45

Tgt Ion:152 Resp: 212387
Ion Ratio Lower Upper
152 100
115 63.3 31.4 94.3
150 157.7 0.0 351.0

