

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
 Data File : VN069172.D
 Acq On : 26 Oct 2021 00:01
 Operator : JC/MD
 Sample : M4334-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-REF-4

Quant Time: Oct 26 01:38:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	406859	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	720815	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	715701	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	279026	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	266500	49.680	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.360%
35) Dibromofluoromethane	8.027	113	209829	50.034	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.060%
50) Toluene-d8	10.446	98	898341	53.537	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.080%
62) 4-Bromofluorobenzene	12.733	95	342415	54.086	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	108.180%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
Data File : VN069172.D
Acq On : 26 Oct 2021 00:01
Operator : JC/MD
Sample : M4334-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4

Quant Time: Oct 26 01:38:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration




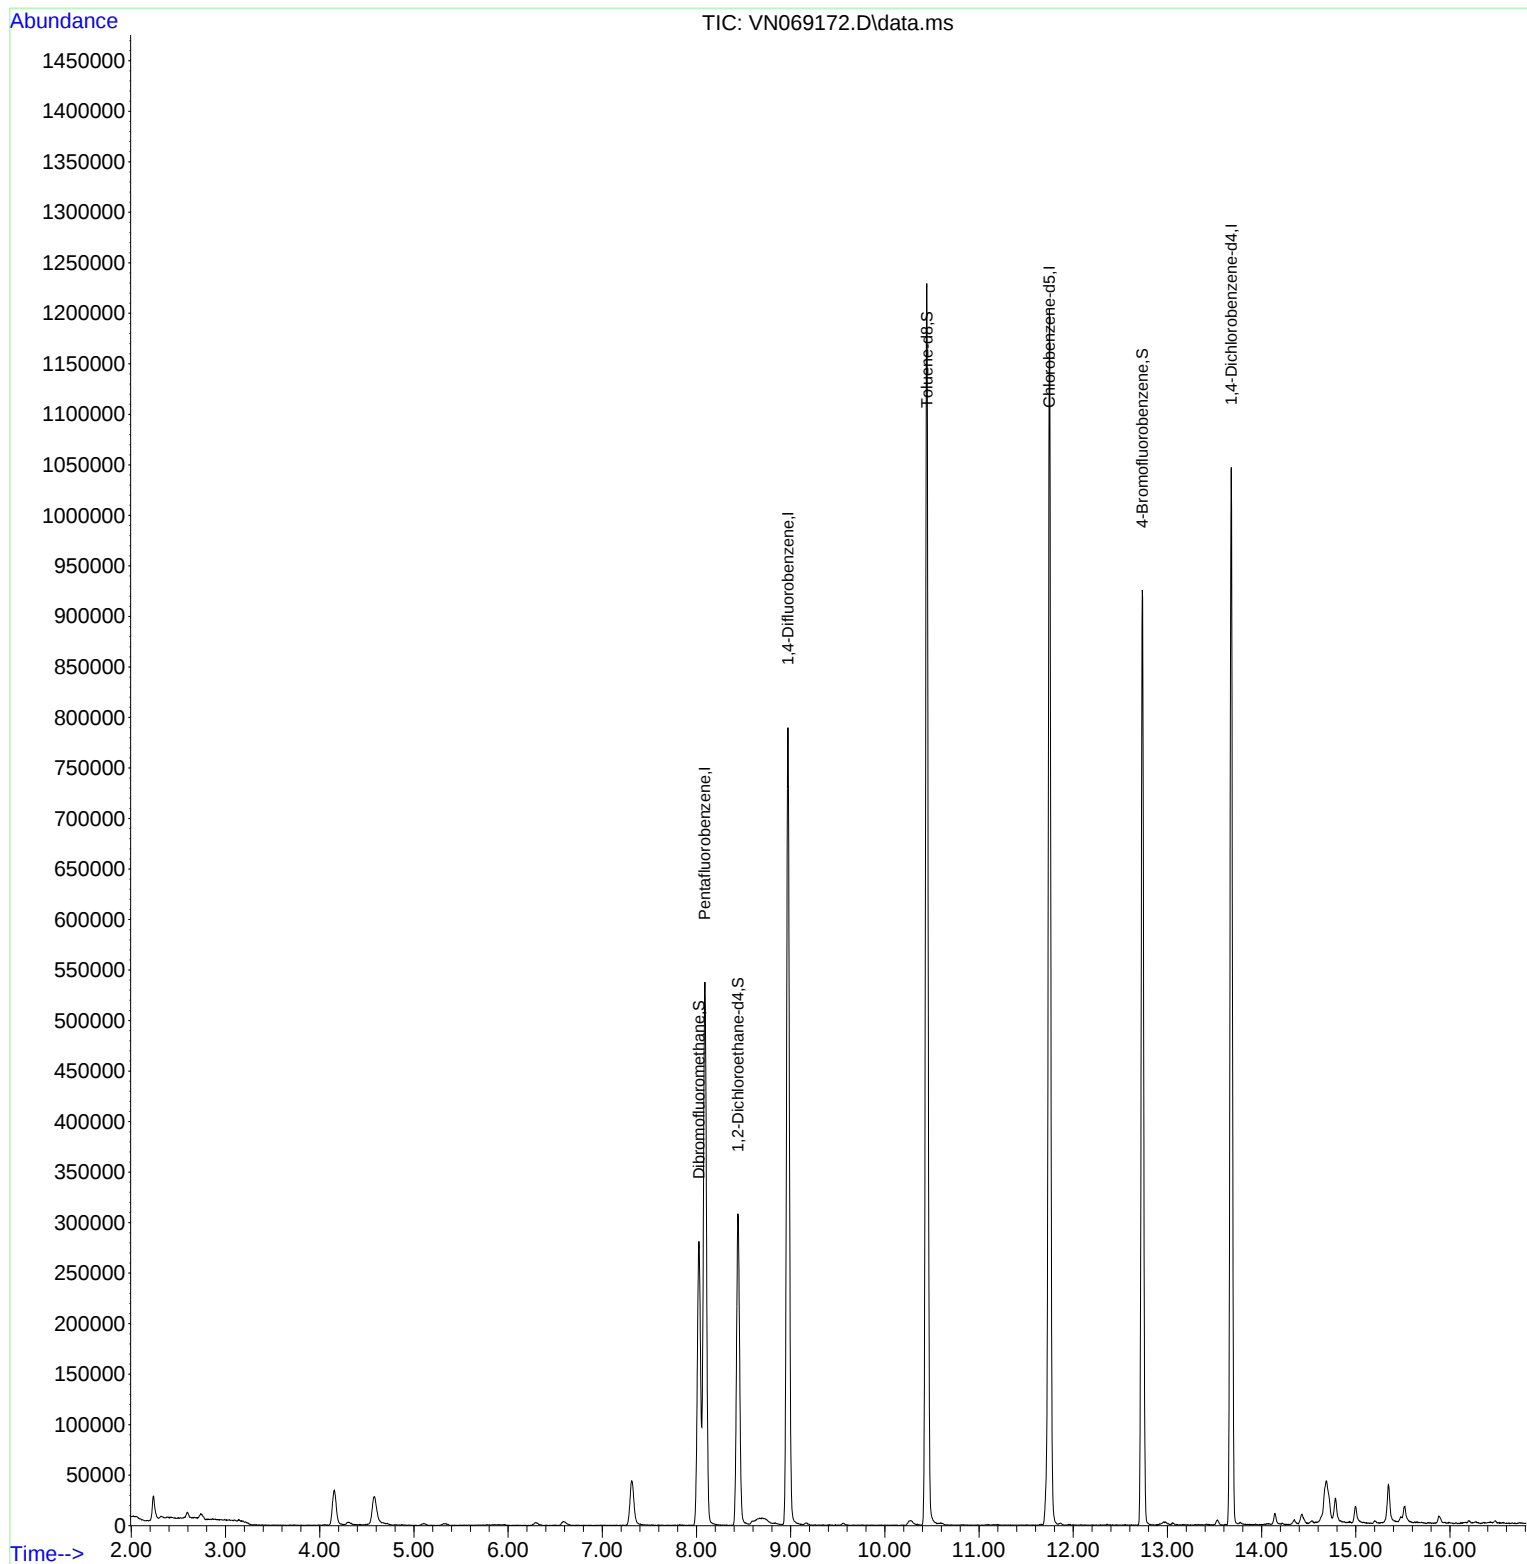




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4


Tgt Ion:168 Resp: 406859
Ion Ratio Lower Upper
168 100
99 61.8 48.9 73.3

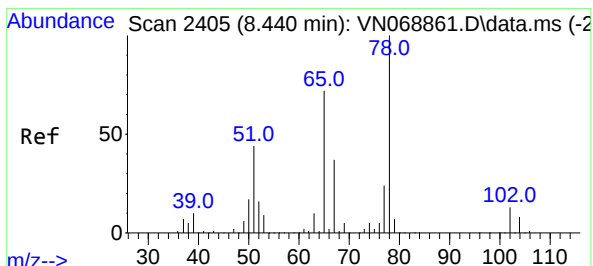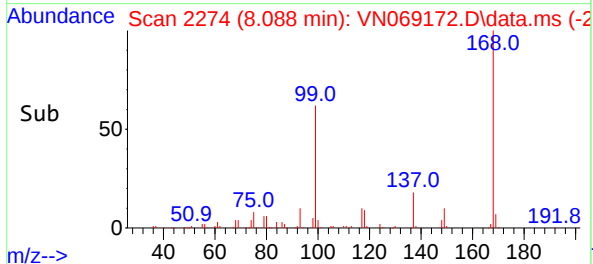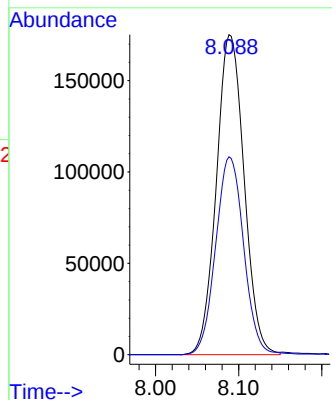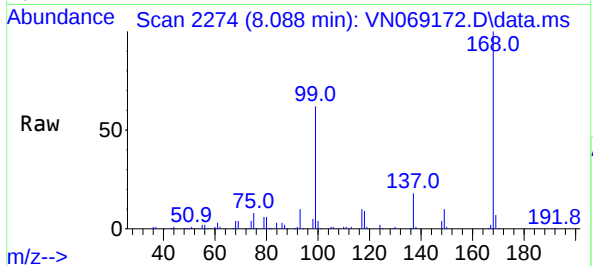

#33
1,2-Dichloroethane-d4
Concen: 49.680 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01

Tgt Ion: 65 Resp: 266500
Ion Ratio Lower Upper
65 100
67 51.9 0.0 103.8

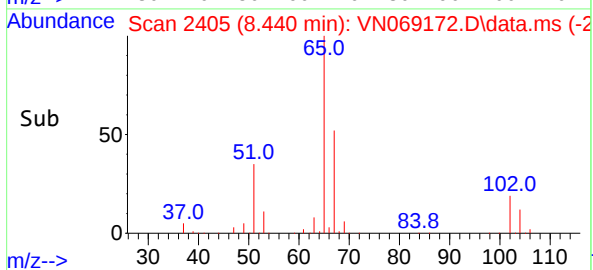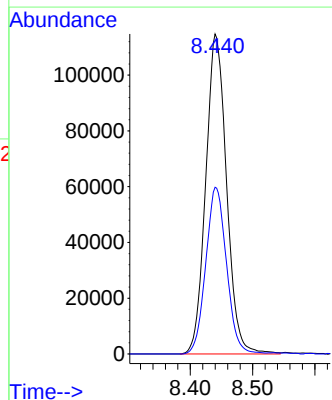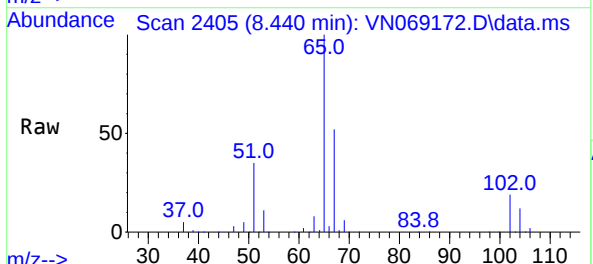




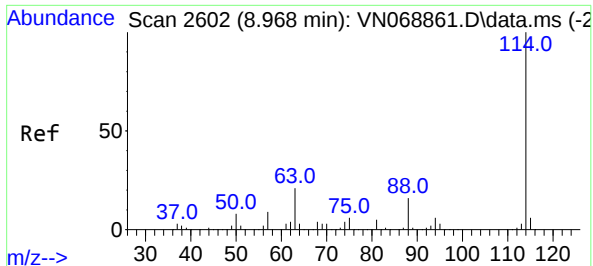


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4




Tgt Ion:114 Resp: 720815
Ion Ratio Lower Upper
114 100
63 20.5 0.0 42.6
88 15.9 0.0 32.0

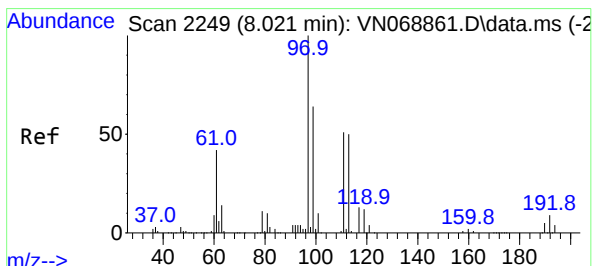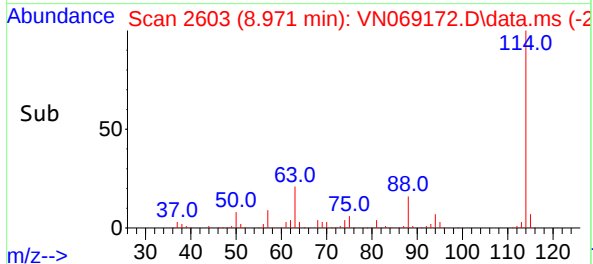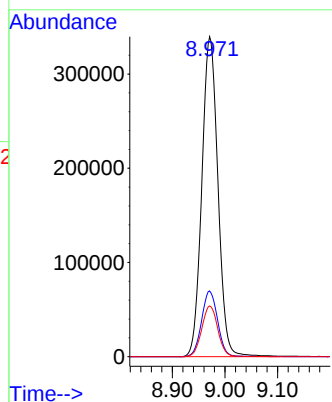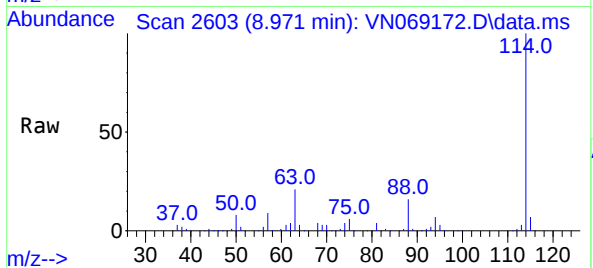


#35

Dibromofluoromethane
Concen: 50.034 ug/l
RT: 8.027 min Scan# 2251
Delta R.T. 0.005 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01

Tgt Ion:113 Resp: 209829
Ion Ratio Lower Upper
113 100
111 103.7 83.2 124.8
192 18.2 15.0 22.4


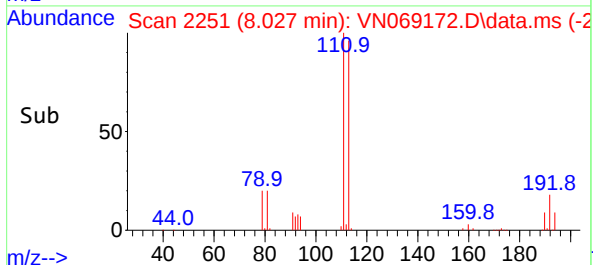
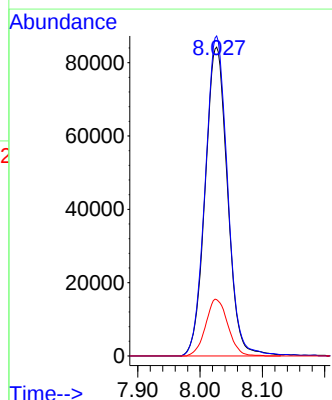
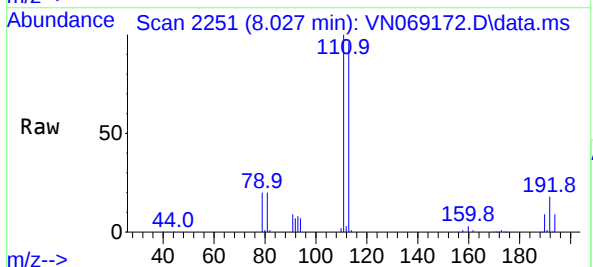


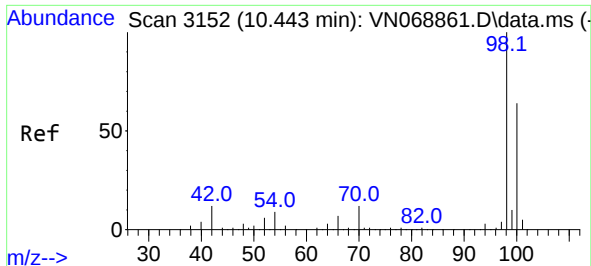

#50
Toluene-d8
Concen: 53.537 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4


Tgt Ion: 98 Resp: 898341
Ion Ratio Lower Upper
98 100
100 64.4 51.5 77.3

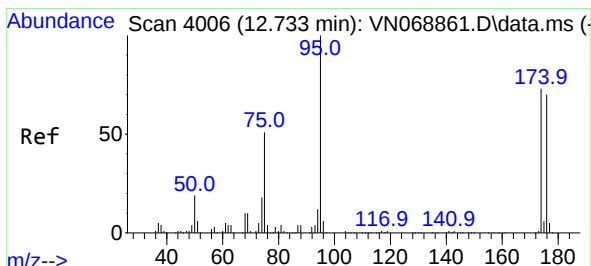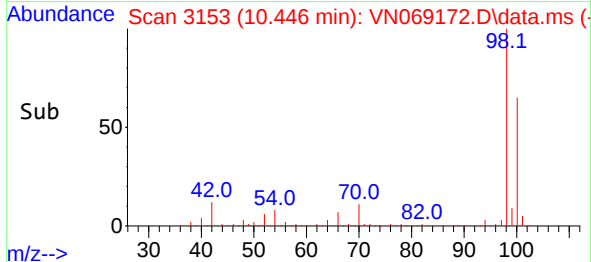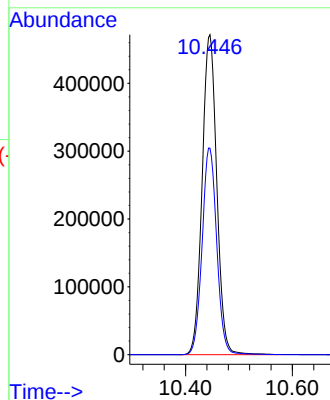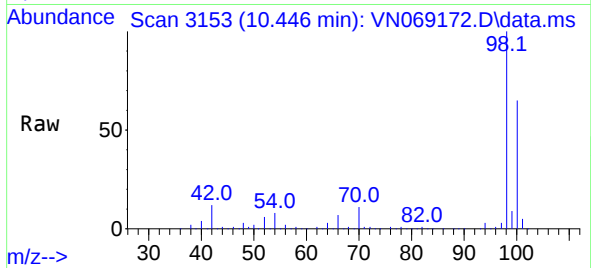

#62
4-Bromofluorobenzene
Concen: 54.086 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01

Tgt Ion: 95 Resp: 342415
Ion Ratio Lower Upper
95 100
174 72.4 0.0 144.8
176 69.8 0.0 140.0


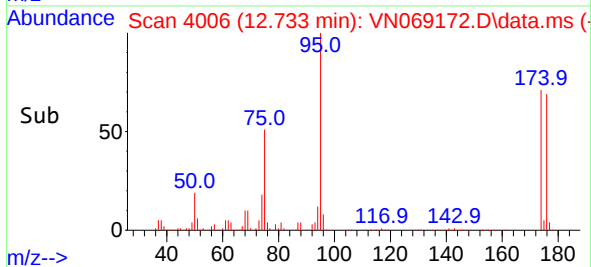
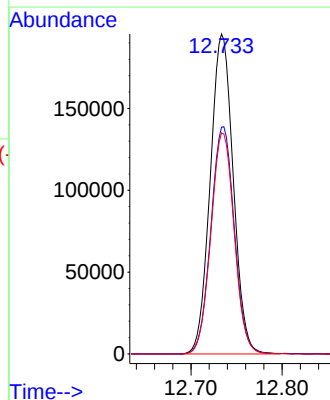
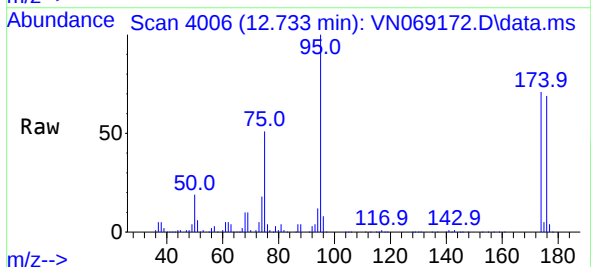


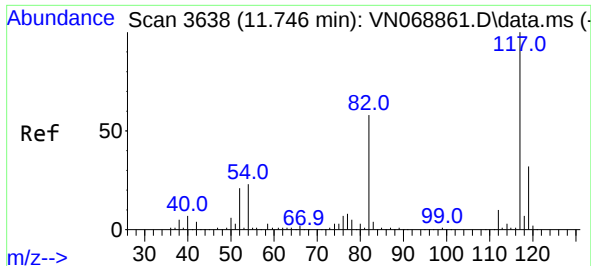

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4

Tgt Ion:117 Resp: 715701
Ion Ratio Lower Upper
117 100
82 56.2 46.4 69.6
119 31.8 26.0 39.0

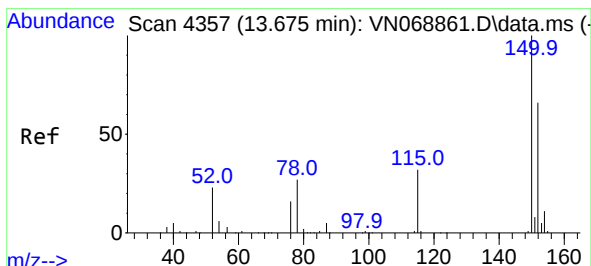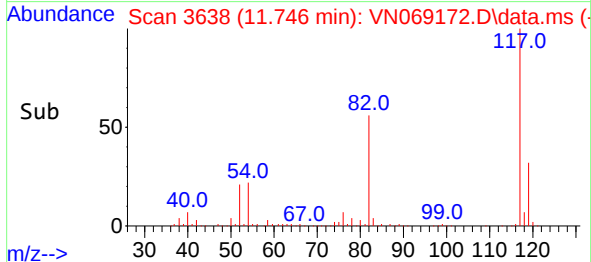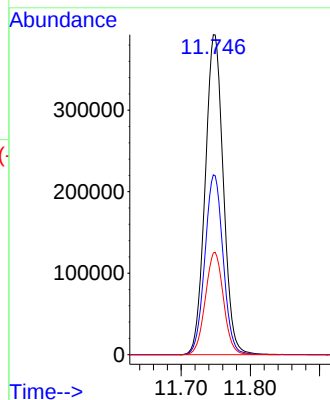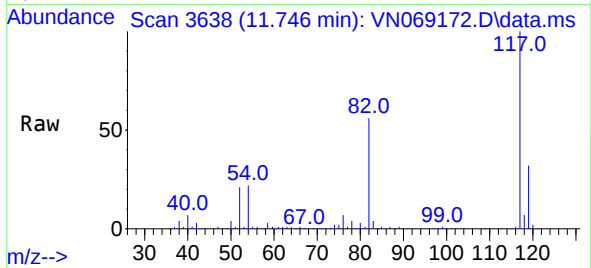

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN069172.D
Acq: 26 Oct 2021 00:01

Tgt Ion:152 Resp: 279026
Ion Ratio Lower Upper
152 100
115 64.3 31.4 94.3
150 159.7 0.0 351.0

