

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
 Data File : VN069163.D
 Acq On : 25 Oct 2021 20:15
 Operator : JC/MD
 Sample : M4307-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.575	938	964	965	rBV3	14645	22780	1.15%	0.223%
2	7.311	1960	1984	1986	rBV2	23348	38618	1.95%	0.378%
3	8.024	2228	2250	2261	rBV2	236561	567060	28.70%	5.553%
4	8.088	2262	2274	2297	rVB	461081	1038998	52.58%	10.174%
5	8.440	2385	2405	2428	rBV	260660	605390	30.64%	5.928%
6	8.971	2582	2603	2628	rBV	672916	1402726	70.99%	13.736%
7	10.443	3131	3152	3196	rBV	1037683	1976002	100.00%	19.350%
8	11.747	3619	3638	3666	rBV	973450	1782155	90.19%	17.451%
9	12.733	3989	4006	4029	rBV	745714	1303021	65.94%	12.760%
10	13.678	4342	4358	4381	rVB	833935	1429206	72.33%	13.995%
11	15.509	5030	5041	5053	rBV	13978	25786	1.30%	0.253%
12	15.702	5100	5113	5128	rVB7	10488	20385	1.03%	0.200%


Sum of corrected areas: 10212127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
Data File : VN069163.D
Acq On : 25 Oct 2021 20:15
Operator : JC/MD
Sample : M4307-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

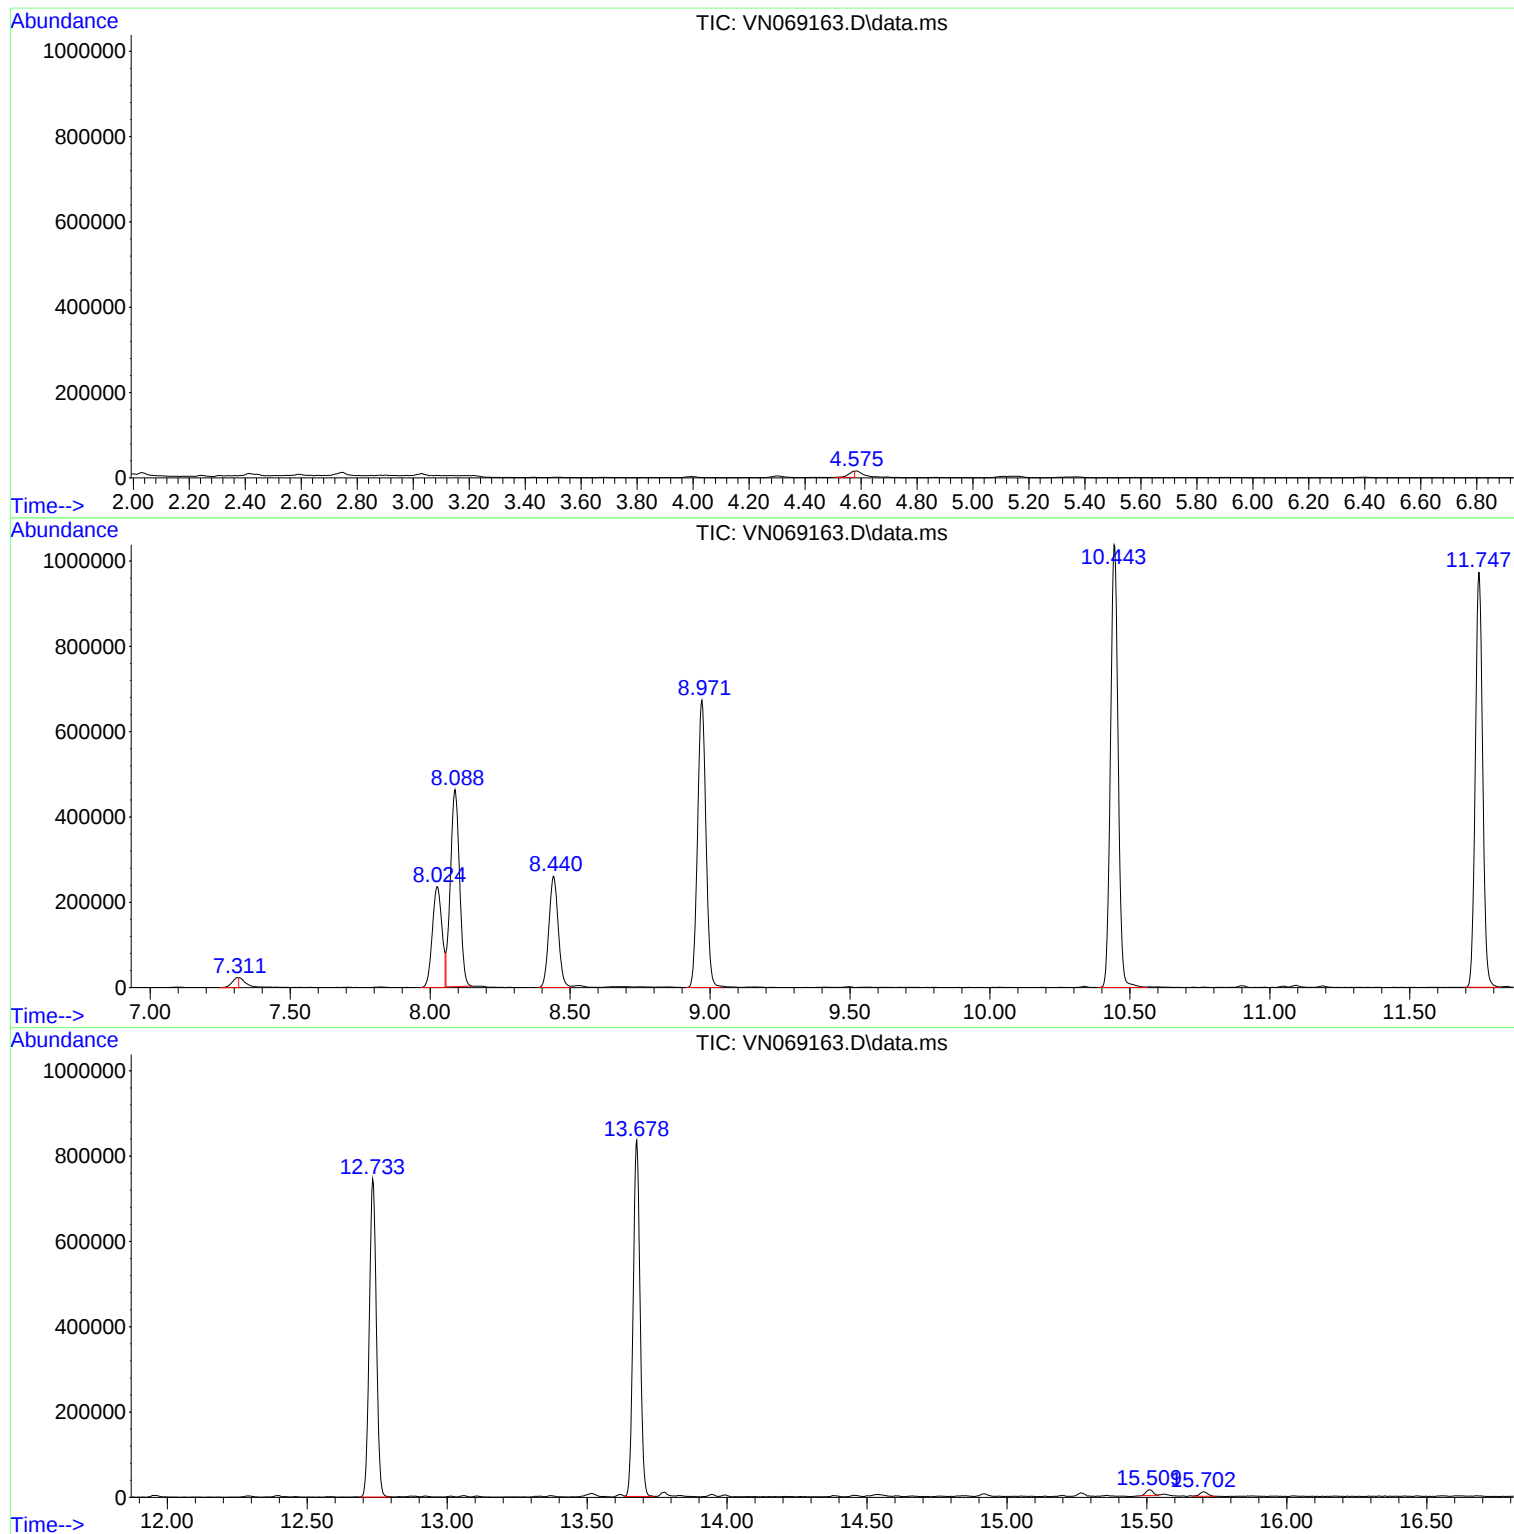

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
Data File : VN069163.D
Acq On : 25 Oct 2021 20:15
Operator : JC/MD
Sample : M4307-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102621\
Data File : VN069163.D
Acq On : 25 Oct 2021 20:15
Operator : JC/MD
Sample : M4307-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
