

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102622\
 Data File : VN075025.D
 Acq On : 26 Oct 2022 16:44
 Operator : JC\MD
 Sample : VN1026WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1026MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M

Title : SW846 8260

Signal : TIC: VN075025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.295	34	41	53	rBV	18429	43707	9.00%	1.646%
2	2.812	125	129	133	rBV	5230	9853	2.03%	0.371%
3	2.895	141	143	151	rVB4	16800	25073	5.16%	0.944%
4	3.242	201	202	216	rVB3	2147	6394	1.32%	0.241%
5	8.171	1031	1040	1045	rBV	68092	166462	34.26%	6.269%
6	8.230	1045	1050	1064	rVB	127810	273569	56.31%	10.302%
7	8.582	1102	1110	1119	rBV2	79824	176128	36.25%	6.633%
8	9.106	1191	1199	1208	rBV	188317	377001	77.60%	14.197%
9	10.571	1440	1448	1462	rBV	270041	485856	100.00%	18.297%
10	11.871	1661	1669	1679	rVB	248646	432330	88.98%	16.281%
11	12.853	1825	1836	1846	rVB	177950	297380	61.21%	11.199%
12	13.794	1989	1996	2004	rBV	218379	361690	74.44%	13.621%




Sum of corrected areas: 2655443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102622\
Data File : VN075025.D
Acq On : 26 Oct 2022 16:44
Operator : JC\MD
Sample : VN1026WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1026MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

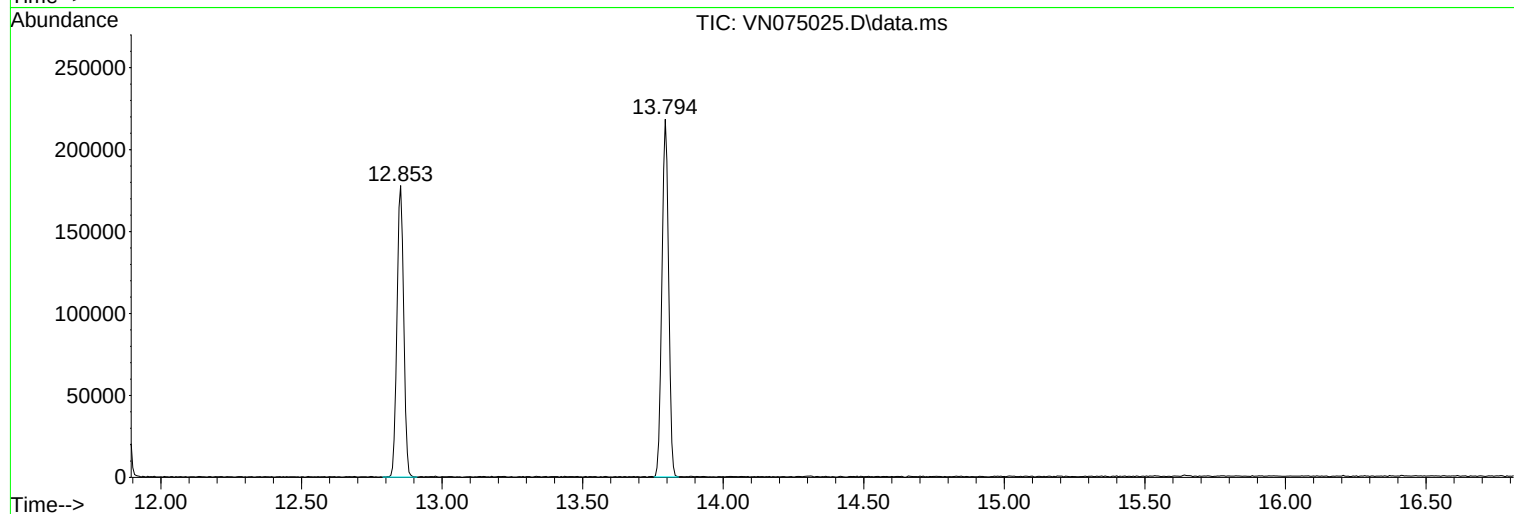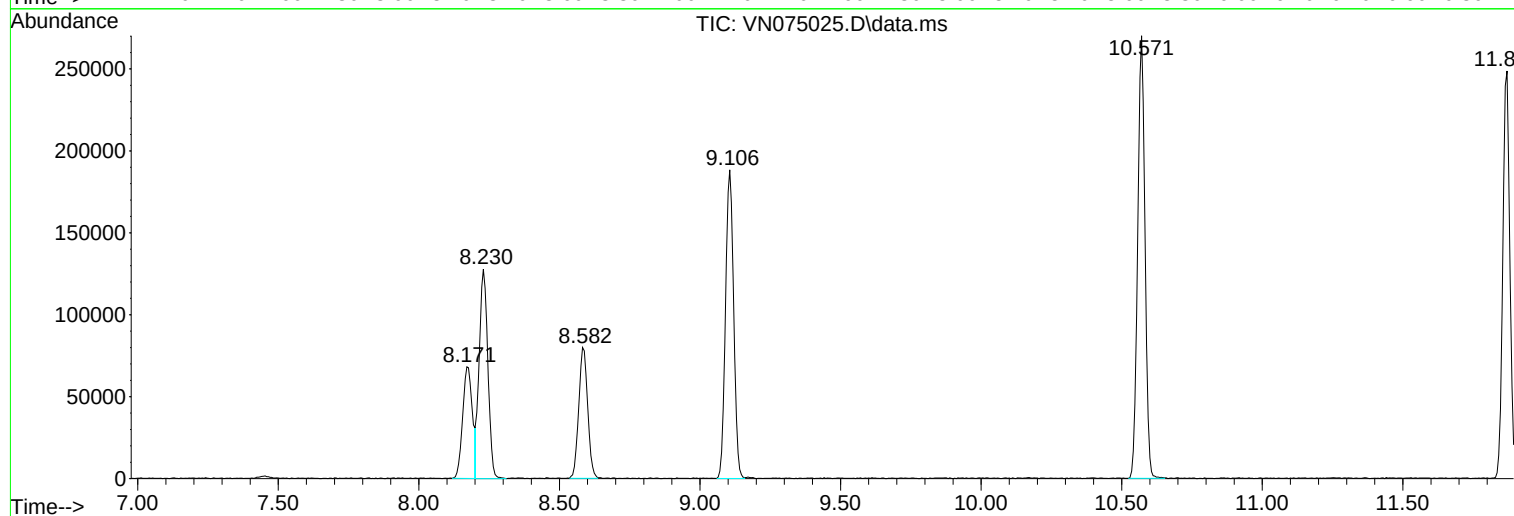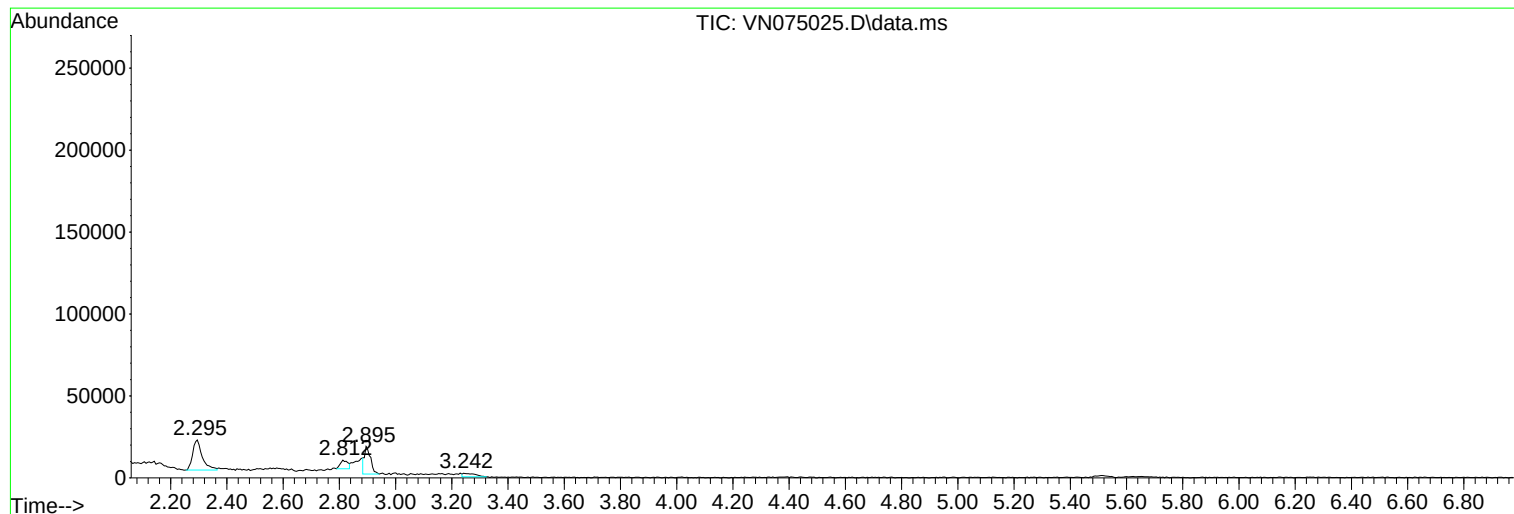

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102622\
Data File : VN075025.D
Acq On : 26 Oct 2022 16:44
Operator : JC\MD
Sample : VN1026WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1026MBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.295	7.99 ug/l	43707	Pentafluorobenzene	8.230

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	74
2			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
3			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

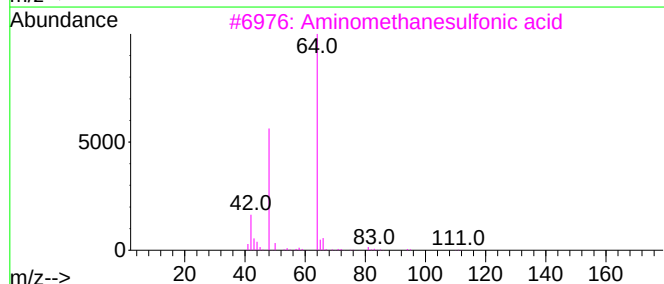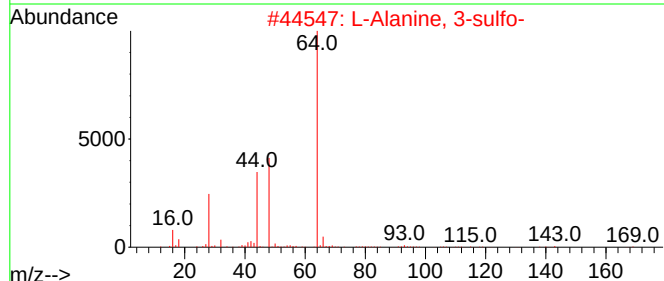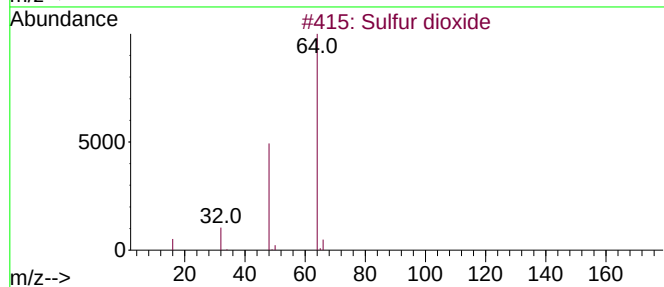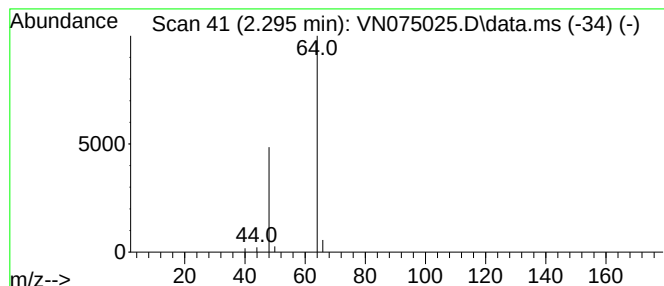

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102622\
Data File : VN075025.D
Acq On : 26 Oct 2022 16:44
Operator : JC\MD
Sample : VN1026WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1026MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.295	8.0	ug/l	43707	1	8.230	273569	50.0