
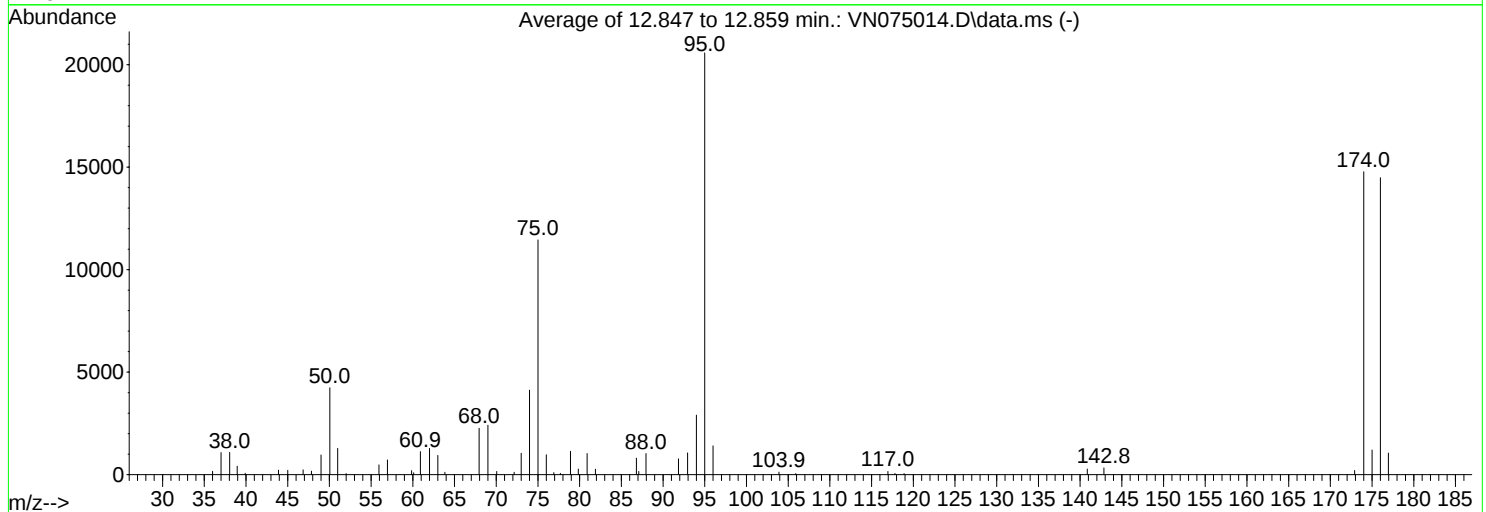


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102622\
 Data File : VN075014.D
 Acq On : 26 Oct 2022 09:52
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Title : SW846 8260
 Last Update : Thu Oct 27 09:48:49 2022

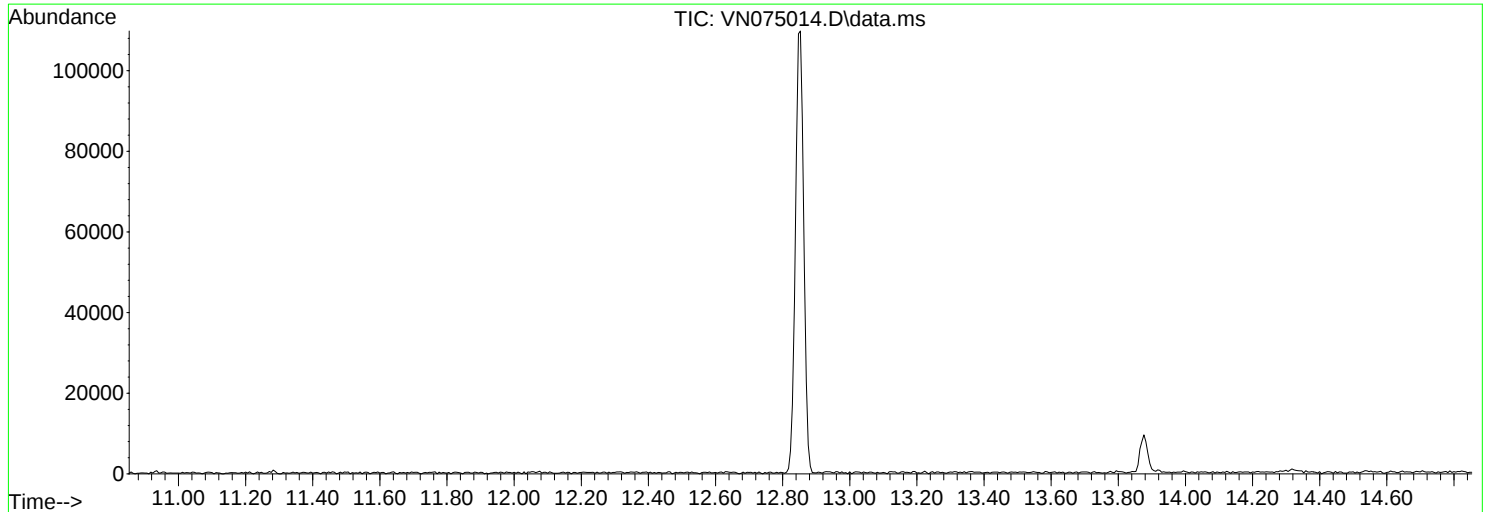

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	4242	PASS
75	95	30	60	55.6	11448	PASS
95	95	100	100	100.0	20576	PASS
96	95	5	9	6.8	1404	PASS
173	174	0.00	2	1.4	202	PASS
174	95	50	100	71.8	14772	PASS
175	174	5	9	8.1	1203	PASS
176	174	95	101	98.1	14488	PASS
177	176	5	9	7.3	1051	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	162	51.00	1283	69.00	2409	80.90	1030
37.00	1078	52.00	51	70.05	157	81.90	261
38.05	1083	55.95	475	72.15	120	86.80	80
38.95	416	56.95	721	73.00	1048	87.10	15
39.90	68	59.85	193	74.00	4121	87.95	1027
43.90	222	60.10	91	75.00	11448	91.85	776
45.00	212	60.90	1126	76.00	965	92.95	1062
46.85	235	62.00	1280	76.90	102	94.00	2905
47.85	175	63.00	933	77.70	66	95.00	20576
49.00	957	63.85	119	78.90	1138	96.00	1404
50.05	4242	67.95	2262	79.85	273	103.90	127

Average of 12.847 to 12.859 min.: VN075014.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.90	55						
116.95	159						
117.80	61						
118.90	57						
140.85	276						
142.85	327						
172.90	202						
174.00	14772						
175.00	1203						
176.00	14488						
176.95	1051						

Instrument :

MSVOA_N

ClientSampleId :

BFB