

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102623\
 Data File : VN079700.D
 Acq On : 26 Oct 2023 17:24
 Operator : JC\MD
 Sample : 04980-02
 Misc : 1.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 27 01:23:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 06 03:34:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	267287	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	503072	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	495615	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	200870	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	209111	48.251	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	96.500%		
35) Dibromofluoromethane	8.165	113	184708	51.091	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	102.180%		
50) Toluene-d8	10.571	98	601839	46.008	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	92.020%		
62) 4-Bromofluorobenzene	12.853	95	236275	56.283	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	112.560%		
Target Compounds						Qvalue
10) Methyl Iodide	4.559	142	816	0.274	ug/l #	38
11) Tert butyl alcohol	5.494	59	11139	17.077	ug/l #	72
13) Acrolein	4.177	56	189	0.291	ug/l	97
15) Acrylonitrile	5.741	53	620	0.328	ug/l	86
18) Methyl Acetate	5.047	43	3919	0.466	ug/l #	55
20) Methylene Chloride	5.259	84	1710	Below Cal	#	84
25) 2-Butanone	7.506	43	2380	0.933	ug/l #	80
29) Tetrahydrofuran	7.859	42	1325	0.803	ug/l #	49
31) Cyclohexane	8.224	56	6992	1.137	ug/l #	29
36) 1,1-Dichloropropene	8.224	75	23536	4.338	ug/l #	48
38) Carbon Tetrachloride	8.224	117	28415	5.231	ug/l #	15
41) Methacrylonitrile	7.847	41	729	0.257	ug/l #	29
51) 4-Methyl-2-Pentanone	10.453	43	2164	0.405	ug/l #	83
59) 2-Hexanone	11.212	43	3922	1.018	ug/l	74
68) m/p-Xylenes	12.076	106	1713	0.246	ug/l	86
74) N-amyl acetate	12.512	43	1653	0.216	ug/l #	76
75) 1,1,2,2-Tetrachloroethane	12.935	83	932	Below Cal	#	60
76) 1,2,3-Trichloropropane	12.853	75	131804	22.758	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	131804	66.032	ug/l #	15
82) 4-Chlorotoluene	13.229	91	2802	0.218	ug/l	97
87) 1,3-Dichlorobenzene	13.735	146	2219	0.305	ug/l	86
88) 1,4-Dichlorobenzene	13.735	146	2219	0.296	ug/l	87
89) n-Butylbenzene	14.059	91	3518	0.341	ug/l	95
90) Hexachloroethane	14.323	117	271	Below Cal	#	21
91) 1,2-Dichlorobenzene	14.117	146	2358	0.333	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	14.723	75	309	0.286	ug/l	81
93) 1,2,4-Trichlorobenzene	15.400	180	2494	1.136	ug/l	94
94) Hexachlorobutadiene	15.500	225	1374	0.804	ug/l	85
95) Naphthalene	15.647	128	9526	1.421	ug/l	98
96) 1,2,3-Trichlorobenzene	15.841	180	2723	1.039	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102623\
Data File : VN079700.D
Acq On : 26 Oct 2023 17:24
Operator : JC\MD
Sample : 04980-02
Misc : 1.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Oct 27 01:23:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 06 03:34:49 2023
Response via : Initial Calibration




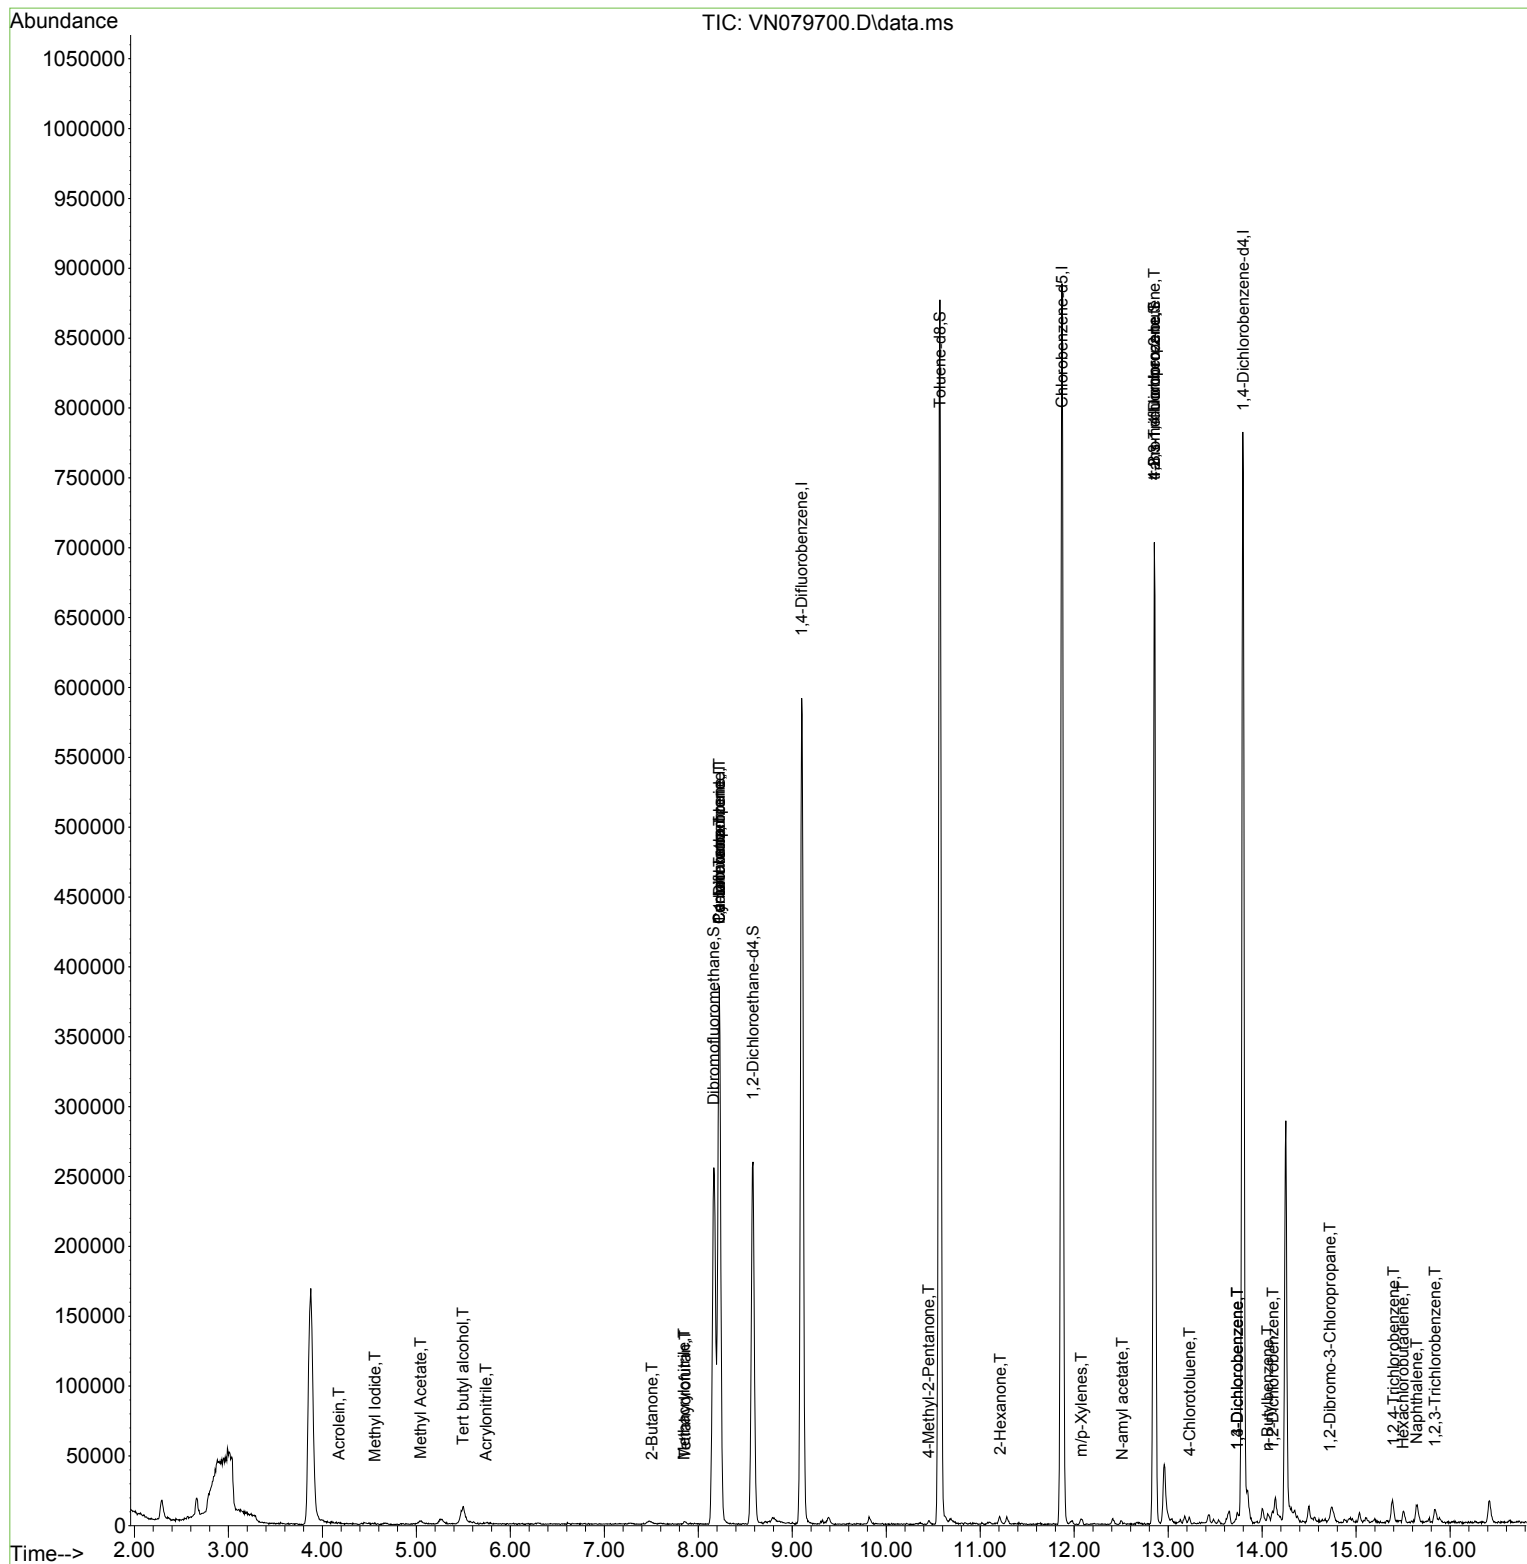




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.006 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 267287
Ion Ratio Lower Upper
168 100
99 63.1 53.0 79.6

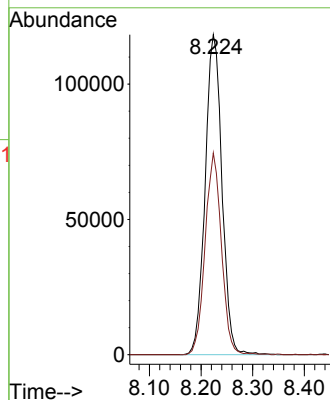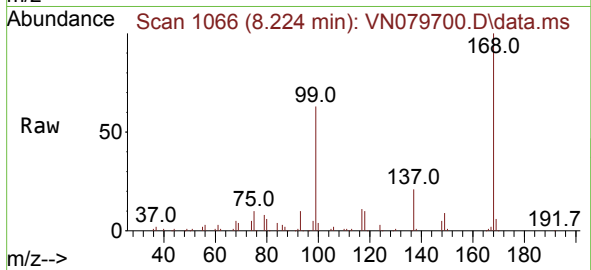

#10
Methyl Iodide
Concen: 0.274 ug/l
RT: 4.559 min Scan# 443
Delta R.T. -0.030 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Tgt Ion:142 Resp: 816
Ion Ratio Lower Upper
142 100
127 0.0 37.6 56.4#
141 0.0 11.4 17.0#



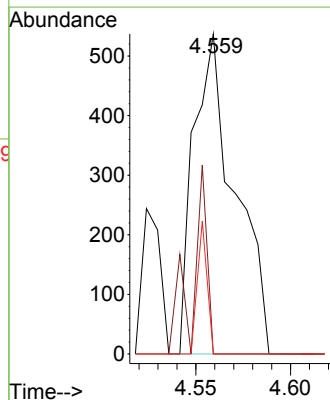





#11
Tert butyl alcohol
Concen: 17.077 ug/l
RT: 5.494 min Scan# 608
Delta R.T. -0.036 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 11139
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

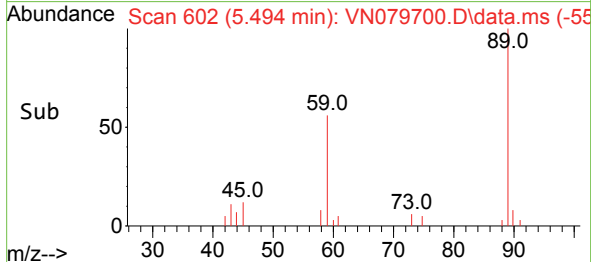

#13
Acrolein
Concen: 0.291 ug/l
RT: 4.177 min Scan# 378
Delta R.T. -0.006 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24


Tgt Ion: 56 Resp: 189
Ion Ratio Lower Upper
56 100
55 70.9 54.5 81.7

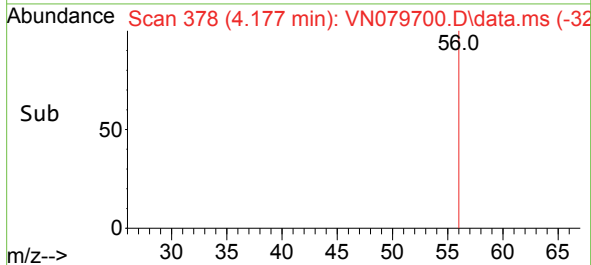






#15
 Acrylonitrile
 Concen: 0.328 ug/l
 RT: 5.741 min Scan# 641
 Delta R.T. 0.017 min
 Lab File: VN079700.D
 Acq: 26 Oct 2023 17:24

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 53	Resp:	620
Ion	Ratio	Lower Upper
53	100	
52	66.9	65.3 97.9
51	31.1	28.9 43.3

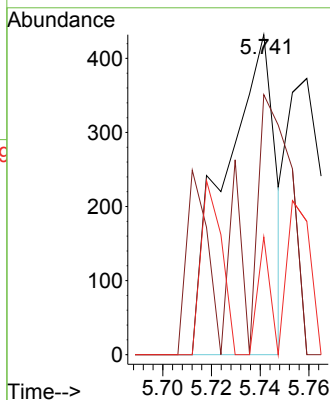

#18
 Methyl Acetate
 Concen: 0.466 ug/l
 RT: 5.047 min Scan# 526
 Delta R.T. 0.018 min
 Lab File: VN079700.D
 Acq: 26 Oct 2023 17:24

Tgt Ion: 43	Resp:	3919
Ion	Ratio	Lower Upper
43	100	
74	7.3	26.2 39.4#


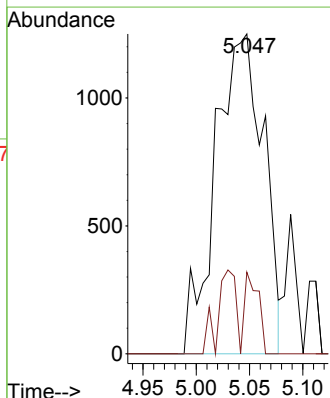
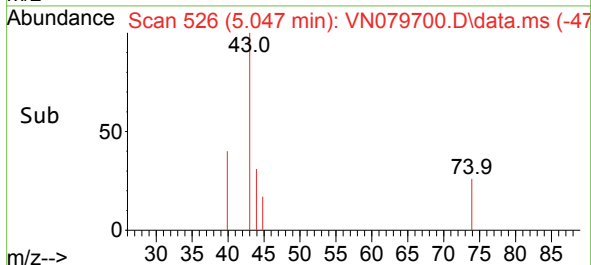
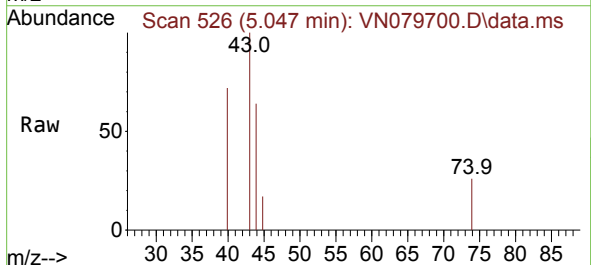


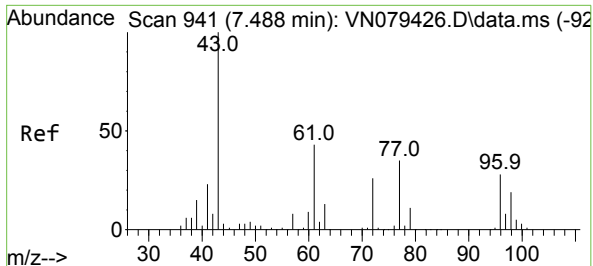

#25
2-Butanone
Concen: 0.933 ug/l
RT: 7.506 min Scan# 941
Delta R.T. 0.018 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2380
Ion Ratio Lower Upper
43 100
72 25.5 30.2 45.2#

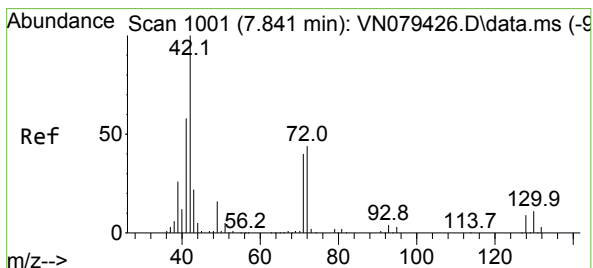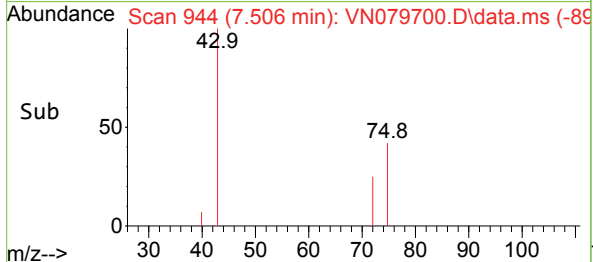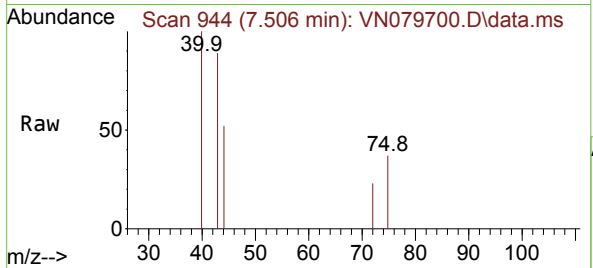

#29
Tetrahydrofuran
Concen: 0.803 ug/l
RT: 7.859 min Scan# 1004
Delta R.T. 0.018 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24


Tgt Ion: 42 Resp: 1325
Ion Ratio Lower Upper
42 100
72 34.6 49.8 74.6#
71 8.5 47.4 71.2#

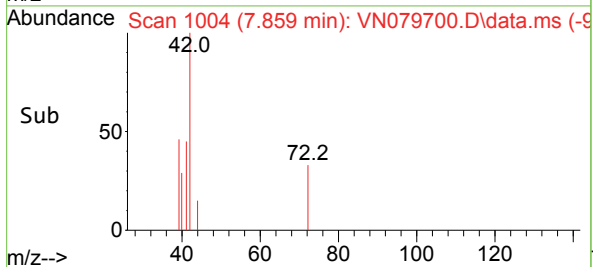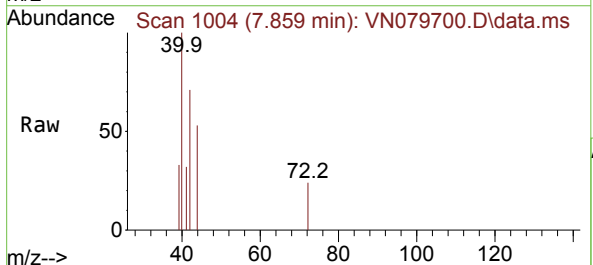






#31
Cyclohexane
Concen: 1.137 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.041 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Instrument :
MSVOA_N
ClientSampleId :



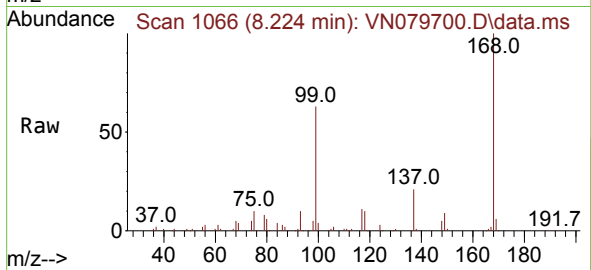



Tgt Ion: 56 Resp: 6992
Ion Ratio Lower Upper
56 100
69 123.1 26.8 40.2#
84 146.1 81.8 122.6#

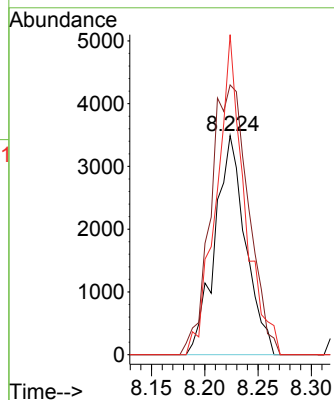

#33
1,2-Dichloroethane-d4
Concen: 48.251 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Tgt Ion: 65 Resp: 209111
Ion Ratio Lower Upper
65 100
67 53.5 0.0 106.6

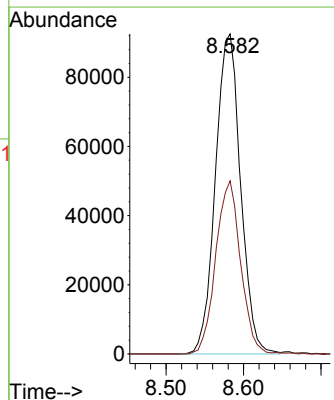



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 503072

Ion Ratio Lower Upper

114 100

63 22.0 0.0 36.4

88 15.3 0.0 30.6



#35

Dibromofluoromethane

Concen: 51.091 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.006 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24




Tgt Ion:113 Resp: 184708


Ion Ratio Lower Upper

113 100

111 105.6 82.6 123.8

192 18.0 12.7 19.1

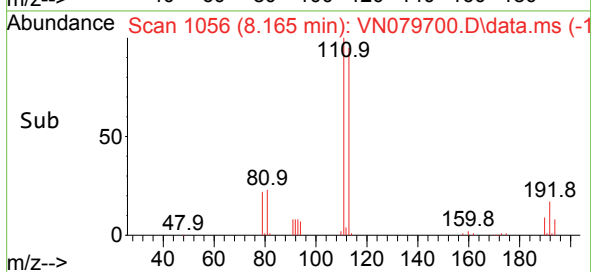



#36

1,1-Dichloropropene

Concen: 4.338 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.153 min


Lab File: VN079700.D

Acq: 26 Oct 2023 17:24

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 23536

Ion Ratio Lower Upper

75 100

110 9.0 19.1 57.3#

77 0.0 25.0 37.4#



#38

Carbon Tetrachloride

Concen: 5.231 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24




Tgt Ion: 117 Resp: 28415


Ion Ratio Lower Upper

117 100

119 3.7 77.3 115.9#

121 0.0 23.3 34.9#


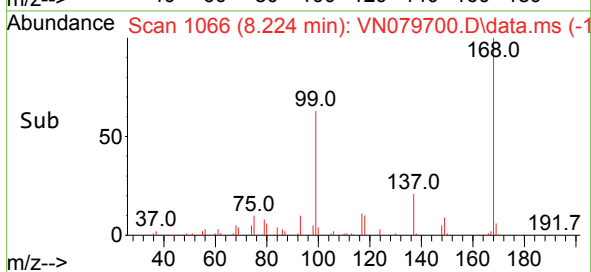




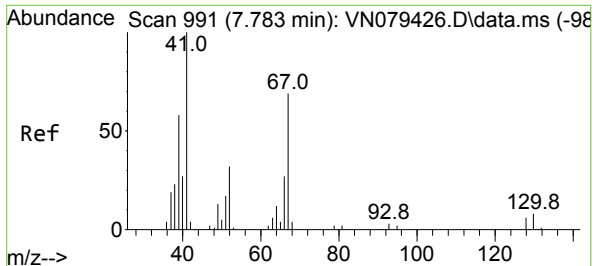

#41
Methacrylonitrile
Concen: 0.257 ug/l
RT: 7.847 min Scan# 1002
Delta R.T. 0.065 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 41 Resp: 729
Ion Ratio Lower Upper
41 100
39 71.9 42.6 64.0#
67 0.0 77.5 116.3#
52 0.0 28.9 43.3#

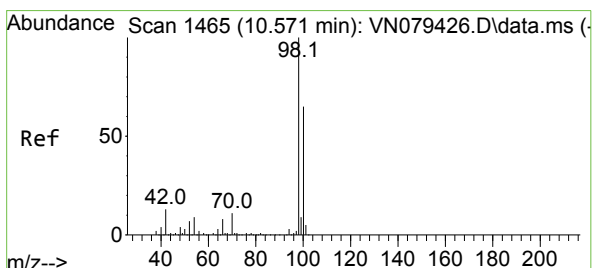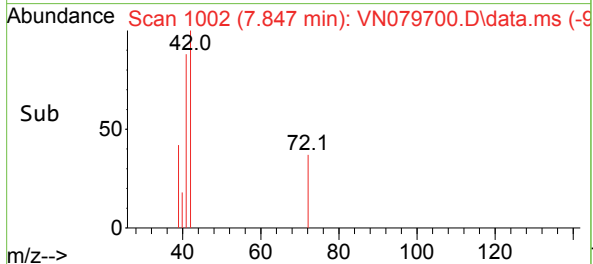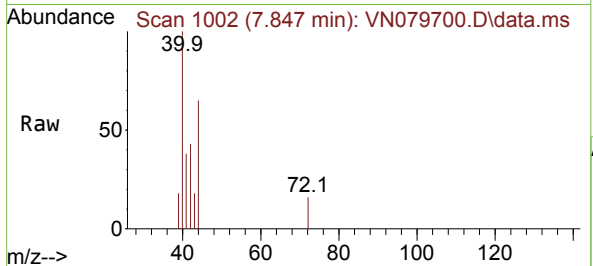

#50
Toluene-d8
Concen: 46.008 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Tgt Ion: 98 Resp: 601839
Ion Ratio Lower Upper
98 100
100 64.4 52.0 78.0


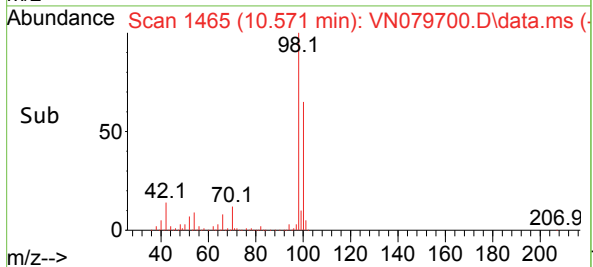

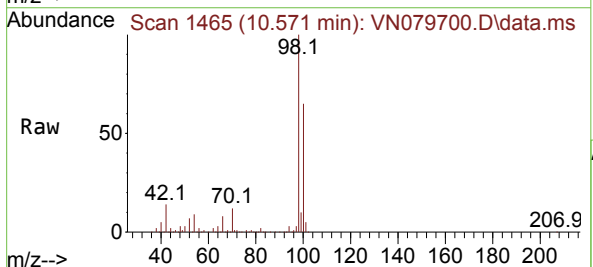




#51
4-Methyl-2-Pentanone
Concen: 0.405 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.006 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2164
Ion Ratio Lower Upper
43 100
58 34.4 36.6 54.8#

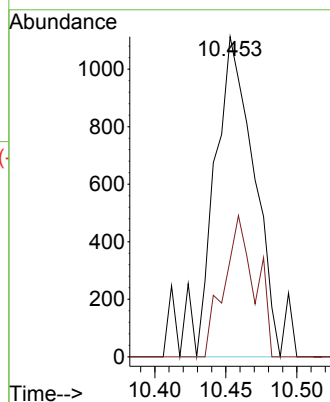

#59
2-Hexanone
Concen: 1.018 ug/l
RT: 11.212 min Scan# 1574
Delta R.T. 0.012 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Tgt Ion: 43 Resp: 3922
Ion Ratio Lower Upper
43 100
58 43.0 31.7 95.1


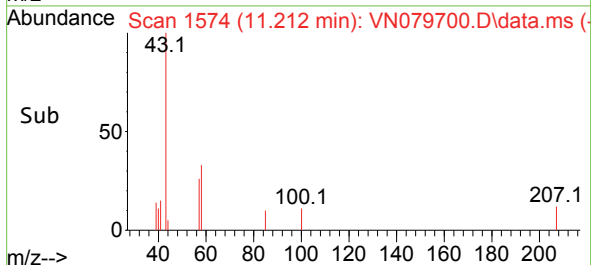
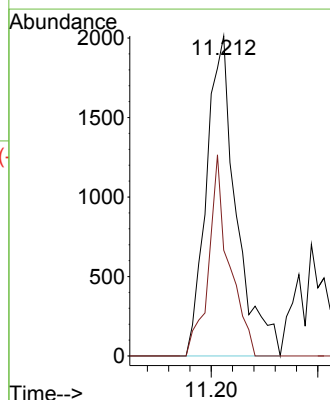





#62
4-Bromofluorobenzene
Concen: 56.283 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 236275
Ion Ratio Lower Upper
95 100
174 75.2 0.0 143.8
176 71.5 0.0 135.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Tgt Ion: 117 Resp: 495615
Ion Ratio Lower Upper
117 100
82 58.9 44.0 66.0
119 32.1 25.6 38.4









#68
m/p-Xylenes
Concen: 0.246 ug/l
RT: 12.076 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 1713
Ion Ratio Lower Upper
106 100
91 178.4 159.6 239.4



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. 0.006 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24

Tgt Ion:152 Resp: 200870
Ion Ratio Lower Upper
152 100
115 63.2 32.3 96.8
150 158.5 0.0 355.8

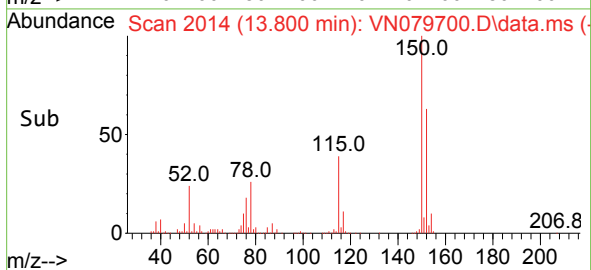

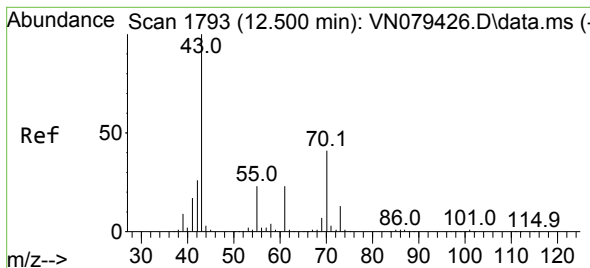

#74

N-amy1 acetate

Concen: 0.216 ug/l

RT: 12.512 min Scan# 1

Delta R.T. 0.012 min


Lab File: VN079700.D

Acq: 26 Oct 2023 17:24

Instrument :

MSVOA_N

ClientSampleId :

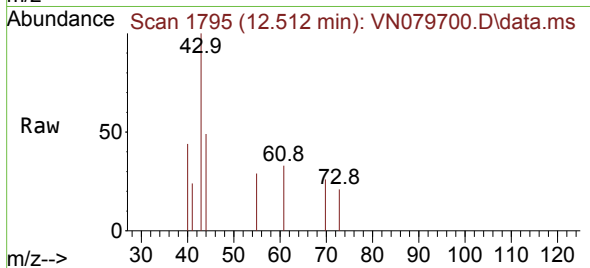

Tgt Ion: 43 Resp: 1653




Ion Ratio Lower Upper

43 100

70 29.3 43.4 65.2#

55 19.1 21.4 32.0#

61 21.2 22.8 34.2#

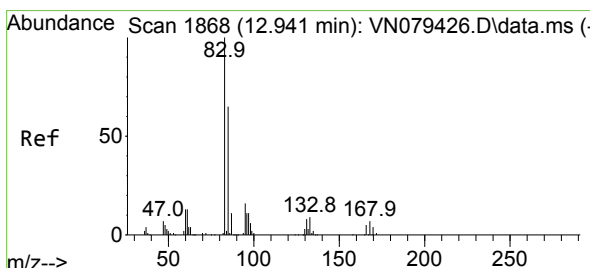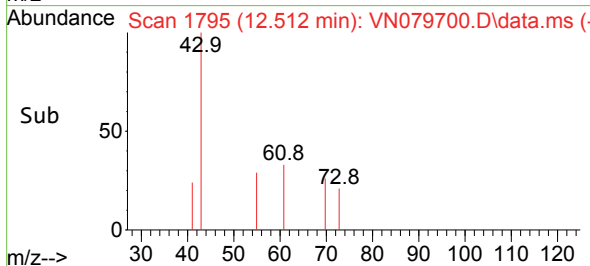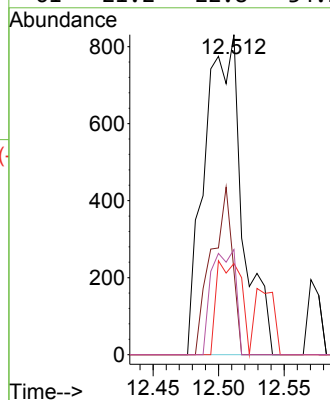

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.935 min Scan# 1867

Delta R.T. -0.006 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24




Tgt Ion: 83 Resp: 932


Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 96.4 31.9 95.7#

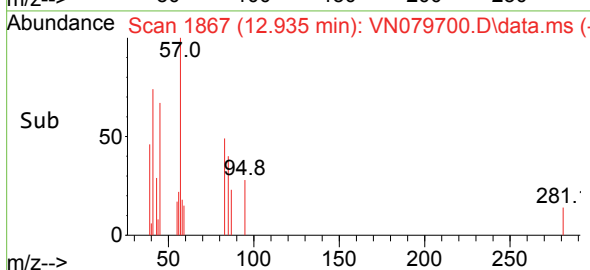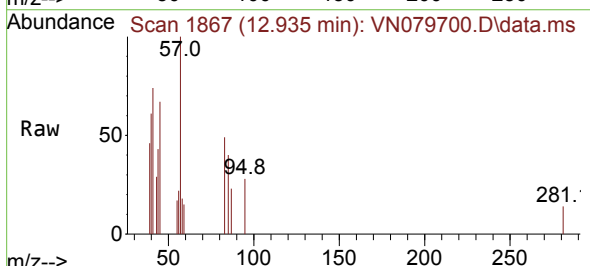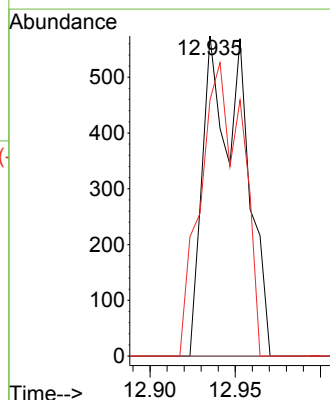



#76

1,2,3-Trichloropropane

Concen: 22.758 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 131804

Ion Ratio Lower Upper

75 100

77 1.2 84.5 253.5#

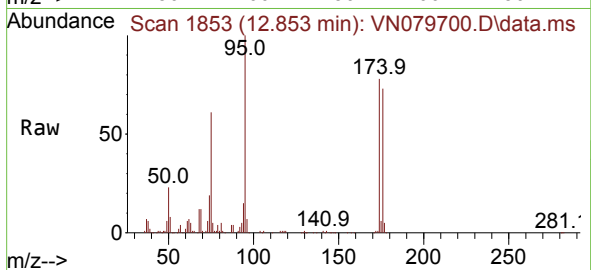

#81

trans-1,4-Dichloro-2-butene

Concen: 66.032 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24




Tgt Ion: 75 Resp: 131804


Ion Ratio Lower Upper

75 100

53 0.0 67.4 101.2#


89 0.0 38.8 58.2#

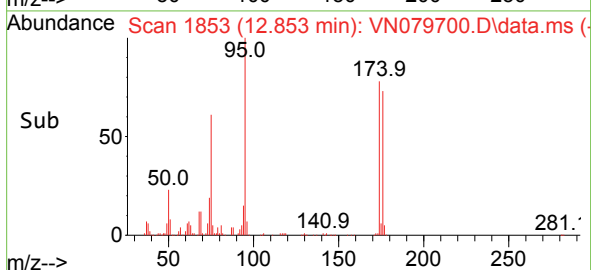






#82
4-Chlorotoluene
Concen: 0.218 ug/l
RT: 13.229 min Scan# 1916
Delta R.T. 0.006 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 91 Resp: 2802
Ion Ratio Lower Upper
91 100
126 34.9 16.7 50.0

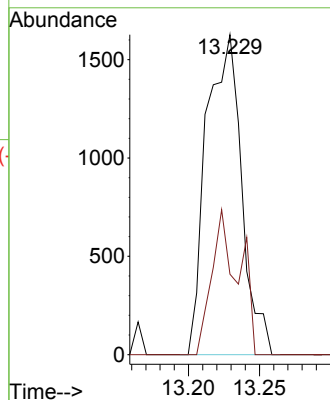


#87
1,3-Dichlorobenzene
Concen: 0.305 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. -0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24



Tgt Ion: 146 Resp: 2219
Ion Ratio Lower Upper
146 100
111 42.4 22.1 66.3
148 47.3 32.0 96.0

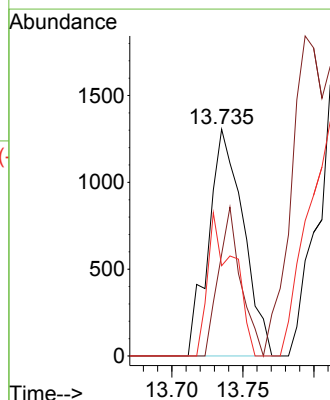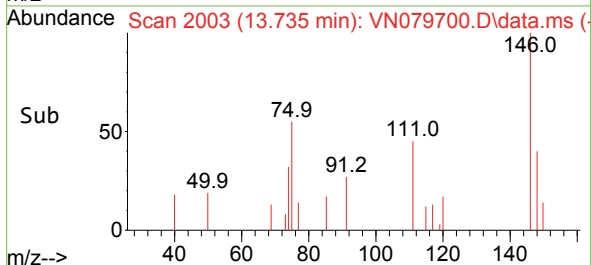



#88

1,4-Dichlorobenzene

Concen: 0.296 ug/l

RT: 13.735 min Scan# 2017

Delta R.T. -0.082 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:146 Resp: 2219

Ion Ratio Lower Upper

146 100

111 42.4 20.6 61.8

148 47.3 31.6 94.8

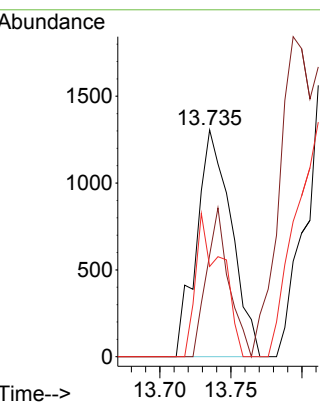

#89

n-Butylbenzene

Concen: 0.341 ug/l

RT: 14.059 min Scan# 2058

Delta R.T. -0.000 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24




Tgt Ion: 91 Resp: 3518


Ion Ratio Lower Upper

91 100

92 49.1 26.4 79.0

134 23.1 12.6 37.6

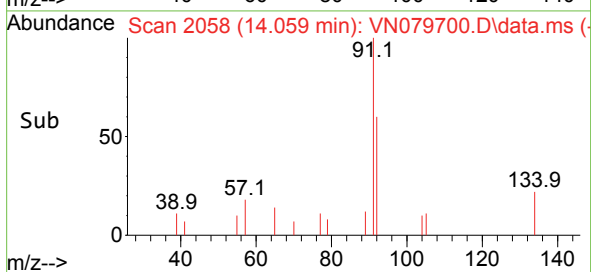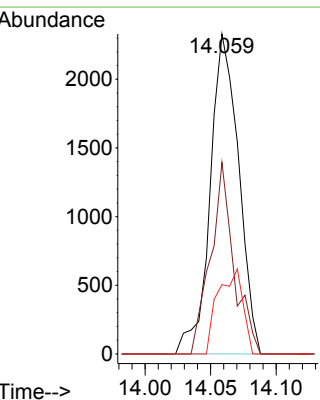



#90

Hexachloroethane

Concen: Below Cal

RT: 14.323 min Scan# 2105

Delta R.T. -0.012 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:117 Resp: 271

Ion Ratio Lower Upper

117 100

201 0.0 29.3 88.0#



#91

1,2-Dichlorobenzene

Concen: 0.333 ug/l

RT: 14.117 min Scan# 2068

Delta R.T. 0.006 min

Lab File: VN079700.D

Acq: 26 Oct 2023 17:24




Tgt Ion:146 Resp: 2358


Ion Ratio Lower Upper

146 100

111 46.9 22.0 66.0

148 63.0 31.8 95.3


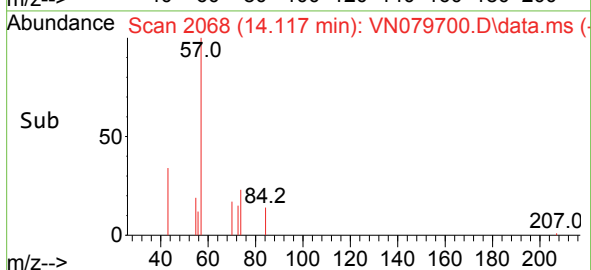






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.286 ug/l
 RT: 14.723 min Scan# 2171
 Delta R.T. -0.000 min
 Lab File: VN079700.D
 Acq: 26 Oct 2023 17:24




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 309
 Ion Ratio Lower Upper
 75 100
 155 70.2 39.1 117.2
 157 127.5 50.3 150.9



#93
 1,2,4-Trichlorobenzene
 Concen: 1.136 ug/l
 RT: 15.400 min Scan# 2286
 Delta R.T. -0.000 min
 Lab File: VN079700.D
 Acq: 26 Oct 2023 17:24


Tgt Ion: 180 Resp: 2494
 Ion Ratio Lower Upper
 180 100
 182 97.5 46.1 138.2
 145 28.8 16.6 49.8

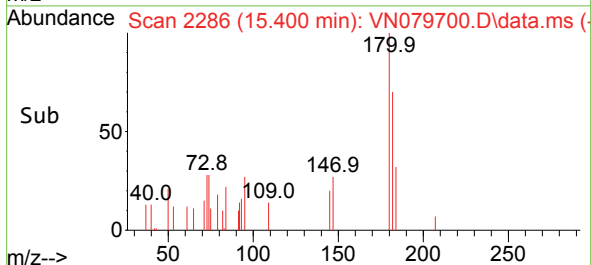






#94
Hexachlorobutadiene
Concen: 0.804 ug/l
RT: 15.500 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:225 Resp: 1374
Ion Ratio Lower Upper
225 100
223 84.6 31.3 93.8
227 64.9 31.9 95.9

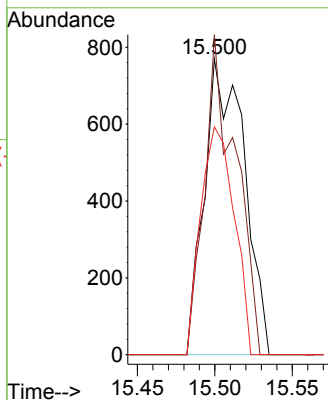


#95
Naphthalene
Concen: 1.421 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN079700.D
Acq: 26 Oct 2023 17:24




Tgt Ion:128 Resp: 9526
Ion Ratio Lower Upper
128 100
127 13.5 10.0 15.0
129 11.3 8.7 13.1

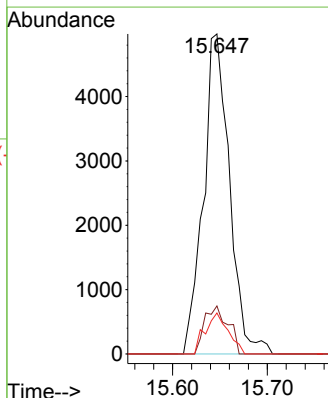



#96
 1,2,3-Trichlorobenzene
 Concen: 1.039 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN079700.D
 Acq: 26 Oct 2023 17:24

Instrument :
 MSVOA_N
 ClientSampleId :

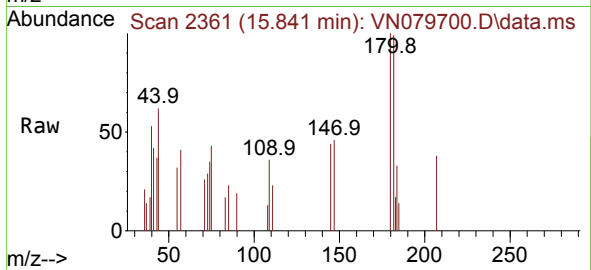

Tgt Ion	Ratio	Lower	Upper
180	100		
182	97.0	46.2	138.6
145	44.0	17.5	52.6

