

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102623\
 Data File : VN079700.D
 Acq On : 26 Oct 2023 17:24
 Operator : JC\MD
 Sample : 04980-02
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SEWER-SLUDGE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Title : SW846 8260

Signal : TIC: VN079700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.295	51	58	67	rBV2	13418	31302	1.90%	0.297%
2	2.659	116	120	127	rBV	11607	21053	1.28%	0.200%
3	3.877	311	327	344	rBV	169150	592686	36.06%	5.629%
4	5.500	600	603	614	rVB	11576	24760	1.51%	0.235%
5	8.165	1046	1056	1061	rBV	255437	629446	38.30%	5.978%
6	8.224	1061	1066	1082	rVB	384590	842087	51.24%	7.998%
7	8.582	1117	1127	1138	rBV	259406	589367	35.86%	5.598%
8	9.100	1206	1215	1226	rBV	590996	1219210	74.19%	11.580%
9	10.571	1456	1465	1480	rBV	876334	1643394	100.00%	15.608%
10	11.871	1678	1686	1698	rBV	888171	1587928	96.62%	15.081%
11	12.853	1844	1853	1864	rBV	703044	1212742	73.79%	11.518%
12	12.959	1864	1871	1881	rBV2	42190	94809	5.77%	0.900%
13	13.653	1978	1989	1994	rBV6	9426	21775	1.33%	0.207%
14	13.735	1994	2003	2007	rBV8	8086	18858	1.15%	0.179%
15	13.794	2007	2013	2020	rBV	775393	1323530	80.54%	12.570%
16	14.000	2042	2048	2055	rBV4	10155	20675	1.26%	0.196%
17	14.141	2068	2072	2077	rVB2	12388	17891	1.09%	0.170%
18	14.253	2084	2091	2100	rBV	285586	469101	28.54%	4.455%
19	14.500	2126	2133	2137	rBV4	12276	22895	1.39%	0.217%
20	14.741	2165	2174	2183	rBV7	10917	31255	1.90%	0.297%
21	15.388	2277	2284	2290	rBV6	16242	33118	2.02%	0.315%
22	15.653	2323	2329	2335	rVB3	11853	24852	1.51%	0.236%
23	15.841	2356	2361	2367	rBV5	9478	20943	1.27%	0.199%
24	16.417	2452	2459	2467	rBV6	15844	35330	2.15%	0.336%




Sum of corrected areas: 10529007

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102623\
Data File : VN079700.D
Acq On : 26 Oct 2023 17:24
Operator : JC\MD
Sample : 04980-02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SEWER-SLUDGE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

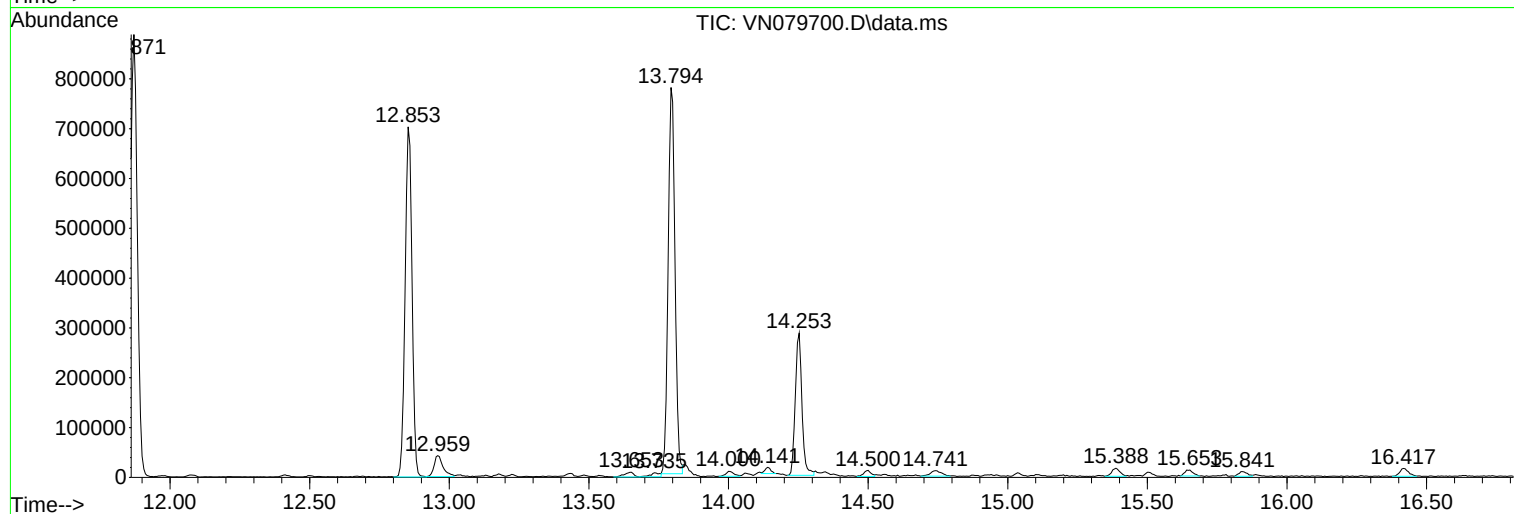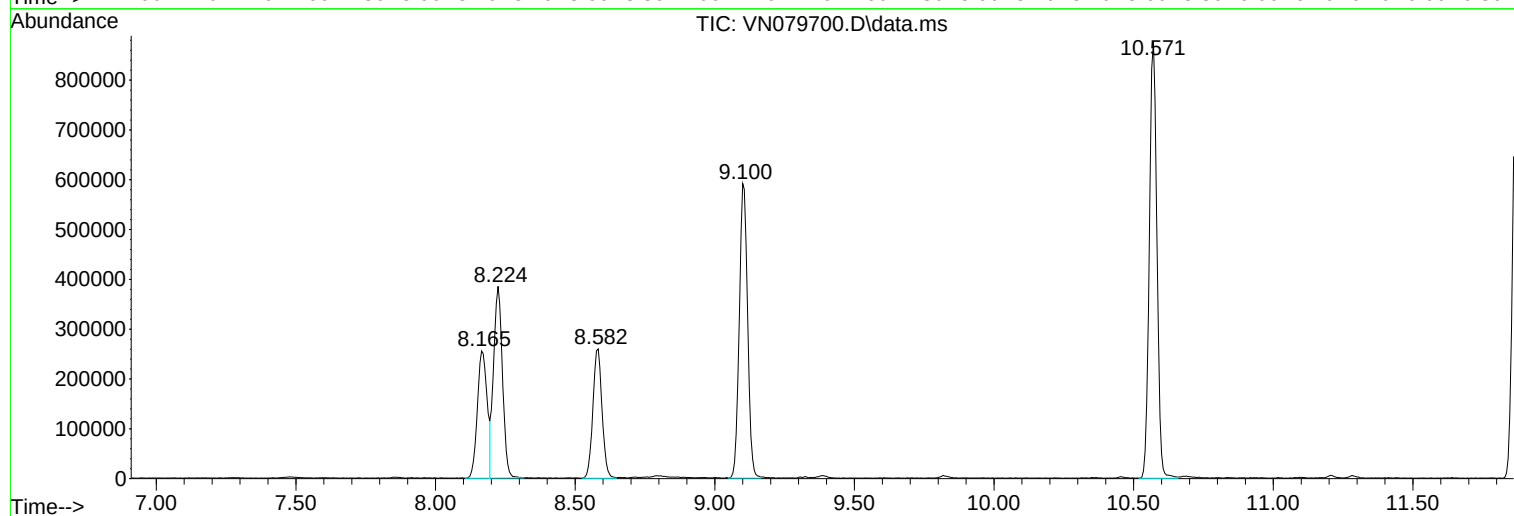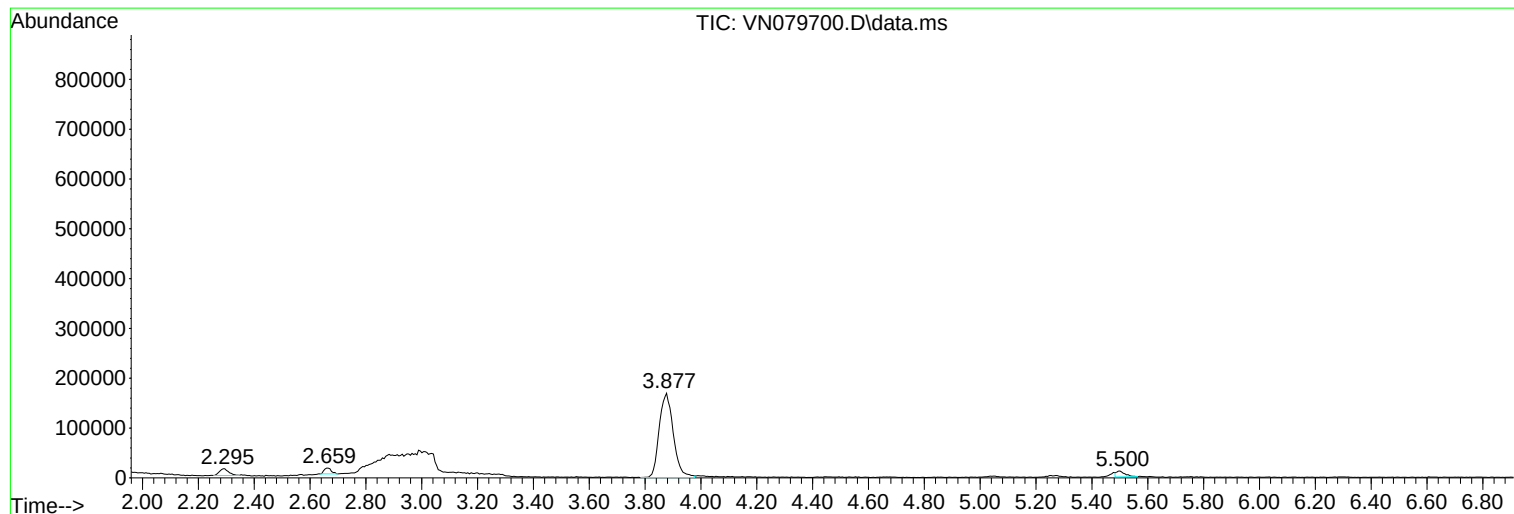

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102623\
Data File : VN079700.D
Acq On : 26 Oct 2023 17:24
Operator : JC\MD
Sample : 04980-02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SEWER-SLUDGE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102623\
Data File : VN079700.D
Acq On : 26 Oct 2023 17:24
Operator : JC\MD
Sample : 04980-02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SEWER-SLUDGE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------