
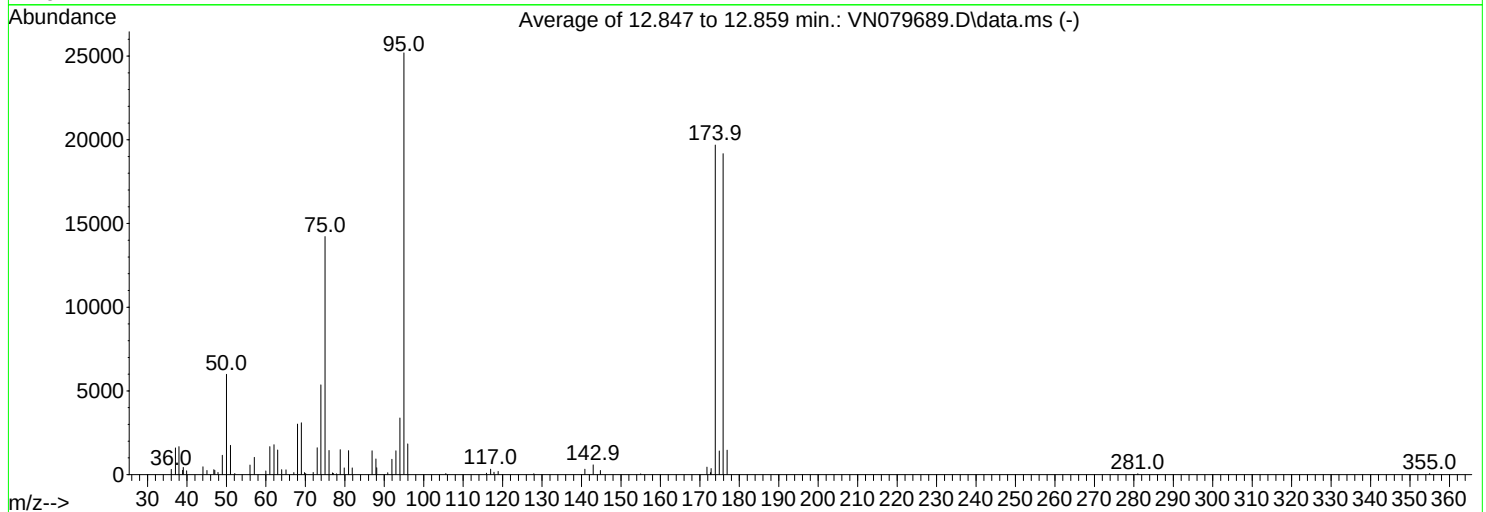


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN102623\  
Data File : VN079689.D  
Acq On : 26 Oct 2023 09:18  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N100523W.M  
Title : SW846 8260  
Last Update : Fri Oct 06 03:34:49 2023

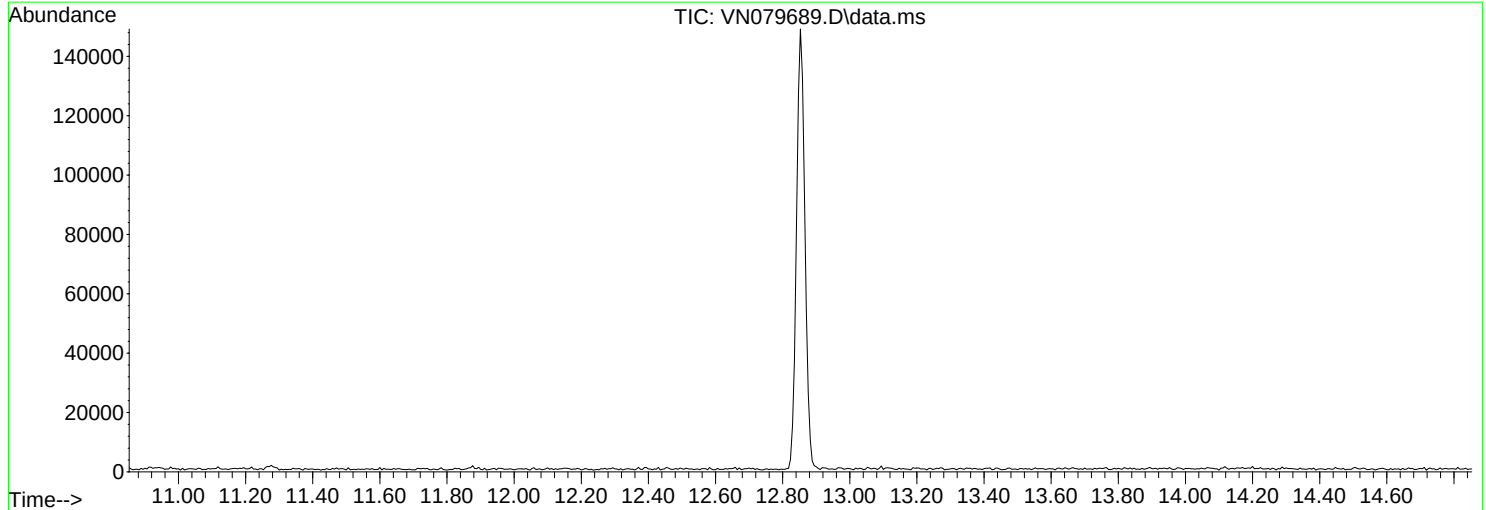

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 23.8  | 5990  | PASS      |
| 75     | 95      | 30     | 60     | 56.4  | 14220 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 25192 | PASS      |
| 96     | 95      | 5      | 9      | 7.3   | 1831  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.8   | 359   | PASS      |
| 174    | 95      | 50     | 100    | 78.2  | 19688 | PASS      |
| 175    | 174     | 5      | 9      | 7.2   | 1412  | PASS      |
| 176    | 174     | 95     | 101    | 97.4  | 19168 | PASS      |
| 177    | 176     | 5      | 9      | 7.6   | 1460  | PASS      |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.00 | 314    | 48.95 | 1153   | 65.10 | 288    | 76.90 | 101    |
| 37.05 | 1593   | 50.00 | 5990   | 67.10 | 128    | 77.10 | 61     |
| 37.95 | 1669   | 51.00 | 1748   | 68.00 | 3018   | 77.90 | 51     |
| 38.90 | 261    | 52.10 | 67     | 69.00 | 3094   | 78.85 | 149    |
| 39.05 | 428    | 55.95 | 571    | 69.80 | 127    | 79.85 | 405    |
| 39.90 | 234    | 57.05 | 1034   | 70.10 | 70     | 80.95 | 1436   |
| 44.05 | 468    | 60.00 | 224    | 72.00 | 134    | 81.90 | 406    |
| 45.05 | 245    | 61.00 | 1671   | 73.00 | 1604   | 86.90 | 1424   |
| 46.80 | 298    | 62.05 | 1784   | 73.95 | 5358   | 87.90 | 933    |
| 47.05 | 259    | 63.00 | 1470   | 75.00 | 14220  | 88.10 | 412    |
| 47.85 | 134    | 64.00 | 298    | 76.00 | 1440   | 90.90 | 115    |

Average of 12.847 to 12.859 min.: VN079689.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 91.95  | 919    | 140.85 | 327    | 281.00 | 54     |     |        |
| 92.95  | 1428   | 142.95 | 587    | 355.00 | 65     |     |        |
| 93.95  | 3380   | 144.80 | 253    |        |        |     |        |
| 95.00  | 25192  | 155.00 | 51     |        |        |     |        |
| 95.95  | 1831   | 171.80 | 451    |        |        |     |        |
| 105.60 | 64     | 172.70 | 126    |        |        |     |        |
| 115.90 | 87     | 172.85 | 359    |        |        |     |        |
| 116.95 | 328    | 173.90 | 19688  |        |        |     |        |
| 117.80 | 145    | 174.90 | 1412   |        |        |     |        |
| 118.85 | 193    | 175.90 | 19168  |        |        |     |        |
| 127.90 | 56     | 176.90 | 1460   |        |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB