


1,2,3-Trichlorobenzene

Response Ratio

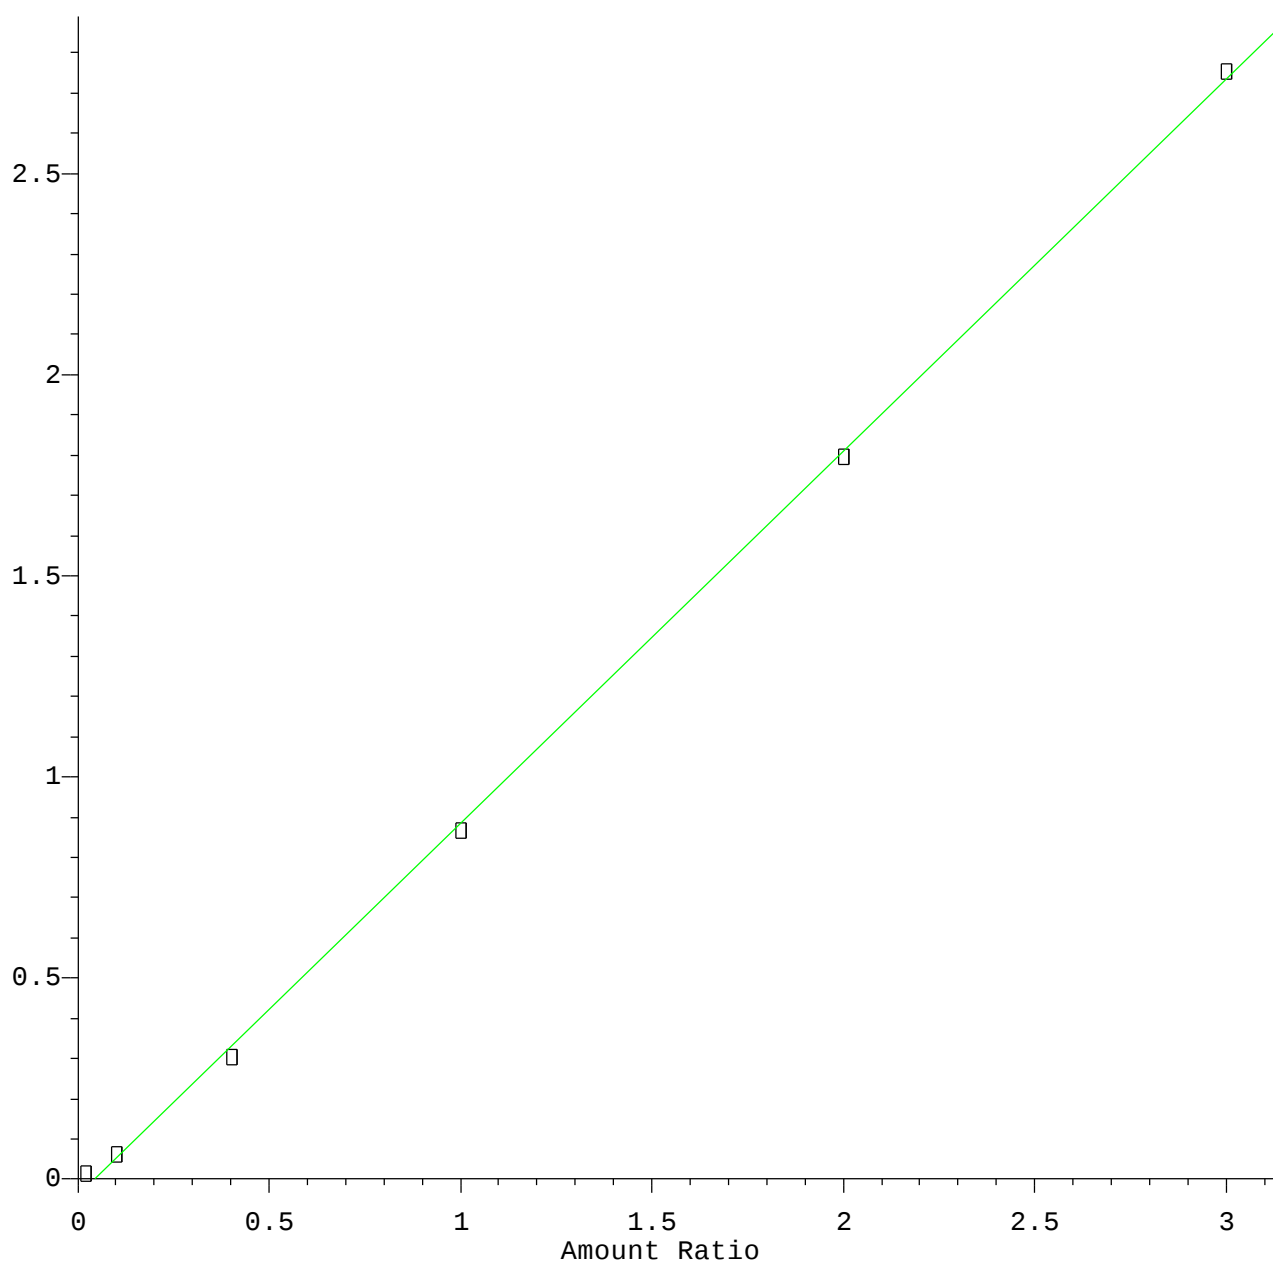


Resp Ratio = 9.25e-001 * Amt - 4.03e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Calibration Table Last Updated: Tue Oct 27 12:23:17 2020

Naphthalene

Response Ratio

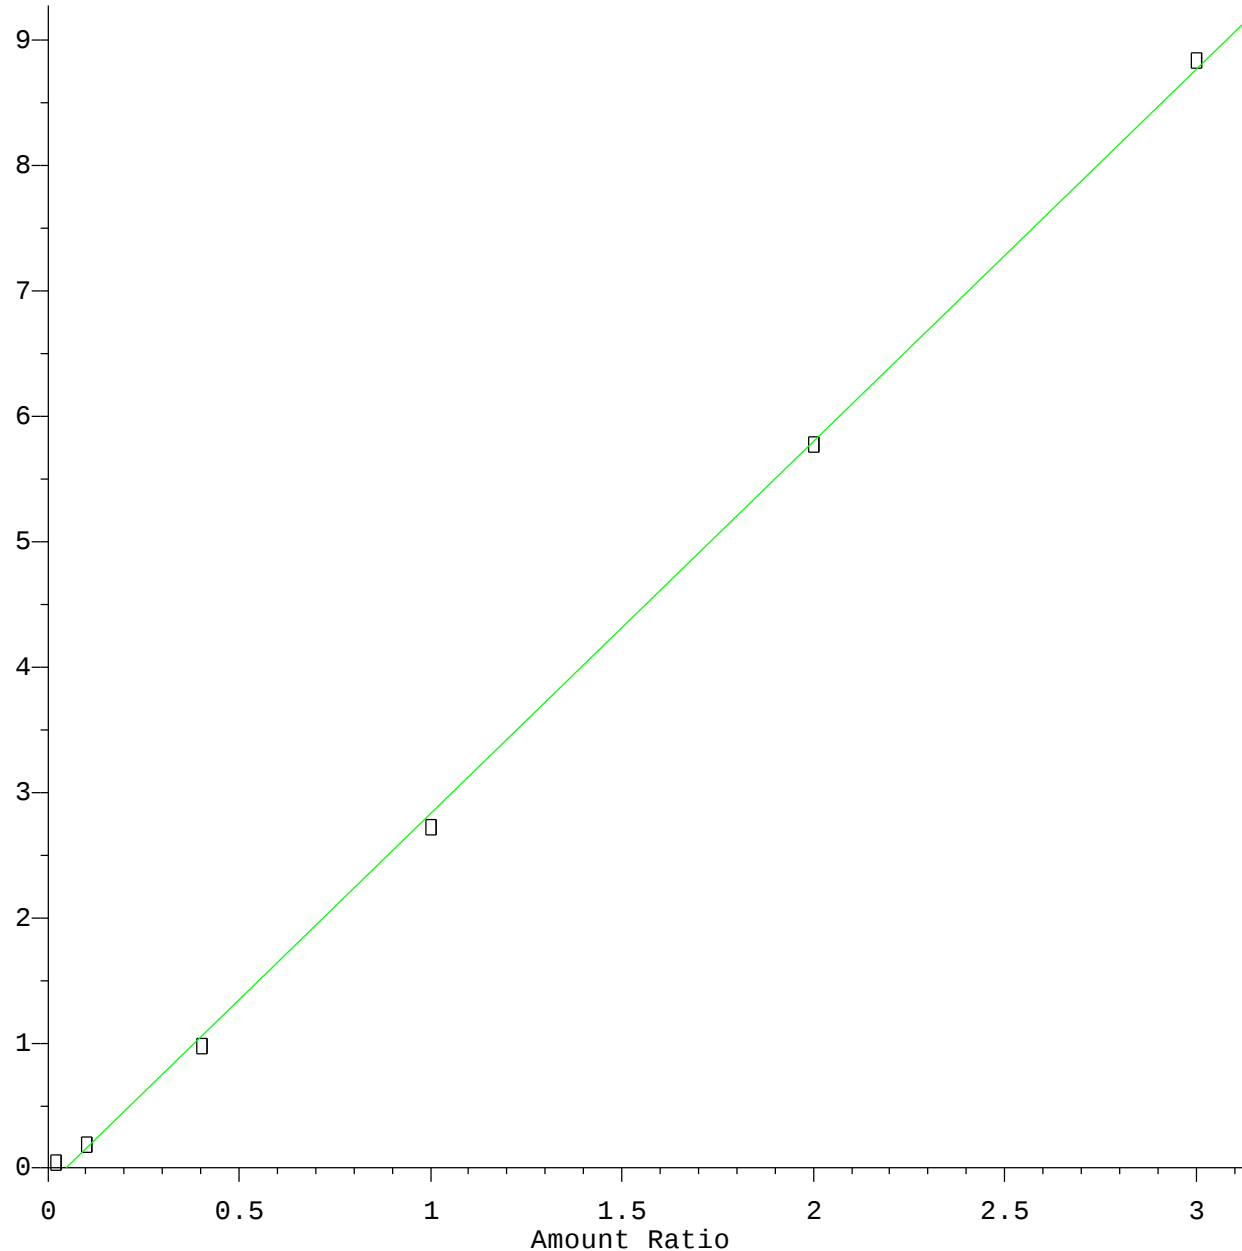


Resp Ratio = 2.97e+000 * Amt - 1.42e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Calibration Table Last Updated: Tue Oct 27 12:23:17 2020


1,2,4-Trichlorobenzene

Response Ratio

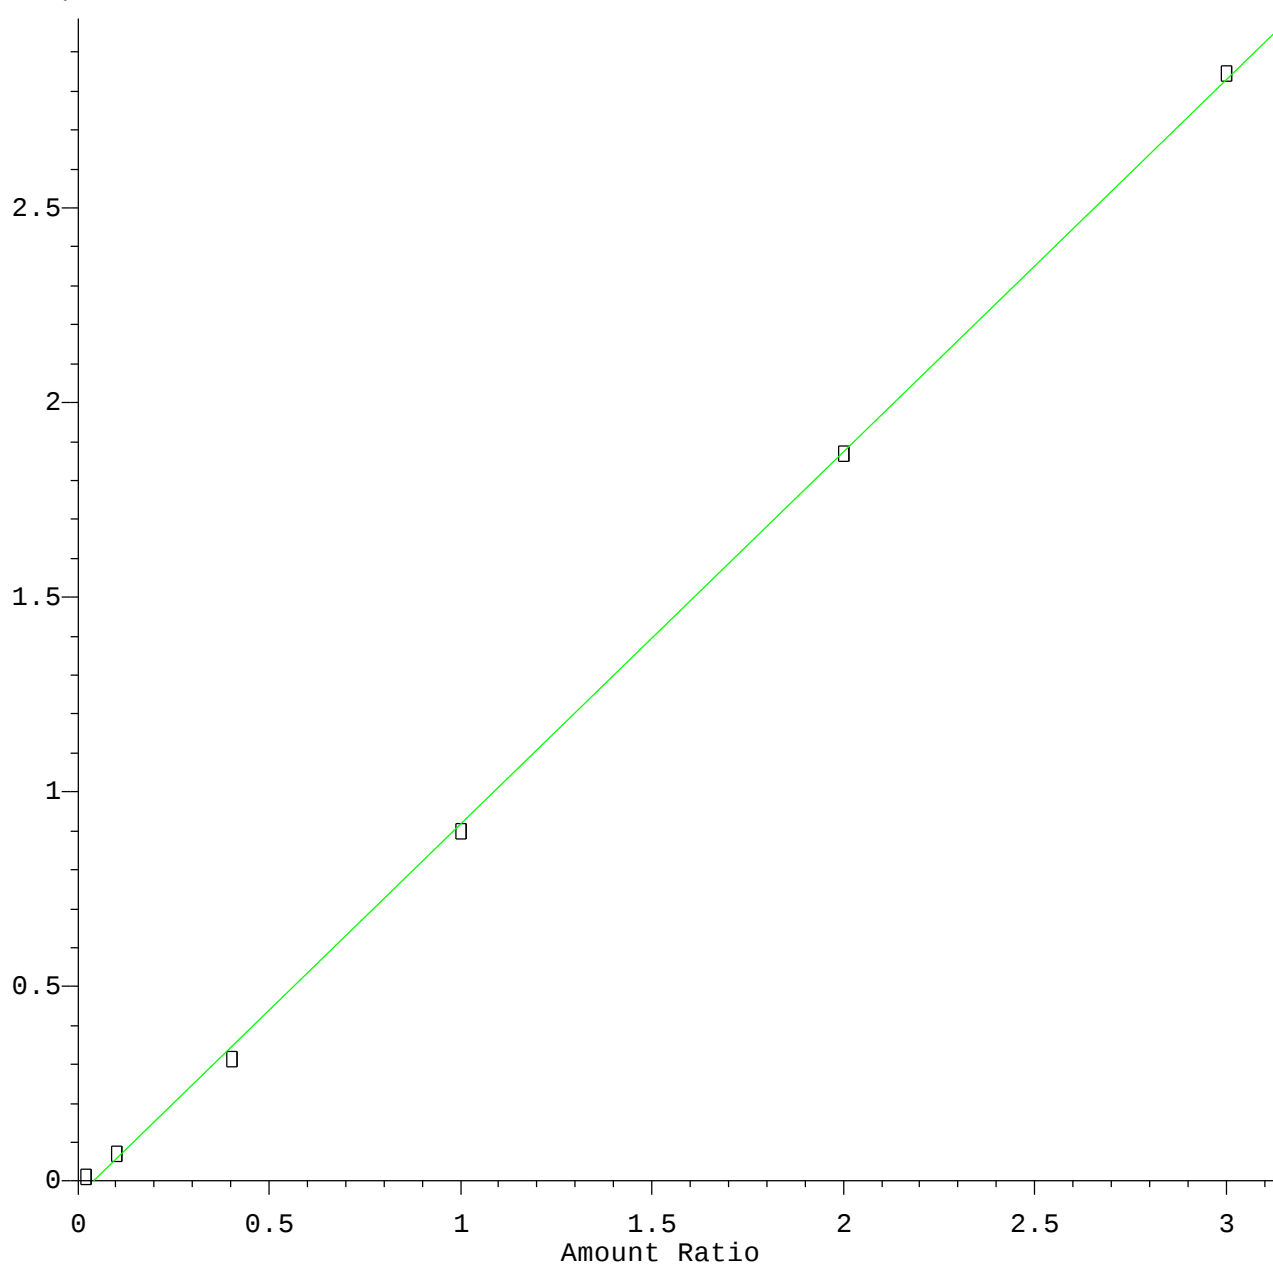


Resp Ratio = $9.56 \times 10^{-1} \times \text{Amt} - 3.86 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Calibration Table Last Updated: Tue Oct 27 12:23:17 2020

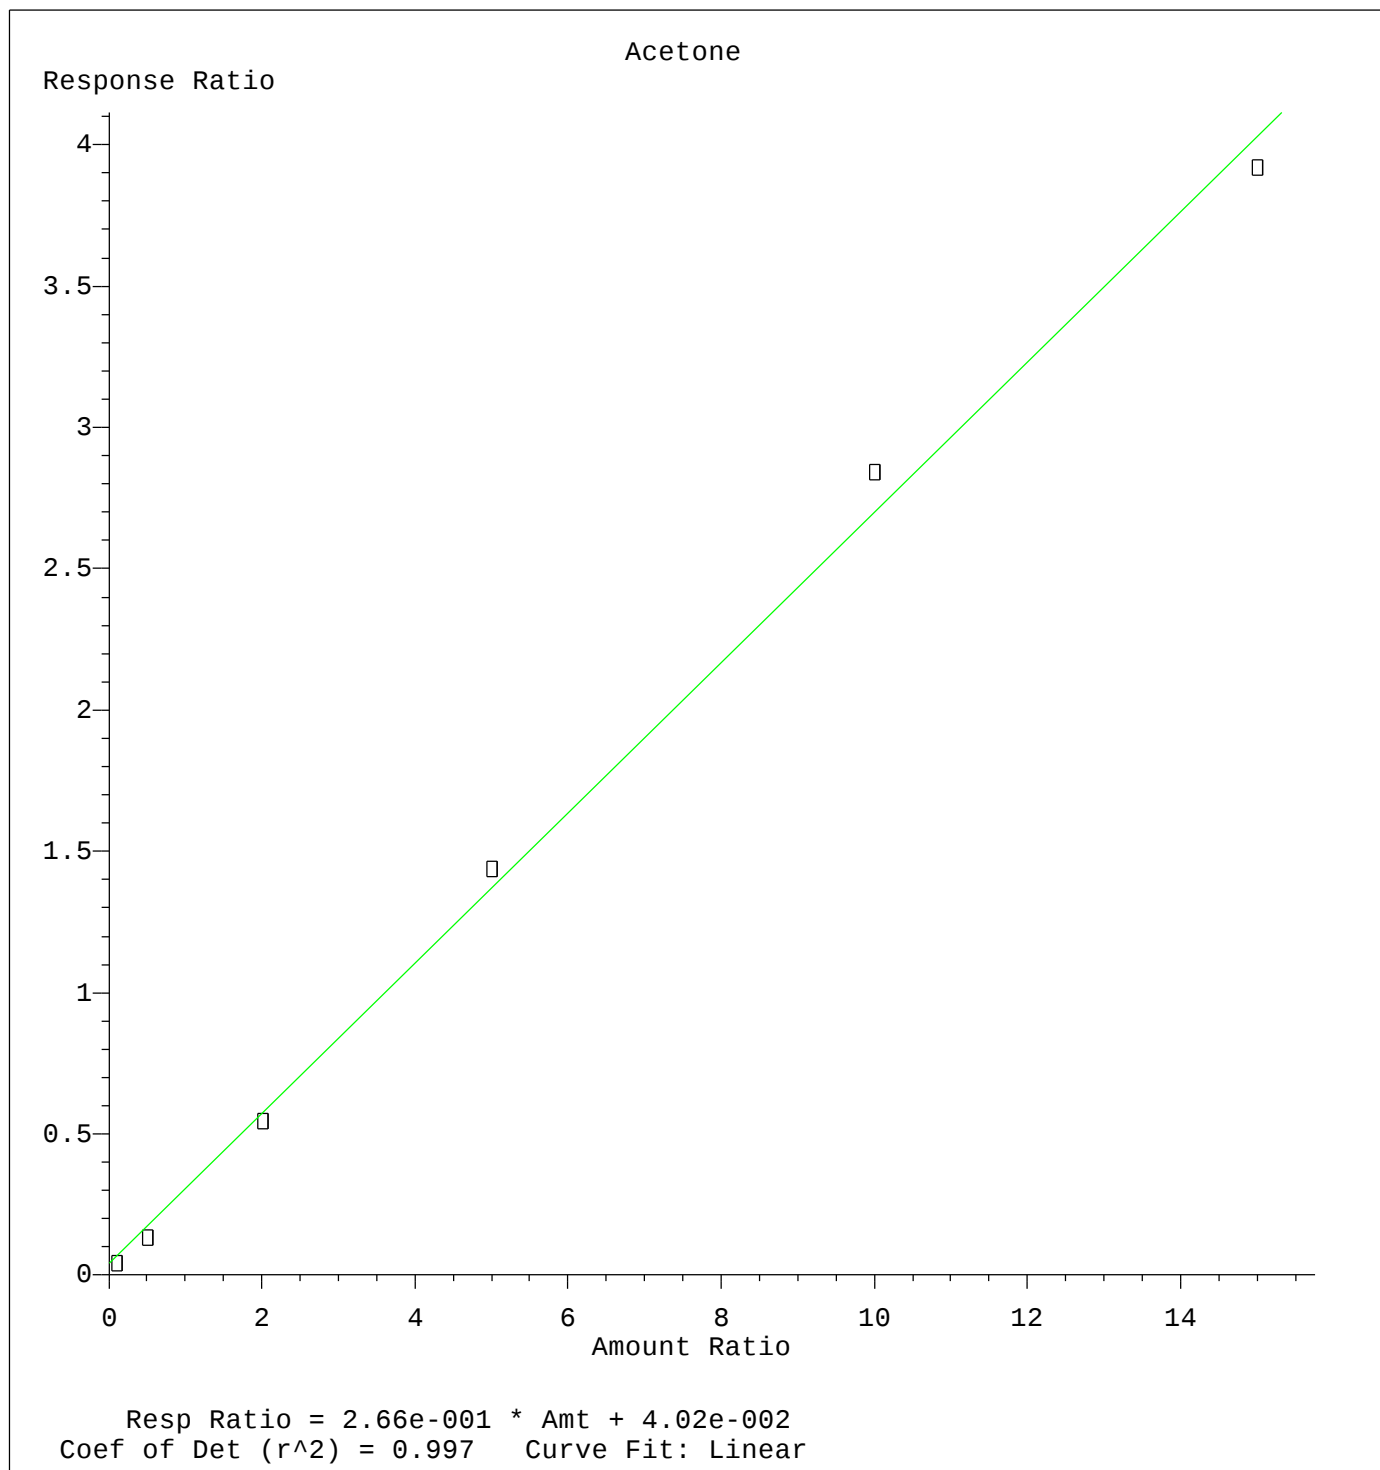

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Calibration Table Last Updated: Tue Oct 27 12:23:17 2020

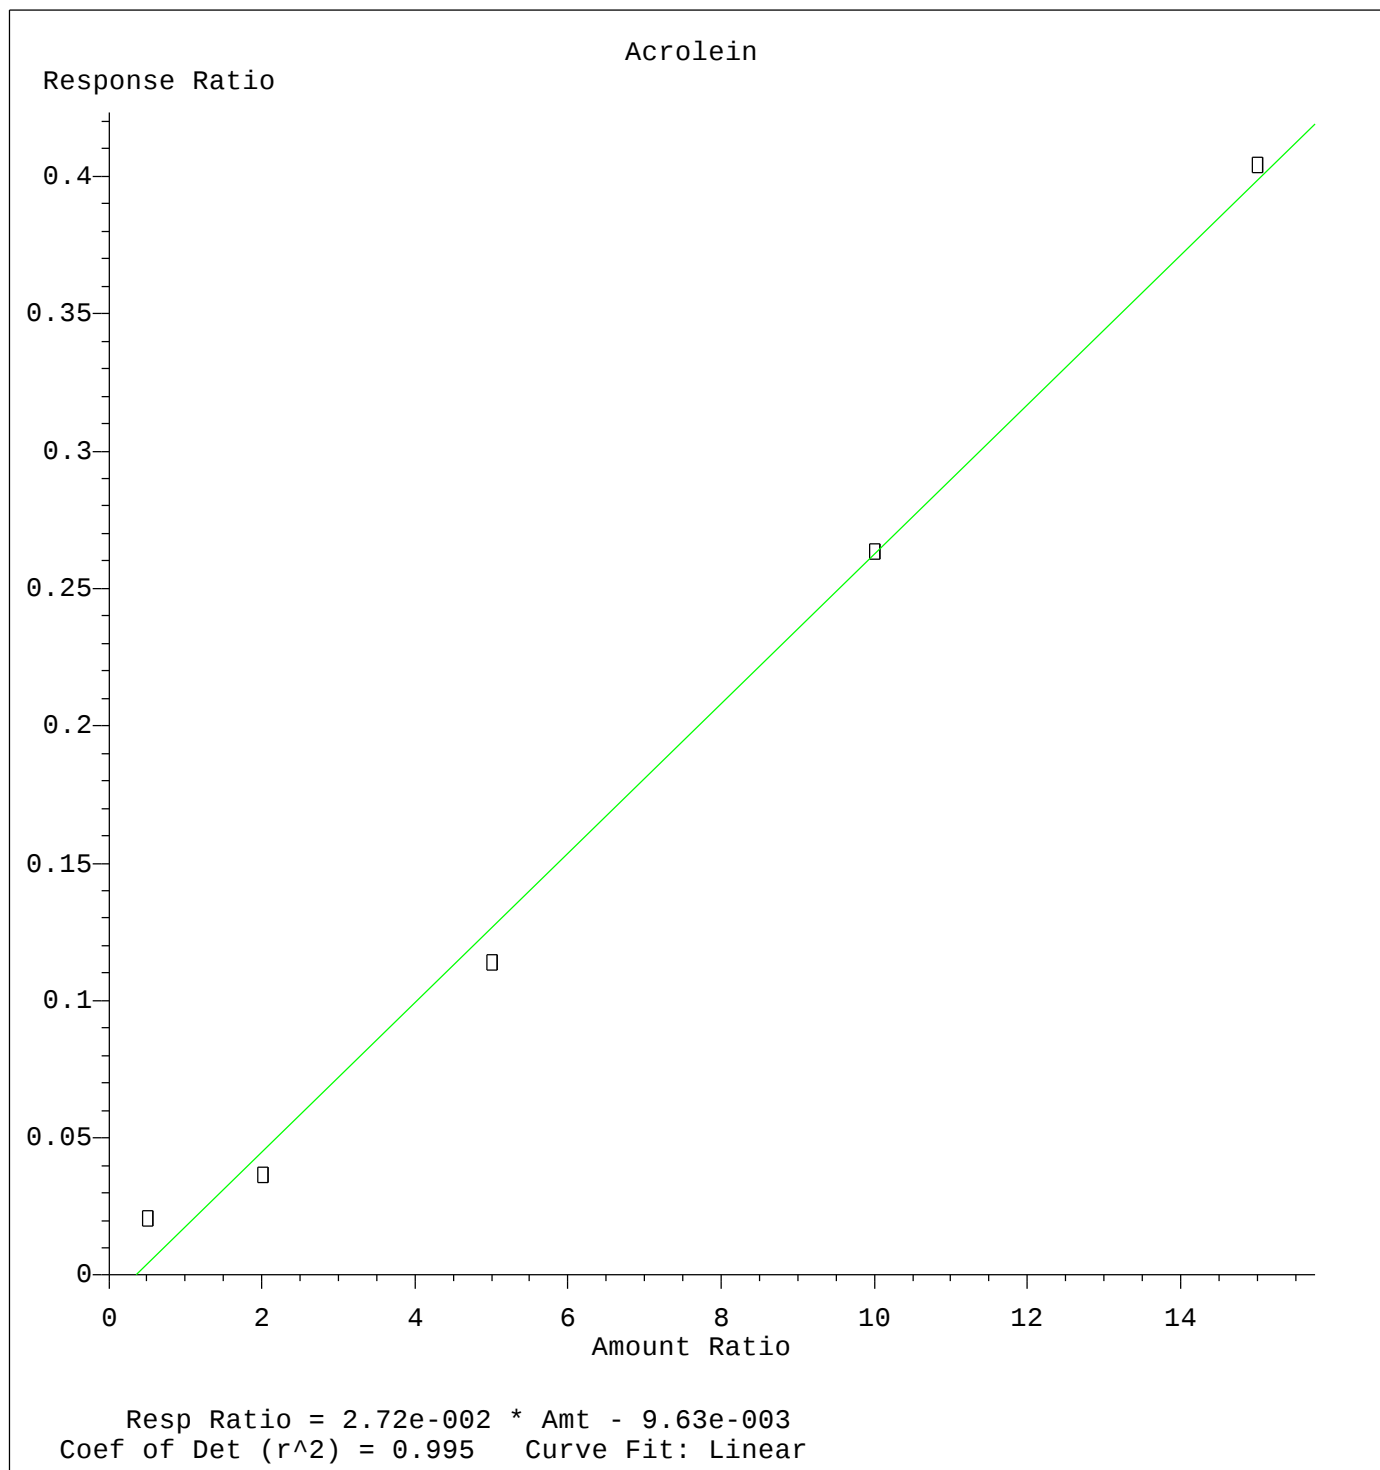

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Calibration Table Last Updated: Tue Oct 27 12:23:17 2020