

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102720\  
Data File : VN064337.D  
Acq On : 27 Oct 2020 19:37  
Operator : JC/MD  
Sample : L4520-01  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PS-FRAC

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON  
Sampling : 1  
Start Thrs: 0.2  
Stop Thrs : 0

Filtering: 5  
Min Area: 3 % of largest Peak  
Max Peaks: 100  
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N102720W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.241       | 455           | 467         | 483          | rBV3     | 7289           | 19943         | 1.52%           | 0.272%        |
| 2         | 7.547       | 1787          | 1806        | 1818         | rBV2     | 171358         | 428146        | 32.68%          | 5.832%        |
| 3         | 7.624       | 1818          | 1830        | 1853         | rVB      | 290076         | 696545        | 53.16%          | 9.488%        |
| 4         | 7.987       | 1923          | 1943        | 1961         | rBV      | 192818         | 451447        | 34.46%          | 6.150%        |
| 5         | 8.550       | 2102          | 2118        | 2137         | rBV      | 455302         | 944814        | 72.11%          | 12.870%       |
| 6         | 10.061      | 2573          | 2588        | 2603         | rBV      | 699309         | 1310197       | 100.00%         | 17.847%       |
| 7         | 11.379      | 2984          | 2998        | 3018         | rBV      | 731261         | 1270712       | 96.99%          | 17.309%       |
| 8         | 12.376      | 3292          | 3308        | 3328         | rBV      | 616444         | 1050149       | 80.15%          | 14.305%       |
| 9         | 13.318      | 3588          | 3601        | 3623         | rBV      | 681194         | 1169229       | 89.24%          | 15.927%       |


Sum of corrected areas: 7341182

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102720\  
Data File : VN064337.D  
Acq On : 27 Oct 2020 19:37  
Operator : JC/MD  
Sample : L4520-01  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PS-FRAC

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_N\METHODS\82N102720W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

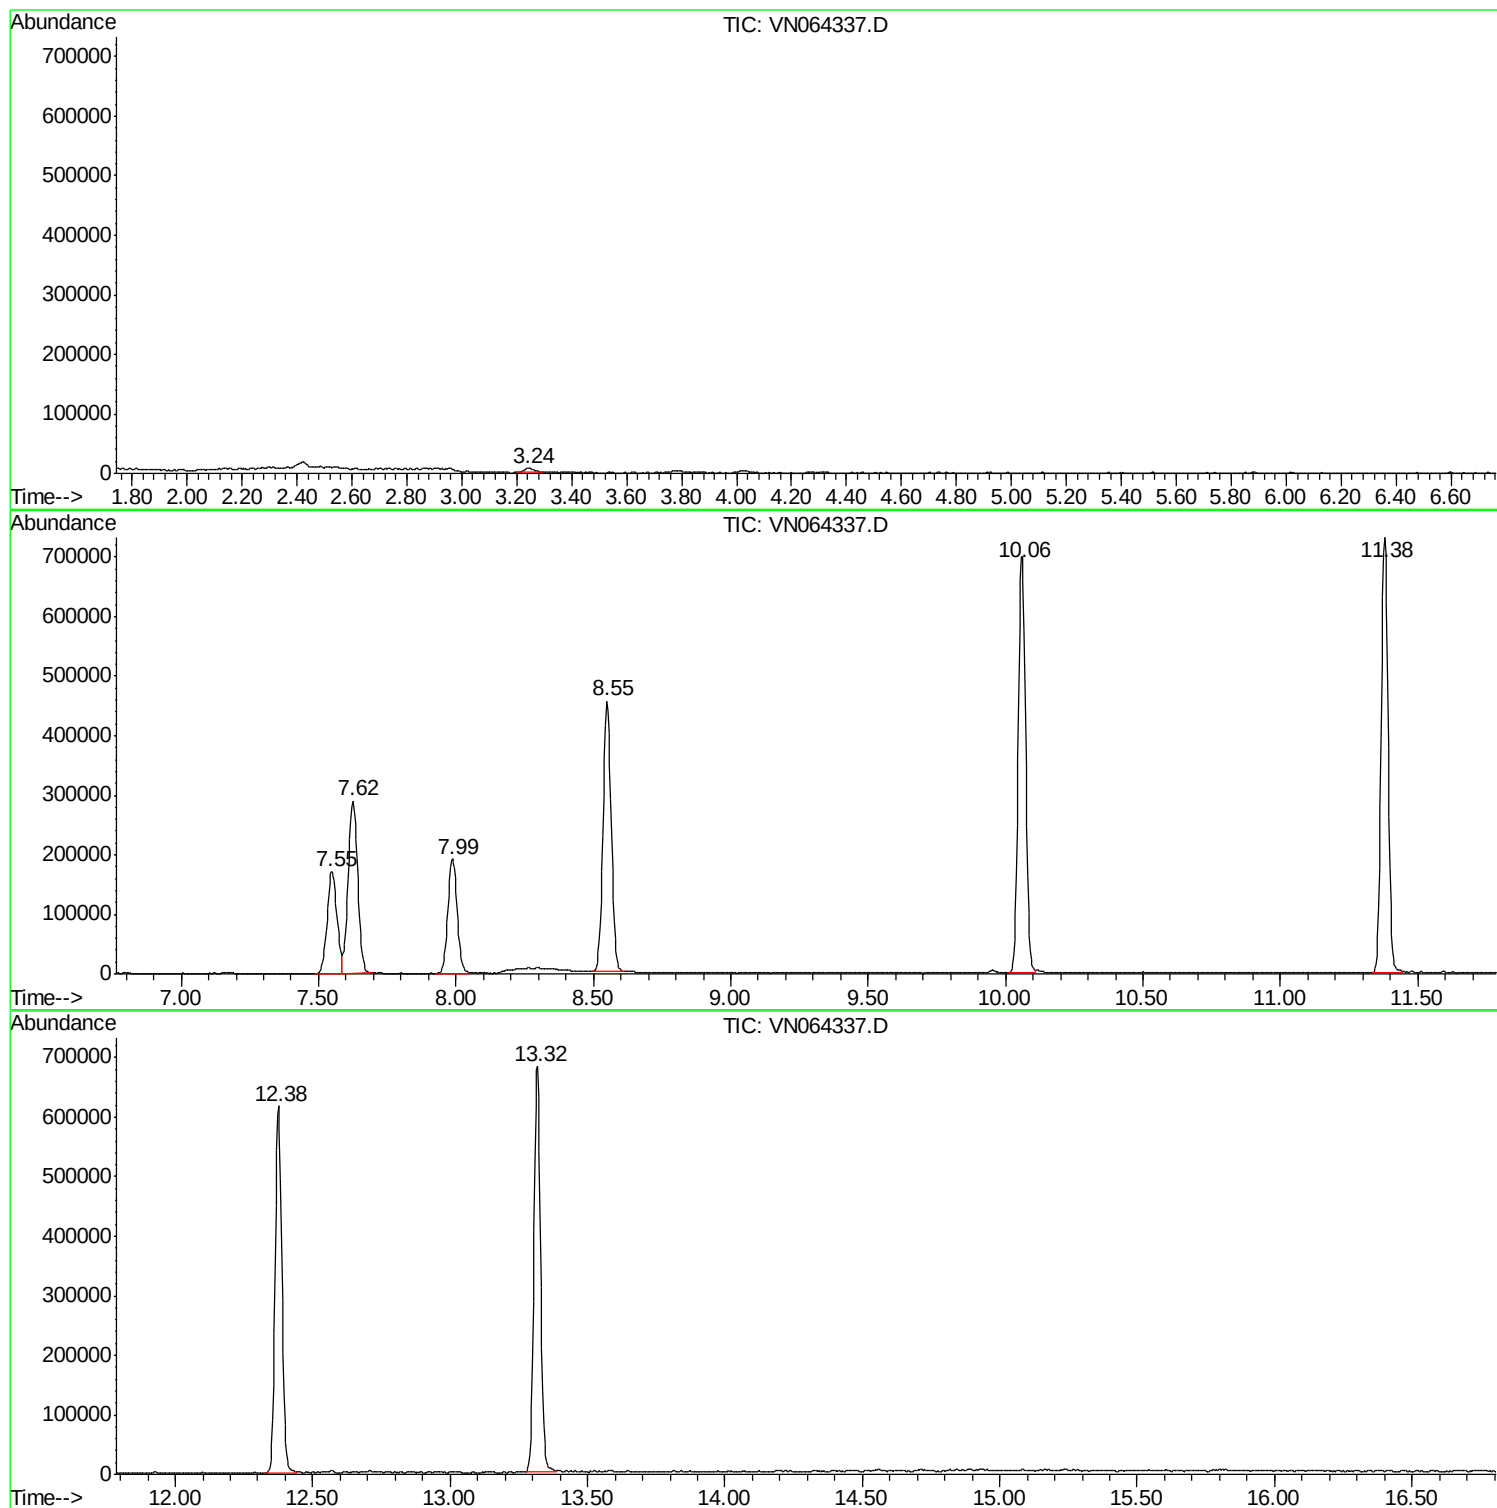

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_N\DATA\VN102720\  
Data File : VN064337.D  
Acq On : 27 Oct 2020 19:37  
Operator : JC/MD  
Sample : L4520-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PS-FRAC

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_N\METHODS\82N102720W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_N\DATA\VN102720\  
Data File : VN064337.D  
Acq On : 27 Oct 2020 19:37  
Operator : JC/MD  
Sample : L4520-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PS-FRAC

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_N\METHODS\82N102720W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |