


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102720\
 Data File : VN064316.D
 Acq On : 27 Oct 2020 9:26
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
 Title : SW846 8260
 Last Update : Tue Oct 27 12:23:17 2020

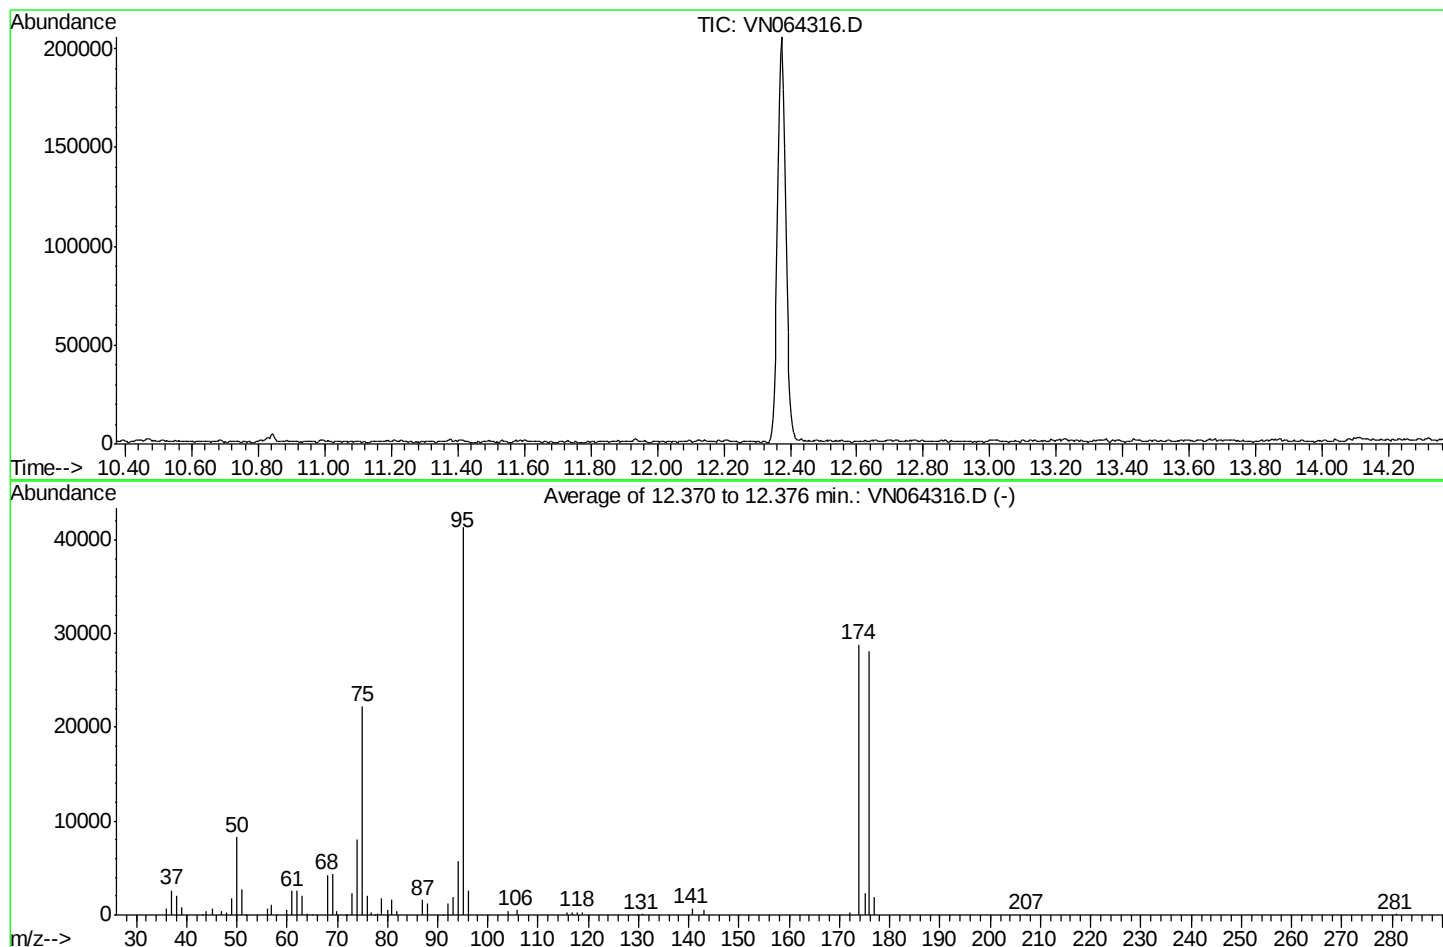

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	8273	PASS
75	95	30	60	53.8	22229	PASS
95	95	100	100	100.0	41330	PASS
96	95	5	9	6.4	2652	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.8	28837	PASS
175	174	5	9	8.2	2362	PASS
176	174	95	101	97.4	28074	PASS
177	176	5	9	7.0	1952	PASS