

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069183.D
 Acq On : 26 Oct 2021 14:14
 Operator : JC/MD
 Sample : M4337-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-5-PS

Quant Time: Oct 27 06:54:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	345102	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	597484	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	575868	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	220627	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	225810	49.628	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.260%
35) Dibromofluoromethane	8.024	113	174453	50.185	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.360%
50) Toluene-d8	10.446	98	740416	53.233	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	106.460%
62) 4-Bromofluorobenzene	12.734	95	269070	51.274	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	102.540%
Target Compounds						
16) Acetone	4.309	43	3880	2.285	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069183.D
Acq On : 26 Oct 2021 14:14
Operator : JC/MD
Sample : M4337-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS

Quant Time: Oct 27 06:54:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration



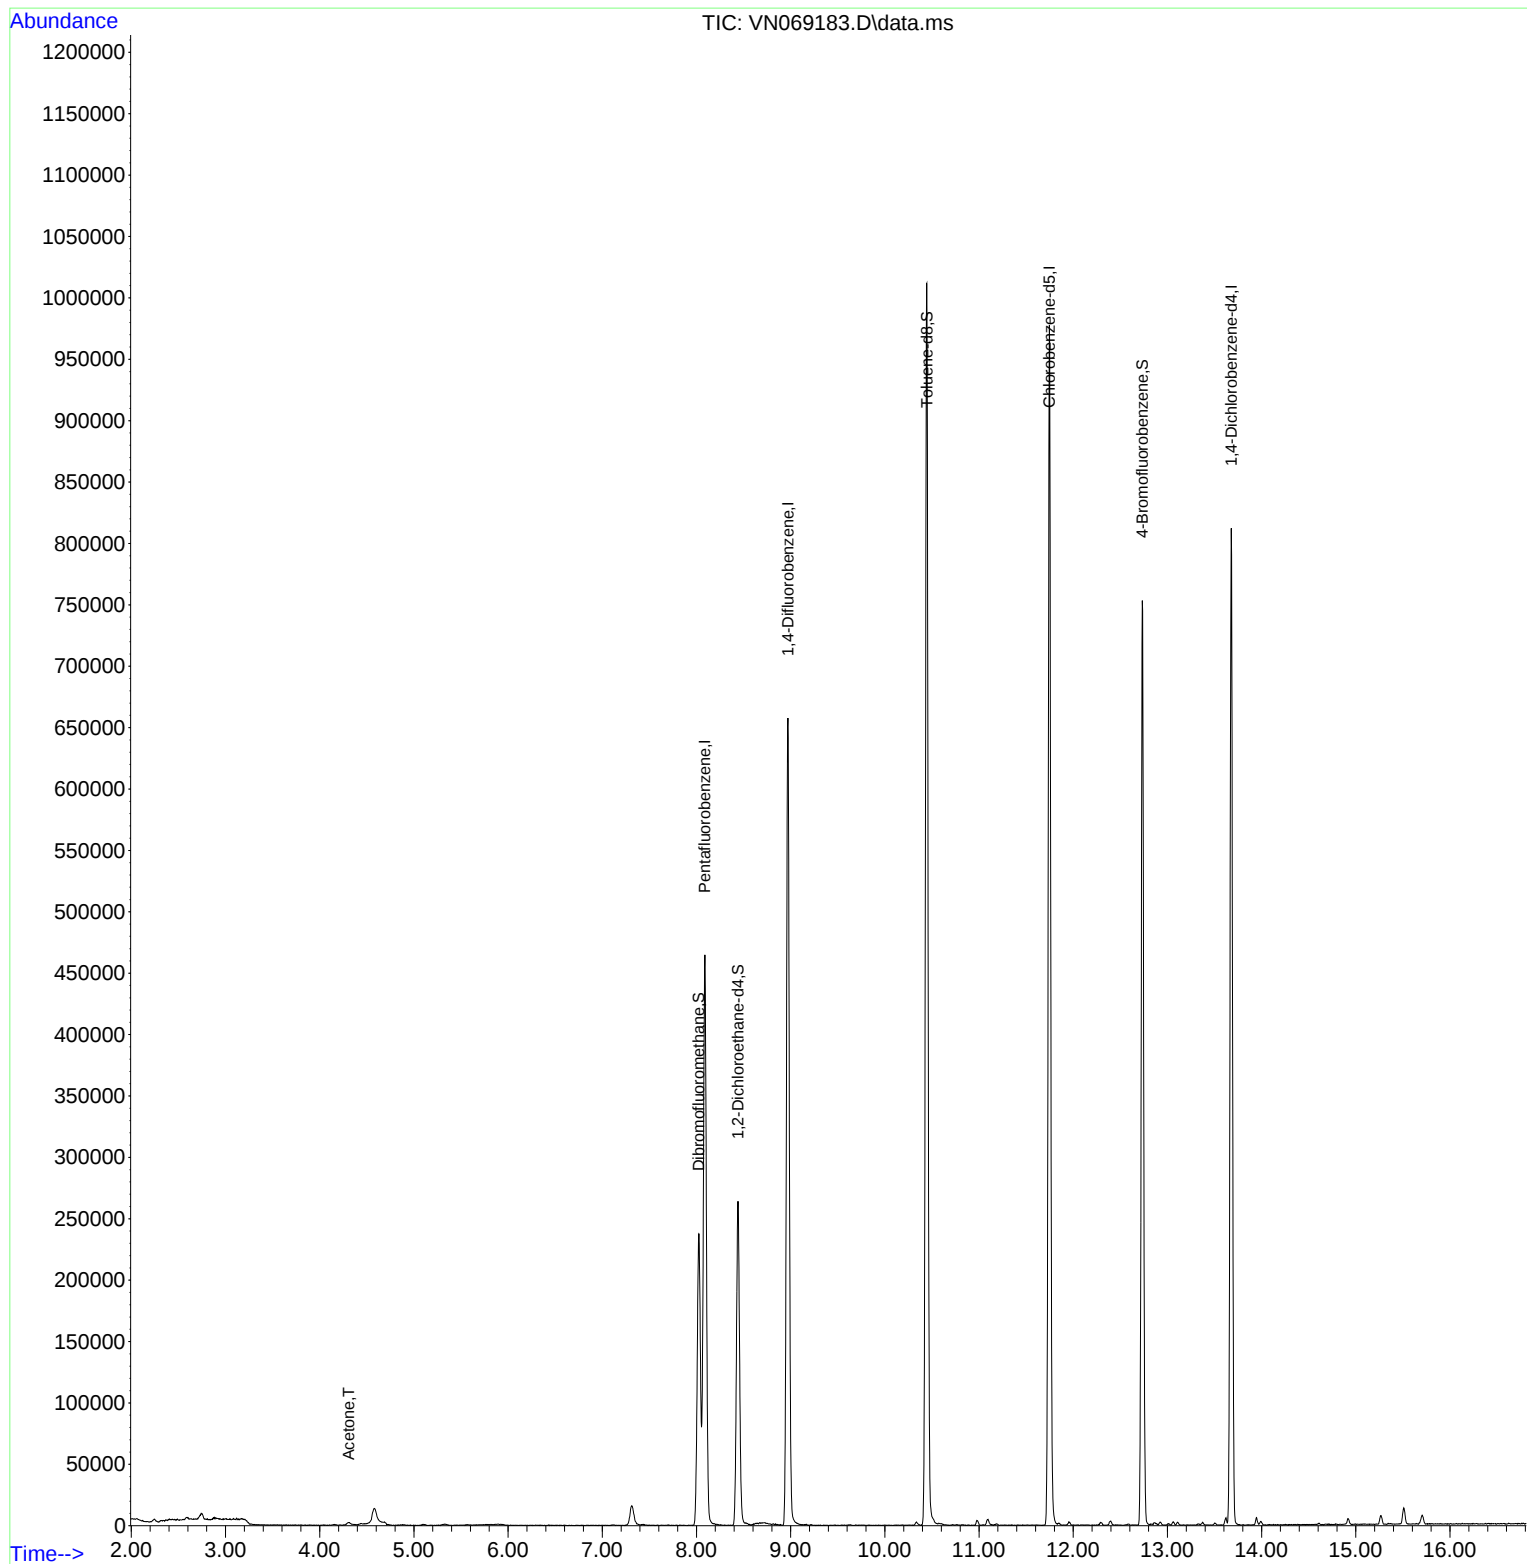


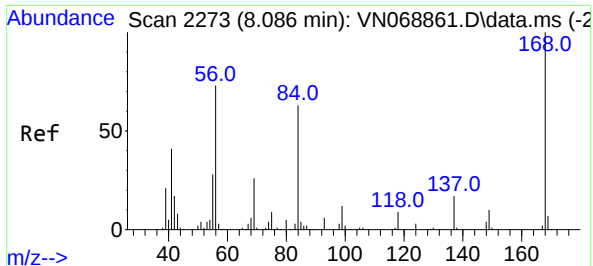

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14




Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS


Tgt Ion:168 Resp: 345102
Ion Ratio Lower Upper
168 100
99 60.0 48.9 73.3

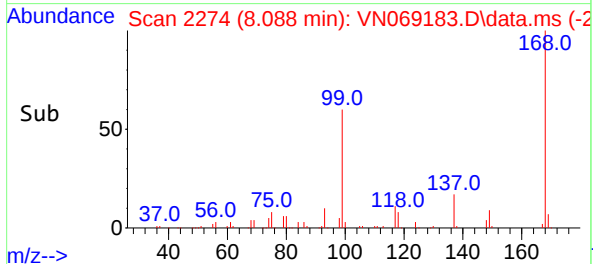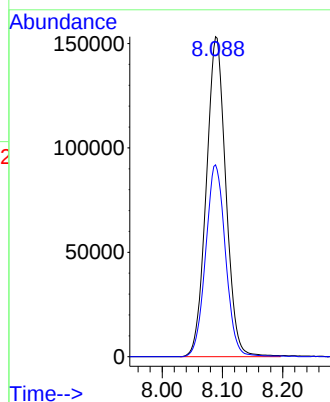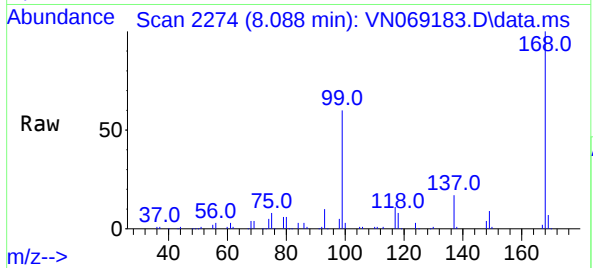

#16
Acetone
Concen: 2.285 ug/l
RT: 4.309 min Scan# 865
Delta R.T. 0.024 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14

Tgt Ion: 43 Resp: 3880
Ion Ratio Lower Upper
43 100
58 30.0 24.5 36.7

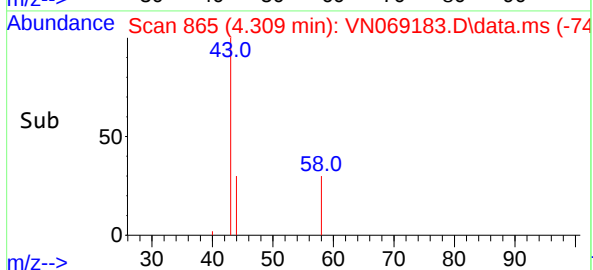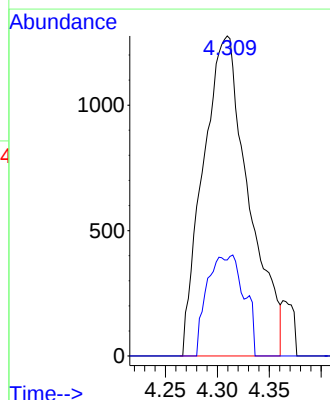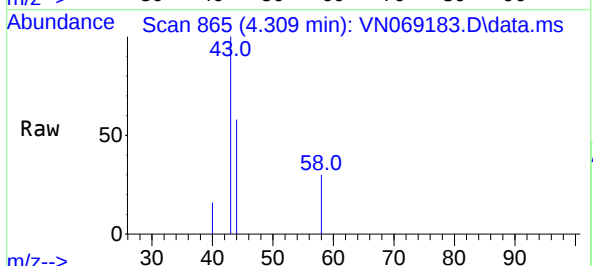




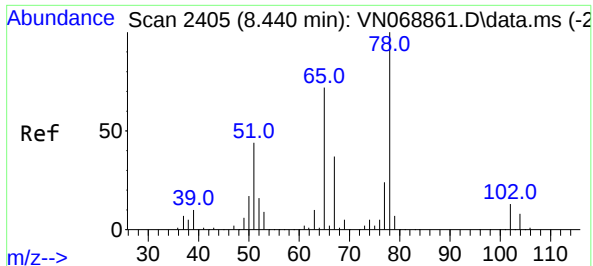


#33

1,2-Dichloroethane-d4
Concen: 49.628 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14

Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS




Tgt Ion: 65 Resp: 225810
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.8

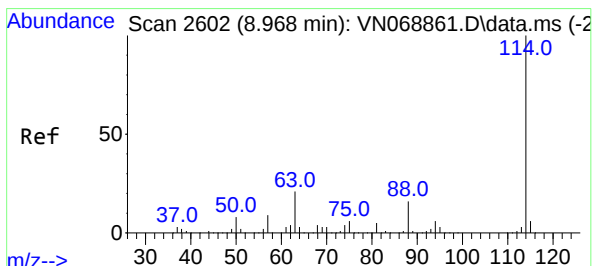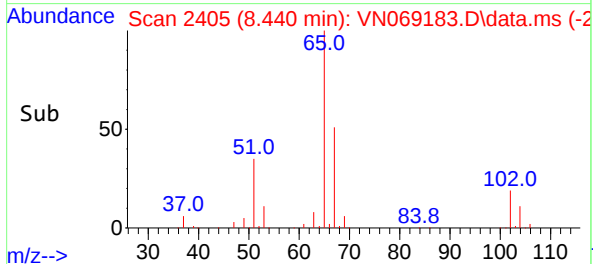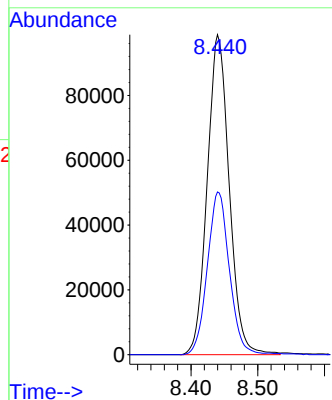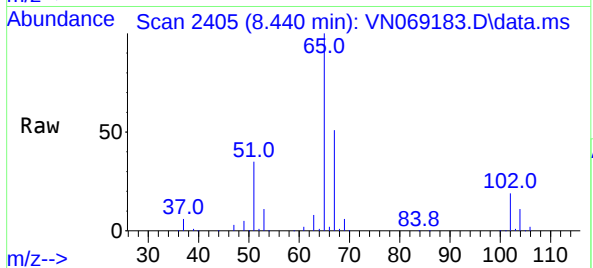


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14

Tgt Ion: 114 Resp: 597484
Ion Ratio Lower Upper
114 100
63 20.5 0.0 42.6
88 15.9 0.0 32.0


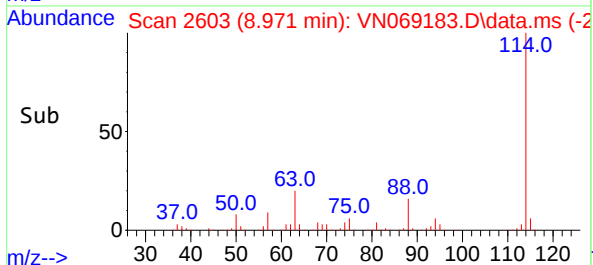
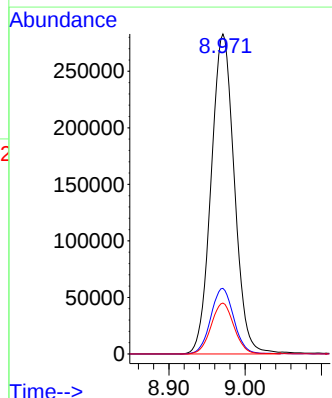
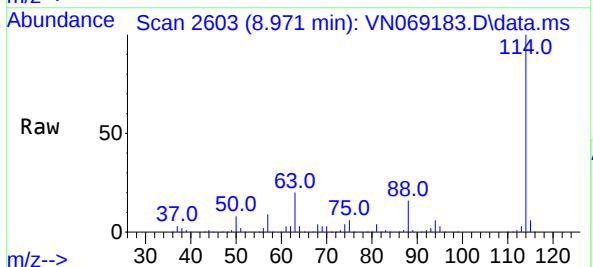


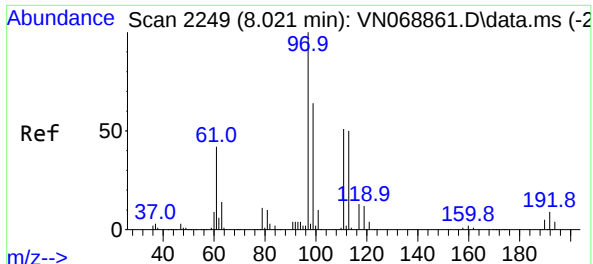

#35
Dibromofluoromethane
Concen: 50.185 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14




Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS


Tgt Ion:113 Resp: 174453
Ion Ratio Lower Upper
113 100
111 104.7 83.2 124.8
192 18.2 15.0 22.4

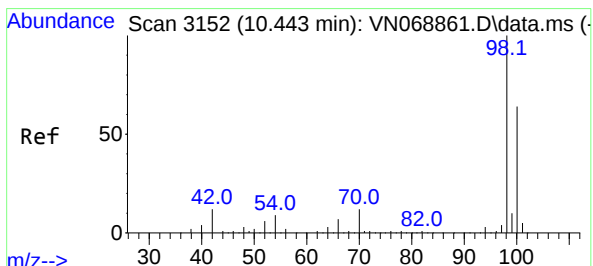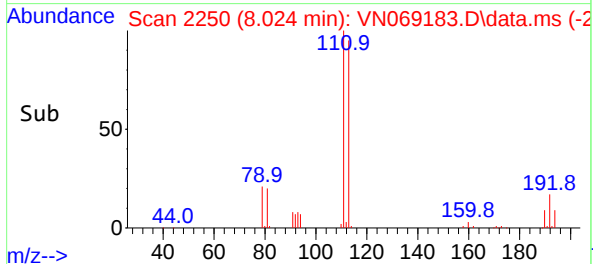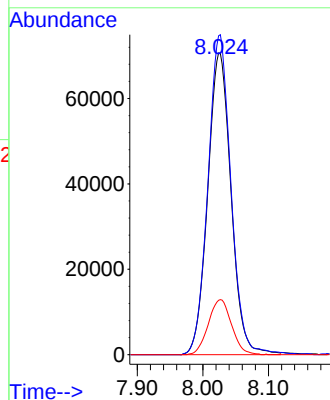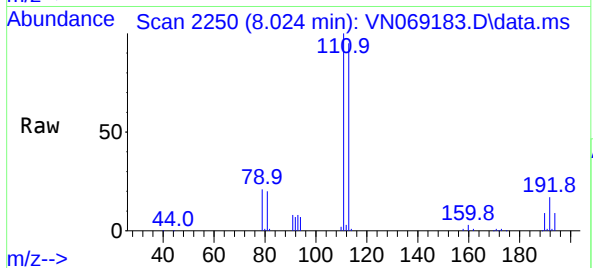

#50
Toluene-d8
Concen: 53.233 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14

Tgt Ion: 98 Resp: 740416
Ion Ratio Lower Upper
98 100
100 64.1 51.5 77.3


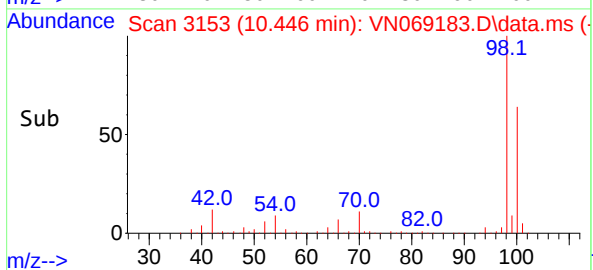
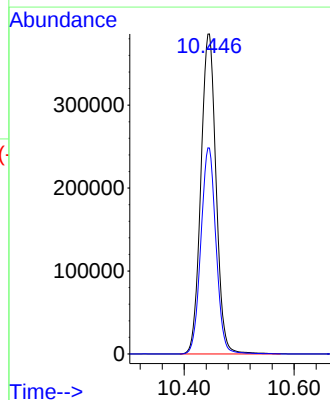
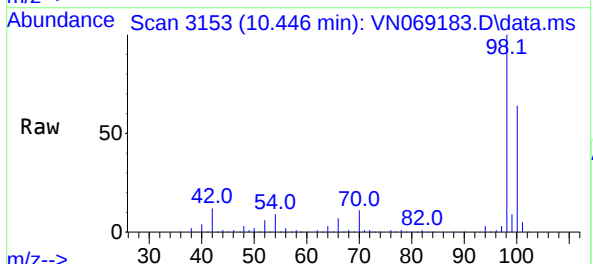


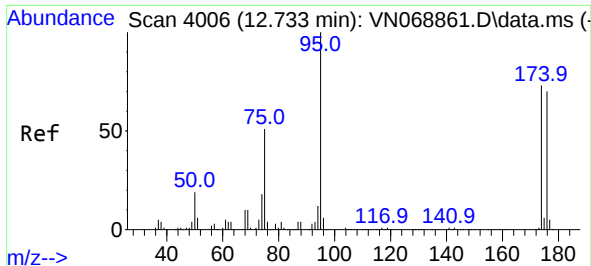

#62
4-Bromofluorobenzene
Concen: 51.274 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14




Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS


Tgt Ion: 95 Resp: 269070
Ion Ratio Lower Upper
95 100
174 74.0 0.0 144.8
176 71.7 0.0 140.0

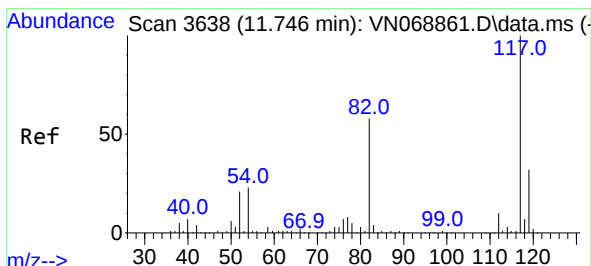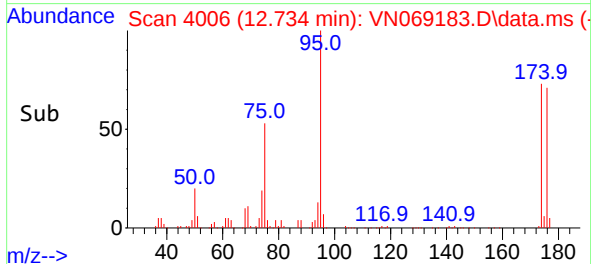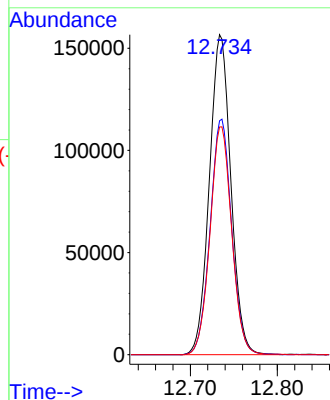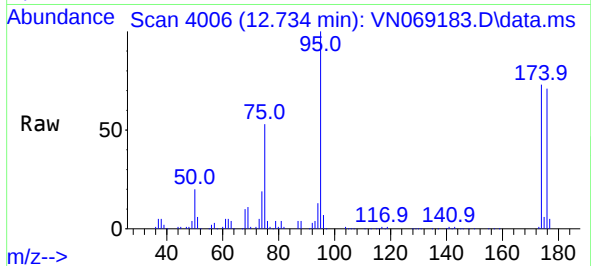

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069183.D
Acq: 26 Oct 2021 14:14

Tgt Ion: 117 Resp: 575868
Ion Ratio Lower Upper
117 100
82 56.3 46.4 69.6
119 31.9 26.0 39.0

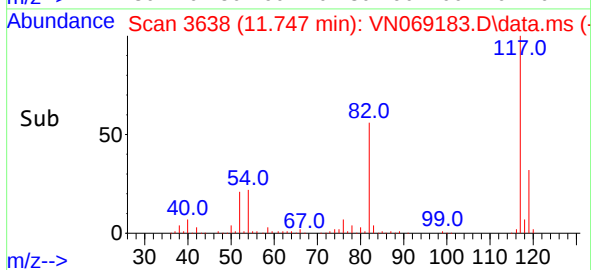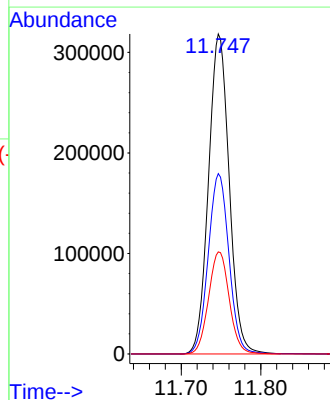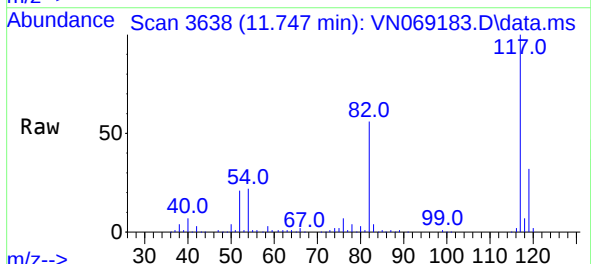

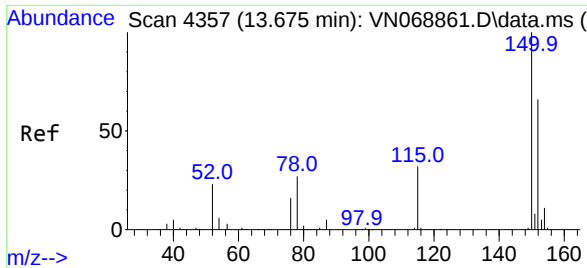

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 4358
 Delta R.T. 0.003 min
 Lab File: VN069183.D
 Acq: 26 Oct 2021 14:14

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-5-PS

Tgt Ion:152 Resp: 220627
 Ion Ratio Lower Upper
 152 100
 115 63.4 31.4 94.3
 150 157.6 0.0 351.0

