

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069201.D
 Acq On : 26 Oct 2021 22:38
 Operator : JC/MD
 Sample : VN1027WBL02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1027WBL02

Quant Time: Oct 27 09:23:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	320406	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	559521	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	541219	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	204227	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	210218	49.762	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.520%
35) Dibromofluoromethane	8.027	113	164982	50.680	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.360%
50) Toluene-d8	10.443	98	694071	53.287	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	106.580%
62) 4-Bromofluorobenzene	12.733	95	253668	51.619	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	103.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069201.D
Acq On : 26 Oct 2021 22:38
Operator : JC/MD
Sample : VN1027WBL02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1027WBL02

Quant Time: Oct 27 09:23:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration




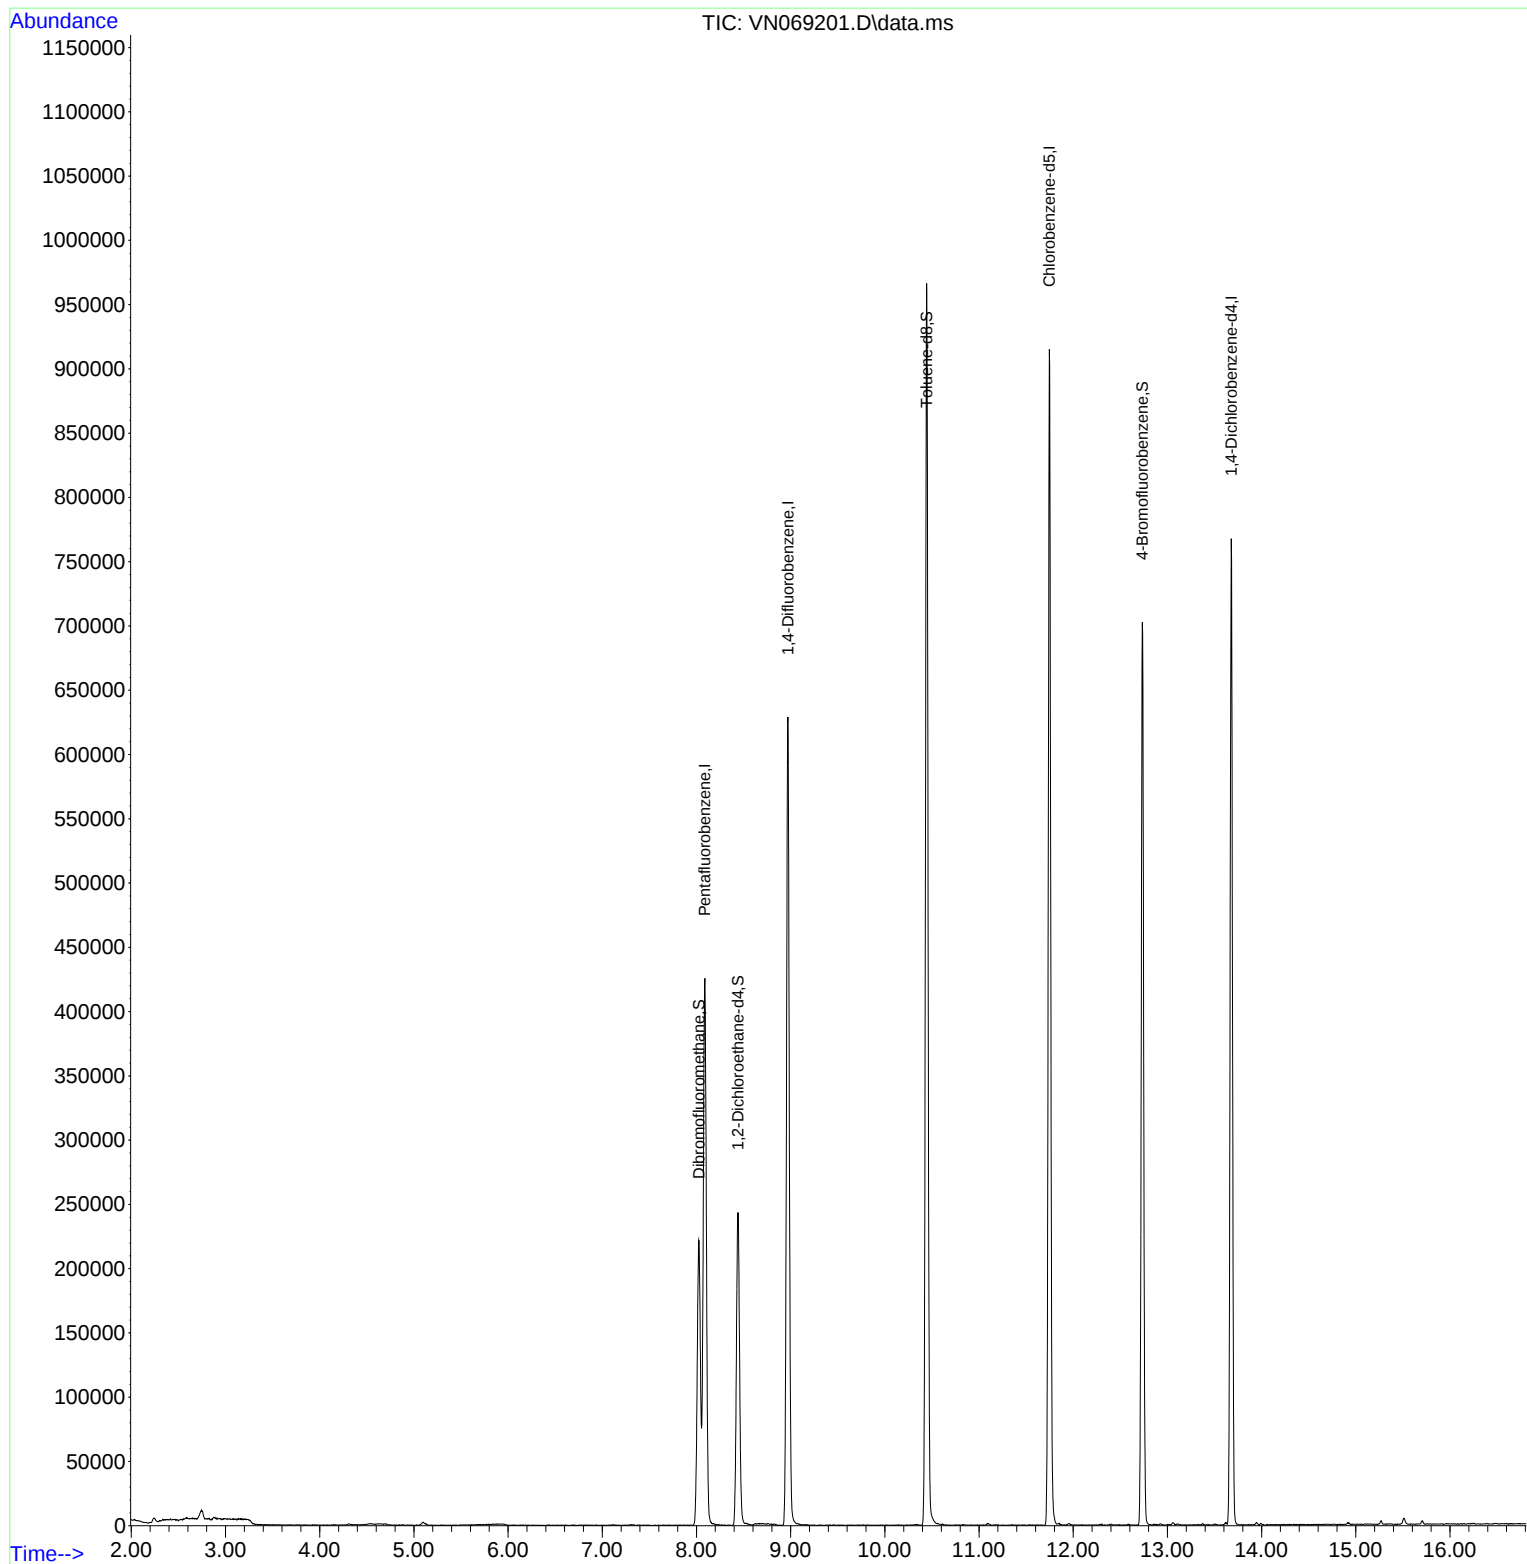


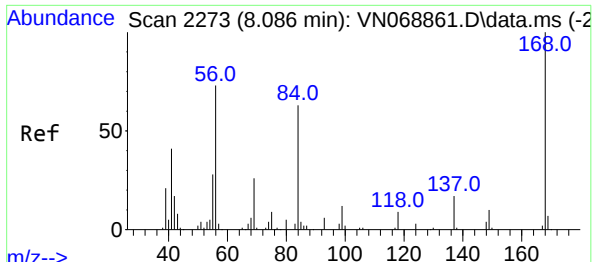

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38




Instrument :
MSVOA_N
ClientSampleId :
VN1027WBL02


Tgt Ion:168 Resp: 320406
Ion Ratio Lower Upper
168 100
99 62.3 48.9 73.3

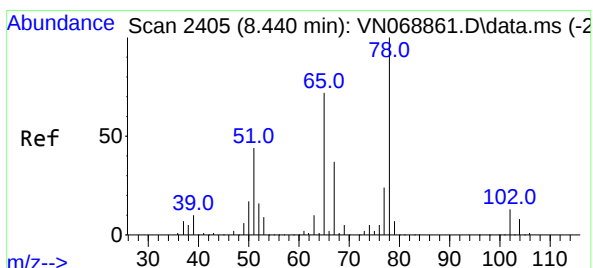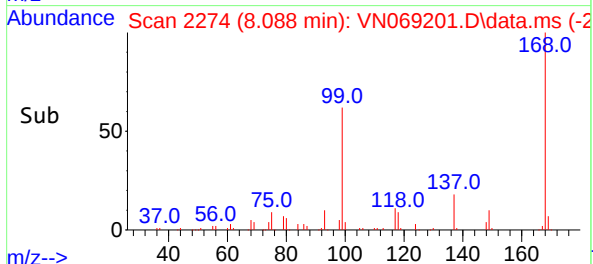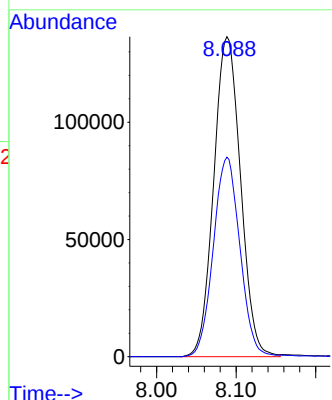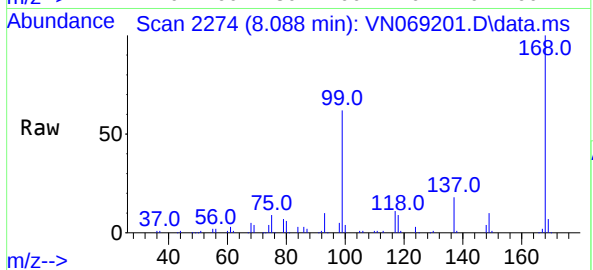

#33
1,2-Dichloroethane-d4
Concen: 49.762 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38

Tgt Ion: 65 Resp: 210218
Ion Ratio Lower Upper
65 100
67 51.8 0.0 103.8

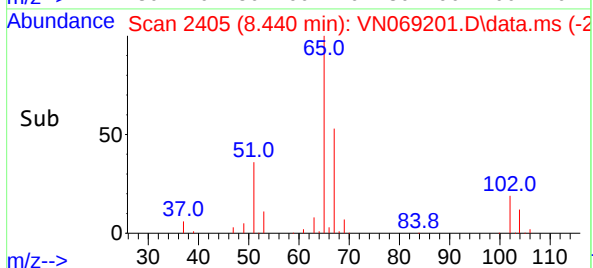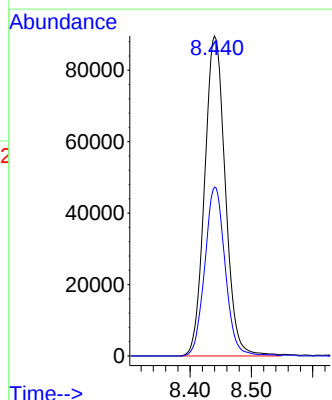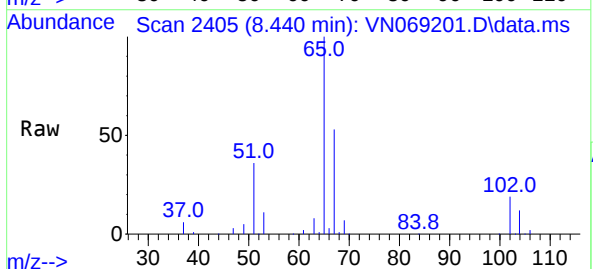




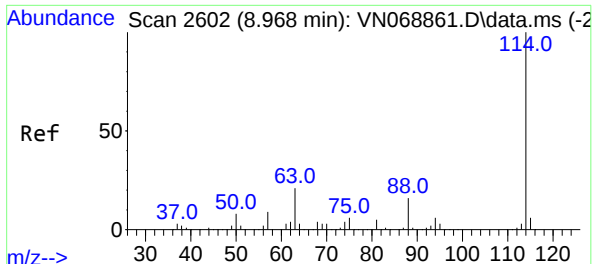


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38

Instrument :
MSVOA_N
ClientSampleId :
VN1027WBL02




Tgt Ion:114 Resp: 559521
Ion Ratio Lower Upper
114 100
63 20.9 0.0 42.6
88 15.8 0.0 32.0

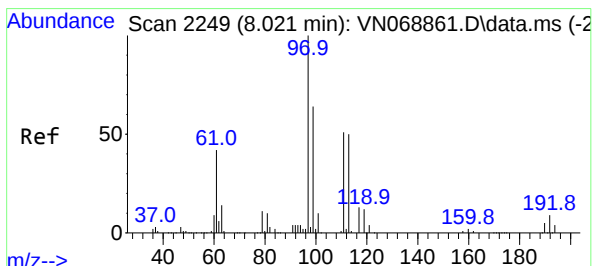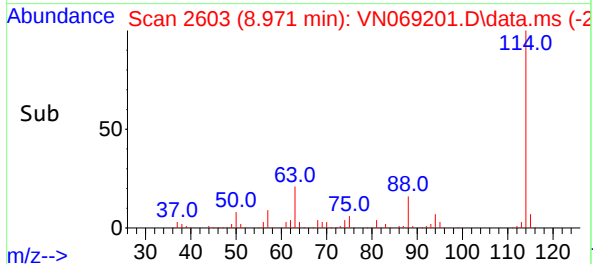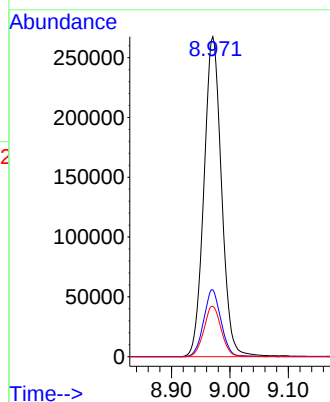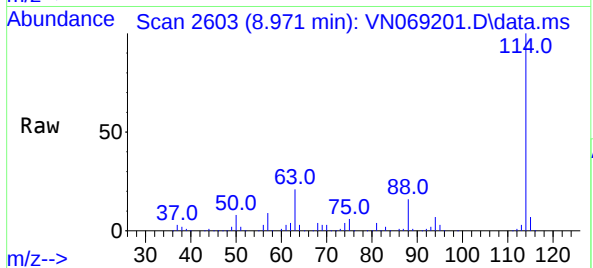


#35

Dibromofluoromethane
Concen: 50.680 ug/l
RT: 8.027 min Scan# 2251
Delta R.T. 0.005 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38

Tgt Ion:113 Resp: 164982
Ion Ratio Lower Upper
113 100
111 101.7 83.2 124.8
192 18.4 15.0 22.4


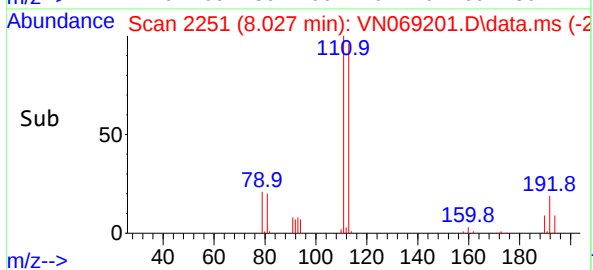
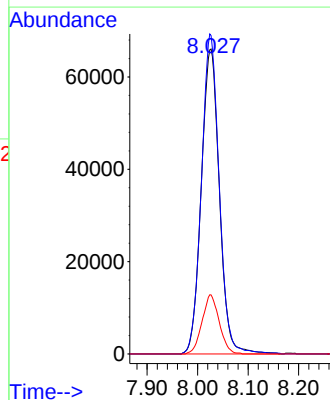
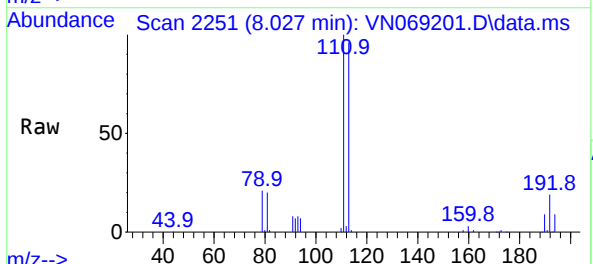


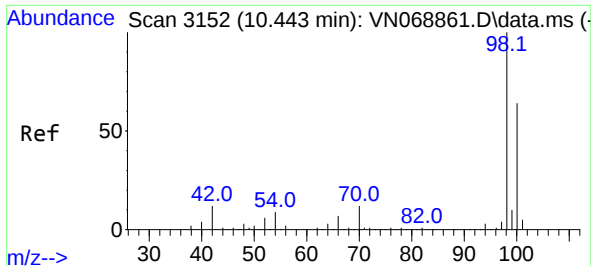

#50
Toluene-d8
Concen: 53.287 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38




Instrument :
MSVOA_N
ClientSampleId :
VN1027WBL02


Tgt Ion: 98 Resp: 694071
Ion Ratio Lower Upper
98 100
100 64.4 51.5 77.3

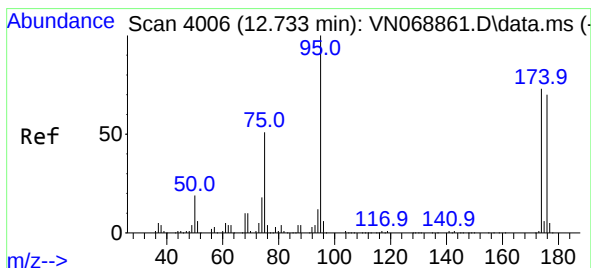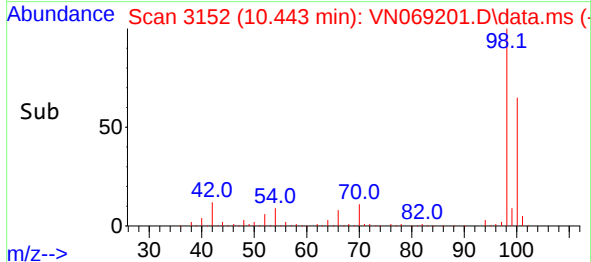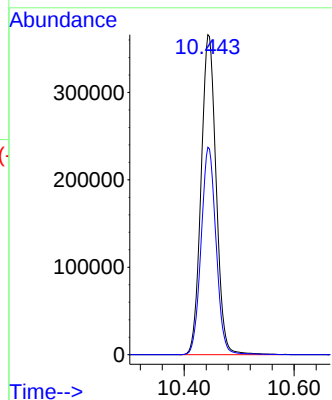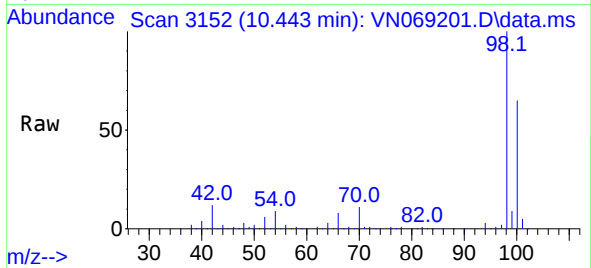

#62
4-Bromofluorobenzene
Concen: 51.619 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38

Tgt Ion: 95 Resp: 253668
Ion Ratio Lower Upper
95 100
174 74.2 0.0 144.8
176 71.5 0.0 140.0


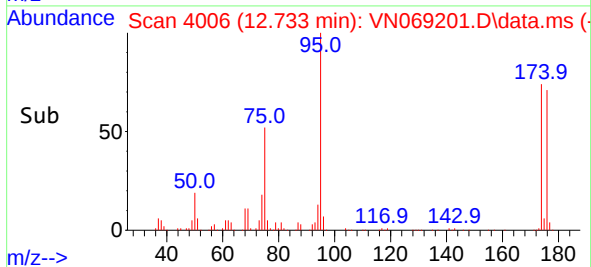
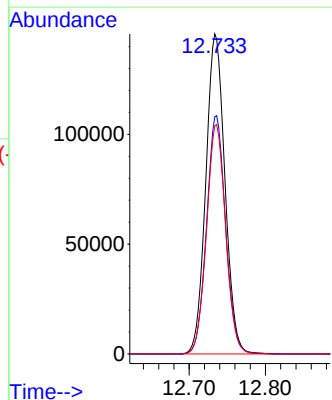
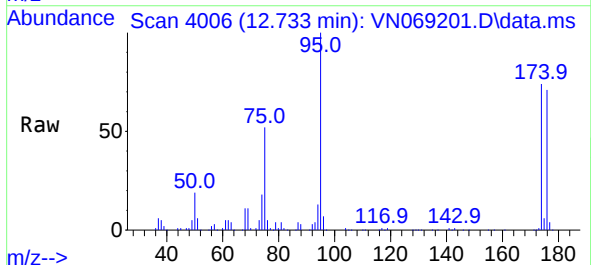


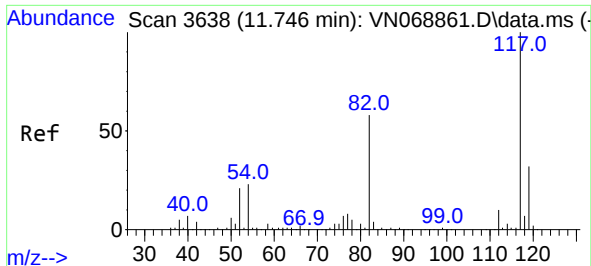

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38

Instrument :
MSVOA_N
ClientSampleId :
VN1027WBL02

Tgt Ion:117 Resp: 541219
Ion Ratio Lower Upper
117 100
82 56.6 46.4 69.6
119 32.4 26.0 39.0

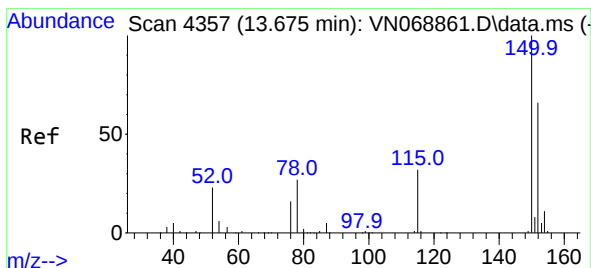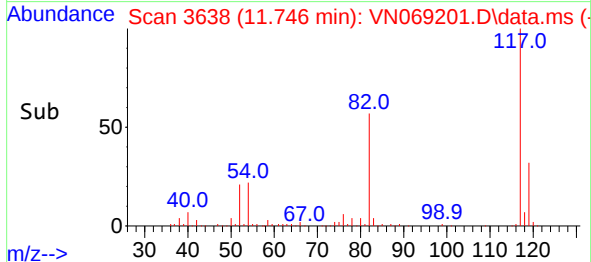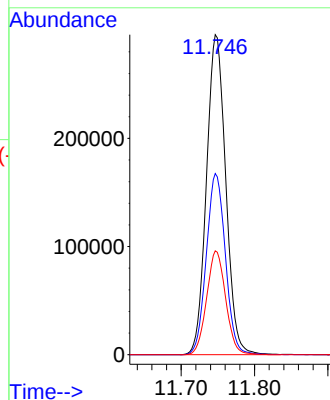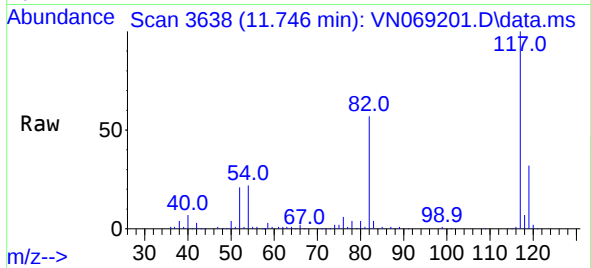

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN069201.D
Acq: 26 Oct 2021 22:38

Tgt Ion:152 Resp: 204227
Ion Ratio Lower Upper
152 100
115 62.5 31.4 94.3
150 156.9 0.0 351.0

