

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069183.D
 Acq On : 26 Oct 2021 14:14
 Operator : JC/MD
 Sample : M4337-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-5-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.578	936	965	995	rBV2	12453	46878	2.41%	0.463%
2	7.313	1962	1985	2006	rBV	15906	47006	2.41%	0.464%
3	8.024	2227	2250	2261	rBV2	237638	564026	28.98%	5.565%
4	8.088	2262	2274	2307	rVB2	463690	1040446	53.45%	10.265%
5	8.440	2385	2405	2433	rBV	263977	602438	30.95%	5.944%
6	8.971	2583	2603	2640	rBV	657528	1390185	71.42%	13.716%
7	10.446	3133	3153	3192	rBV	1011406	1946591	100.00%	19.206%
8	11.747	3619	3638	3670	rBV	977189	1775391	91.21%	17.517%
9	12.734	3989	4006	4033	rBV	752897	1288557	66.20%	12.713%
10	13.678	4342	4358	4382	rVB	810982	1410071	72.44%	13.912%
11	15.509	5028	5041	5056	rVB2	13102	23881	1.23%	0.236%


Sum of corrected areas: 10135470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069183.D
Acq On : 26 Oct 2021 14:14
Operator : JC/MD
Sample : M4337-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

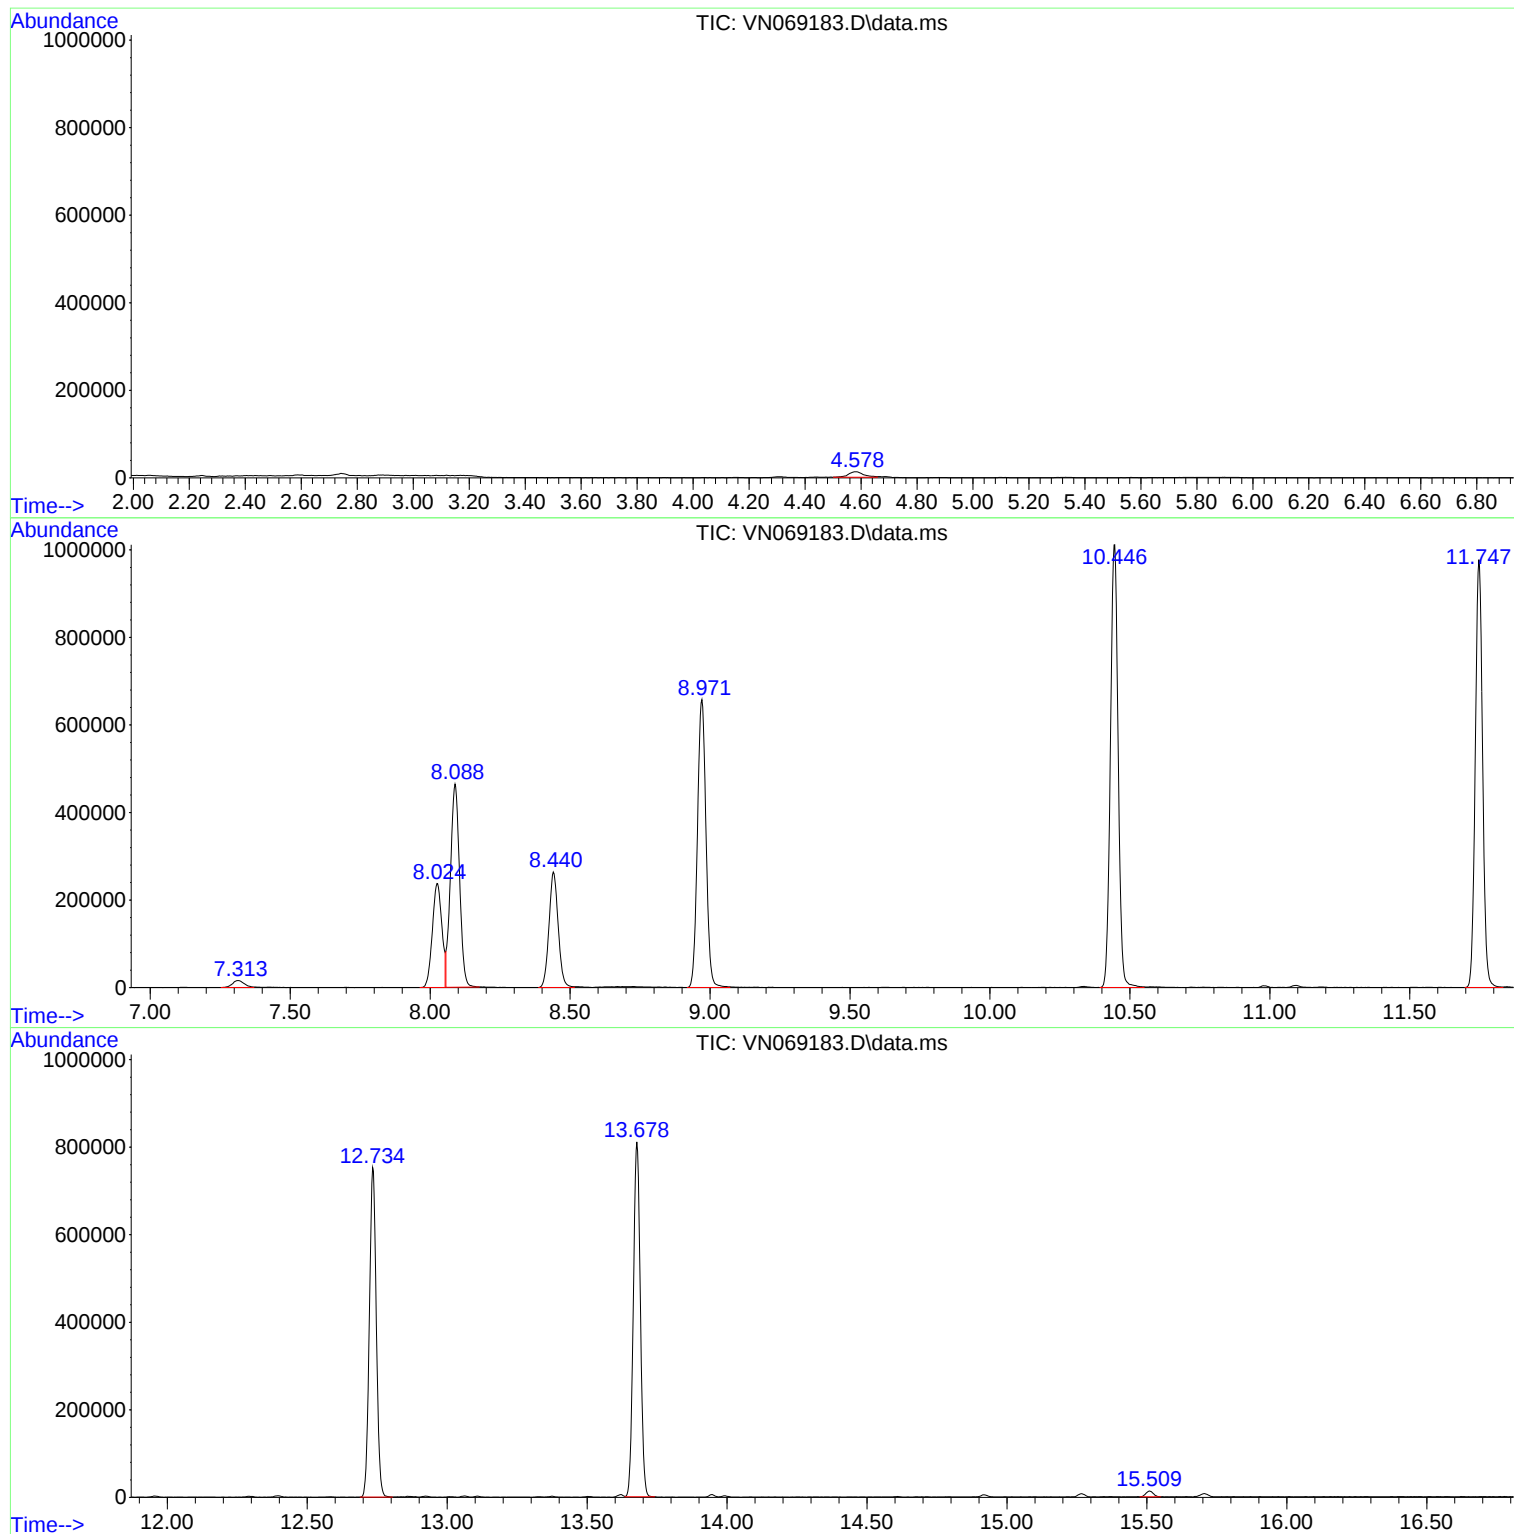

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069183.D
Acq On : 26 Oct 2021 14:14
Operator : JC/MD
Sample : M4337-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069183.D
Acq On : 26 Oct 2021 14:14
Operator : JC/MD
Sample : M4337-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
