

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069187.D
 Acq On : 26 Oct 2021 15:54
 Operator : JC/MD
 Sample : M4337-05
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-6-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.577	943	965	991	rBV2	22280	76710	4.01%	0.767%
2	7.316	1962	1986	2006	rBV2	34450	99540	5.20%	0.995%
3	8.024	2229	2250	2261	rBV	231395	554475	28.98%	5.542%
4	8.088	2262	2274	2306	rVB	448308	1016014	53.10%	10.155%
5	8.440	2384	2405	2430	rBV	258672	594015	31.05%	5.937%
6	8.971	2583	2603	2638	rBV	647661	1362861	71.23%	13.621%
7	10.443	3133	3152	3189	rBV	1012654	1913302	100.00%	19.122%
8	10.979	3339	3352	3366	rBV3	40461	71985	3.76%	0.719%
9	11.746	3620	3638	3667	rBV	942051	1714046	89.59%	17.131%
10	12.733	3987	4006	4030	rBV	727742	1256801	65.69%	12.561%
11	13.677	4340	4358	4386	rBV	798683	1345775	70.34%	13.450%


Sum of corrected areas: 10005524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069187.D
Acq On : 26 Oct 2021 15:54
Operator : JC/MD
Sample : M4337-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-6-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

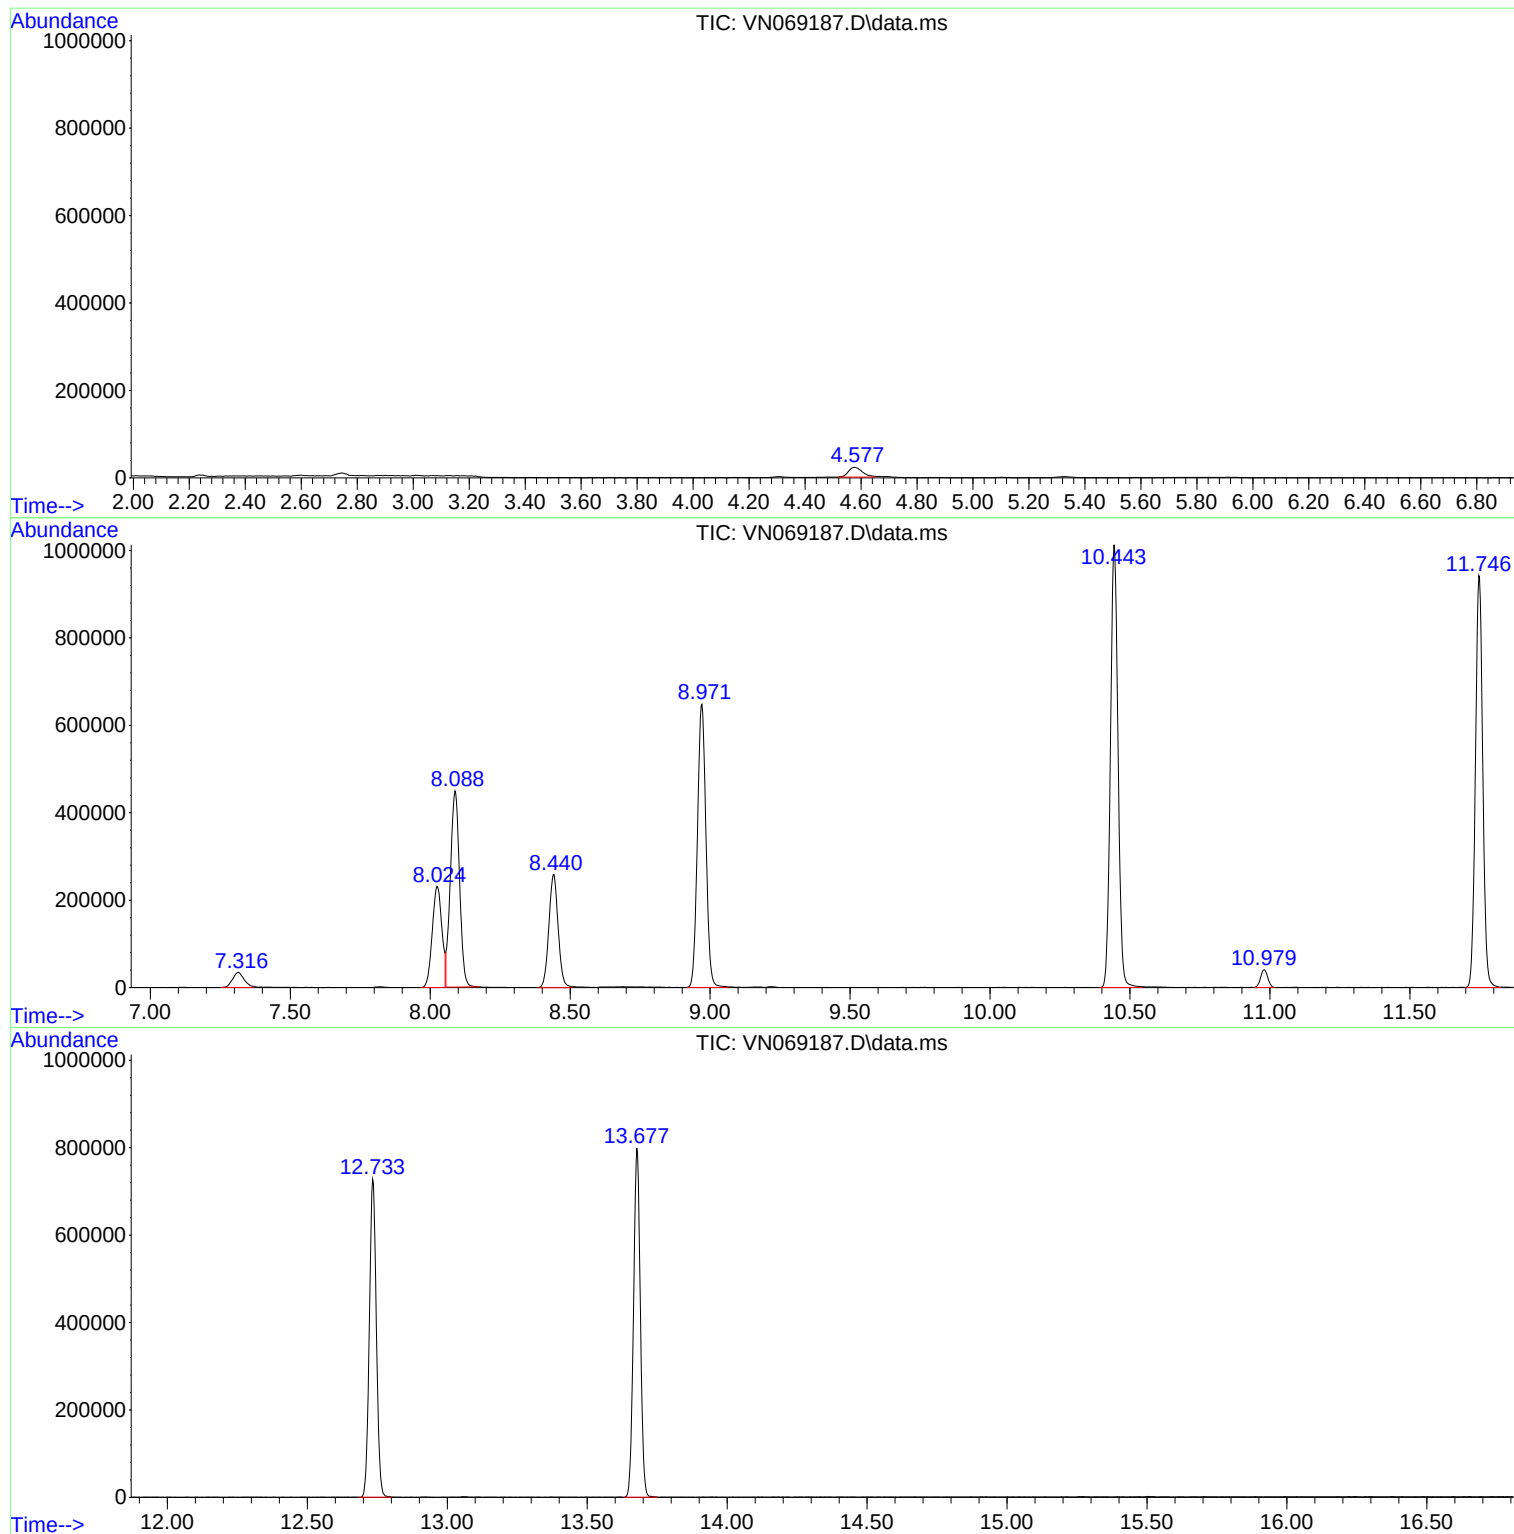

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069187.D
Acq On : 26 Oct 2021 15:54
Operator : JC/MD
Sample : M4337-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-6-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069187.D
Acq On : 26 Oct 2021 15:54
Operator : JC/MD
Sample : M4337-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-6-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
